

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010821\
 Data File : PP032617.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2021 12:16
 Operator : DD\AJ
 Sample : M1044-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 03:16:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.748	4.031	1484582	1281085	27.147	26.468
2) SA Decachlor...	10.585	9.316	1078727	1032084	24.096	23.244

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010821\
Data File : PP032617.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 12:16
Operator : DD\AJ
Sample : M1044-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:16:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

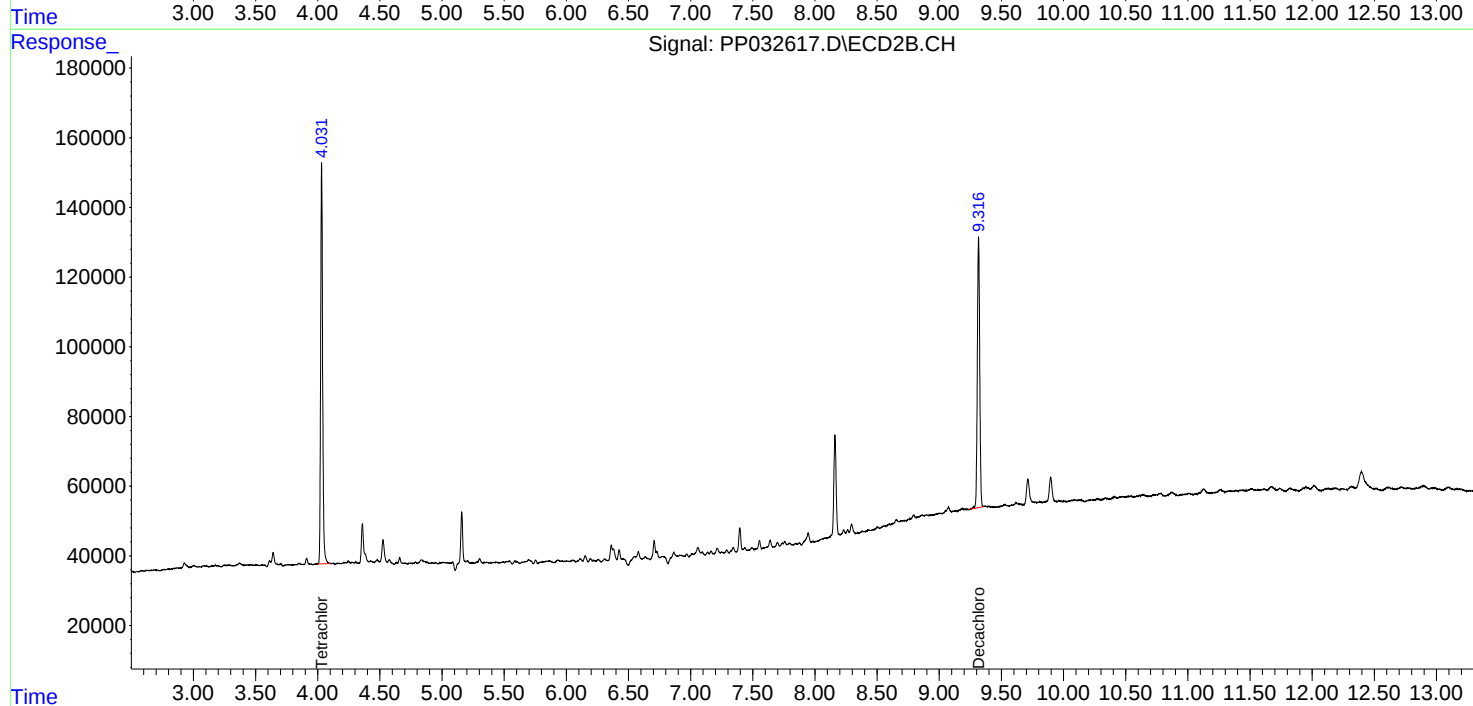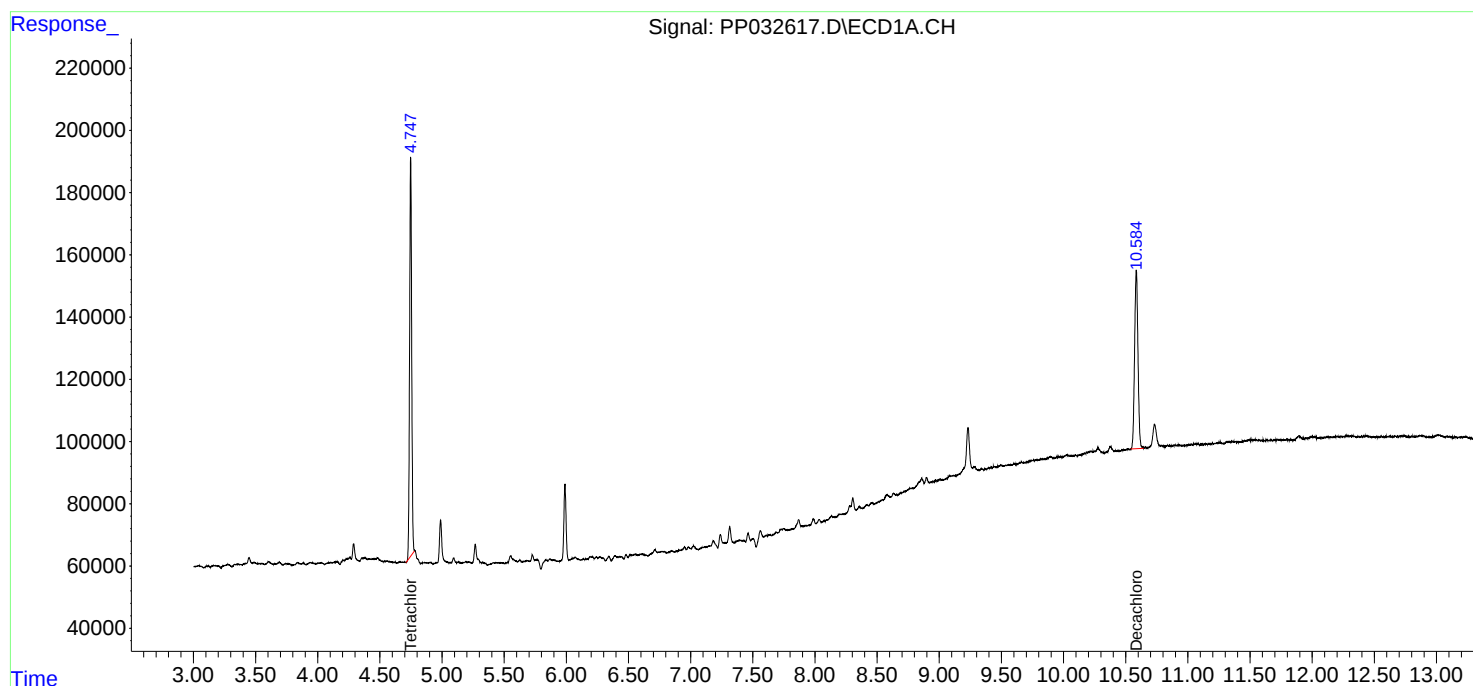


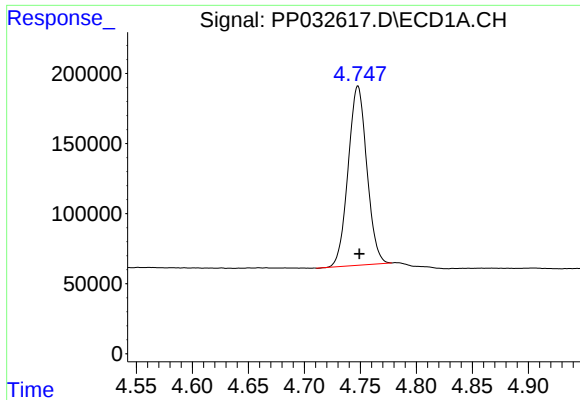

#1 Tetrachloro-m-xylene


R.T.: 4.748 min
Delta R.T.: -0.001 min
Response: 1484582
Conc: 27.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-4

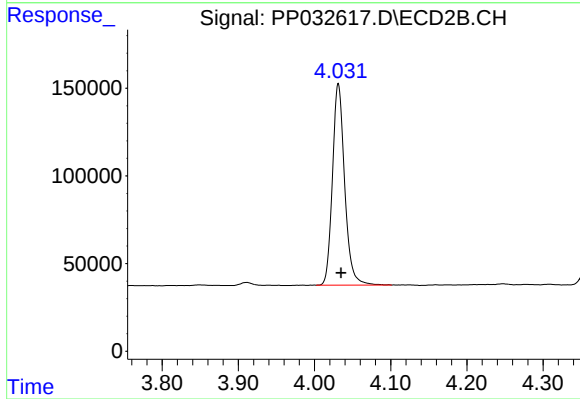


#1 Tetrachloro-m-xylene

R.T.: 4.031 min
Delta R.T.: -0.004 min
Response: 1281085
Conc: 26.47 ng/ml

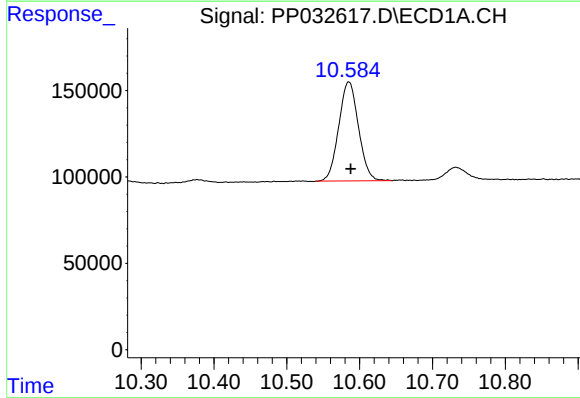

#2 Decachlorobiphenyl

R.T.: 10.585 min
Delta R.T.: -0.003 min
Response: 1078727
Conc: 24.10 ng/ml

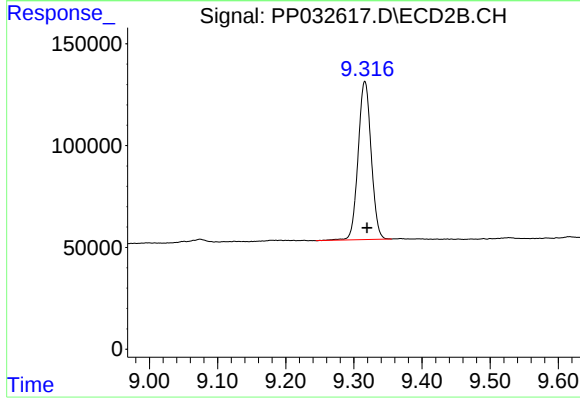

#2 Decachlorobiphenyl

R.T.: 9.316 min
Delta R.T.: -0.003 min
Response: 1032084
Conc: 23.24 ng/ml