

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010821\
 Data File : PP032622.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2021 13:55
 Operator : DD\AJ
 Sample : M1044-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-10

Manual Integrations
 APPROVED

Ankita
 1/11/2021 11:11:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 03:18:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.746	4.031	1693338	1353708	30.964	27.968
2) SA Decachlor...	10.582	9.316	1175578	1153378	26.259	25.976
Target Compounds						
26) L6 AR-1254-1	6.953	6.150	173451	191362	87.072m	76.218
27) L6 AR-1254-2	7.181	6.308	197583	95788	65.219	44.698 #
28) L6 AR-1254-3	7.558	6.728	242223	269563	74.348	75.375
29) L6 AR-1254-4	7.851	6.969	98794	81617	42.876m	39.623
30) L6 AR-1254-5	8.278	7.395	193368	239358	78.741	77.403m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010821\
Data File : PP032622.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 13:55
Operator : DD\AJ
Sample : M1044-09
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
TP-10


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:18:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

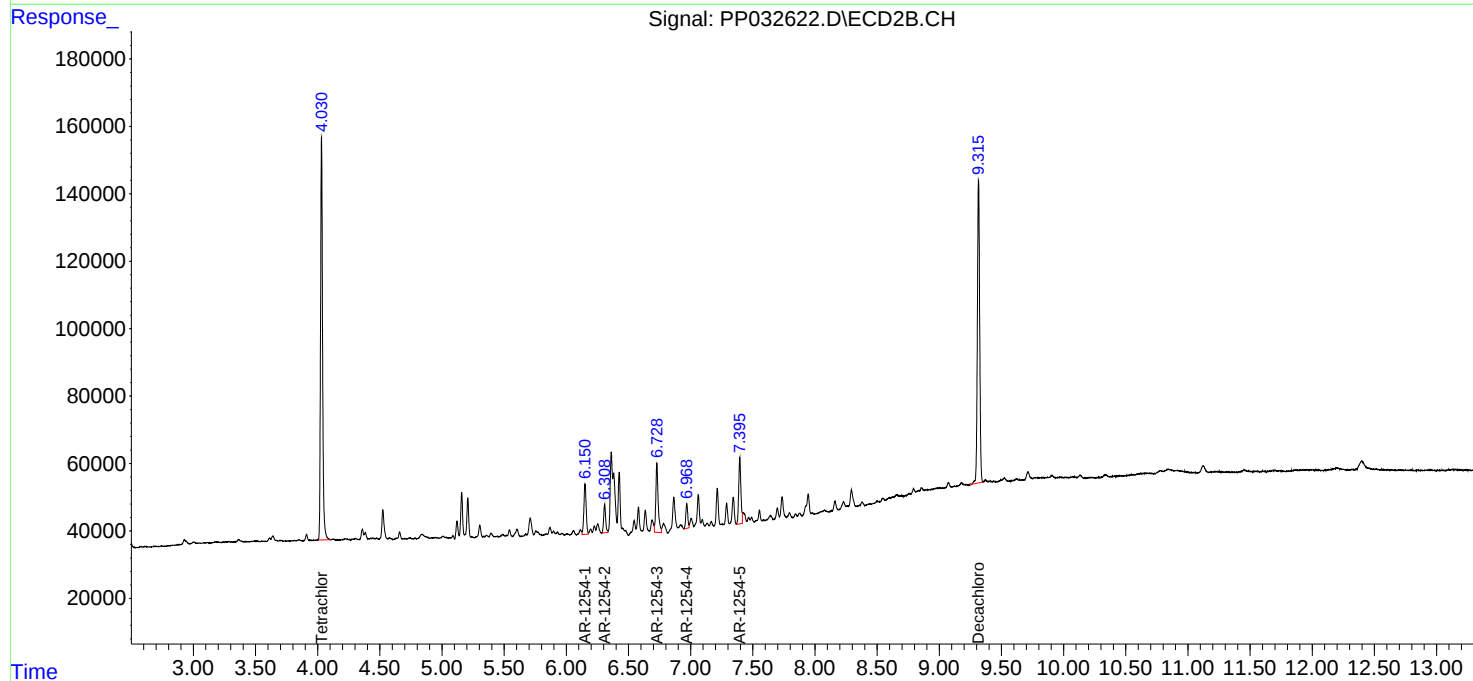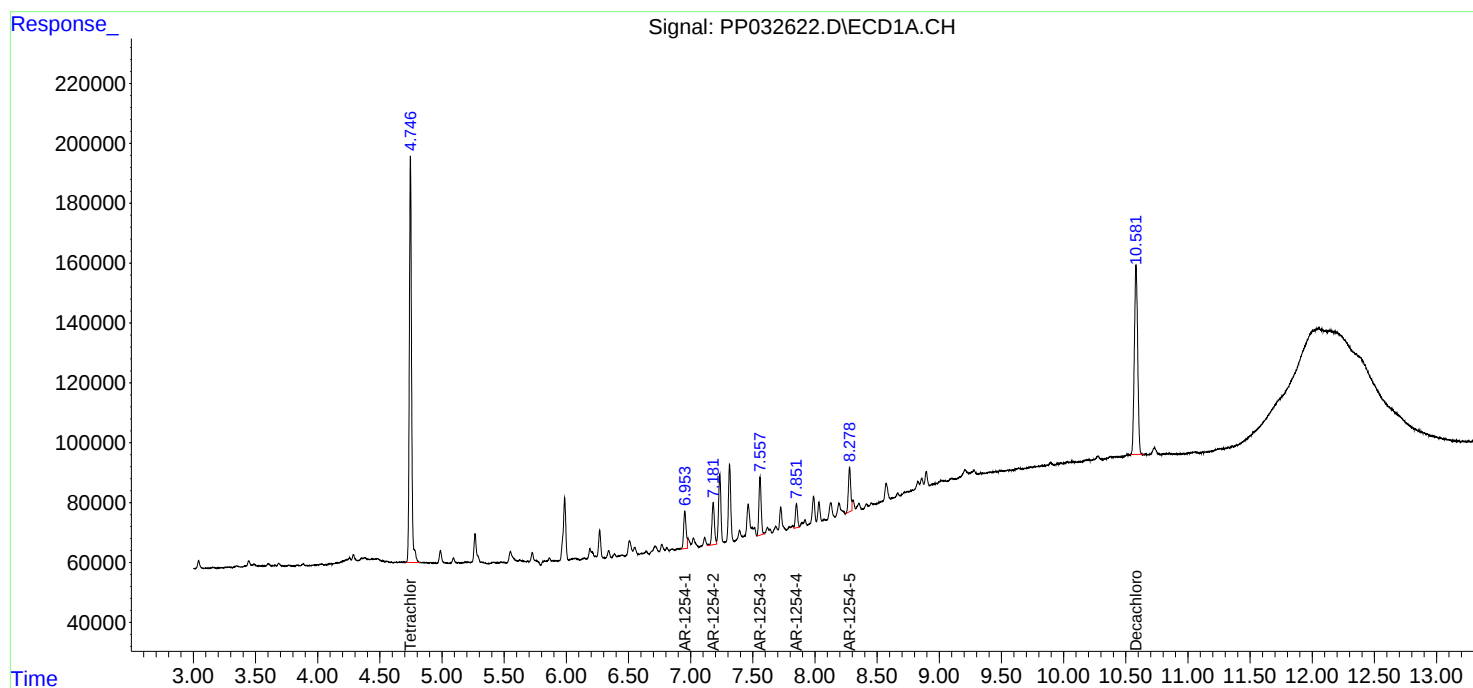

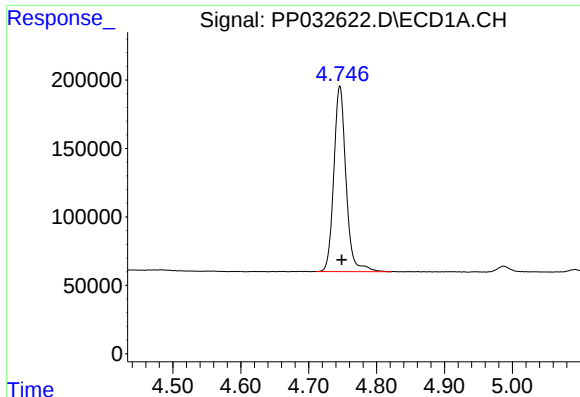


#1 Tetrachloro-m-xylene

R.T.: 4.746 min
Delta R.T.: -0.003 min
Response: 1693338
Conc: 30.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:57 AM

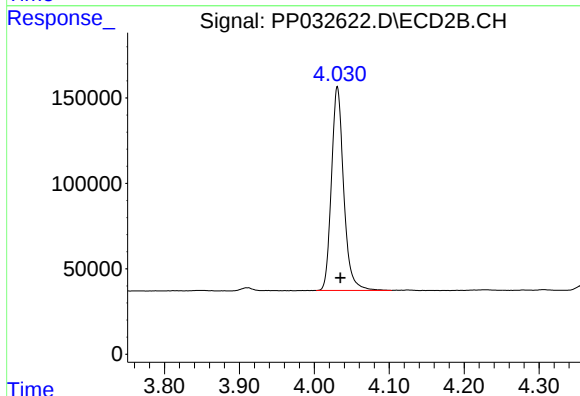


#1 Tetrachloro-m-xylene

R.T.: 4.031 min
Delta R.T.: -0.004 min
Response: 1353708
Conc: 27.97 ng/ml

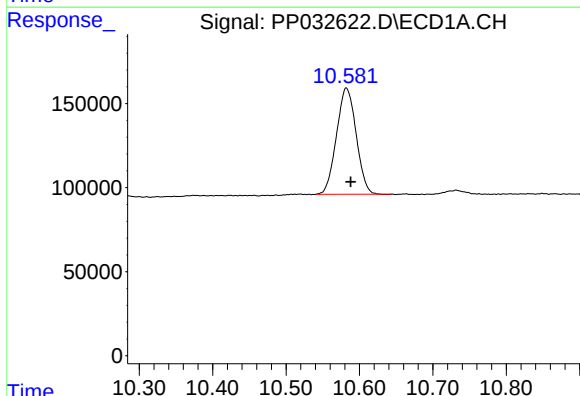


#2 Decachlorobiphenyl

R.T.: 10.582 min
Delta R.T.: -0.006 min
Response: 1175578
Conc: 26.26 ng/ml

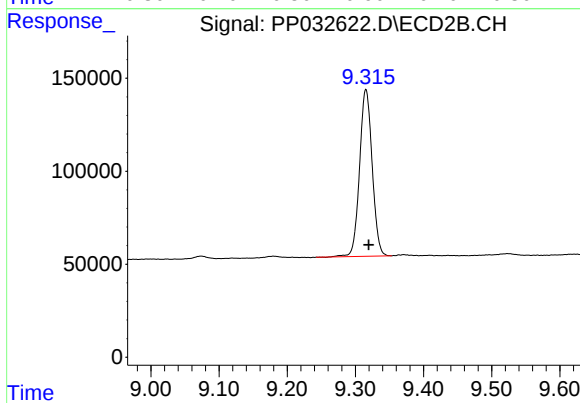

#2 Decachlorobiphenyl

R.T.: 9.316 min
Delta R.T.: -0.004 min
Response: 1153378
Conc: 25.98 ng/ml

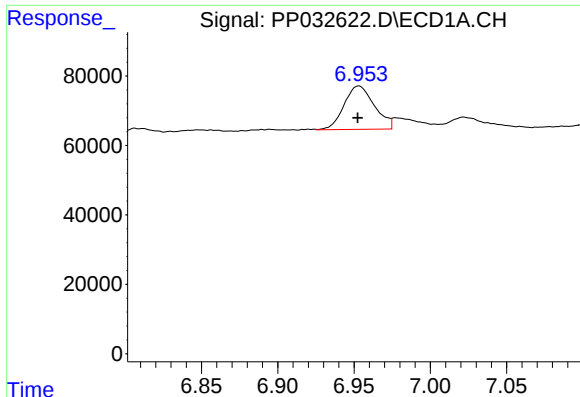


#26 AR-1254-1

R.T.: 6.953 min
Delta R.T.: 0.000 min
Response: 173451
Conc: 87.07 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:57 AM

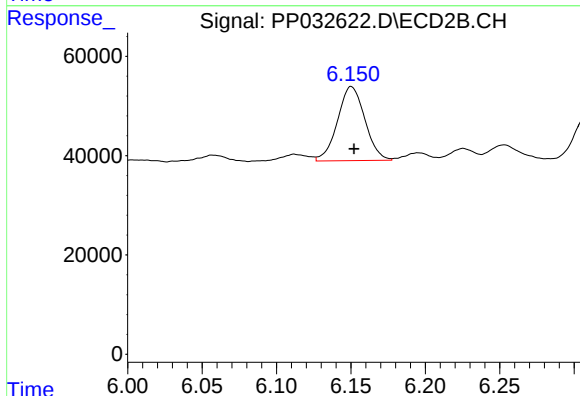


#26 AR-1254-1

R.T.: 6.150 min
Delta R.T.: -0.002 min
Response: 191362
Conc: 76.22 ng/ml

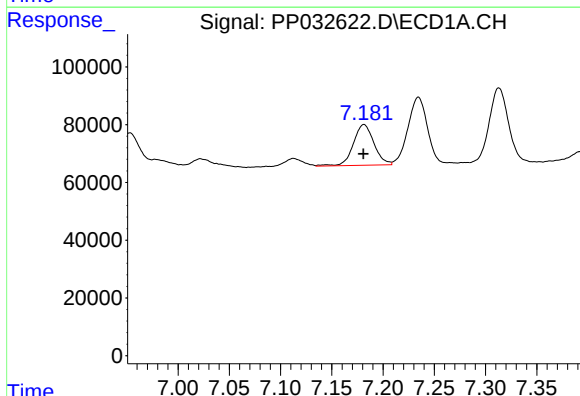


#27 AR-1254-2

R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 197583
Conc: 65.22 ng/ml

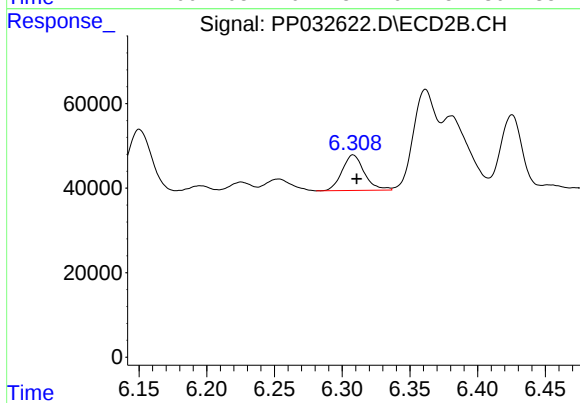

#27 AR-1254-2

R.T.: 6.308 min
Delta R.T.: -0.003 min
Response: 95788
Conc: 44.70 ng/ml

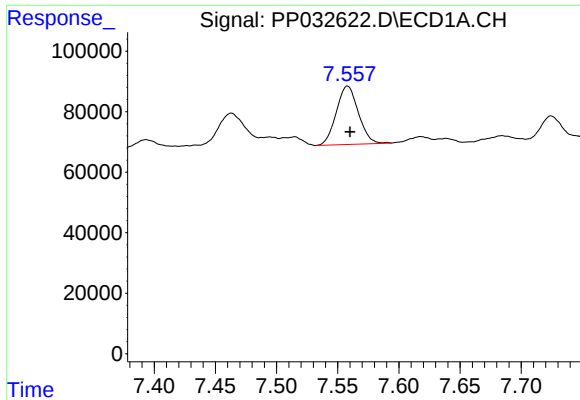


#28 AR-1254-3

R.T.: 7.558 min
Delta R.T.: -0.002 min
Response: 242223
Conc: 74.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-10


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:57 AM

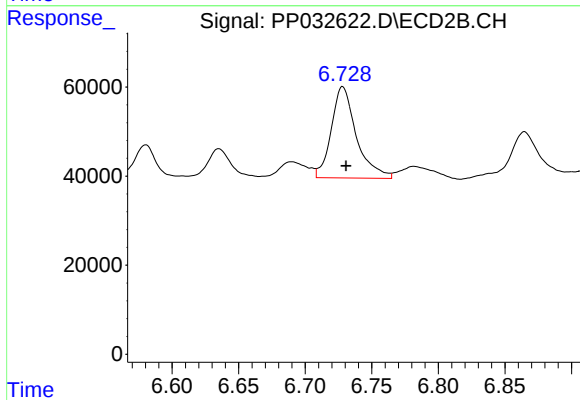


#28 AR-1254-3

R.T.: 6.728 min
Delta R.T.: -0.003 min
Response: 269563
Conc: 75.37 ng/ml

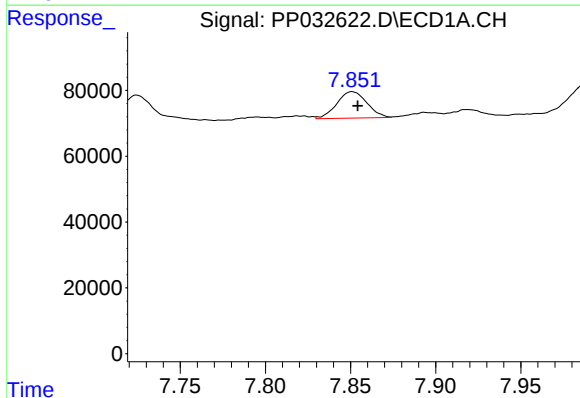


#29 AR-1254-4

R.T.: 7.851 min
Delta R.T.: -0.004 min
Response: 98794
Conc: 42.88 ng/ml m

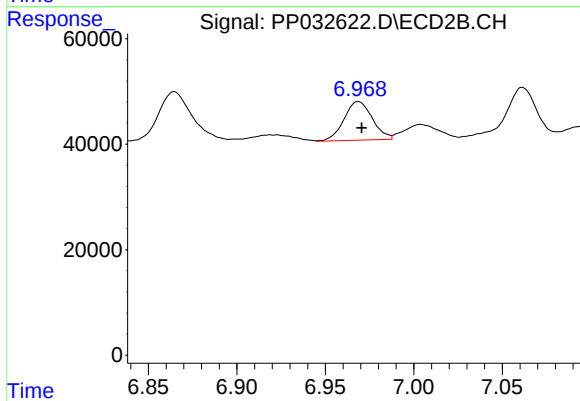

#29 AR-1254-4

R.T.: 6.969 min
Delta R.T.: -0.002 min
Response: 81617
Conc: 39.62 ng/ml

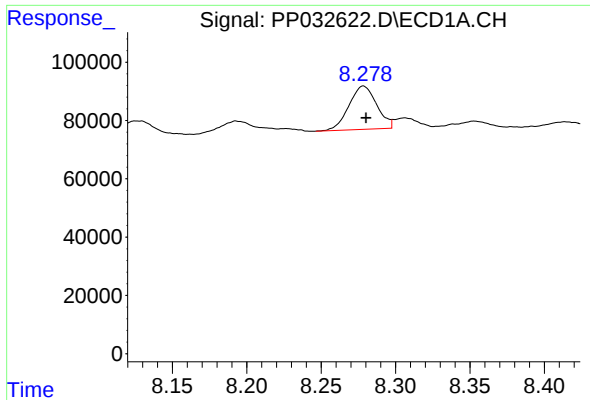


#30 AR-1254-5

R.T.: 8.278 min
Delta R.T.: -0.002 min
Response: 193368
Conc: 78.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-10

Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:57 AM

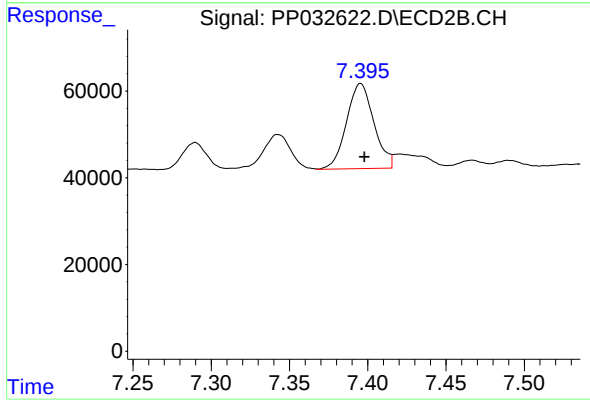

#30 AR-1254-5

R.T.: 7.395 min
Delta R.T.: -0.003 min
Response: 239358
Conc: 77.40 ng/ml m