

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010821\
 Data File : PP032623.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2021 14:12
 Operator : DD\AJ
 Sample : M1044-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-11

Manual Integrations
 APPROVED

Ankita
 1/11/2021 11:11:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 03:18:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.746	4.032	1631139	1324321	29.826	27.361
2) SA Decachlor...	10.584	9.315	1205100	1140697	26.918	25.691m
Target Compounds						
26) L6 AR-1254-1	6.952	6.151	586856	645405	294.601m	257.059
27) L6 AR-1254-2	7.181	6.309	718261	409828	237.086	191.239
28) L6 AR-1254-3	7.558	6.729	895534	930412	274.874	260.161
29) L6 AR-1254-4	7.852	6.969	446540	367560	193.797	178.440
30) L6 AR-1254-5	8.278	7.395	812644	815328	330.912	263.661m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010821\
Data File : PP032623.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 14:12
Operator : DD\AJ
Sample : M1044-11
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:18:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

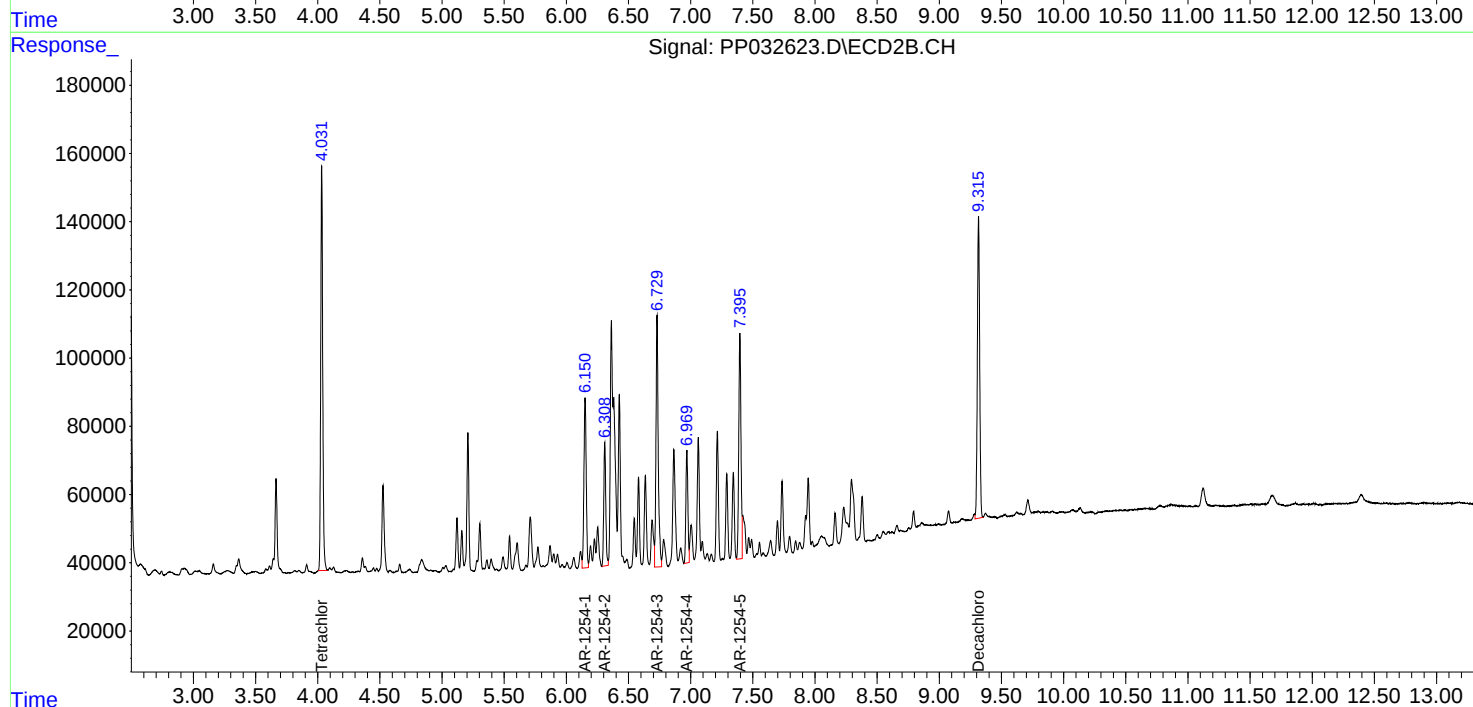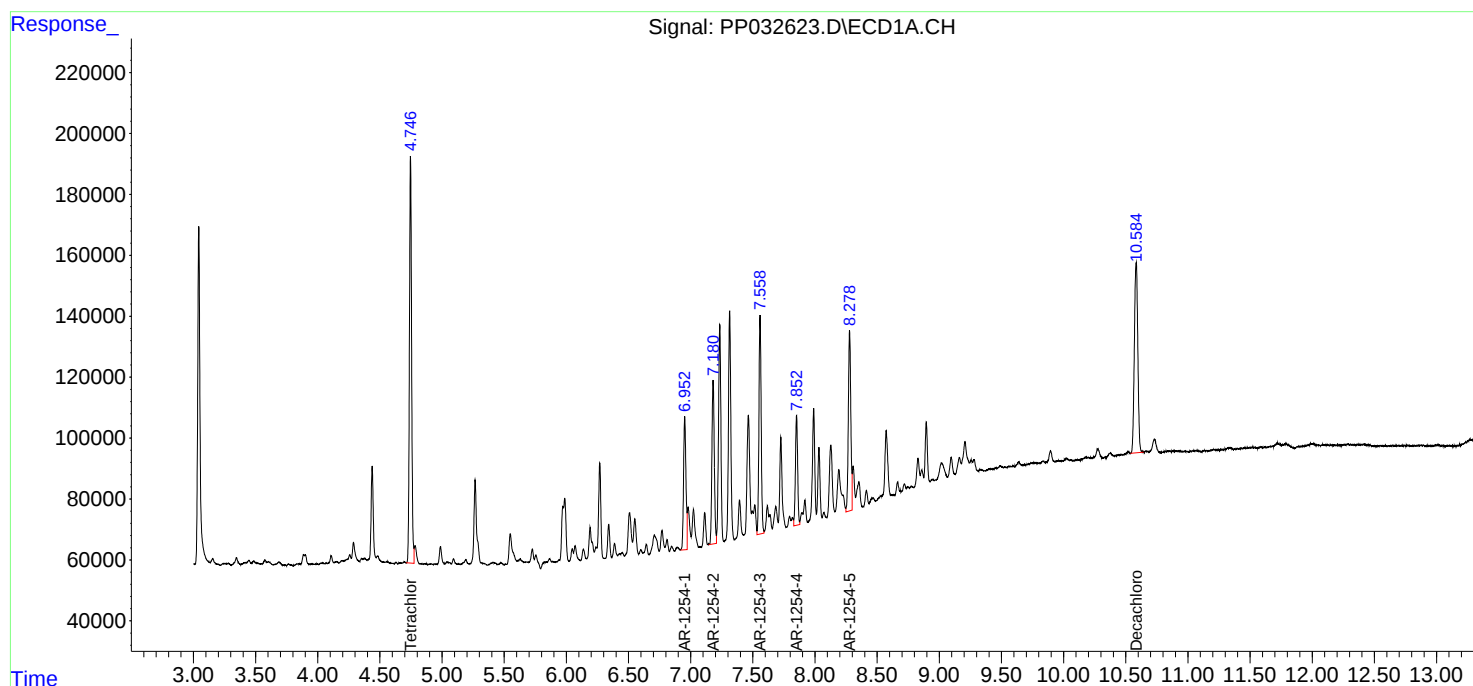

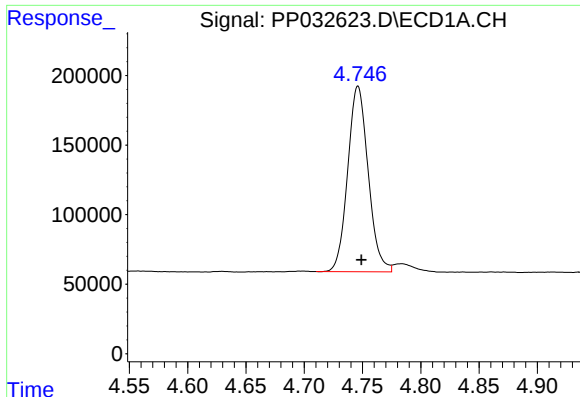


#1 Tetrachloro-m-xylene

R.T.: 4.746 min
Delta R.T.: -0.003 min
Response: 1631139
Conc: 29.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:59 AM

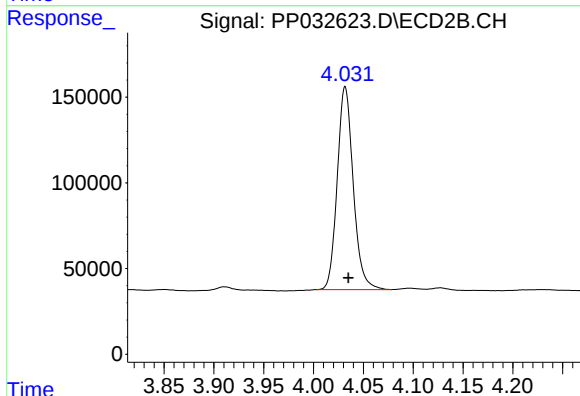


#1 Tetrachloro-m-xylene

R.T.: 4.032 min
Delta R.T.: -0.003 min
Response: 1324321
Conc: 27.36 ng/ml

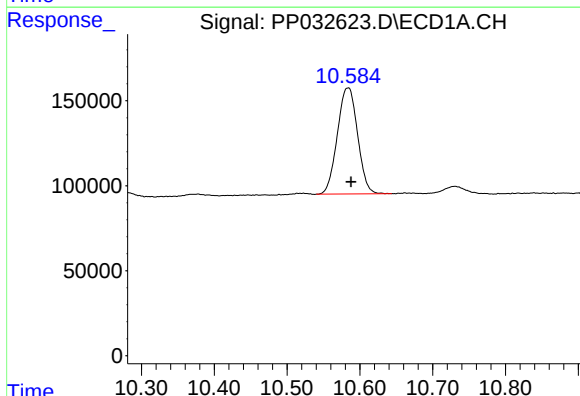


#2 Decachlorobiphenyl

R.T.: 10.584 min
Delta R.T.: -0.004 min
Response: 1205100
Conc: 26.92 ng/ml

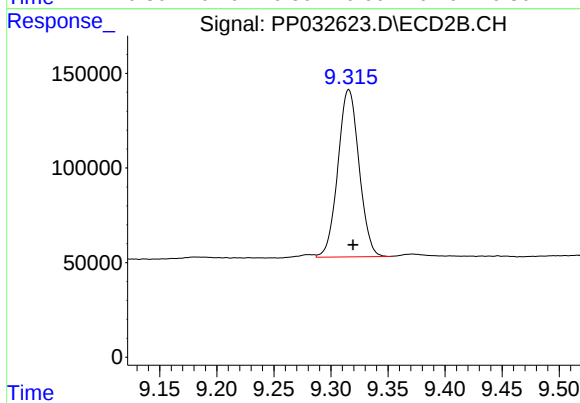

#2 Decachlorobiphenyl

R.T.: 9.315 min
Delta R.T.: -0.004 min
Response: 1140697
Conc: 25.69 ng/ml m

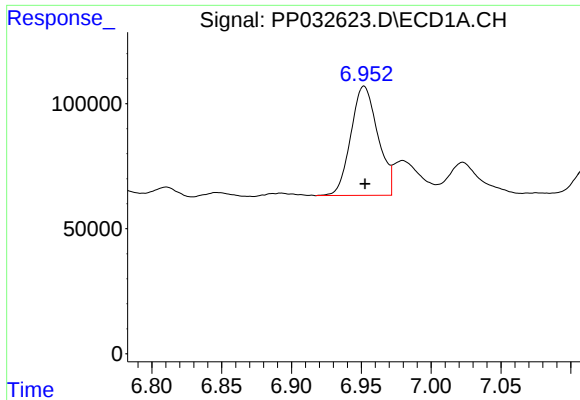


#26 AR-1254-1

R.T.: 6.952 min
Delta R.T.: 0.000 min
Response: 586856
Conc: 294.60 ng/ml m

Instrument :
ECD_P
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:59 AM

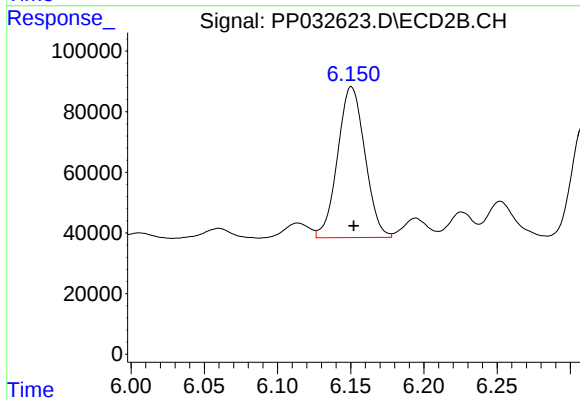


#26 AR-1254-1

R.T.: 6.151 min
Delta R.T.: -0.002 min
Response: 645405
Conc: 257.06 ng/ml

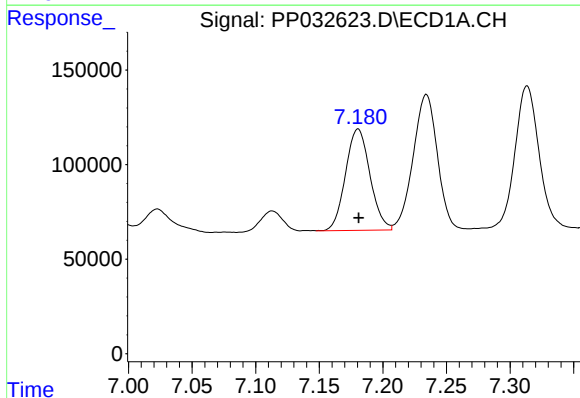


#27 AR-1254-2

R.T.: 7.181 min
Delta R.T.: 0.000 min
Response: 718261
Conc: 237.09 ng/ml

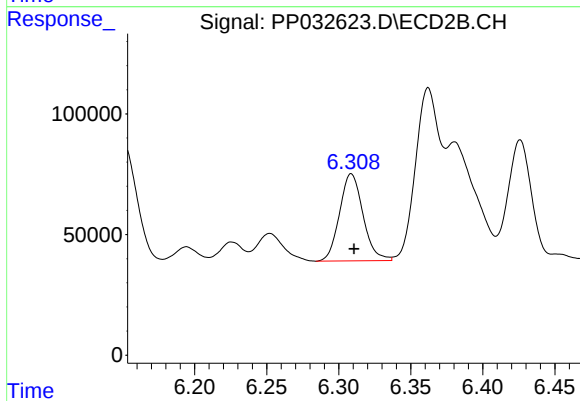

#27 AR-1254-2

R.T.: 6.309 min
Delta R.T.: -0.002 min
Response: 409828
Conc: 191.24 ng/ml

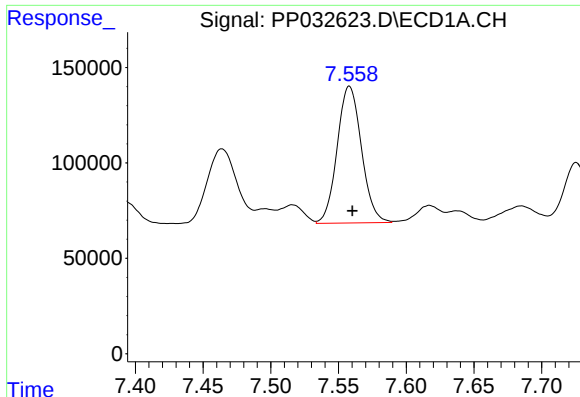


#28 AR-1254-3

R.T.: 7.558 min
Delta R.T.: -0.002 min
Response: 895534
Conc: 274.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-11


Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:59 AM

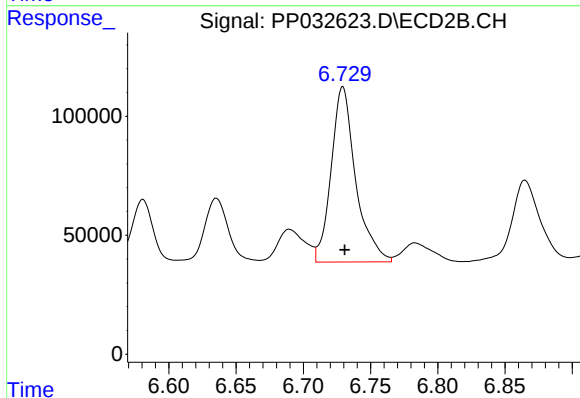


#28 AR-1254-3

R.T.: 6.729 min
Delta R.T.: -0.001 min
Response: 930412
Conc: 260.16 ng/ml

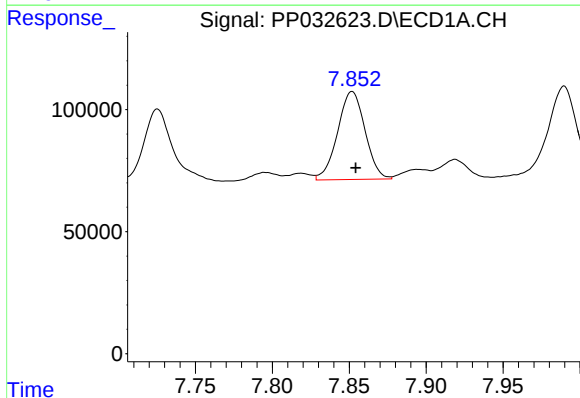


#29 AR-1254-4

R.T.: 7.852 min
Delta R.T.: -0.002 min
Response: 446540
Conc: 193.80 ng/ml

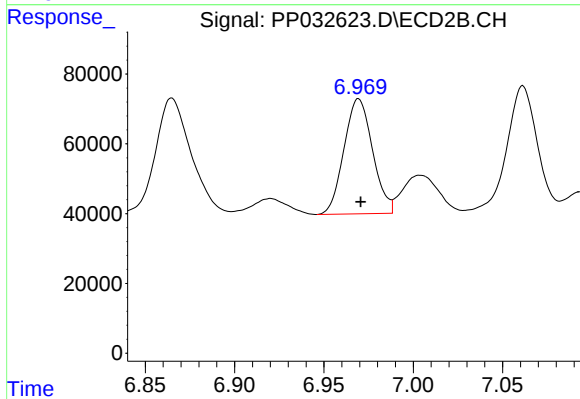

#29 AR-1254-4

R.T.: 6.969 min
Delta R.T.: -0.001 min
Response: 367560
Conc: 178.44 ng/ml

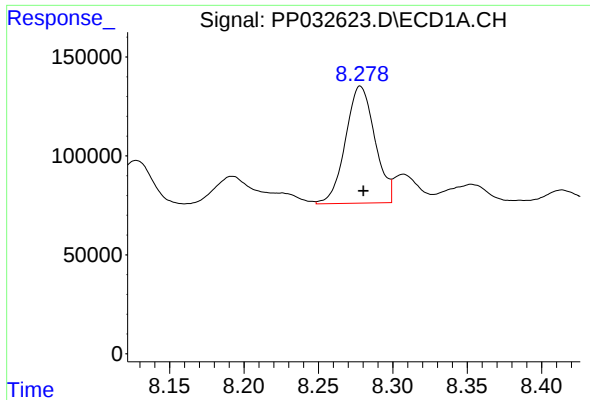


#30 AR-1254-5

R.T.: 8.278 min
Delta R.T.: -0.002 min
Response: 812644
Conc: 330.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-11

Manual Integrations
APPROVED

Ankita
1/11/2021 11:11:59 AM

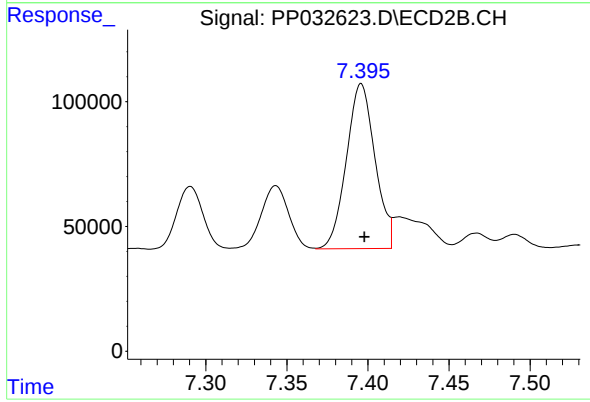

#30 AR-1254-5

R.T.: 7.395 min
Delta R.T.: -0.002 min
Response: 815328
Conc: 263.66 ng/ml m