

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010824\
 Data File : PP062767.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2024 11:32
 Operator : YP\AJ
 Sample : P1039-01RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TREMONT-AVE-DRUM-27-POLYRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/09/2024
 Supervised By :Ankita Jodhani 01/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 20:39:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 22 03:29:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.682	32708031	52156820	15.045m	17.478

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010824\
Data File : PP062767.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2024 11:32
Operator : YP\AJ
Sample : P1039-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TREMONT-AVE-DRUM-27-POLYRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2024
Supervised By :Ankita Jodhani 01/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 20:39:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP122123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 22 03:29:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

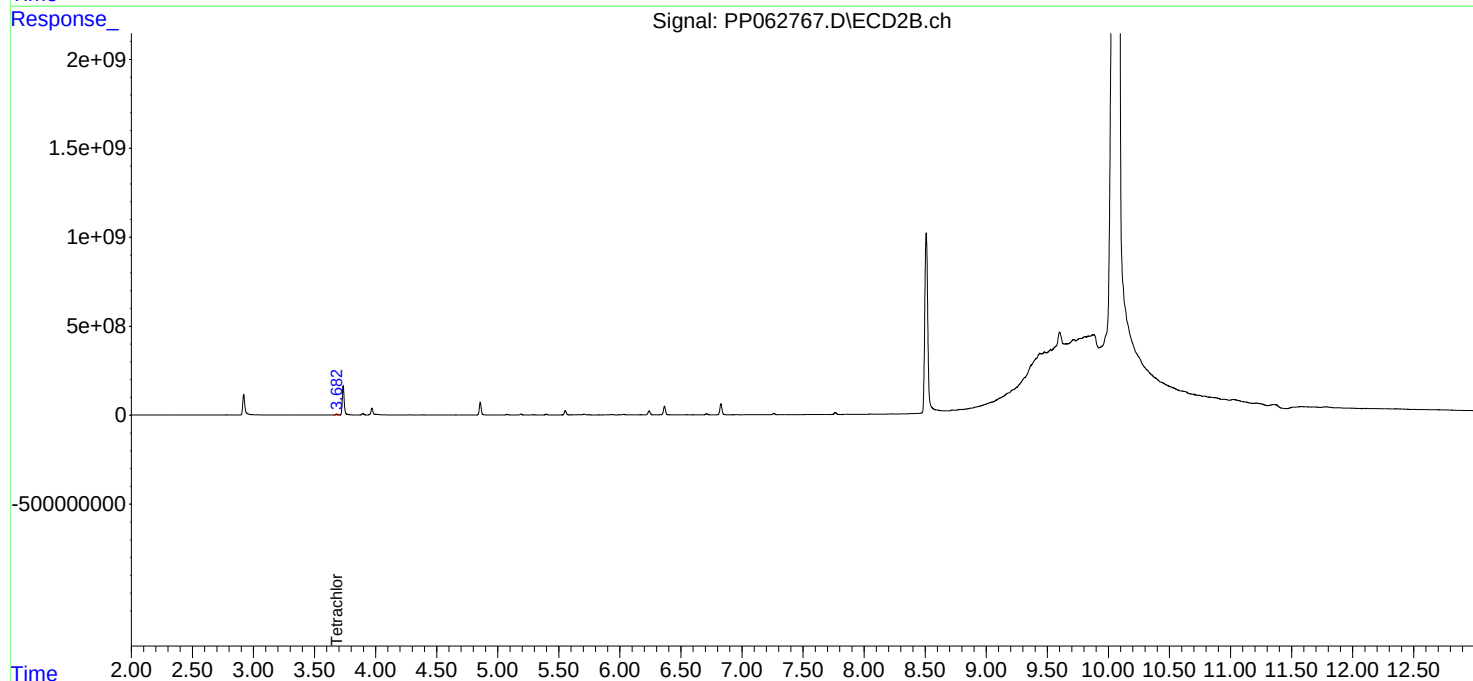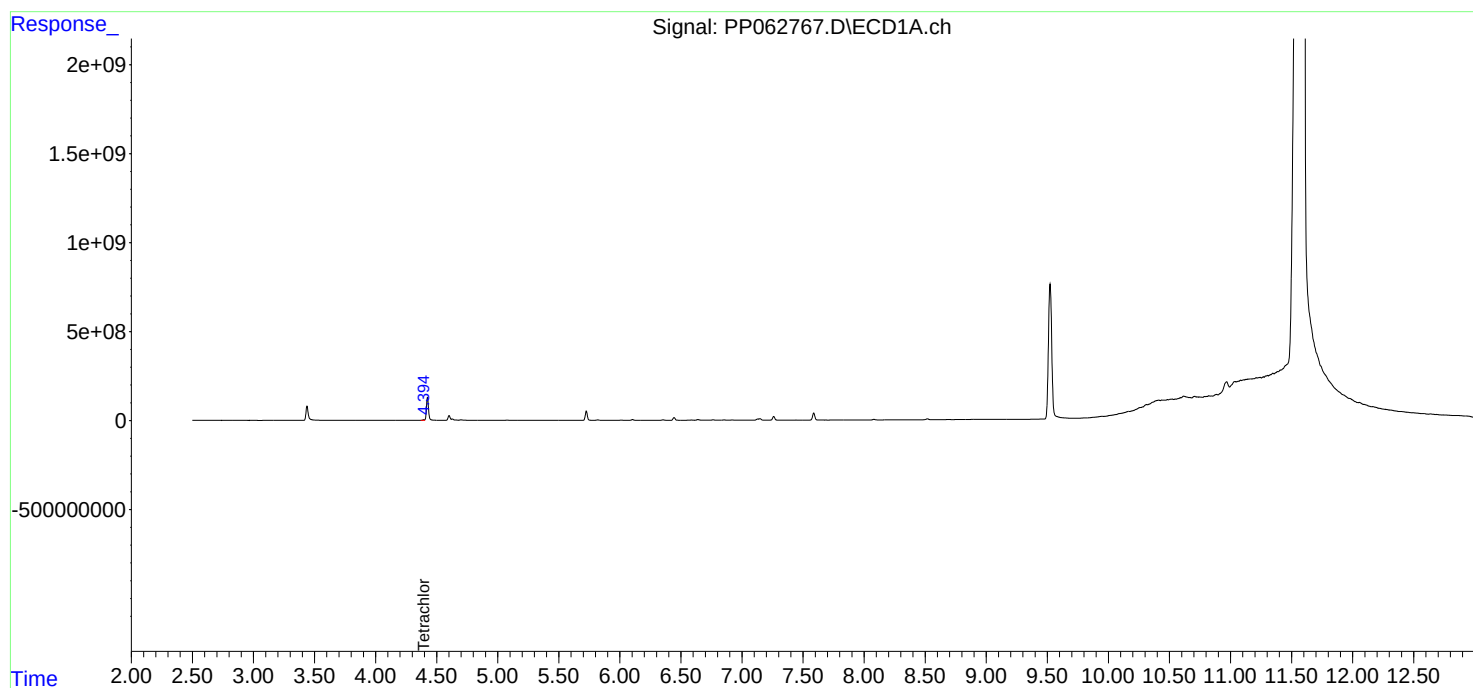

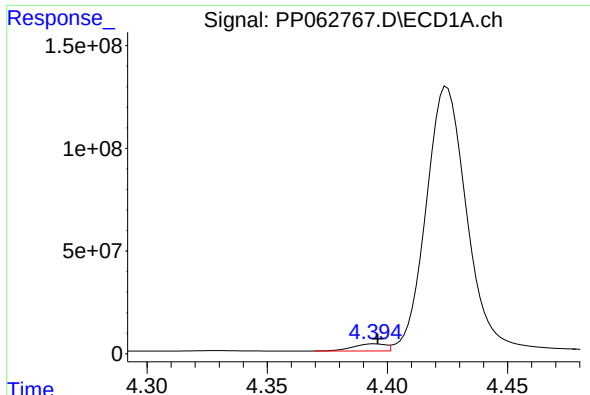

#1 Tetrachloro-m-xylene

R.T.: 4.394 min
Delta R.T.: -0.002 min
Response: 32708031
Conc: 15.04 ng/ml

Instrument :

ECD_P


ClientSampleId :

TREMONT-AVE-DRUM-27-POLYRE

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 01/09/2024
Supervised By :Ankita Jodhani 01/09/2024

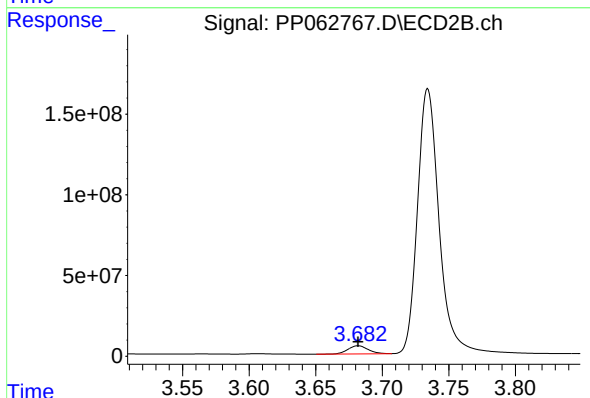


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: 0.000 min
Response: 52156820
Conc: 17.48 ng/ml

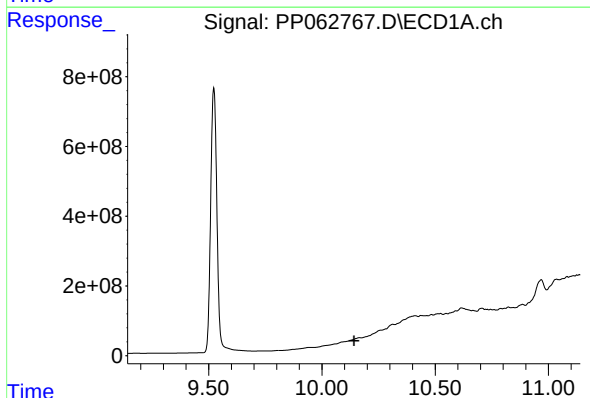

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.142 min
Response: 0
Conc: N.D.

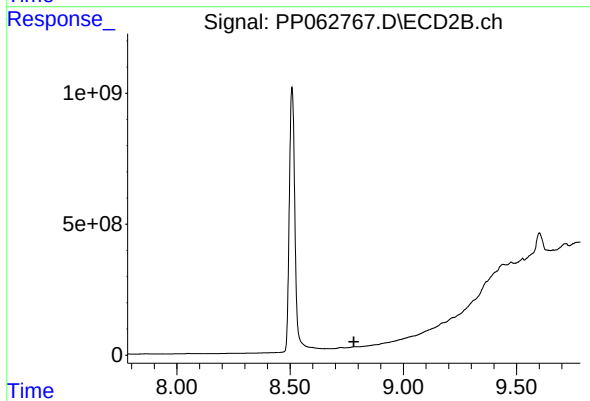

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.782 min
Response: 0
Conc: N.D.