

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR123124\
 Data File : PR069951.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Dec 2024 12:47
 Operator : AJ\MA
 Sample : P5398-13
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PCB-GPC2-BLANK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 01 01:59:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR122024CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Dec 21 03:09:04 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.970	0	259017	N.D.	0.046 #
Target Compounds							
27)	L6 AR-1254-2	0.000	5.067	0	49404	N.D.	0.217 #
28)	L6 AR-1254-3	0.000	5.475	0	1078958	N.D.	3.088 #
29)	L6 AR-1254-4	0.000	5.732	0	141352	N.D.	0.683 #
31)	L7 AR-1260-1	0.000	5.645	0	276536	N.D.	1.176 #
32)	L7 AR-1260-2	0.000	5.848	0	210316	N.D.	0.784 #
33)	L7 AR-1260-3	0.000	6.004	0	510747	N.D.	1.999 #
34)	L7 AR-1260-4	0.000	6.530	0	129513	N.D.	0.596 #
35)	L7 AR-1260-5	0.000	6.820 ^f	0	194433	N.D.	0.389 #
37)	L8 AR-1262-2	0.000	6.820	0	194433	N.D.	0.350 #
45)	L9 AR-1268-5	0.000	8.025	0	723022	N.D.	0.447 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR123124\
Data File : PR069951.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Dec 2024 12:47
Operator : AJ\MA
Sample : P5398-13
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PCB-GPC2-BLANK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 01 01:59:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR122024CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Dec 21 03:09:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

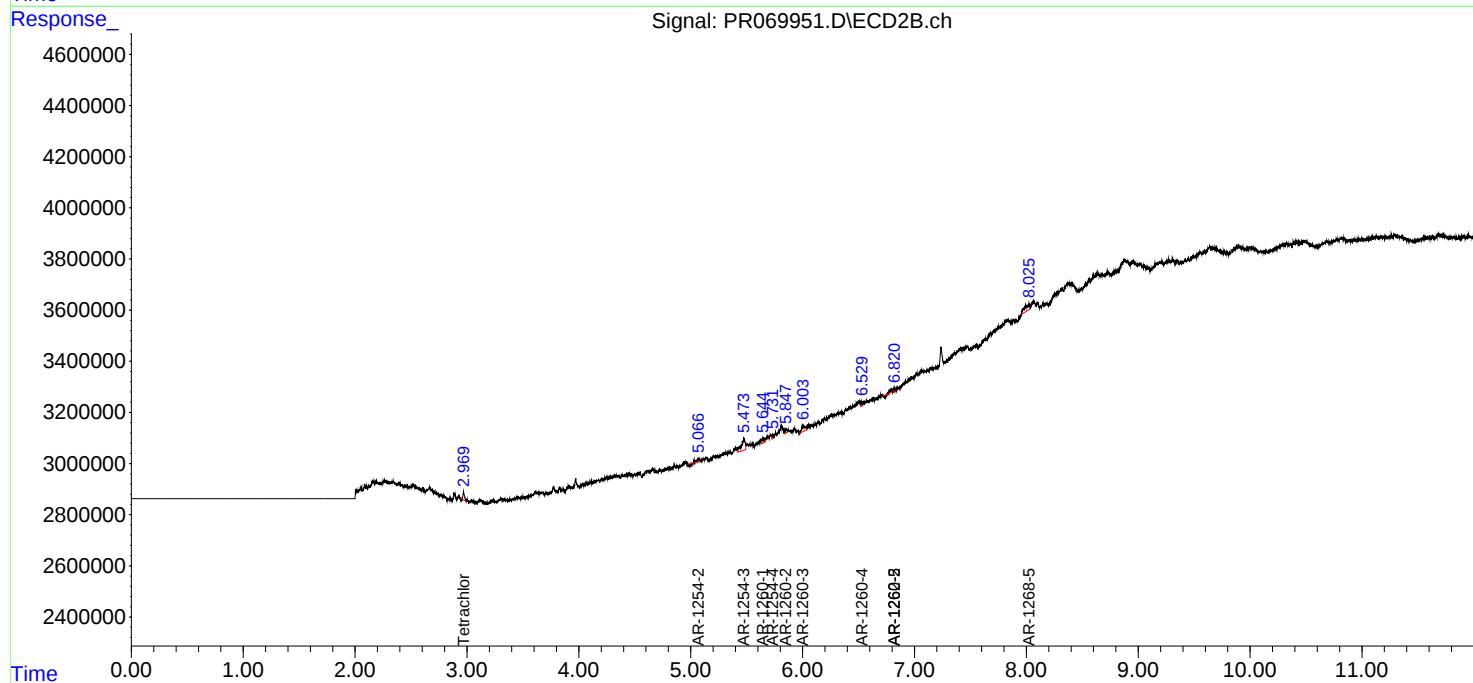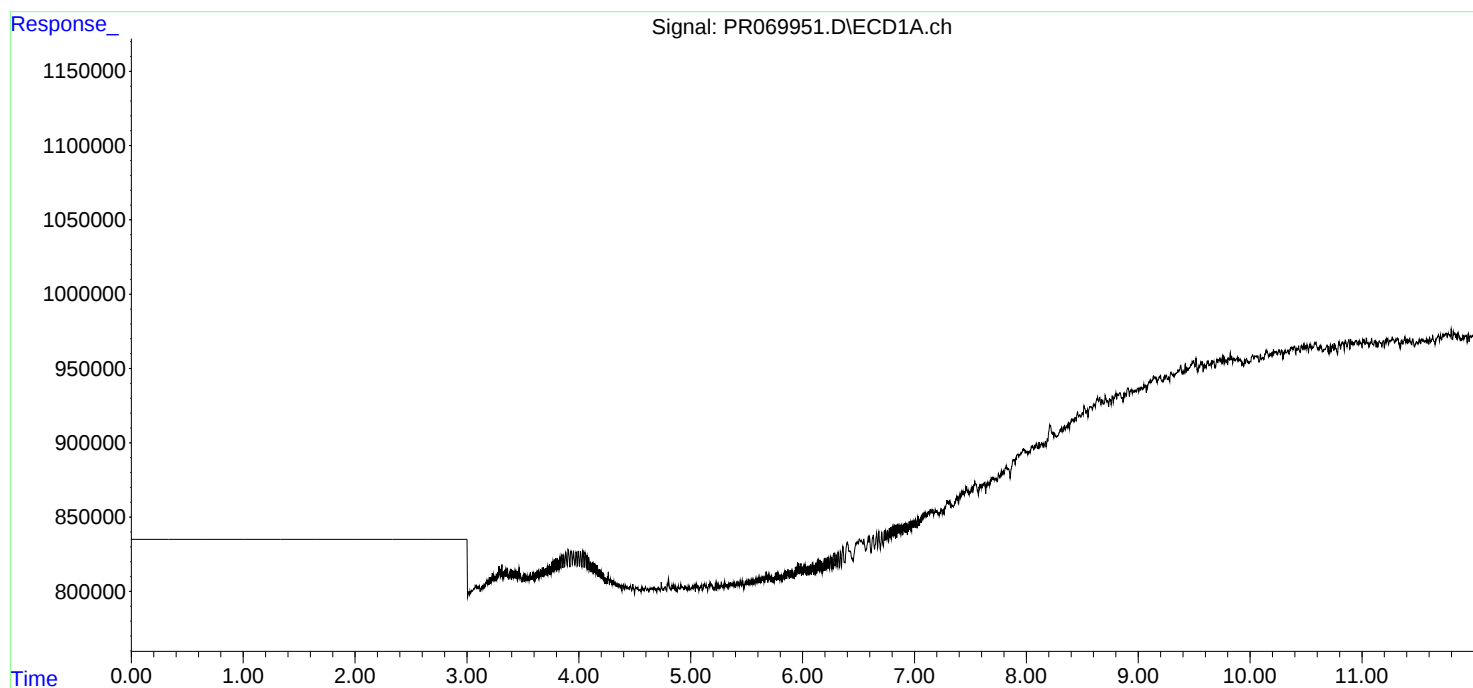


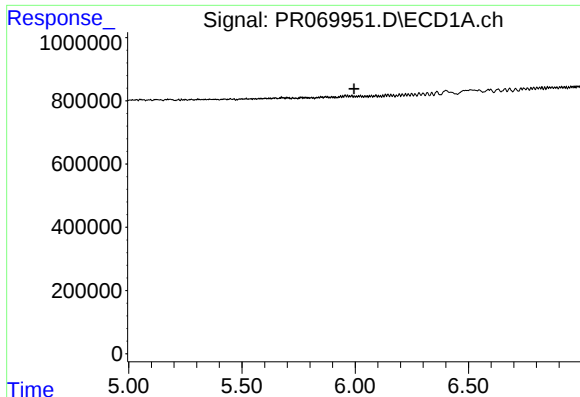

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 5.995 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-GPC2-BLANK

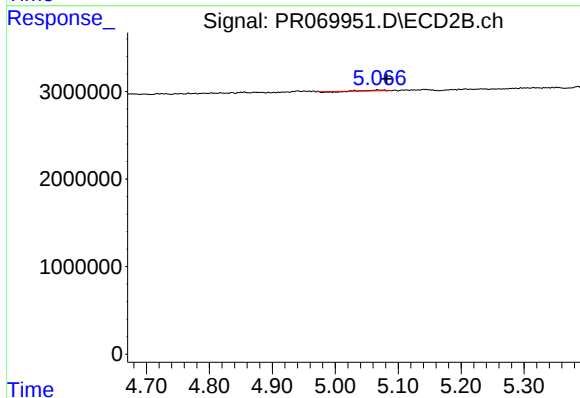


#27 AR-1254-2

R.T.: 5.067 min
Delta R.T.: -0.015 min
Response: 49404
Conc: 0.22 ng/ml

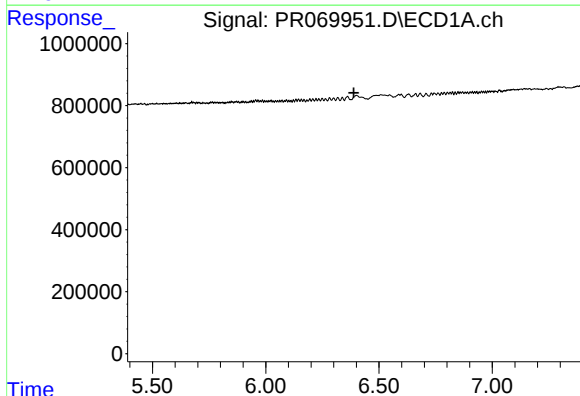


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

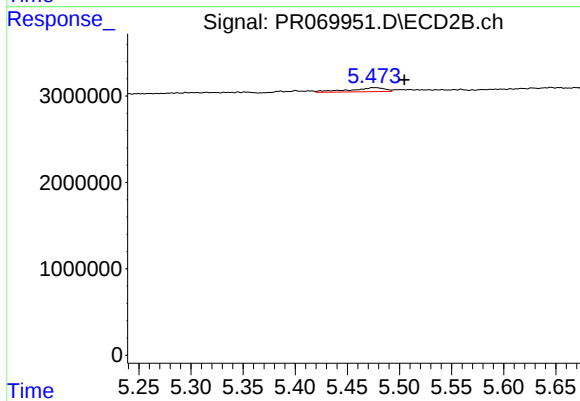

#28 AR-1254-3


R.T.: 5.475 min
Delta R.T.: -0.030 min
Response: 1078958
Conc: 3.09 ng/ml

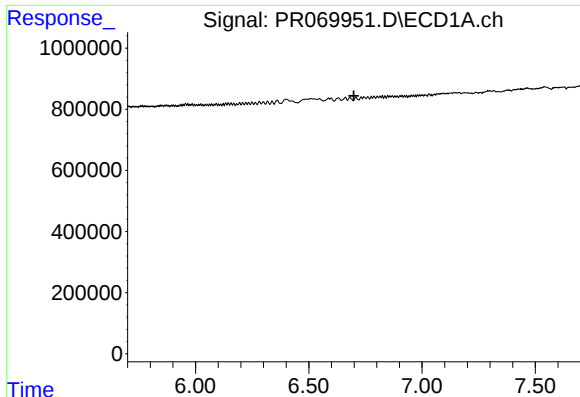

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 6.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-GPC2-BLANK

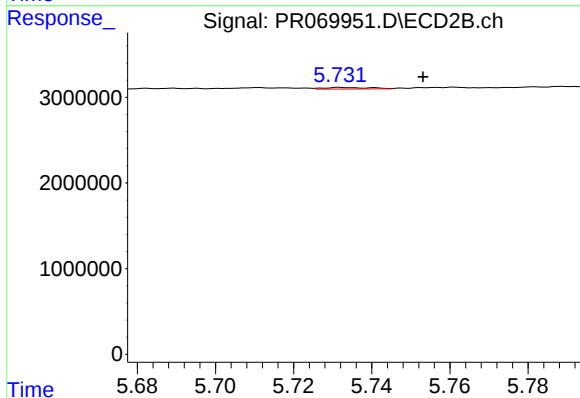


#29 AR-1254-4

R.T.: 5.732 min
Delta R.T.: -0.021 min
Response: 141352
Conc: 0.68 ng/ml

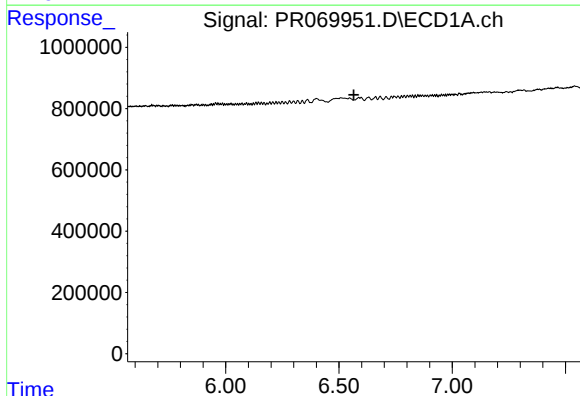


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T.: 6.566 min
Response: 0
Conc: N.D.

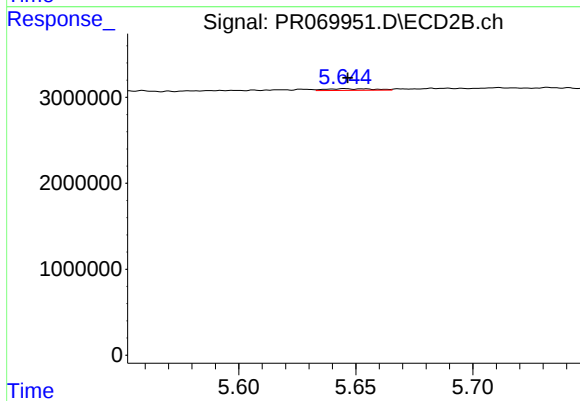

#31 AR-1260-1


R.T.: 5.645 min
Delta R.T.: -0.001 min
Response: 276536
Conc: 1.18 ng/ml

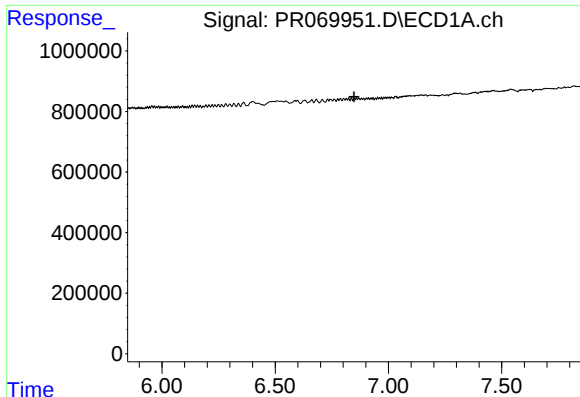

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 6.848 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-GPC2-BLANK

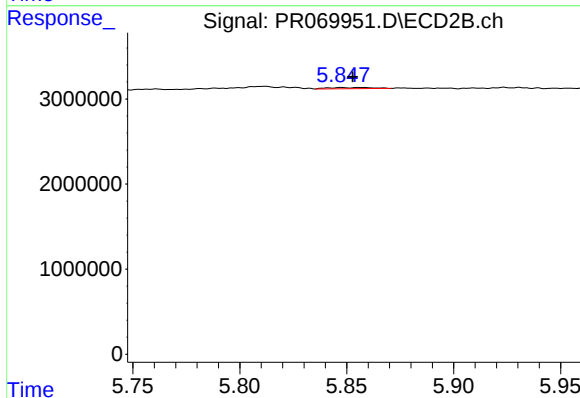


#32 AR-1260-2

R.T.: 5.848 min
Delta R.T.: -0.005 min
Response: 210316
Conc: 0.78 ng/ml

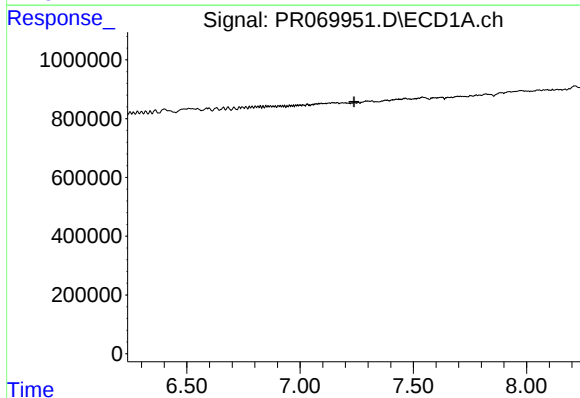


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.238 min
Response: 0
Conc: N.D.

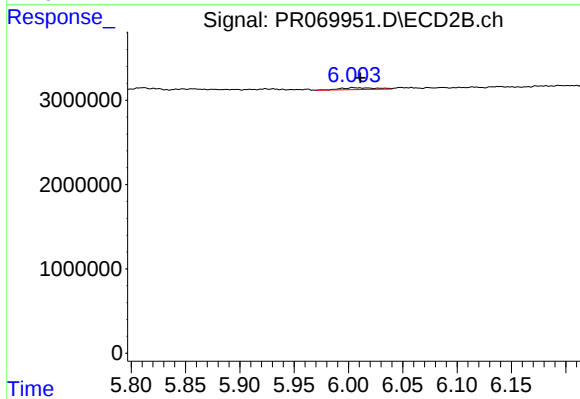

#33 AR-1260-3


R.T.: 6.004 min
Delta R.T.: -0.007 min
Response: 510747
Conc: 2.00 ng/ml

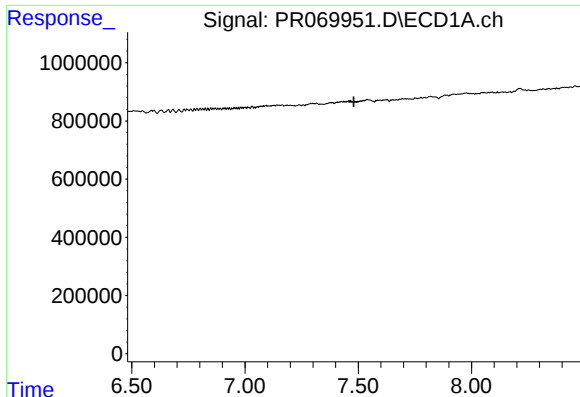

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-GPC2-BLANK

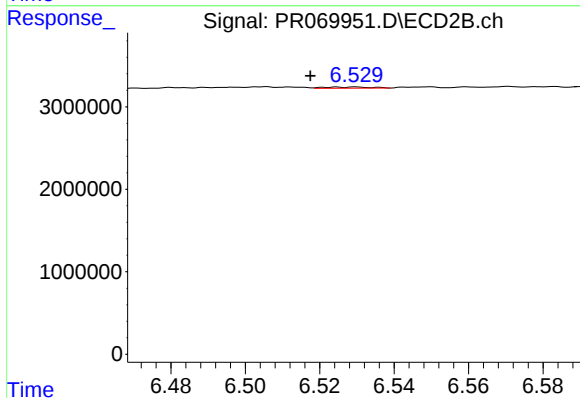


#34 AR-1260-4

R.T.: 6.530 min
Delta R.T.: 0.012 min
Response: 129513
Conc: 0.60 ng/ml

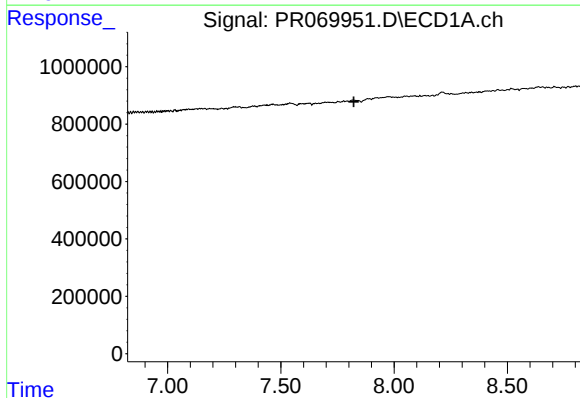


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 7.822 min
Response: 0
Conc: N.D.

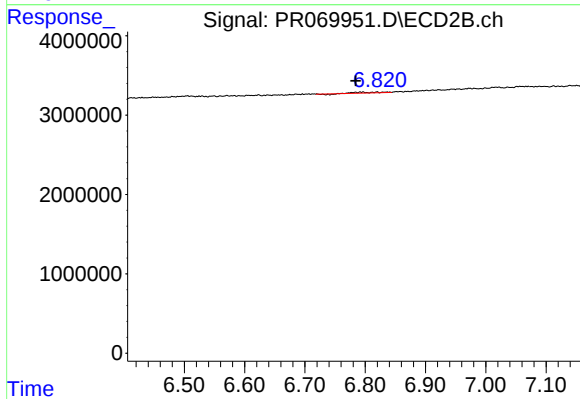

#35 AR-1260-5


R.T.: 6.820 min
Delta R.T.: 0.035 min
Response: 194433
Conc: 0.39 ng/ml

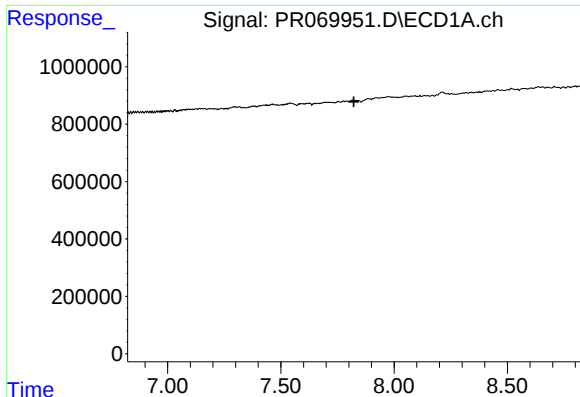

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PCB-GPC2-BLANK

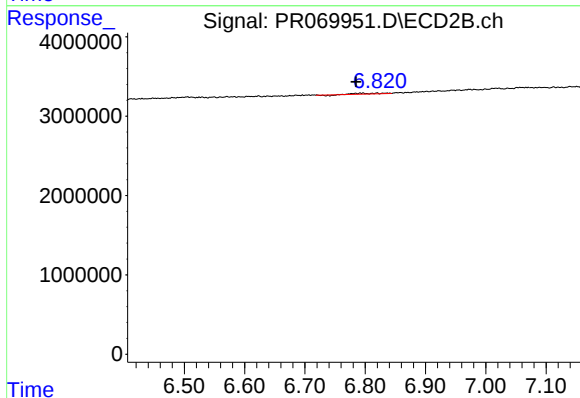


#37 AR-1262-2

R.T.: 6.820 min
Delta R.T.: 0.035 min
Response: 194433
Conc: 0.35 ng/ml

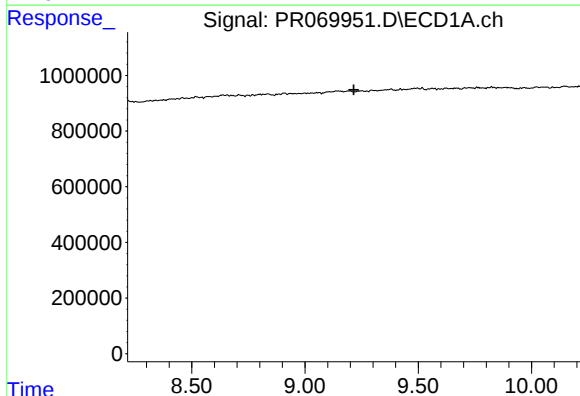

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.216 min
Response: 0
Conc: N.D.

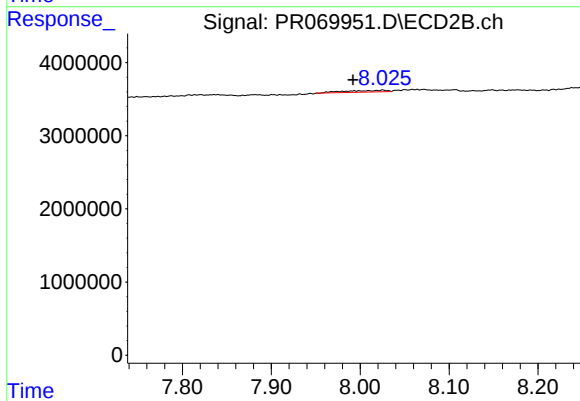

#45 AR-1268-5

R.T.: 8.025 min
Delta R.T.: 0.033 min
Response: 723022
Conc: 0.45 ng/ml