

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010919\
 Data File : PP028718.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jan 2019 14:48
 Operator : EI\MA
 Sample : K1074-11
 Misc : hexane
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 00:58:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010319.M
 Quant Title : 8080.M
 QLast Update : Fri Jan 04 01:40:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.135	12.247	33265905	53669264	129.386	122.931
Target Compounds							
1) T	Dalapon	3.325	3.046	13661709	16353922	22.341	27.975 #
2) T	3,5-DICHL...	10.599	0.000	6468410	0	12.944	N.D. #
5) T	DICAMBA	12.504	12.487	3358393	-471338	2.145	N.D. #
6) T	MCP	12.824	0.000	114.1E6	0	216.100	N.D. #
8) T	DICHLORPROP	0.000	13.683	0	131.0E6	N.D.	301.579 #
12) T	2,4,5-T	0.000	15.984	0	26048978	N.D.	12.008 #
13) T	2,4-DB	16.468	0.000	15597611	0	160.910	N.D. #
16) T	DCPA	18.270	18.204	13808932	6882872	3.345	2.108 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010919\
Data File : PP028718.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jan 2019 14:48
Operator : EI\MA
Sample : K1074-11
Misc : hexane
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 00:58:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010319.M
Quant Title : 8080.M
QLast Update : Fri Jan 04 01:40:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

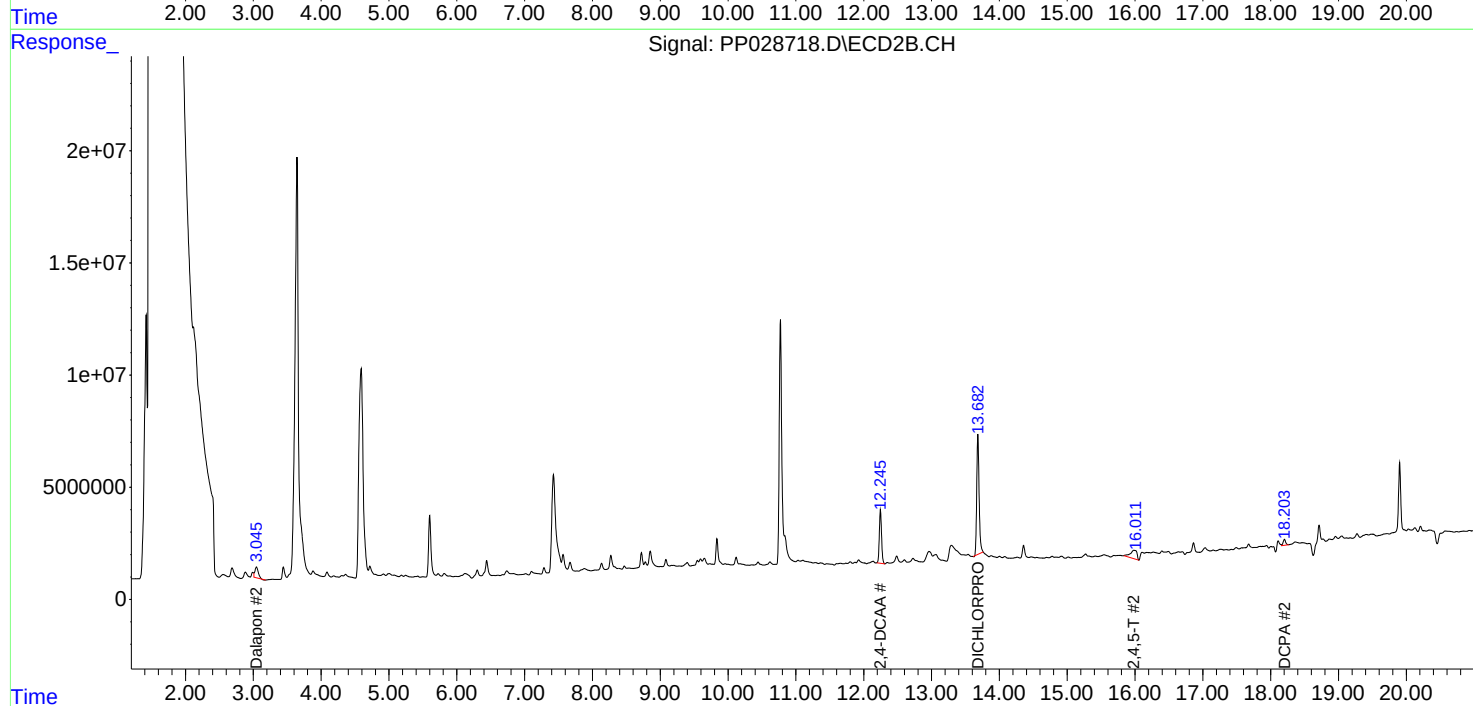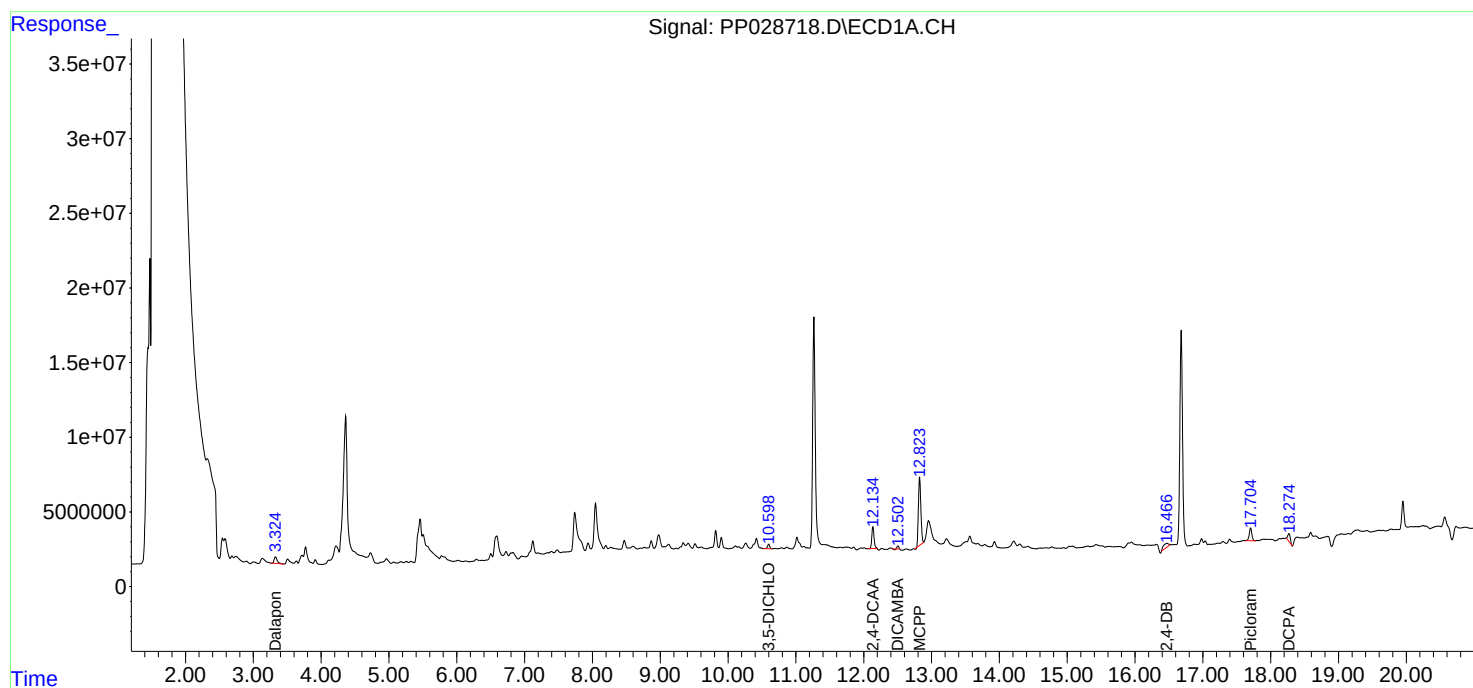


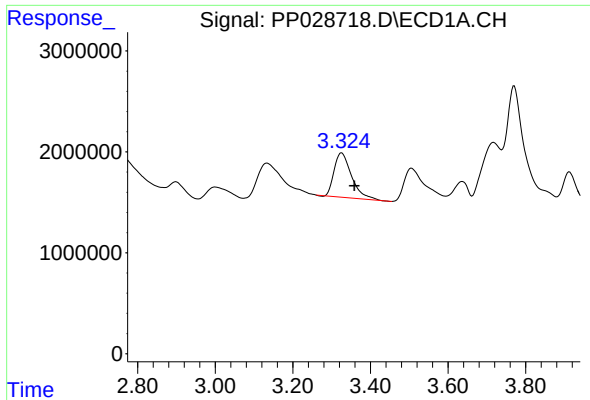

#1 Dalapon


R.T.: 3.325 min
Delta R.T.: -0.034 min
Response: 13661709
Conc: 22.34 ng/ml

Instrument :
ECD_P
ClientSampleId :

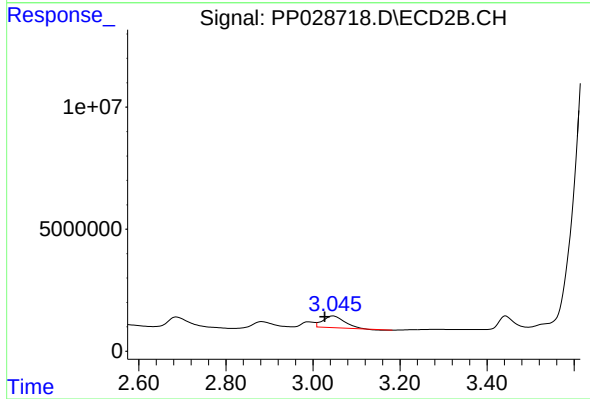


#1 Dalapon

R.T.: 3.046 min
Delta R.T.: 0.019 min
Response: 16353922
Conc: 27.98 ng/ml

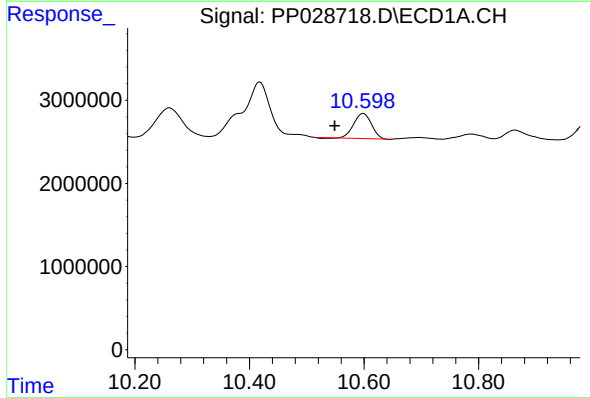


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.599 min
Delta R.T.: 0.050 min
Response: 6468410
Conc: 12.94 ng/ml

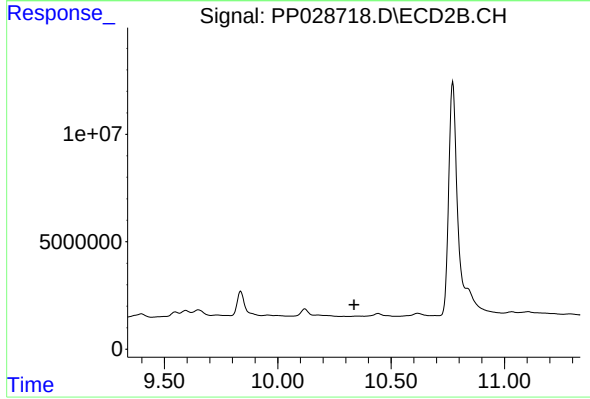

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 10.337 min
Response: 0
Conc: N.D.

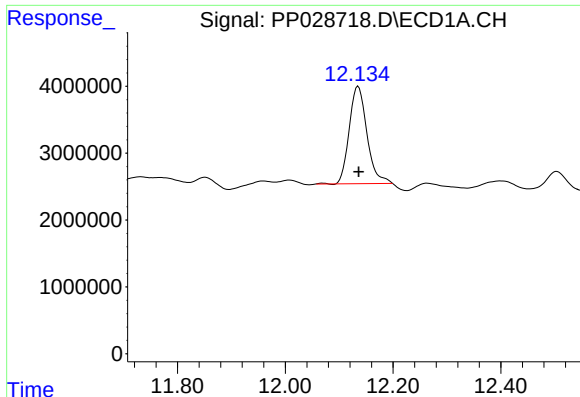

#4 2,4-DCAA


R.T.: 12.135 min
Delta R.T.: 0.000 min
Response: 33265905
Conc: 129.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

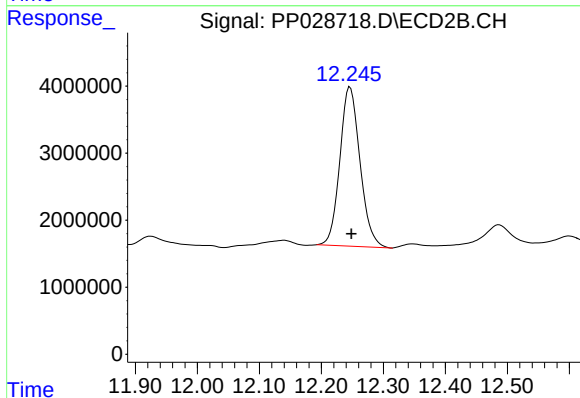


#4 2,4-DCAA

R.T.: 12.247 min
Delta R.T.: -0.002 min
Response: 53669264
Conc: 122.93 ng/ml

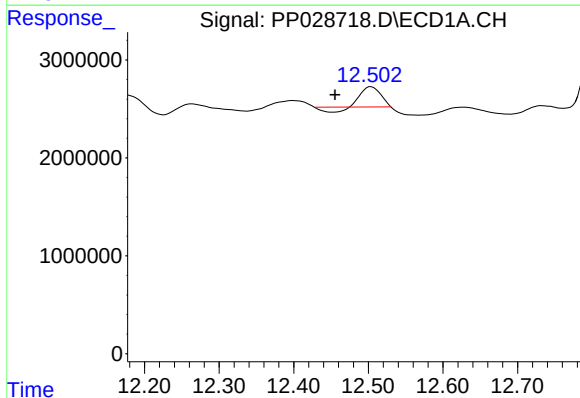


#5 DICAMBA

R.T.: 12.504 min
Delta R.T.: 0.048 min
Response: 3358393
Conc: 2.15 ng/ml

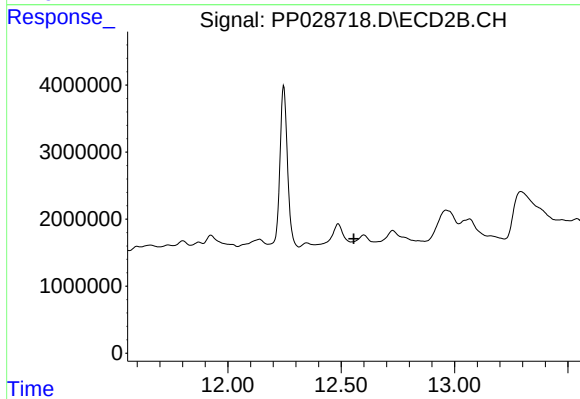

#5 DICAMBA


R.T.: 12.487 min
Delta R.T.: -0.068 min
Response: -471338
Conc: N.D.

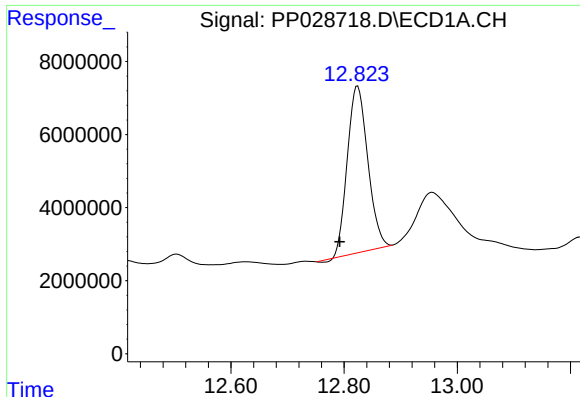

#6 MCPP


R.T.: 12.824 min
Delta R.T.: 0.032 min
Response: 114132412
Conc: 216.10 ug/ml

Instrument :
ECD_P
ClientSampleId :

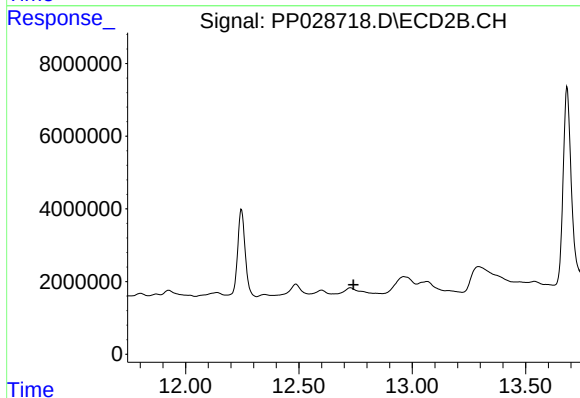


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 12.741 min
Response: 0
Conc: N.D.

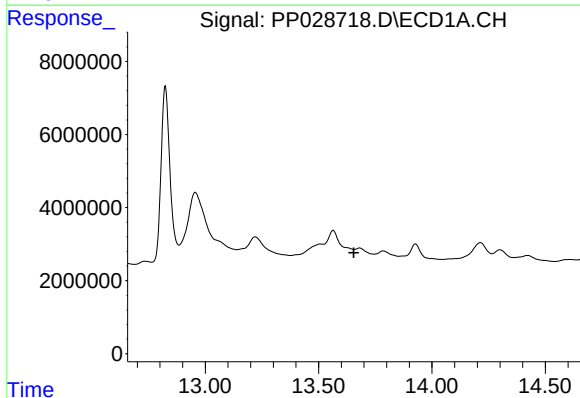


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.655 min
Response: 0
Conc: N.D.

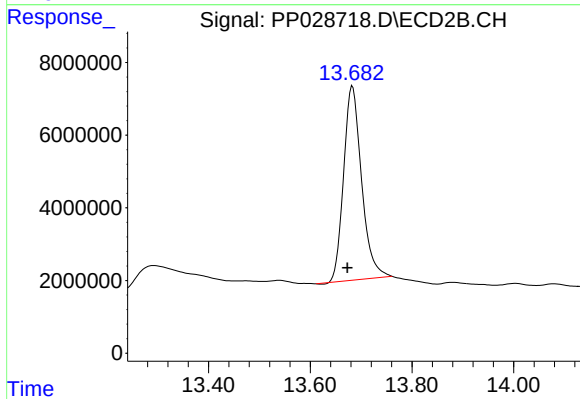

#8 DICHLORPROP


R.T.: 13.683 min
Delta R.T.: 0.010 min
Response: 130962828
Conc: 301.58 ng/ml

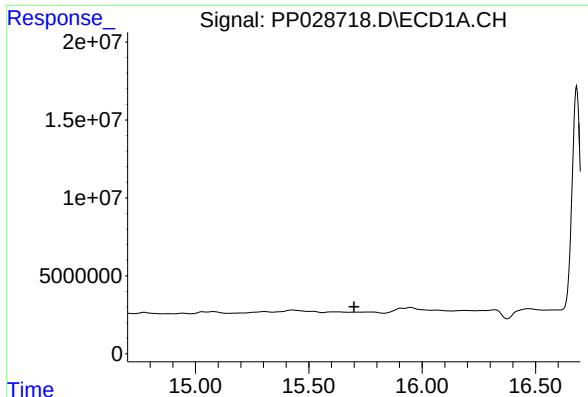

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.699 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

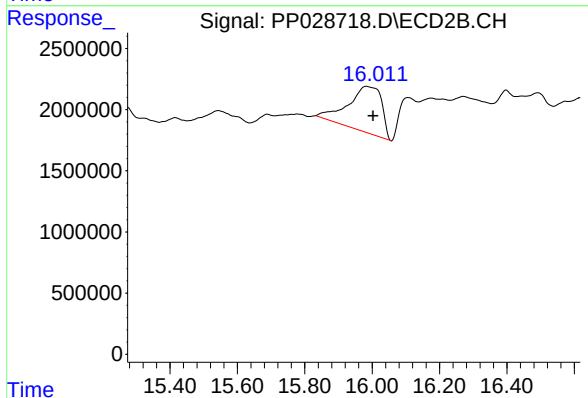


#12 2,4,5-T

R.T.: 15.984 min
Delta R.T.: -0.018 min
Response: 26048978
Conc: 12.01 ng/ml

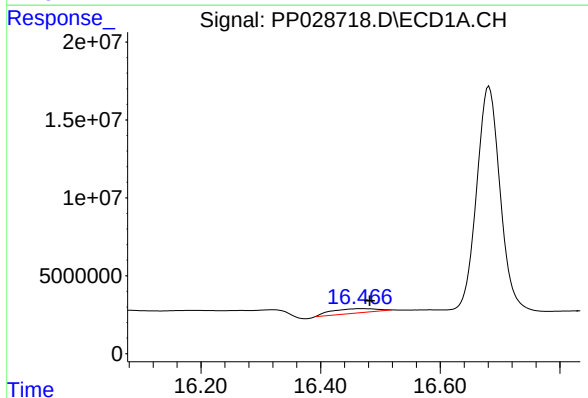


#13 2,4-DB

R.T.: 16.468 min
Delta R.T.: -0.014 min
Response: 15597611
Conc: 160.91 ng/ml

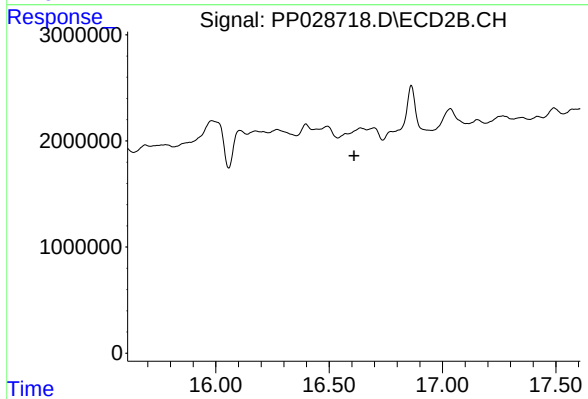

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.610 min
Response: 0
Conc: N.D.

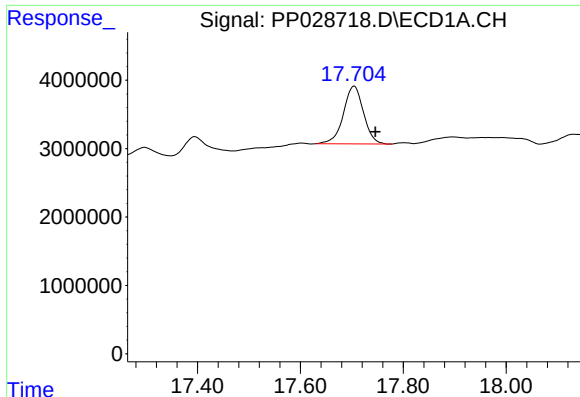

#15 Picloram


R.T.: 17.705 min
Delta R.T.: -0.041 min
Response: 22950934
Conc: 21.41 ng/ml

Instrument :
ECD_P
ClientSampleId :

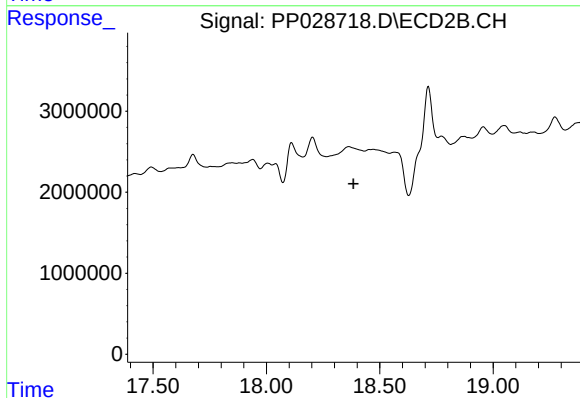


#15 Picloram

R.T.: 18.364 min
Delta R.T.: -0.021 min
Response: 3356712
Conc: N.D.

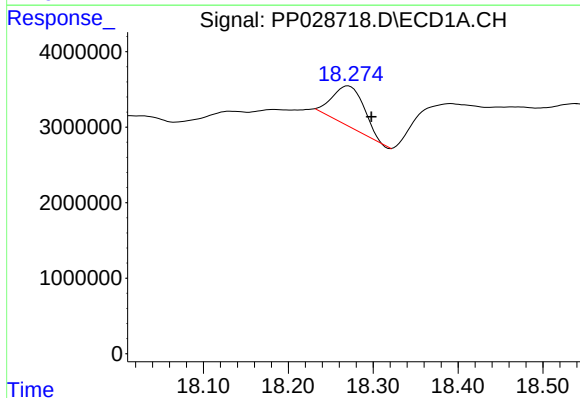

#16 DCPA

R.T.: 18.270 min
Delta R.T.: -0.028 min
Response: 13808932
Conc: 3.34 ng/ml

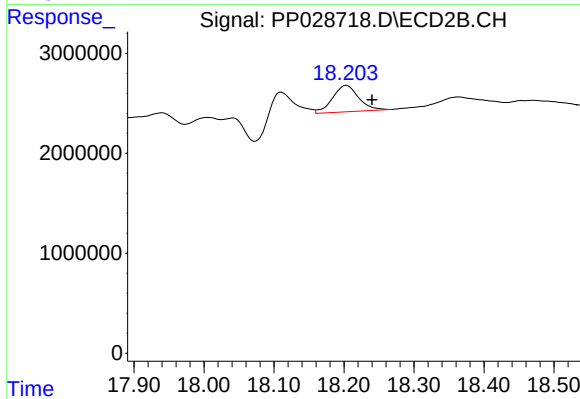

#16 DCPA

R.T.: 18.204 min
Delta R.T.: -0.037 min
Response: 6882872
Conc: 2.11 ng/ml