

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010923\
 Data File : PP054352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jan 2023 23:00
 Operator : YP\AJ
 Sample : 01054-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/10/2023
 Supervised By :Ankita Jodhani 01/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 23:41:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 03:46:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.331	3.588	172.5E6	1096551	85.163m	0.680m#
2) SA Decachlor...	10.119	8.626	19534740	24410363	13.602	17.304m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP010923\
Data File : PP054352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jan 2023 23:00
Operator : YP\AJ
Sample : 01054-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/10/2023
Supervised By :Ankita Jodhani 01/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 23:41:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 03:46:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

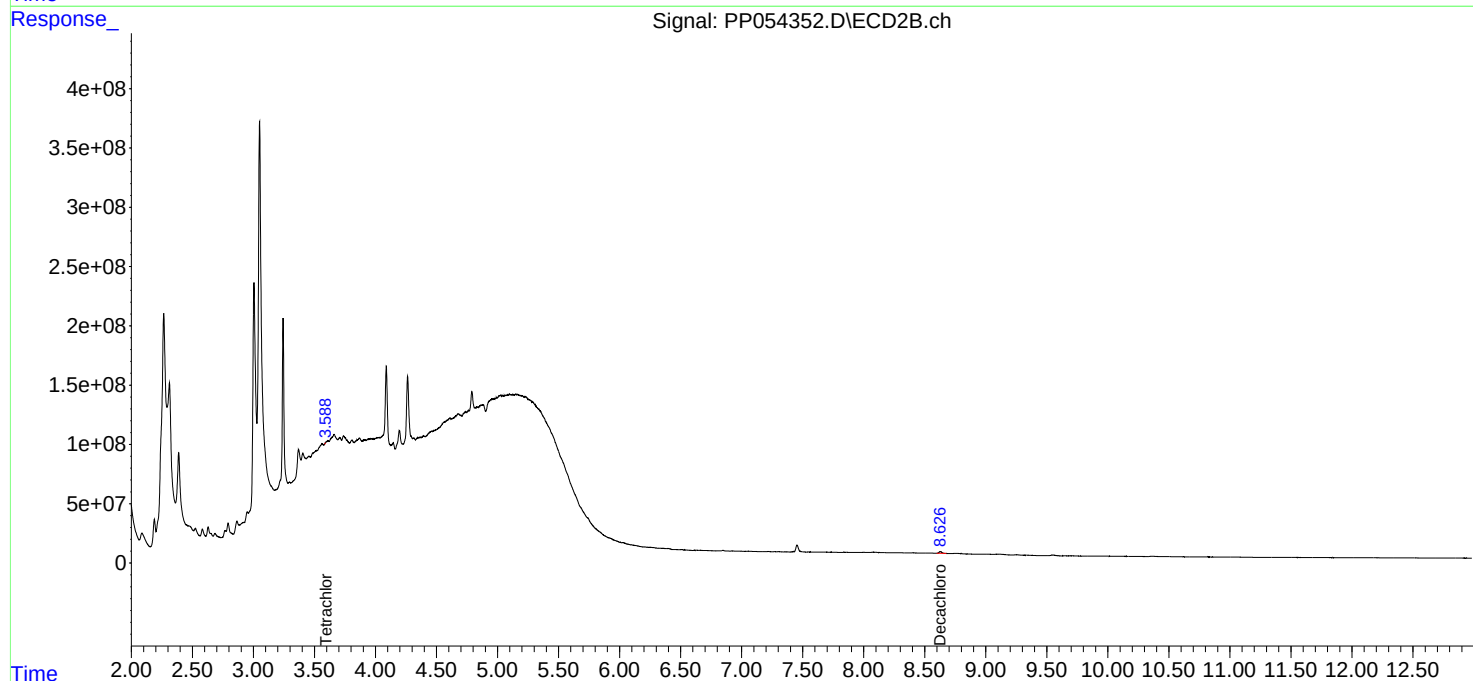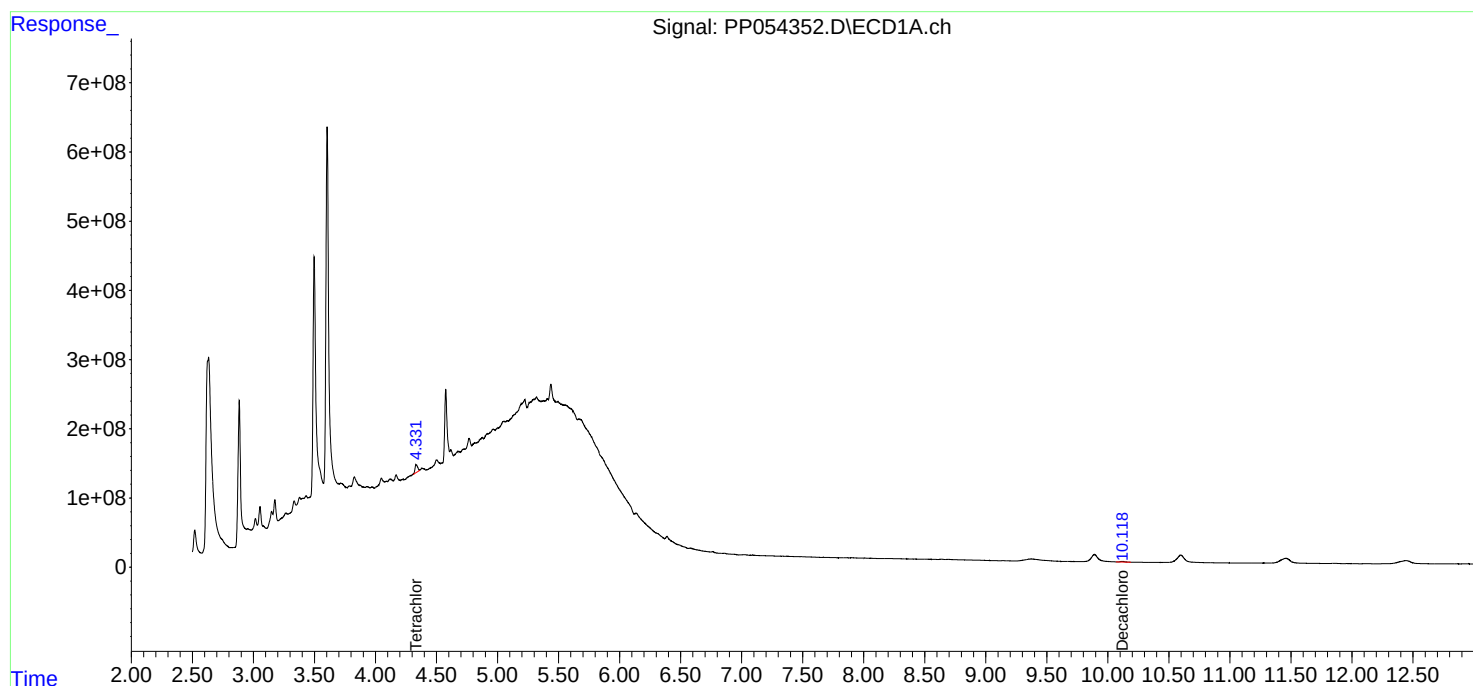

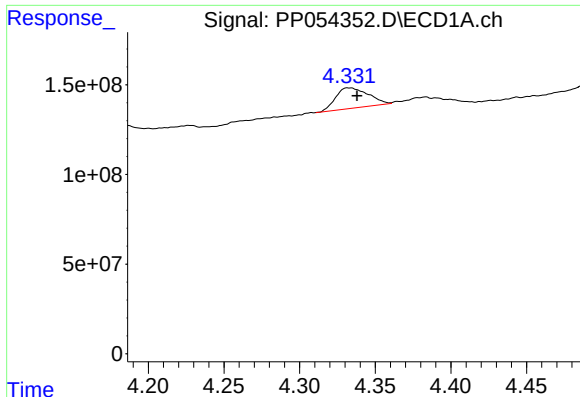


#1 Tetrachloro-m-xylene

R.T.: 4.331 min
Delta R.T.: -0.007 min
Response: 172460450
Conc: 85.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/10/2023
Supervised By :Ankita Jodhani 01/10/2023

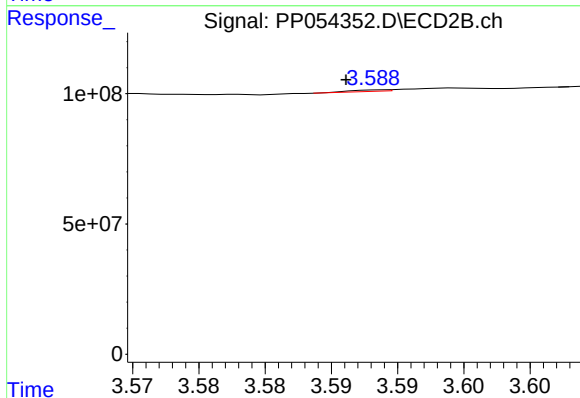


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: 0.002 min
Response: 1096551
Conc: 0.68 ng/ml m

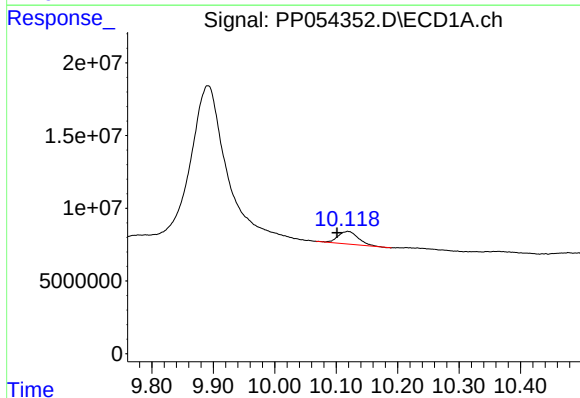

#2 Decachlorobiphenyl

R.T.: 10.119 min
Delta R.T.: 0.018 min
Response: 19534740
Conc: 13.60 ng/ml

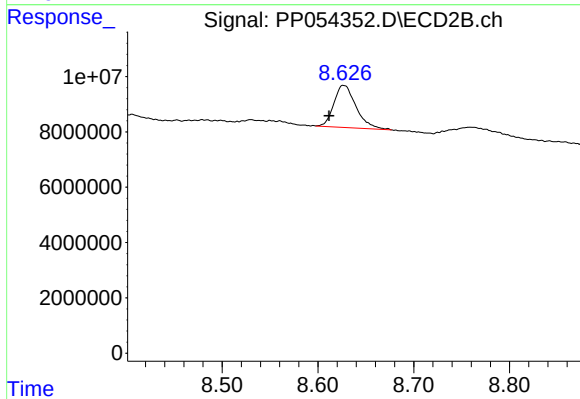

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: 0.014 min
Response: 24410363
Conc: 17.30 ng/ml m