

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011023\
 Data File : PP054427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2023 03:33
 Operator : YP\AJ
 Sample : 01079-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-2-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/11/2023
 Supervised By :Ankita Jodhani 01/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 09:47:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 03:46:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.336	3.585	26496708	19340552	13.084	11.990
2) SA Decachlor...	10.093	8.606	13150853	15716020	9.157m	11.141

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011023\
Data File : PP054427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2023 03:33
Operator : YP\AJ
Sample : 01079-02
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/11/2023
Supervised By :Ankita Jodhani 01/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 09:47:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 03:46:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

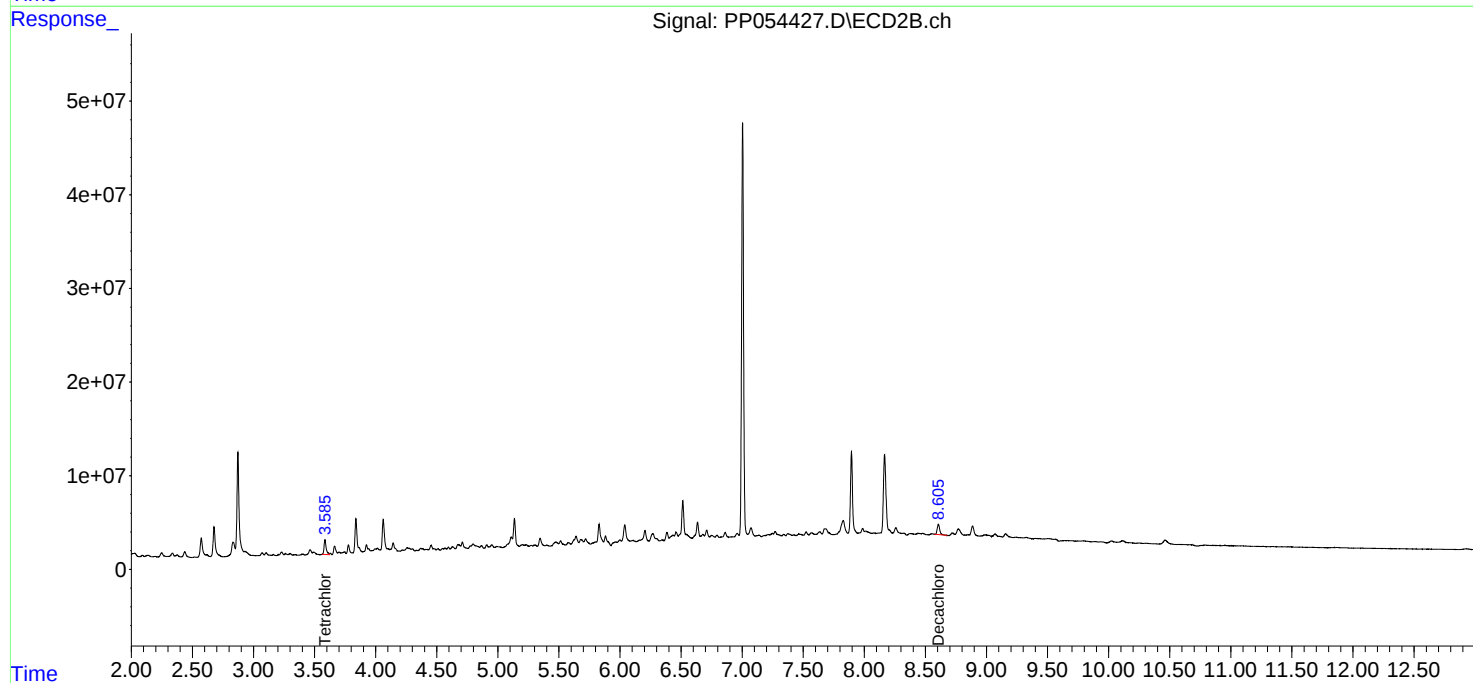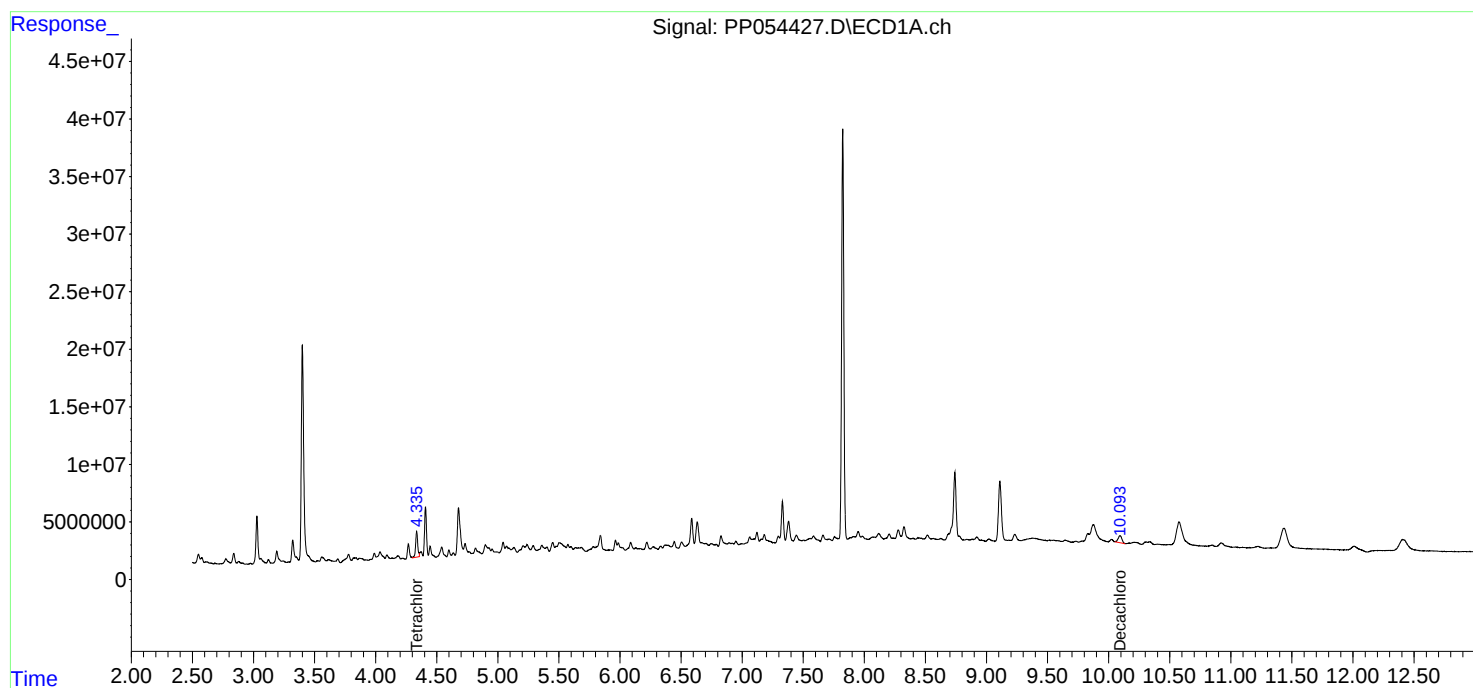

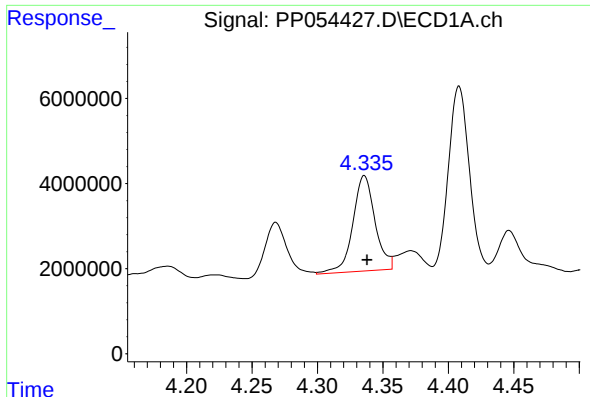


#1 Tetrachloro-m-xylene

R.T.: 4.336 min
Delta R.T.: -0.002 min
Response: 26496708
Conc: 13.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/11/2023
Supervised By :Ankita Jodhani 01/11/2023

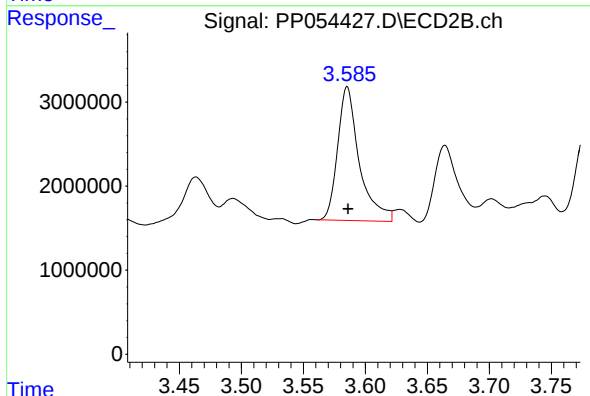


#1 Tetrachloro-m-xylene

R.T.: 3.585 min
Delta R.T.: 0.000 min
Response: 19340552
Conc: 11.99 ng/ml

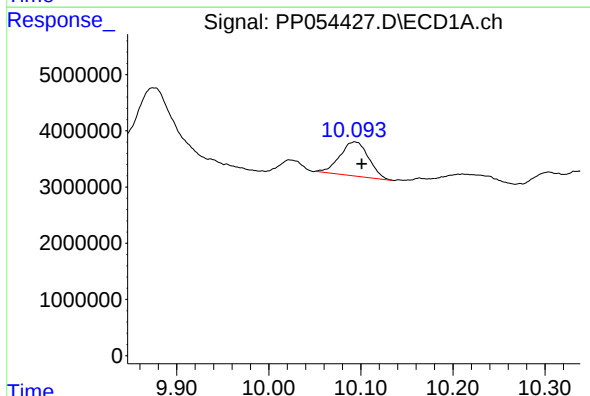

#2 Decachlorobiphenyl

R.T.: 10.093 min
Delta R.T.: -0.008 min
Response: 13150853
Conc: 9.16 ng/ml m

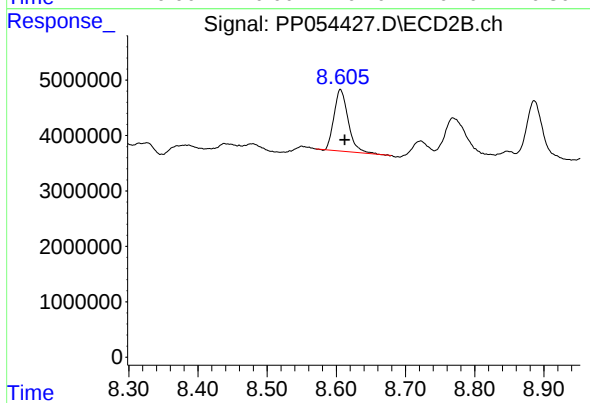

#2 Decachlorobiphenyl

R.T.: 8.606 min
Delta R.T.: -0.006 min
Response: 15716020
Conc: 11.14 ng/ml