

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011023\
 Data File : PP054428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2023 08:54
 Operator : YP\AJ
 Sample : 01079-02RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-2-INFLUENTRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/11/2023
 Supervised By :Ankita Jodhani 01/11/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 09:47:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 03:46:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.587	27485089	19929395	13.572	12.356
2) SA Decachlor...	10.104	8.608	14050741	16289422	9.783m	11.547m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011023\
Data File : PP054428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2023 08:54
Operator : YP\AJ
Sample : 01079-02RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/11/2023
Supervised By :Ankita Jodhani 01/11/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 09:47:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 03:46:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

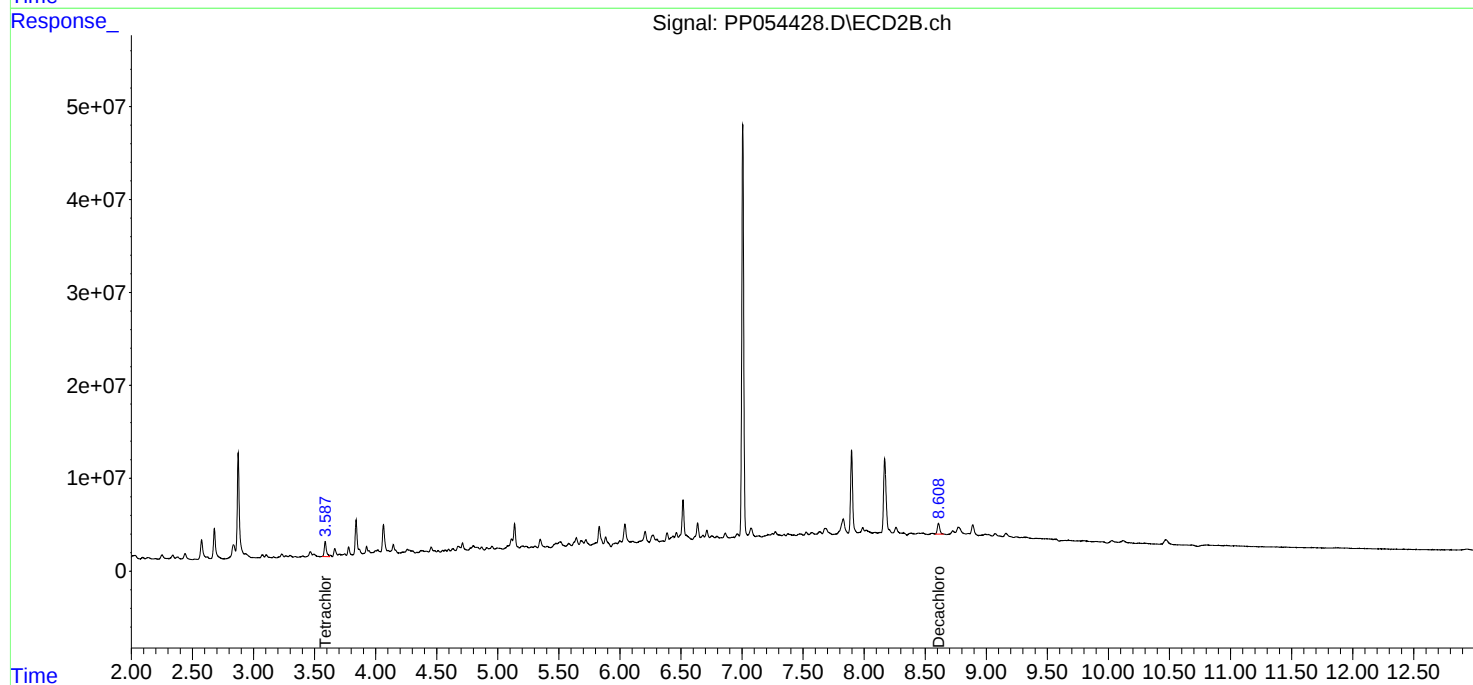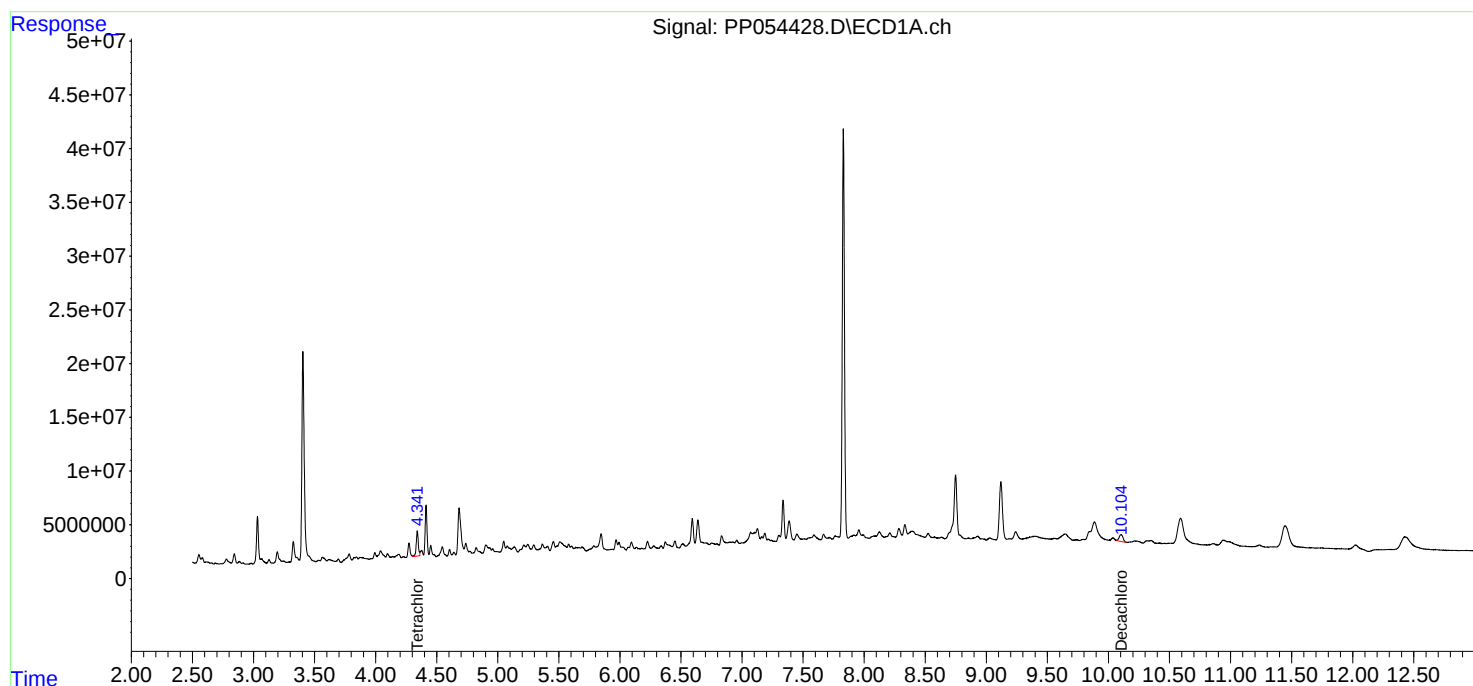

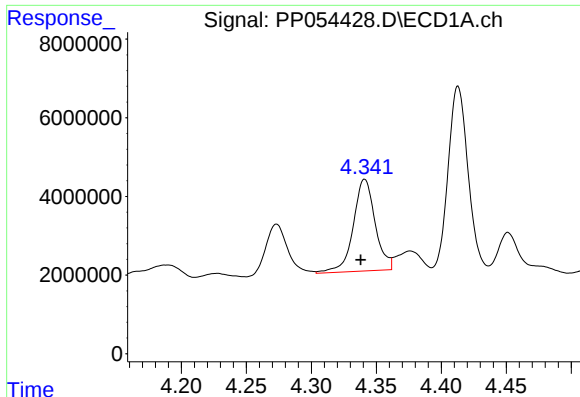


#1 Tetrachloro-m-xylene

R.T.: 4.341 min
Delta R.T.: 0.003 min
Response: 27485089
Conc: 13.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/11/2023
Supervised By :Ankita Jodhani 01/11/2023

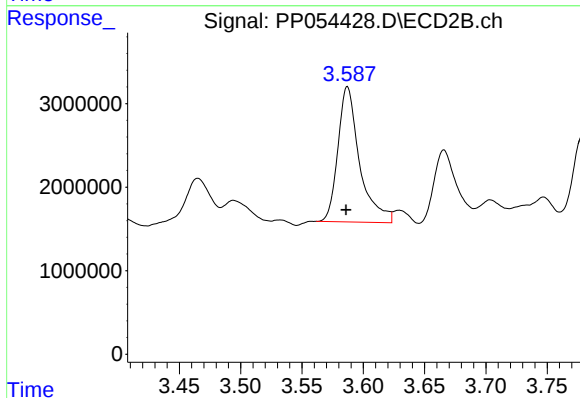


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: 0.000 min
Response: 19929395
Conc: 12.36 ng/ml

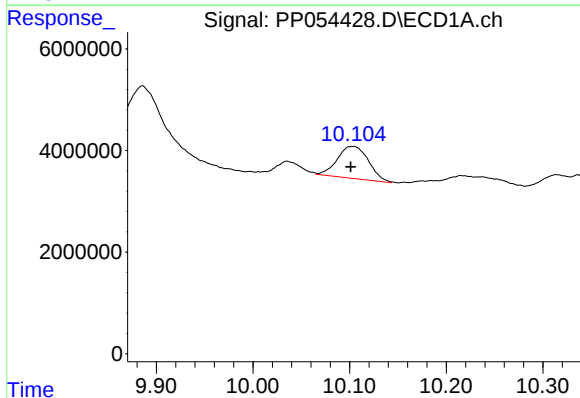

#2 Decachlorobiphenyl

R.T.: 10.104 min
Delta R.T.: 0.003 min
Response: 14050741
Conc: 9.78 ng/ml m

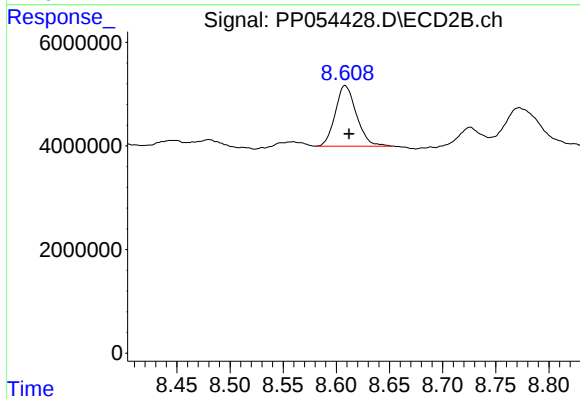

#2 Decachlorobiphenyl

R.T.: 8.608 min
Delta R.T.: -0.004 min
Response: 16289422
Conc: 11.55 ng/ml m