

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011119\
 Data File : PP028774.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jan 2019 19:52
 Operator : EI\MA
 Sample : J1005-02
 Misc : hexane
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 03:43:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010319.M
 Quant Title : 8080.M
 QLast Update : Fri Jan 04 01:40:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.139	12.250	75496071	119.7E6	293.639	274.117
Target Compounds							
1) T	Dalapon	3.324	2.995	75444811	91289921	123.373	156.161 #
6) T	MCP	12.832	0.000	29336374	0	58.598	N.D. #
7) T	MCPA	13.064	13.079	293.2E6	37787278	366.055	25.820 #
8) T	DICHLORPROP	0.000	13.691	0	30606326	N.D.	70.480 #
11) T	2,4,5-TP ...	0.000	15.329	0	8536024	N.D.	3.456 #
12) T	2,4,5-T	0.000	15.993	0	15280239	N.D.	7.044 #
13) T	2,4-DB	16.485	0.000	5918941	0	113.683	N.D. #
16) T	DCPA	0.000	18.241	0	3607641	N.D.	1.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011119\
Data File : PP028774.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jan 2019 19:52
Operator : EI\MA
Sample : J1005-02
Misc : hexane
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 03:43:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010319.M
Quant Title : 8080.M
QLast Update : Fri Jan 04 01:40:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

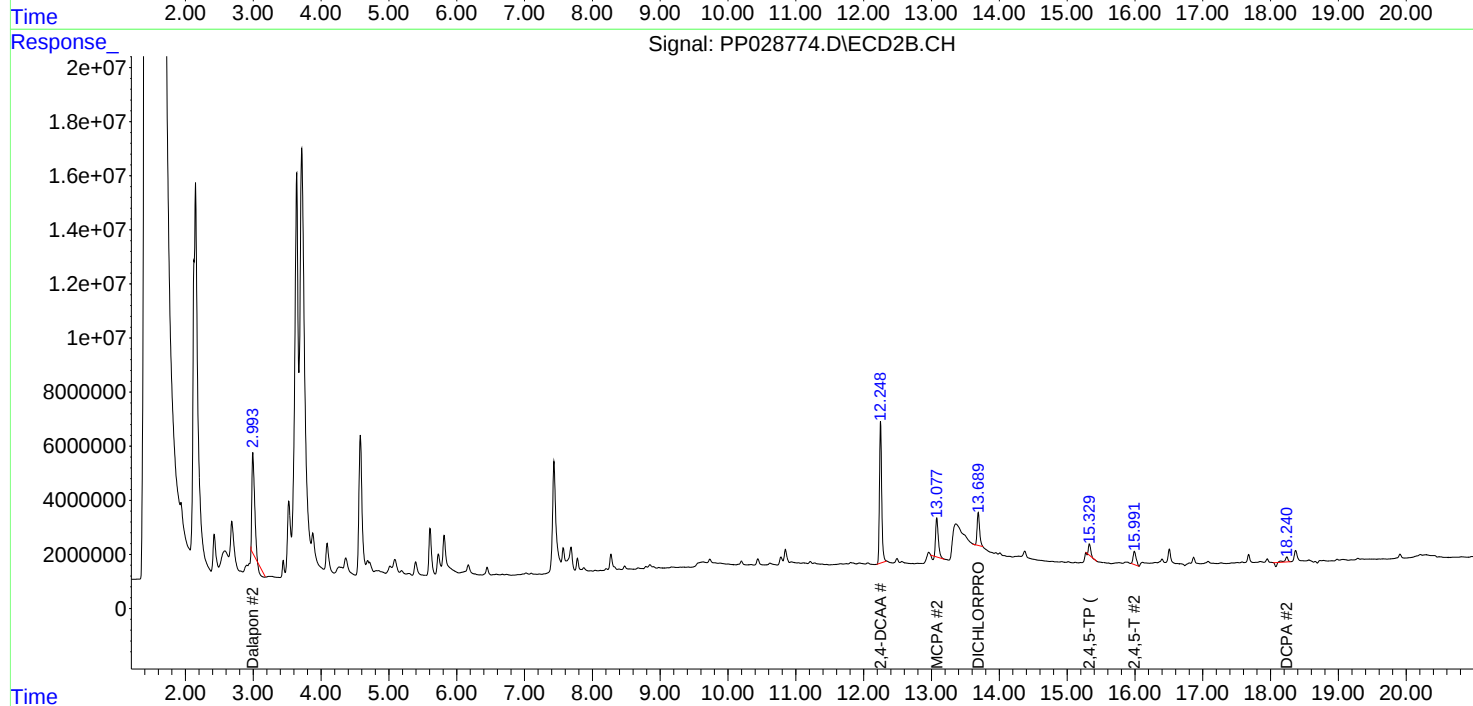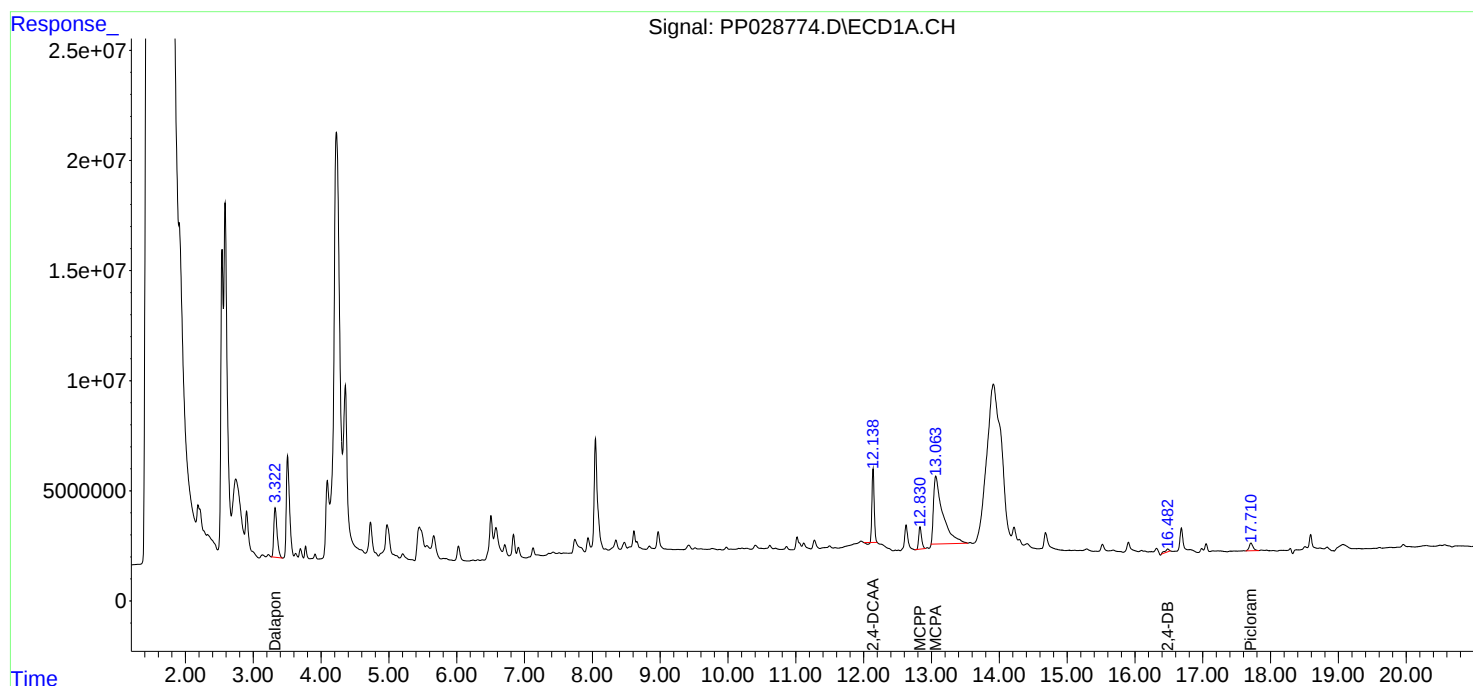


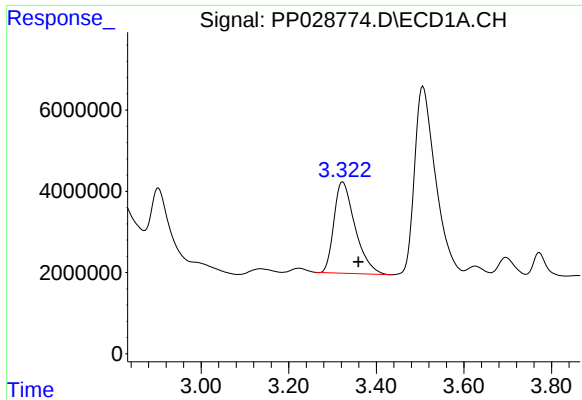

#1 Dalapon


R.T.: 3.324 min
Delta R.T.: -0.035 min
Response: 75444811
Conc: 123.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

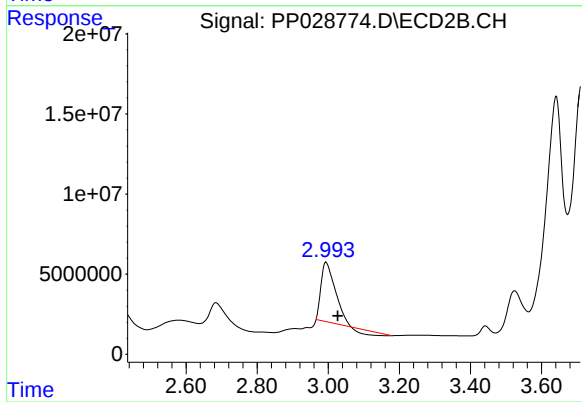


#1 Dalapon

R.T.: 2.995 min
Delta R.T.: -0.032 min
Response: 91289921
Conc: 156.16 ng/ml

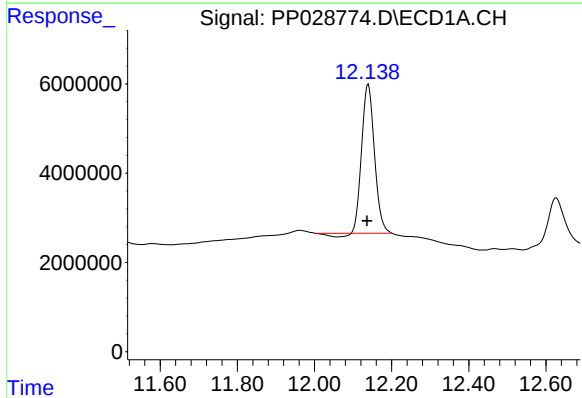


#4 2,4-DCAA

R.T.: 12.139 min
Delta R.T.: 0.003 min
Response: 75496071
Conc: 293.64 ng/ml

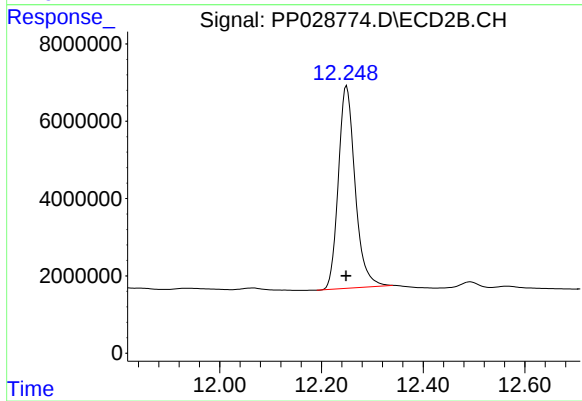

#4 2,4-DCAA


R.T.: 12.250 min
Delta R.T.: 0.001 min
Response: 119674164
Conc: 274.12 ng/ml

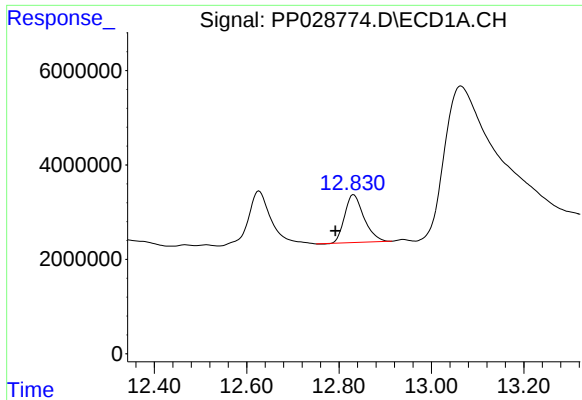

#6 MCPP


R.T.: 12.832 min
Delta R.T.: 0.040 min
Response: 29336374
Conc: 58.60 ug/ml

Instrument :
ECD_P
ClientSampleId :

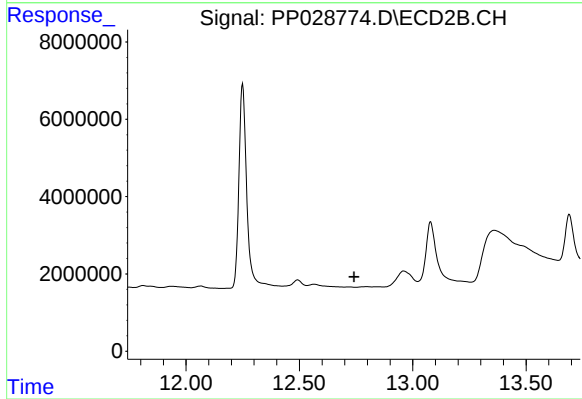


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 12.741 min
Response: 0
Conc: N.D.

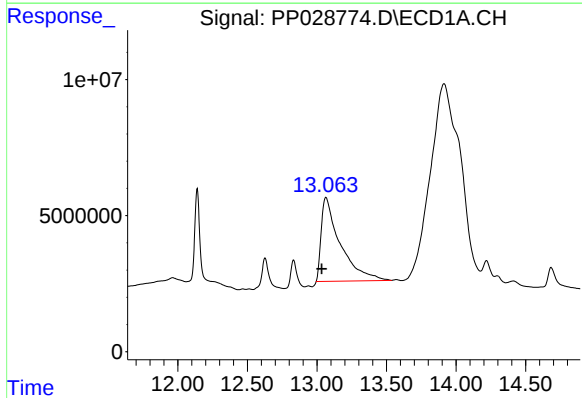


#7 MCPA

R.T.: 13.064 min
Delta R.T.: 0.029 min
Response: 293179580
Conc: 366.06 ug/ml

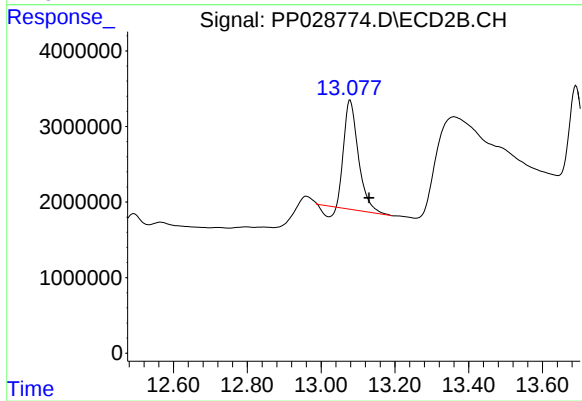

#7 MCPA


R.T.: 13.079 min
Delta R.T.: -0.050 min
Response: 37787278
Conc: 25.82 ug/ml

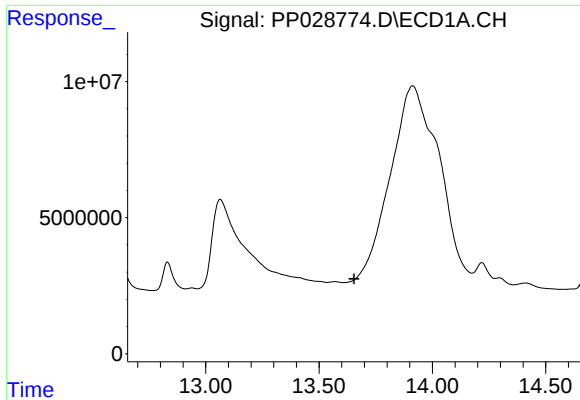

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.655 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

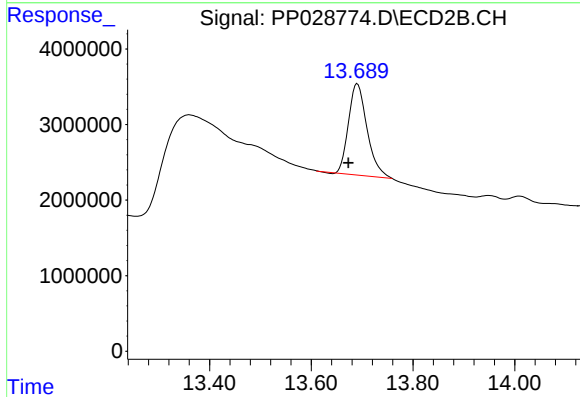


#8 DICHLORPROP

R.T.: 13.691 min
Delta R.T.: 0.018 min
Response: 30606326
Conc: 70.48 ng/ml

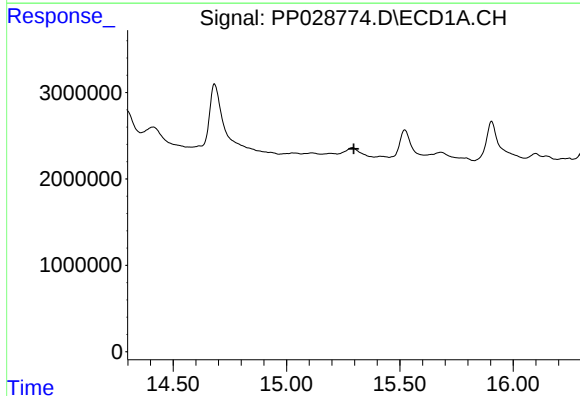


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 15.296 min
Response: 0
Conc: N.D.

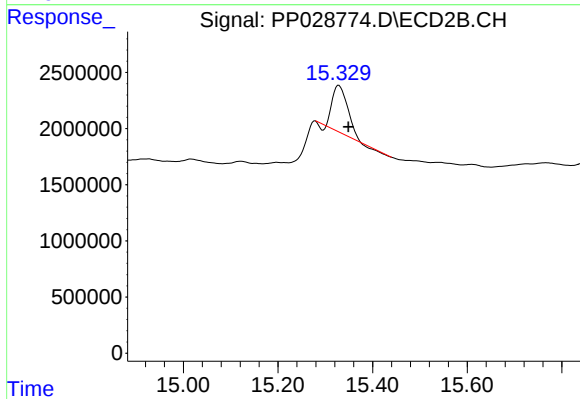

#11 2,4,5-TP (SILVEX)


R.T.: 15.329 min
Delta R.T.: -0.020 min
Response: 8536024
Conc: 3.46 ng/ml

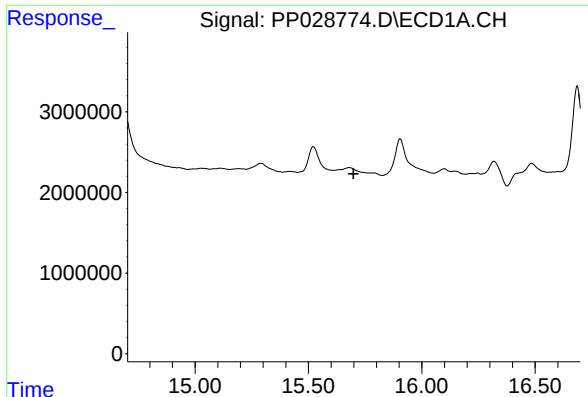

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.699 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

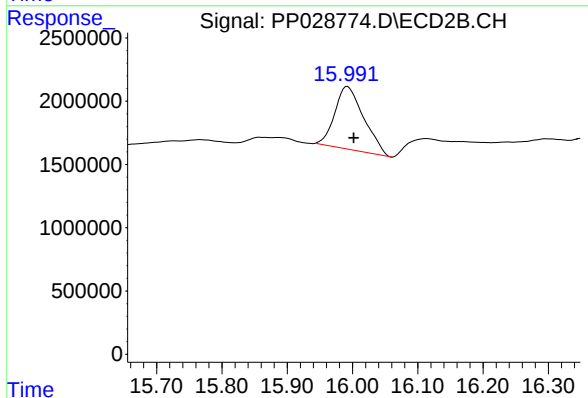


#12 2,4,5-T

R.T.: 15.993 min
Delta R.T.: -0.010 min
Response: 15280239
Conc: 7.04 ng/ml

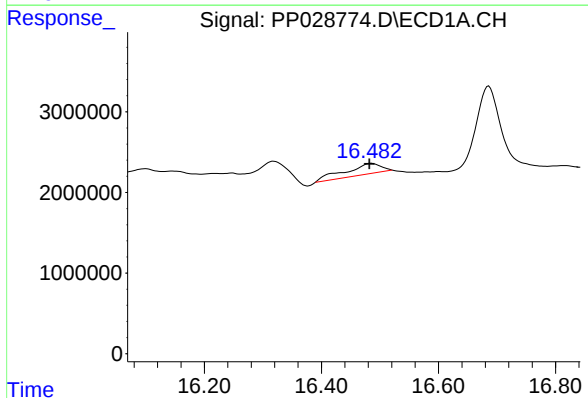


#13 2,4-DB

R.T.: 16.485 min
Delta R.T.: 0.003 min
Response: 5918941
Conc: 113.68 ng/ml

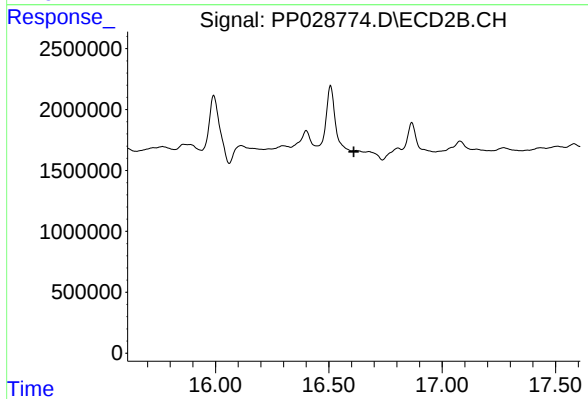

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.610 min
Response: 0
Conc: N.D.

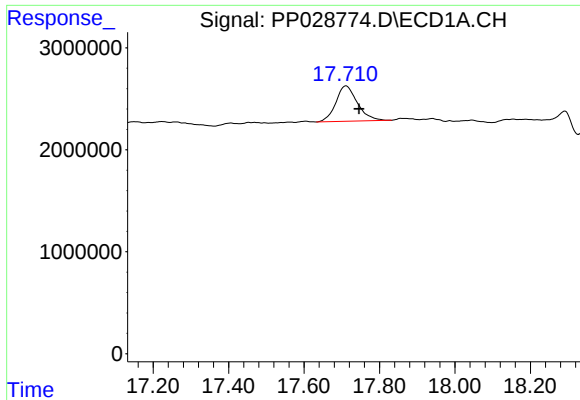

#15 Picloram


R.T.: 17.711 min
Delta R.T.: -0.034 min
Response: 13793280
Conc: 19.31 ng/ml

Instrument :
ECD_P
ClientSampleId :

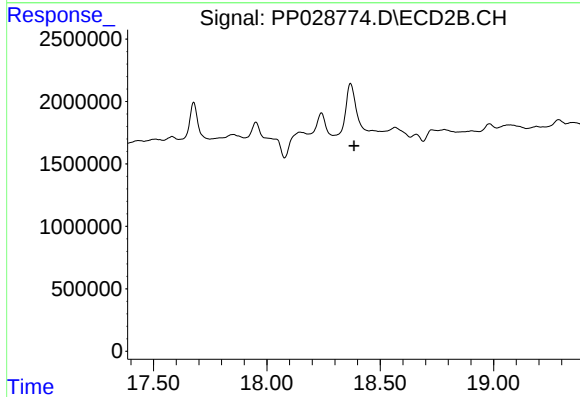


#15 Picloram

R.T.: 18.369 min
Delta R.T.: -0.015 min
Response: 11784149
Conc: N.D.

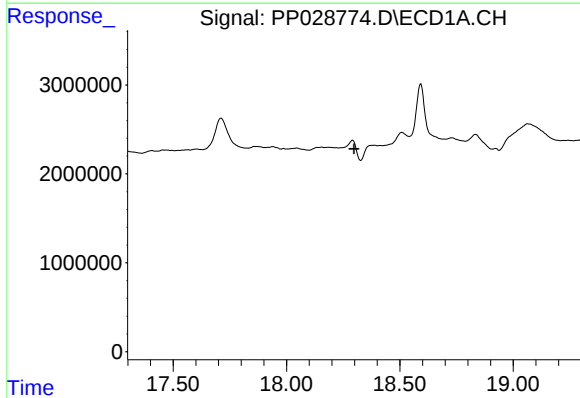

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 18.298 min
Response: 0
Conc: N.D.

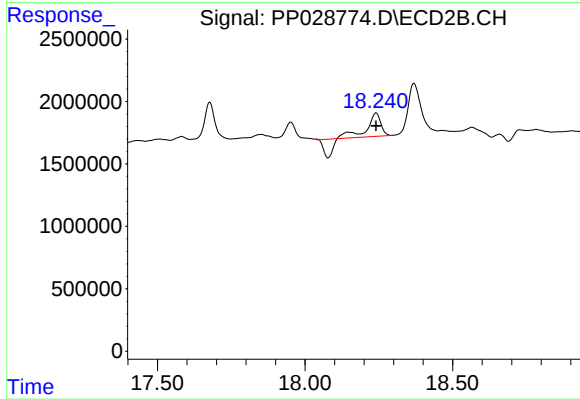

#16 DCPA

R.T.: 18.241 min
Delta R.T.: 0.000 min
Response: 3607641
Conc: 1.10 ng/ml