

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011123\
 Data File : PP054488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2023 03:44
 Operator : YP\AJ
 Sample : 01103-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 332

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/12/2023
 Supervised By :Ankita Jodhani 01/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 05:07:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 03:46:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.587	27528562	20505136	13.594	12.712
2) SA Decachlor...	10.095	8.605	9469613	10868289	6.594m	7.704

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011123\
Data File : PP054488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2023 03:44
Operator : YP\AJ
Sample : 01103-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
332


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/12/2023
Supervised By :Ankita Jodhani 01/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 05:07:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 03:46:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

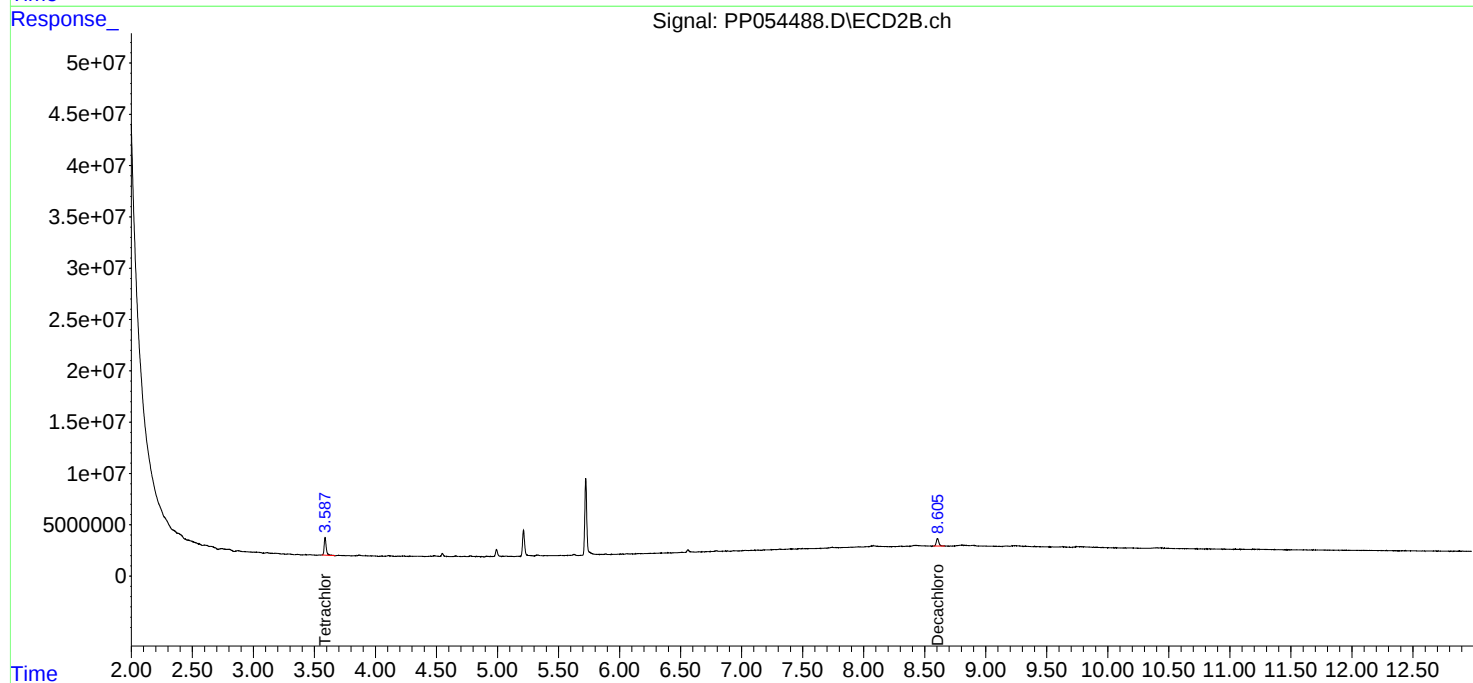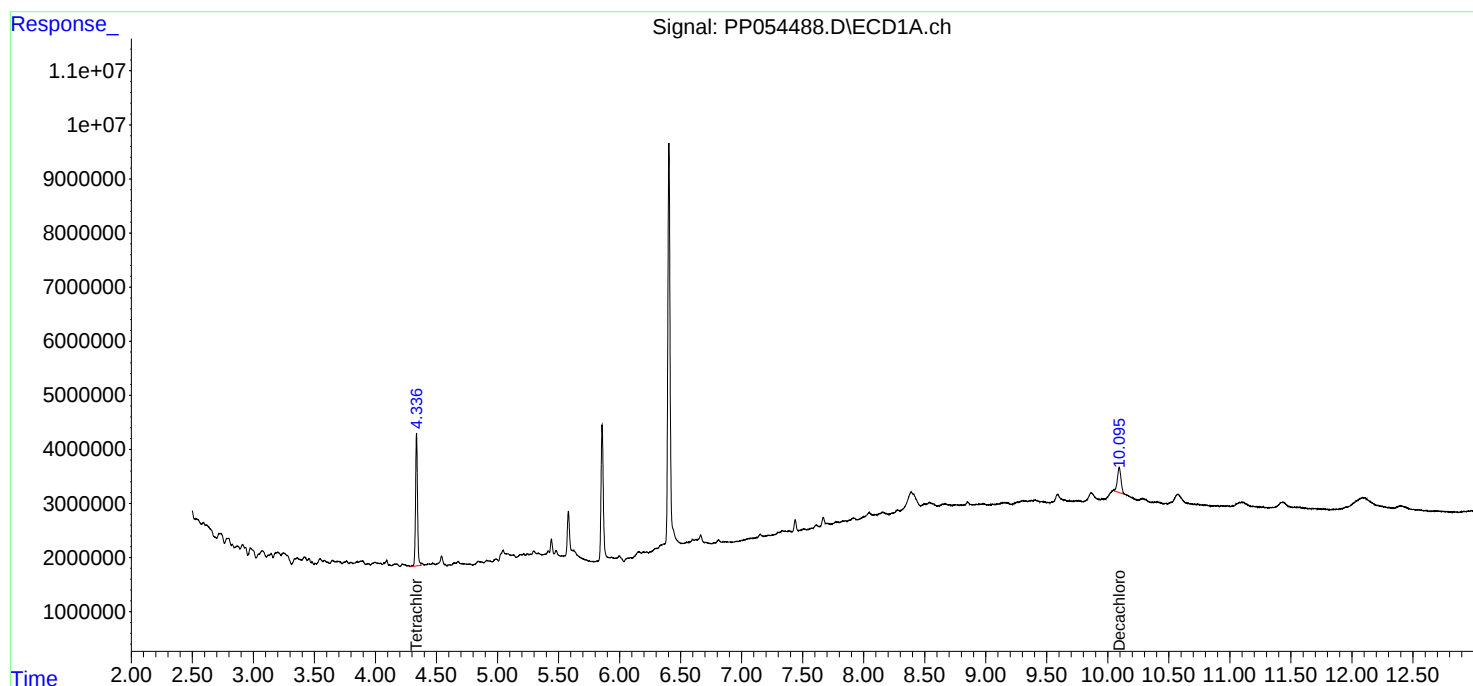

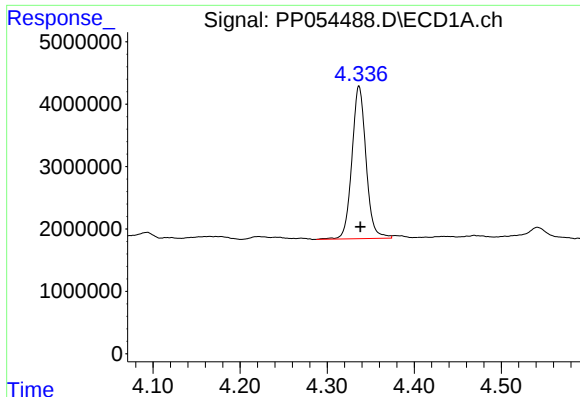


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: -0.001 min
Response: 27528562
Conc: 13.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
332


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/12/2023
Supervised By :Ankita Jodhani 01/12/2023

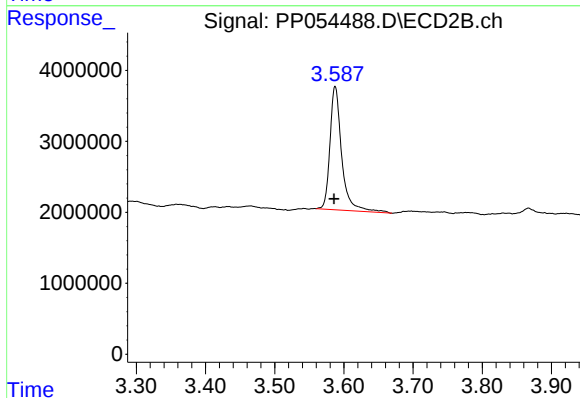


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: 0.001 min
Response: 20505136
Conc: 12.71 ng/ml

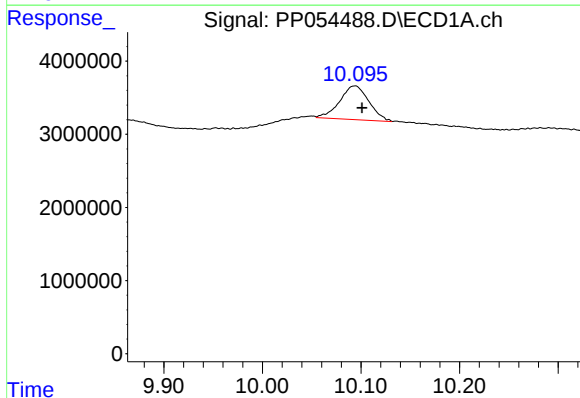

#2 Decachlorobiphenyl

R.T.: 10.095 min
Delta R.T.: -0.007 min
Response: 9469613
Conc: 6.59 ng/ml m

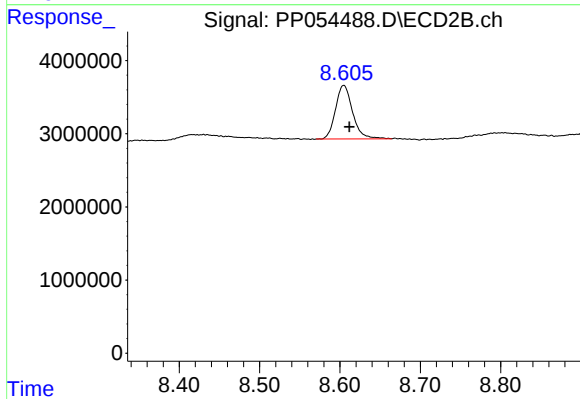

#2 Decachlorobiphenyl

R.T.: 8.605 min
Delta R.T.: -0.007 min
Response: 10868289
Conc: 7.70 ng/ml