

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032640.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 15:14
 Operator : DD\AJ
 Sample : M1077-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JC-03-011121-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:15:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.745	4.023	1342982	1084773	24.557	22.412
2) SA Decachlor...	10.577	9.303	1182599	1003806	26.416	22.607

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032640.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 15:14
Operator : DD\AJ
Sample : M1077-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
JC-03-011121-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:15:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

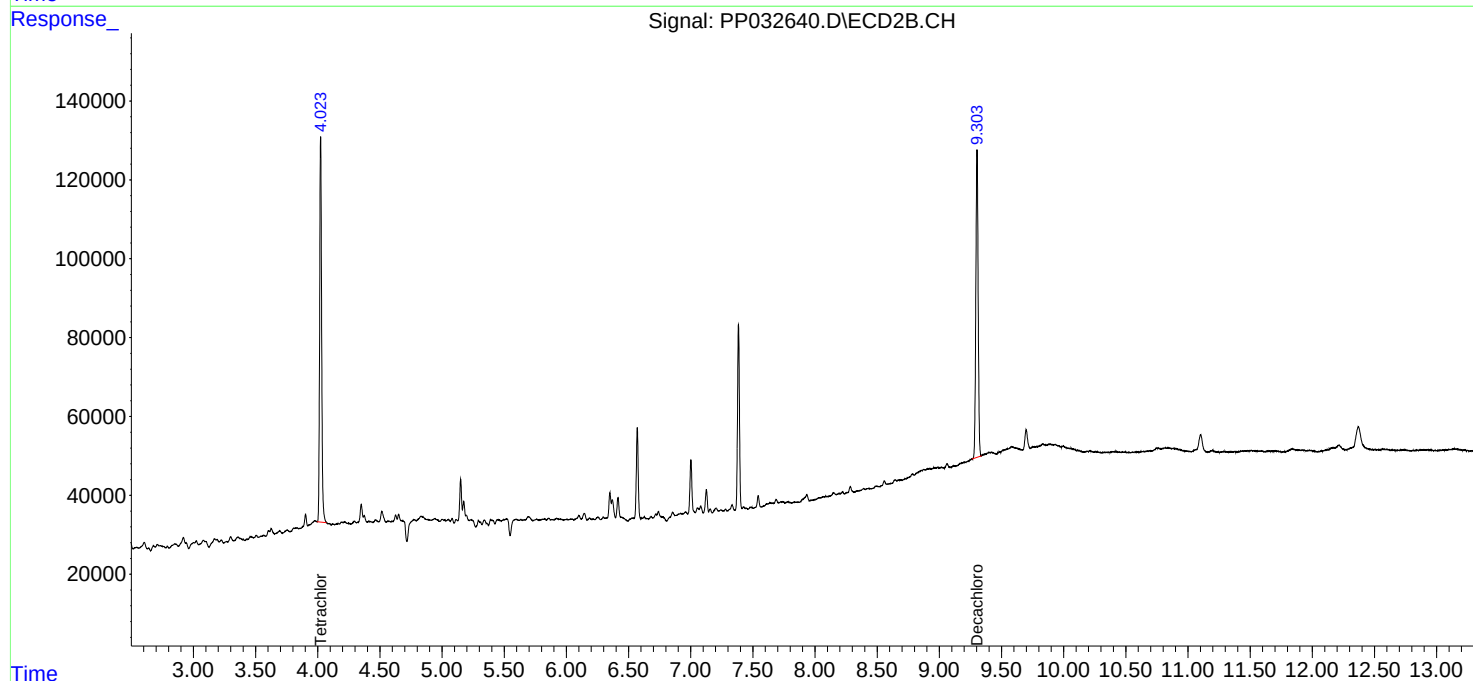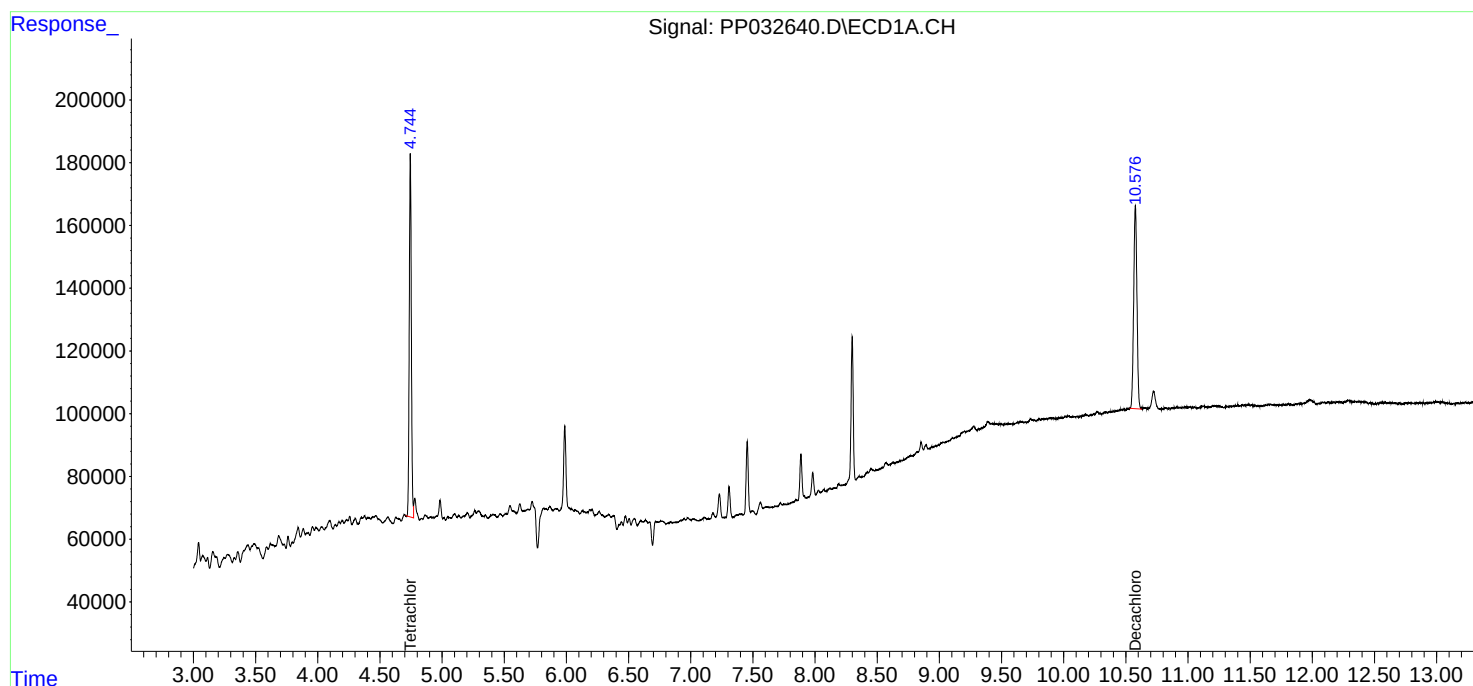


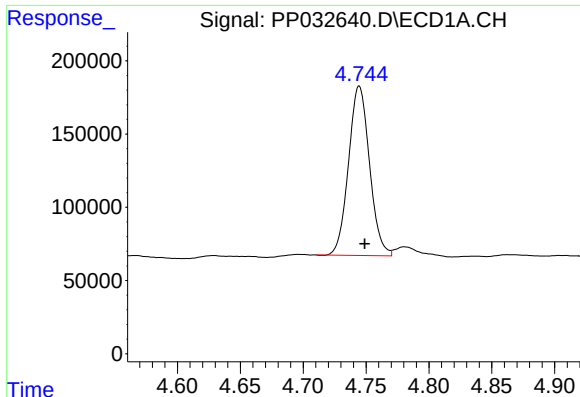

#1 Tetrachloro-m-xylene


R.T.: 4.745 min
Delta R.T.: -0.004 min
Response: 1342982
Conc: 24.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
JC-03-011121-B

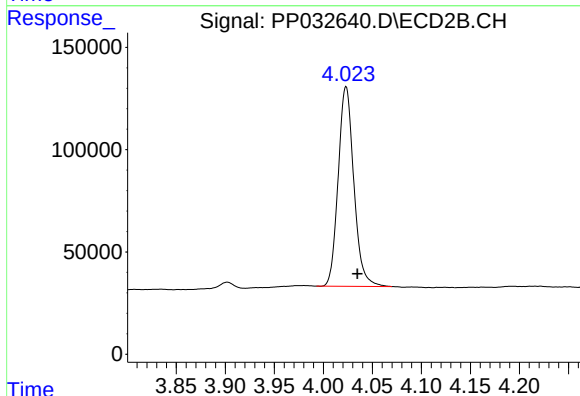


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: -0.012 min
Response: 1084773
Conc: 22.41 ng/ml

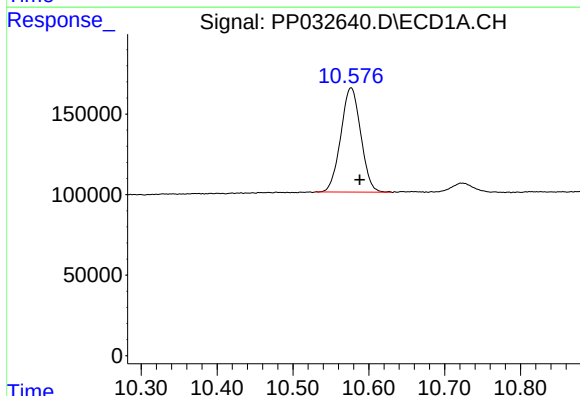

#2 Decachlorobiphenyl

R.T.: 10.577 min
Delta R.T.: -0.011 min
Response: 1182599
Conc: 26.42 ng/ml

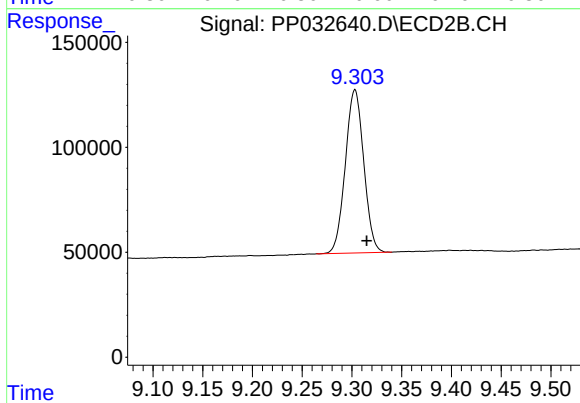

#2 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: -0.012 min
Response: 1003806
Conc: 22.61 ng/ml