

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032642.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 15:47
 Operator : DD\AJ
 Sample : M1081-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S-1

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:37:24 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:16:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.744	4.023	1665020	1300221	30.446	26.863
2) SA Decachlor...	10.576	9.303	1126703	1043697	25.167	23.506m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032642.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 15:47
Operator : DD\AJ
Sample : M1081-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:24 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:16:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

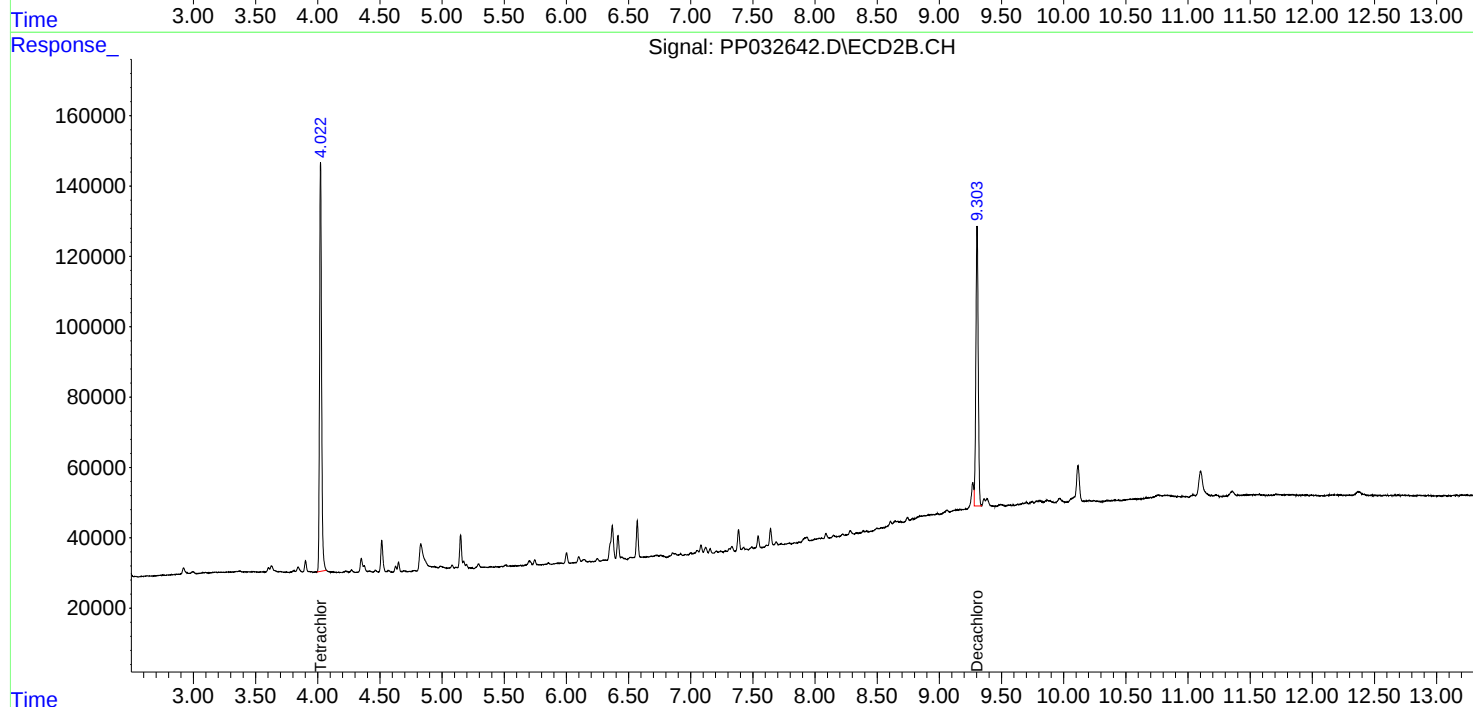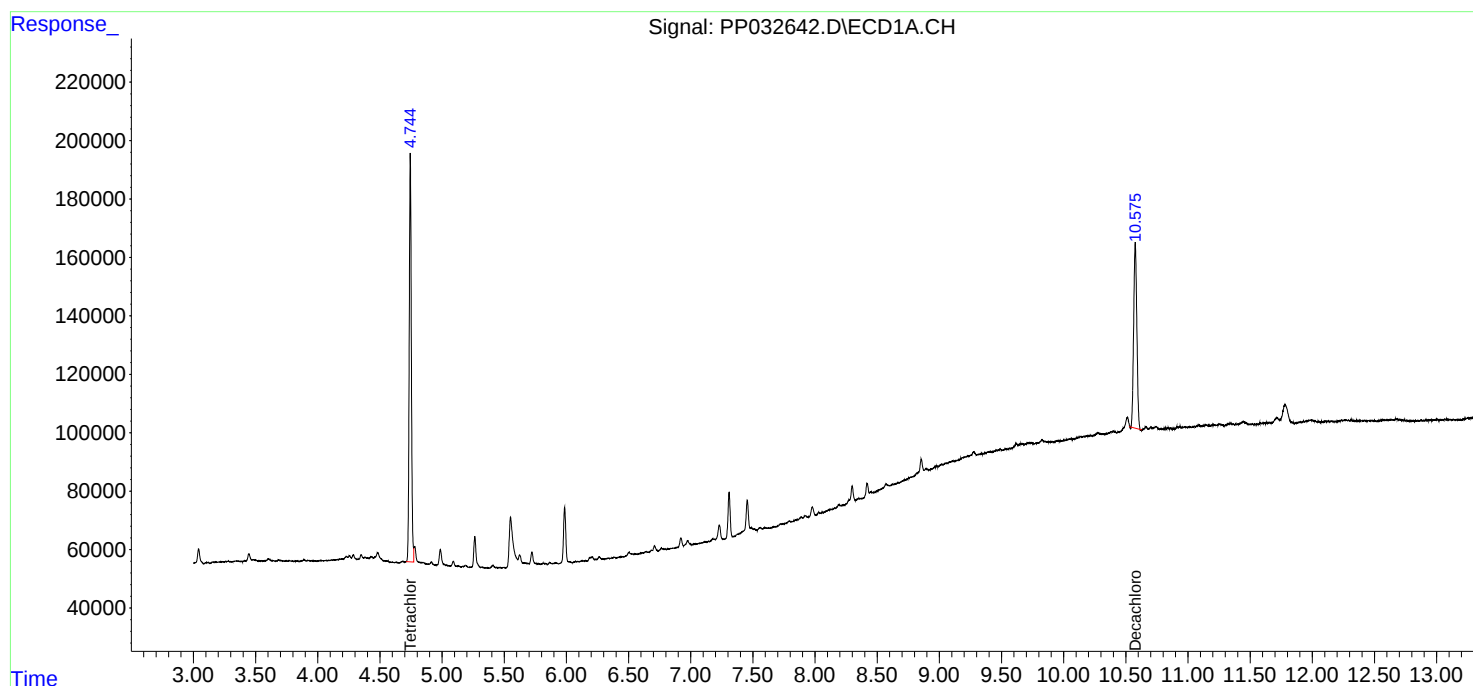

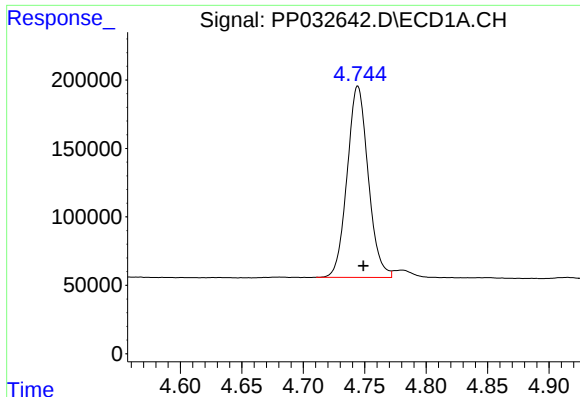


#1 Tetrachloro-m-xylene

R.T.: 4.744 min
Delta R.T.: -0.005 min
Response: 1665020
Conc: 30.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
S-1


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:24 PM

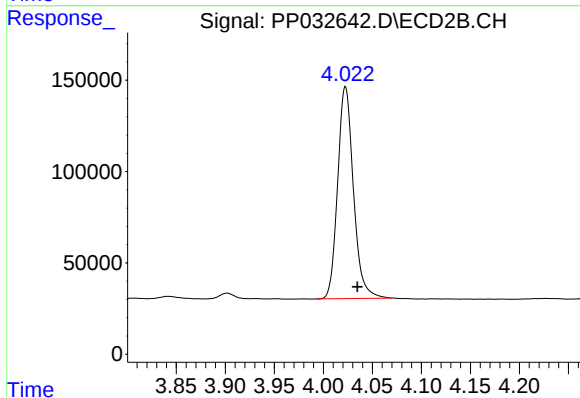


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: -0.012 min
Response: 1300221
Conc: 26.86 ng/ml

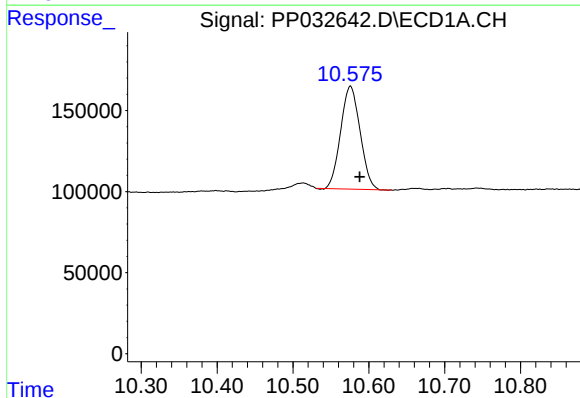

#2 Decachlorobiphenyl

R.T.: 10.576 min
Delta R.T.: -0.012 min
Response: 1126703
Conc: 25.17 ng/ml

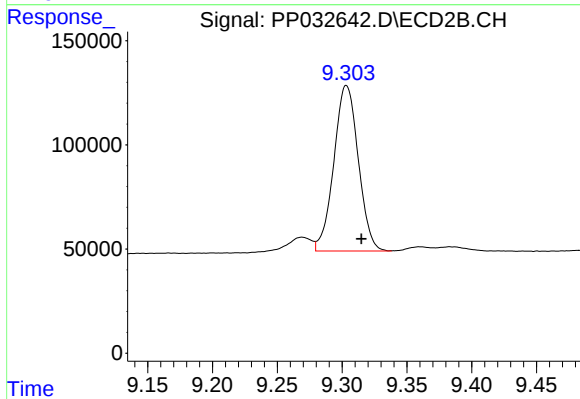

#2 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: -0.012 min
Response: 1043697
Conc: 23.51 ng/ml m