

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032655.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 20:02
 Operator : DD\AJ
 Sample : M1092-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-3A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:37:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:25:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.744	4.020	1797717	1390360	32.872	28.725
2) SA Decachlor...	10.576	9.299f	1138573	1112150	25.432	25.048
Target Compounds						
26) L6 AR-1254-1	6.947	6.137	242638	183462	121.804	73.071 #
27) L6 AR-1254-2	7.176	6.296	319683	228811	105.522	106.770
28) L6 AR-1254-3	7.554	6.716	743476	873916	228.201	244.364
29) L6 AR-1254-4	7.847	6.955f	392893	317997	170.514	154.379
30) L6 AR-1254-5	8.277	7.382f	971438	14188041	395.574m	4588.126 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032655.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 20:02
Operator : DD\AJ
Sample : M1092-07
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
263K-3A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:25:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

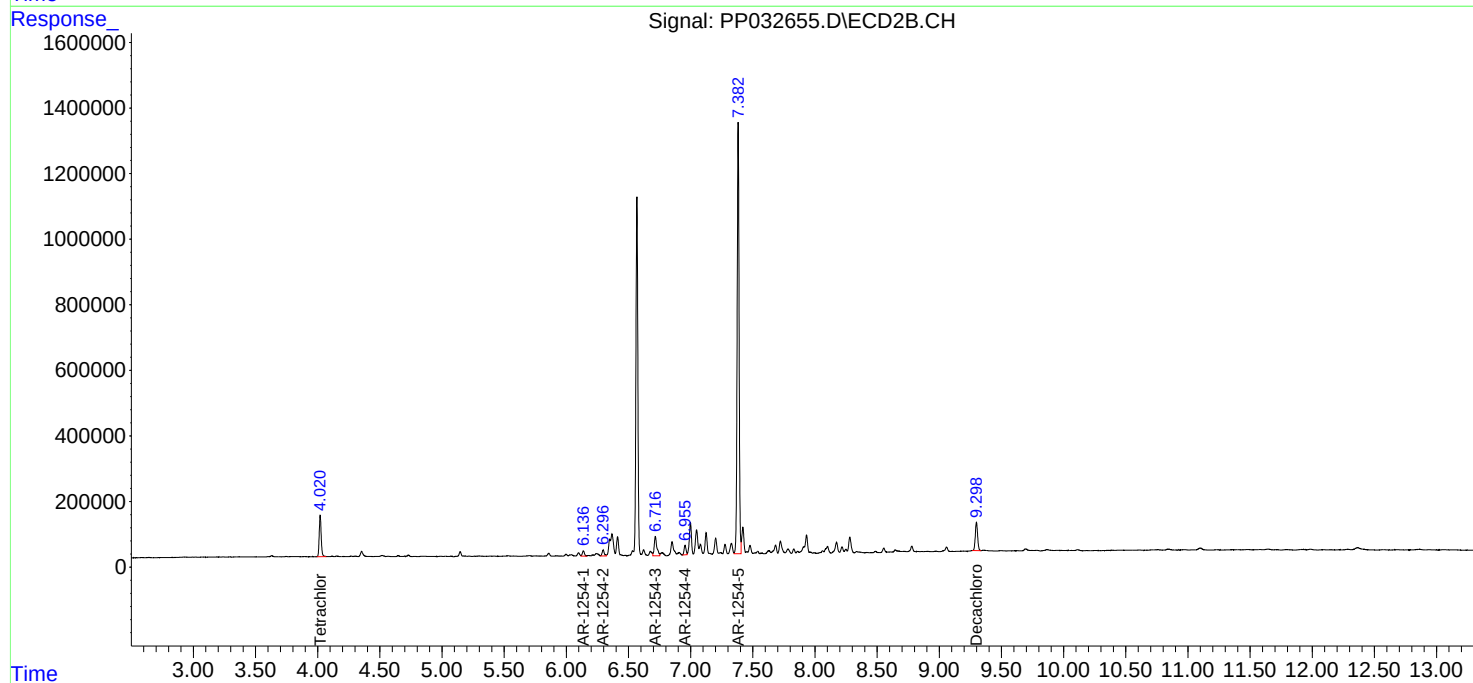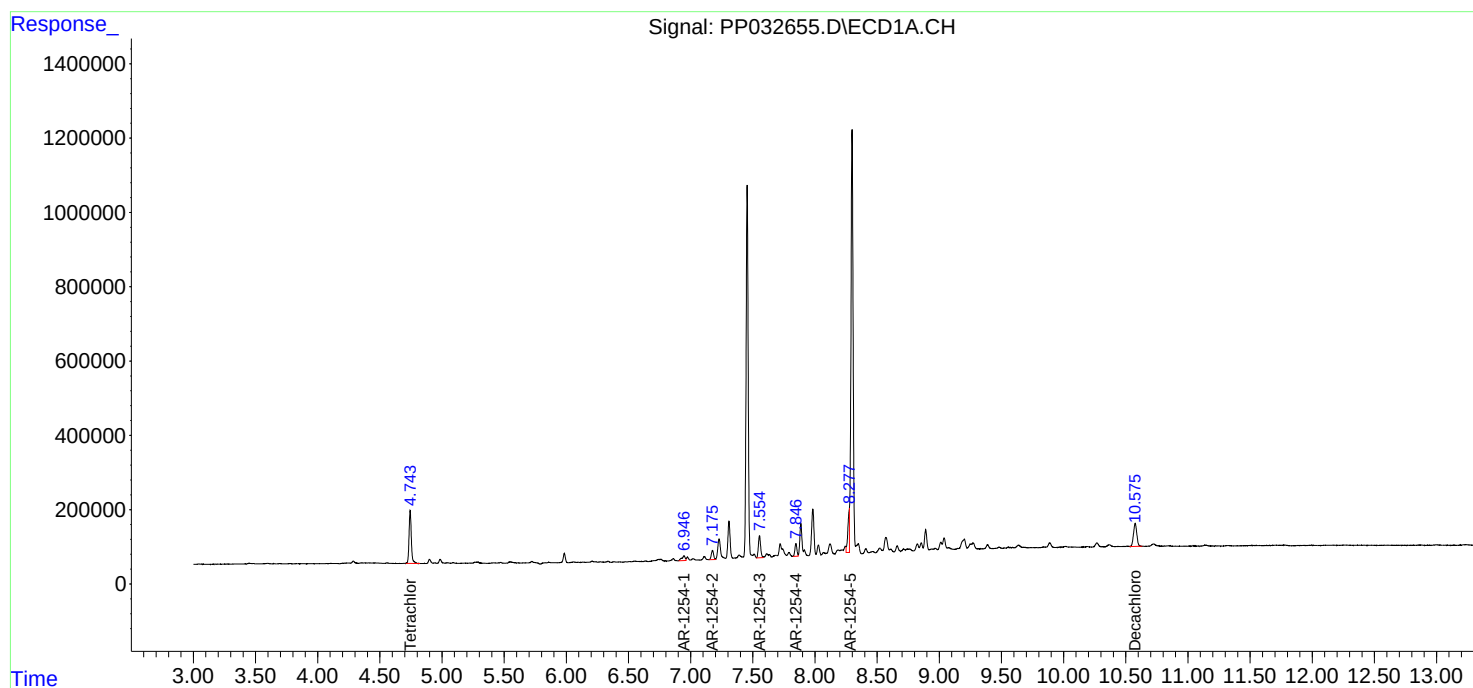

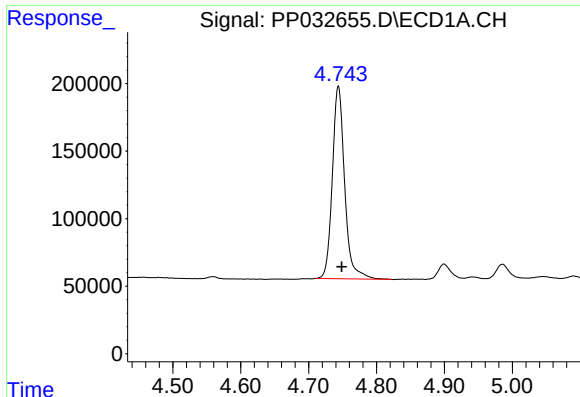


#1 Tetrachloro-m-xylene

R.T.: 4.744 min
Delta R.T.: -0.005 min
Response: 1797717
Conc: 32.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-3A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:53 PM

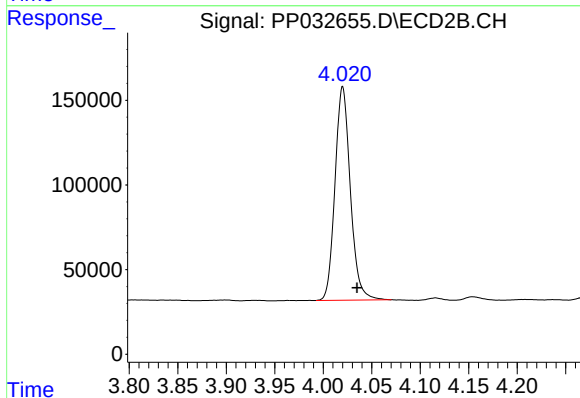


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: -0.015 min
Response: 1390360
Conc: 28.73 ng/ml

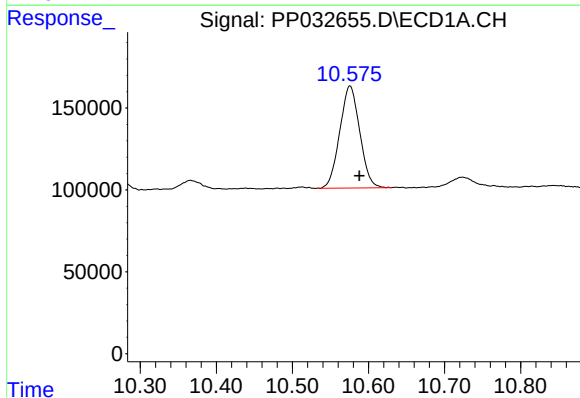


#2 Decachlorobiphenyl

R.T.: 10.576 min
Delta R.T.: -0.012 min
Response: 1138573
Conc: 25.43 ng/ml

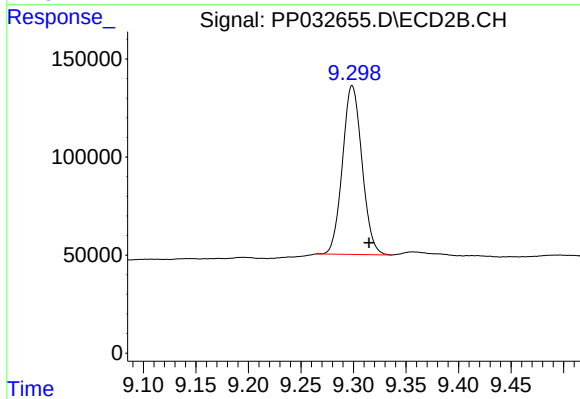

#2 Decachlorobiphenyl

R.T.: 9.299 min
Delta R.T.: -0.016 min
Response: 1112150
Conc: 25.05 ng/ml

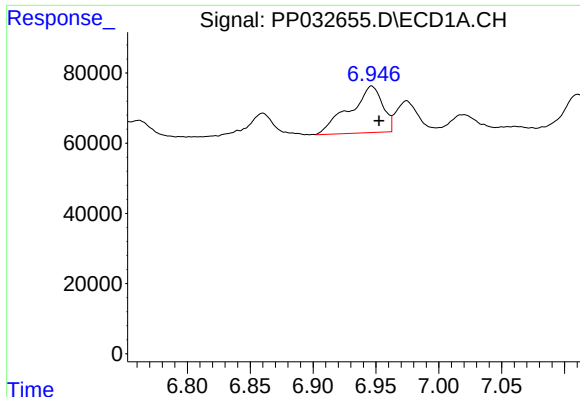


#26 AR-1254-1

R.T.: 6.947 min
Delta R.T.: -0.006 min
Response: 242638
Conc: 121.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-3A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:53 PM

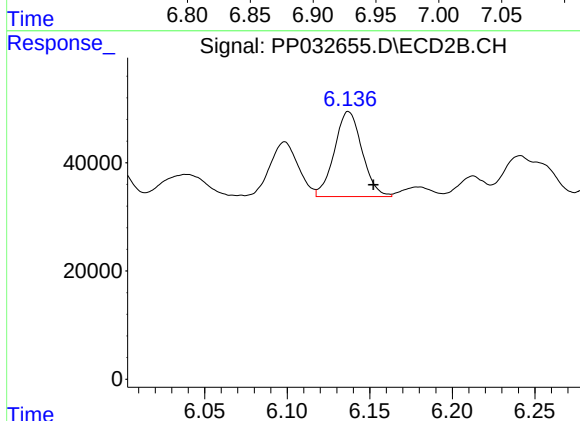


#26 AR-1254-1

R.T.: 6.137 min
Delta R.T.: -0.015 min
Response: 183462
Conc: 73.07 ng/ml

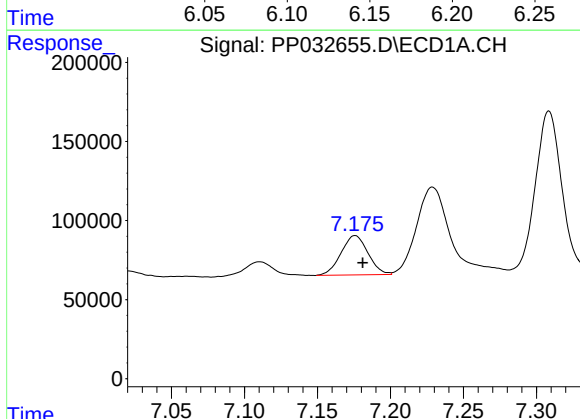


#27 AR-1254-2

R.T.: 7.176 min
Delta R.T.: -0.005 min
Response: 319683
Conc: 105.52 ng/ml

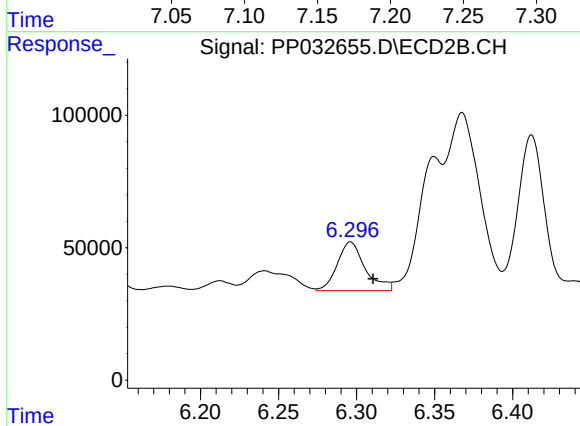

#27 AR-1254-2

R.T.: 6.296 min
Delta R.T.: -0.015 min
Response: 228811
Conc: 106.77 ng/ml

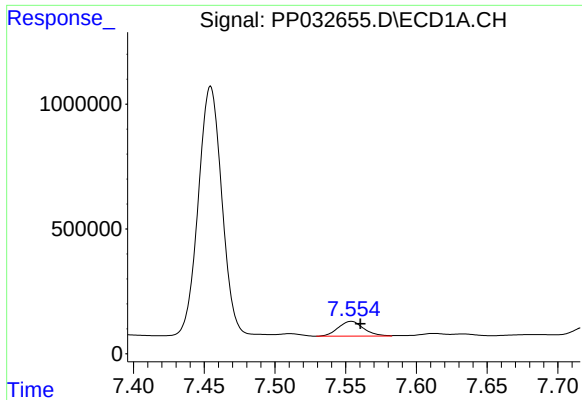


#28 AR-1254-3

R.T.: 7.554 min
Delta R.T.: -0.006 min
Response: 743476
Conc: 228.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-3A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:53 PM

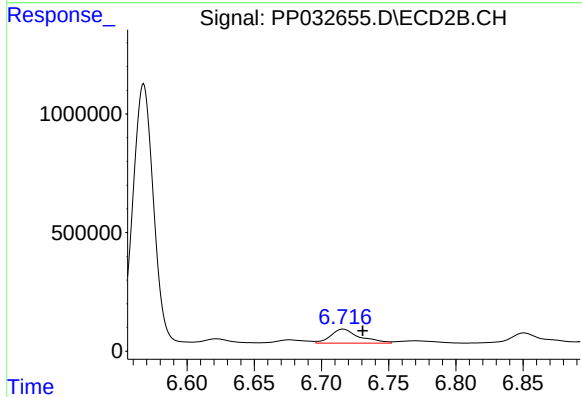


#28 AR-1254-3

R.T.: 6.716 min
Delta R.T.: -0.015 min
Response: 873916
Conc: 244.36 ng/ml

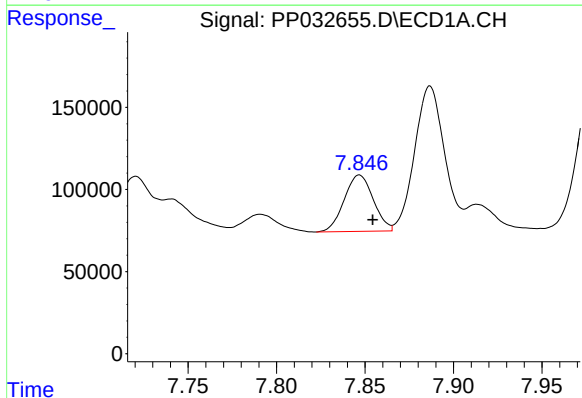


#29 AR-1254-4

R.T.: 7.847 min
Delta R.T.: -0.007 min
Response: 392893
Conc: 170.51 ng/ml

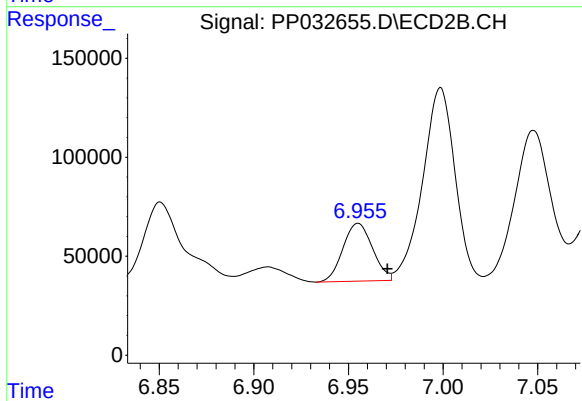

#29 AR-1254-4

R.T.: 6.955 min
Delta R.T.: -0.015 min
Response: 317997
Conc: 154.38 ng/ml

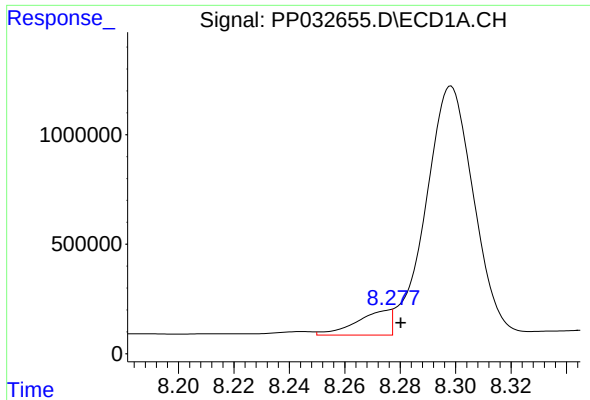


#30 AR-1254-5

R.T.: 8.277 min
Delta R.T.: -0.004 min
Response: 971438
Conc: 395.57 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-3A

Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:53 PM

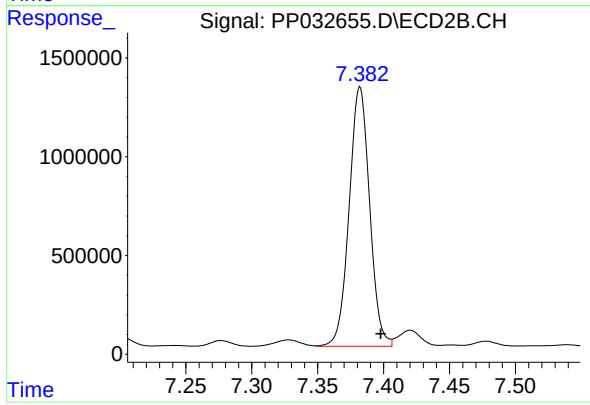

#30 AR-1254-5

R.T.: 7.382 min
Delta R.T.: -0.016 min
Response: 14188041
Conc: 4588.13 ng/ml