

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032656.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 20:19
 Operator : DD\AJ
 Sample : M1092-10
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-4A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:37:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:26:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.744	4.020f	1683797	1326927	30.789	27.415
2)	SA Decachlor...	10.577	9.300f	1041622	1018330	23.267	22.935
Target Compounds							
26)	L6 AR-1254-1	6.946	6.137f	83898	114156	42.117	45.467
27)	L6 AR-1254-2	7.175	6.296	185091	172707	61.095	80.591 #
28)	L6 AR-1254-3	7.554	6.715f	535225	679974	164.281	190.134
29)	L6 AR-1254-4	7.847	6.955f	291133	246765	126.351	119.798
30)	L6 AR-1254-5	8.277	7.382f	867807	7703186	353.375m	2491.055 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032656.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 20:19
Operator : DD\AJ
Sample : M1092-10
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
263K-4A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:26:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

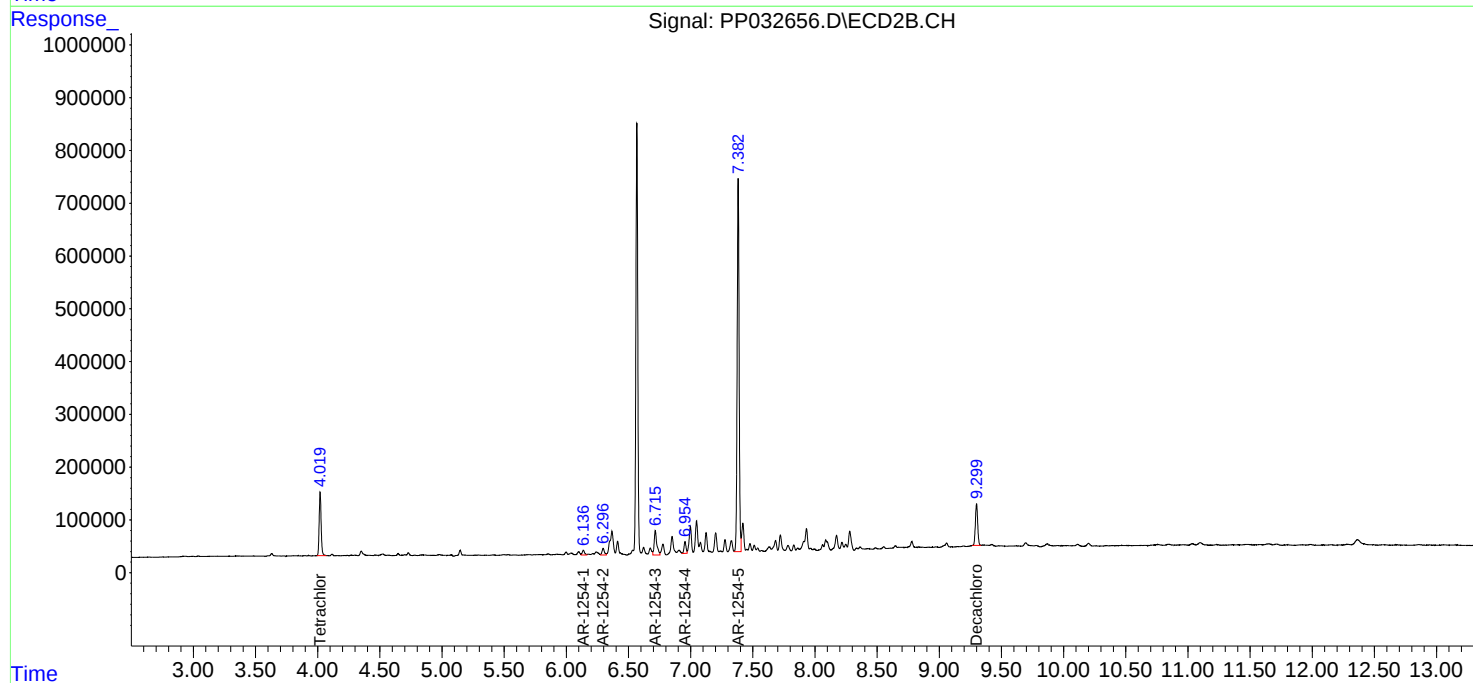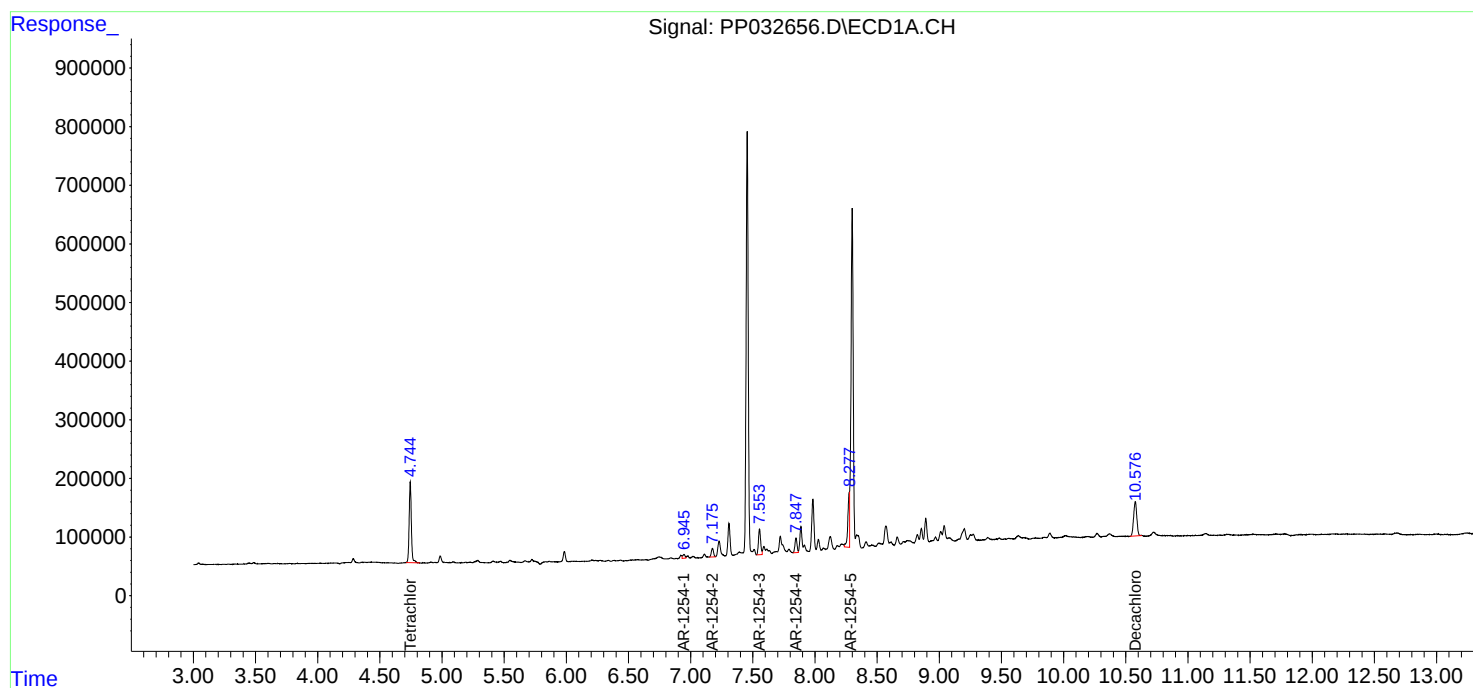

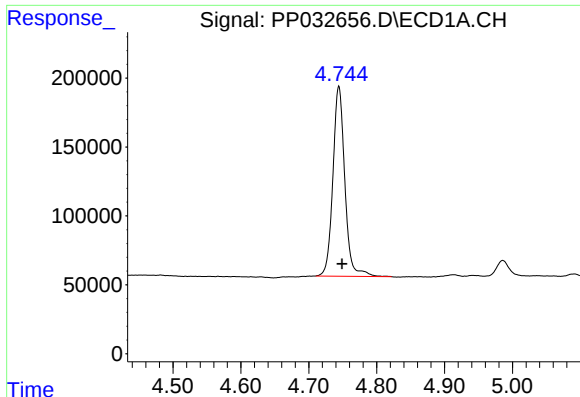


#1 Tetrachloro-m-xylene

R.T.: 4.744 min
Delta R.T.: -0.005 min
Response: 1683797
Conc: 30.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-4A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:55 PM

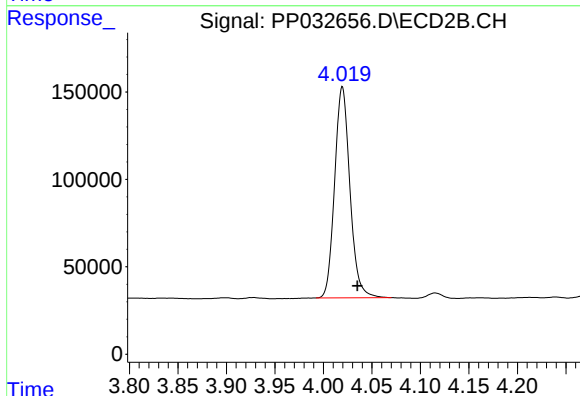


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: -0.015 min
Response: 1326927
Conc: 27.41 ng/ml

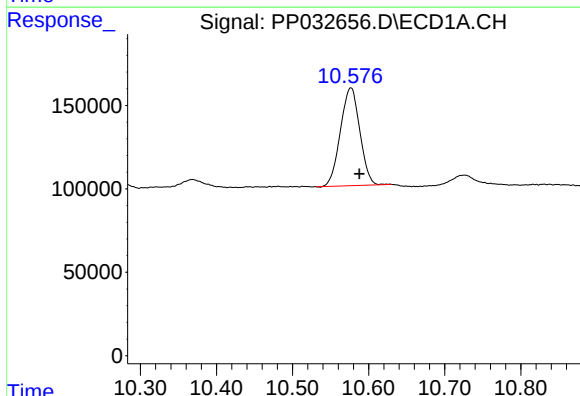


#2 Decachlorobiphenyl

R.T.: 10.577 min
Delta R.T.: -0.011 min
Response: 1041622
Conc: 23.27 ng/ml

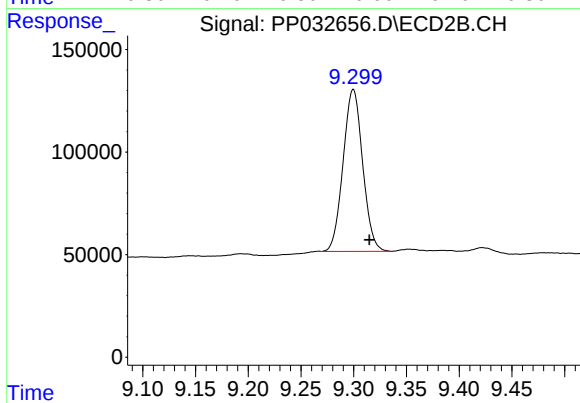

#2 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.015 min
Response: 1018330
Conc: 22.93 ng/ml

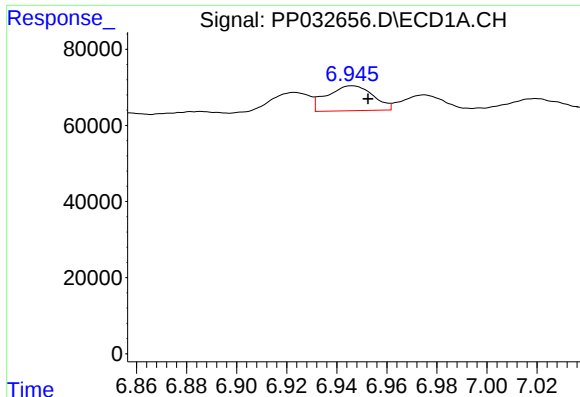


#26 AR-1254-1

R.T.: 6.946 min
Delta R.T.: -0.006 min
Response: 83898
Conc: 42.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-4A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:55 PM

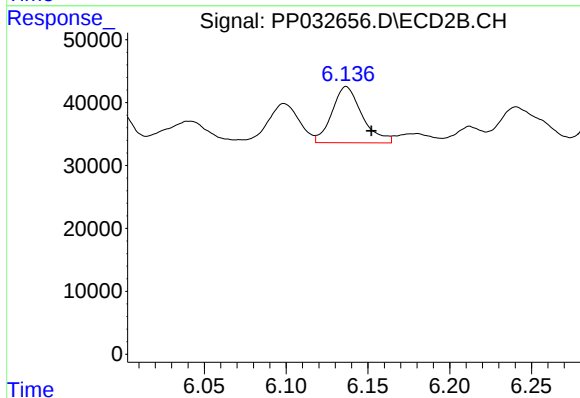


#26 AR-1254-1

R.T.: 6.137 min
Delta R.T.: -0.015 min
Response: 114156
Conc: 45.47 ng/ml

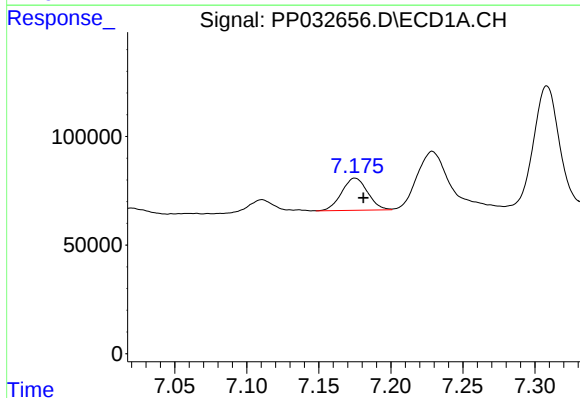


#27 AR-1254-2

R.T.: 7.175 min
Delta R.T.: -0.006 min
Response: 185091
Conc: 61.10 ng/ml

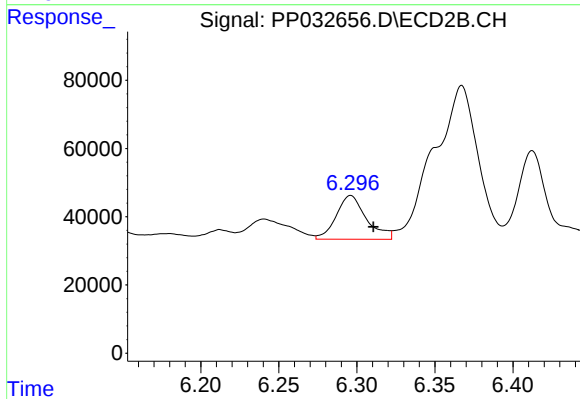

#27 AR-1254-2

R.T.: 6.296 min
Delta R.T.: -0.015 min
Response: 172707
Conc: 80.59 ng/ml

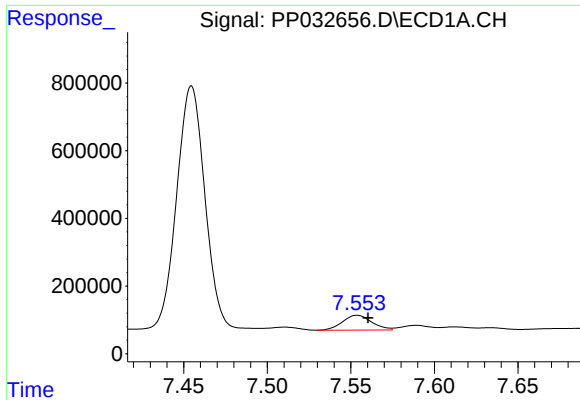


#28 AR-1254-3

R.T.: 7.554 min
Delta R.T.: -0.006 min
Response: 535225
Conc: 164.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-4A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:55 PM

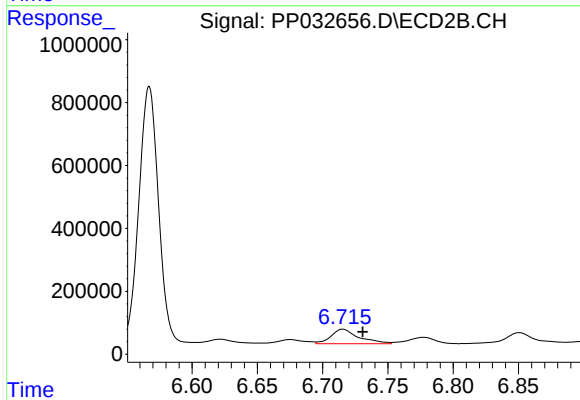


#28 AR-1254-3

R.T.: 6.715 min
Delta R.T.: -0.015 min
Response: 679974
Conc: 190.13 ng/ml

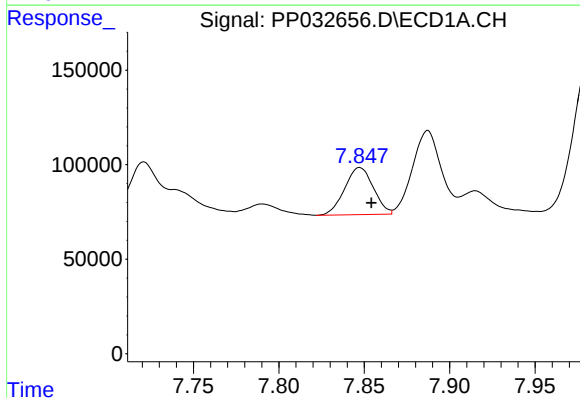


#29 AR-1254-4

R.T.: 7.847 min
Delta R.T.: -0.007 min
Response: 291133
Conc: 126.35 ng/ml

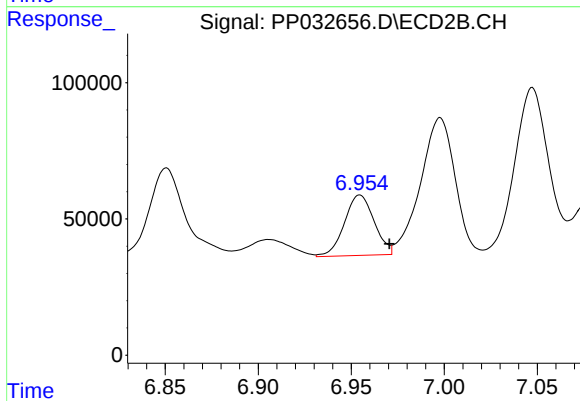

#29 AR-1254-4

R.T.: 6.955 min
Delta R.T.: -0.016 min
Response: 246765
Conc: 119.80 ng/ml

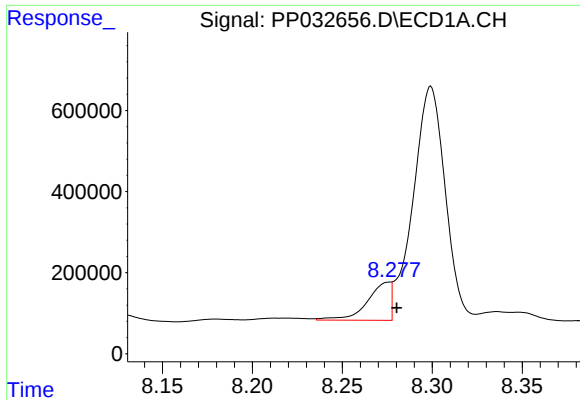


#30 AR-1254-5

R.T.: 8.277 min
Delta R.T.: -0.003 min
Response: 867807
Conc: 353.38 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-4A

Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:55 PM

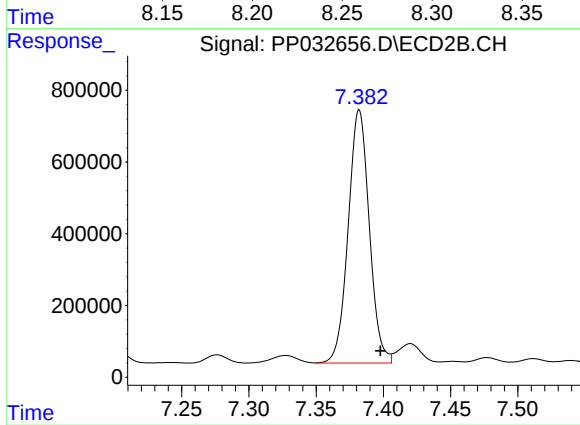

#30 AR-1254-5

R.T.: 7.382 min
Delta R.T.: -0.016 min
Response: 7703186
Conc: 2491.05 ng/ml