

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032657.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 20:36
 Operator : DD\AJ
 Sample : M1092-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-5A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:37:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:26:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.744	4.020f	1689008	1348771	30.885	27.866
2)	SA Decachlor...	10.575	9.301	915150	871309	20.442	19.623
Target Compounds							
26)	L6 AR-1254-1	6.946	6.137f	111689	130827	56.068	52.107
27)	L6 AR-1254-2	7.175	6.297	234668	217505	77.460	101.495 #
28)	L6 AR-1254-3	7.554	6.716	587380	746905	180.289	208.849
29)	L6 AR-1254-4	7.847	6.955f	326600	297067	141.743	144.218
30)	L6 AR-1254-5	8.278	7.382f	894245	9571024	364.141m	3095.076 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032657.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 20:36
Operator : DD\AJ
Sample : M1092-13
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
263K-5A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:26:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

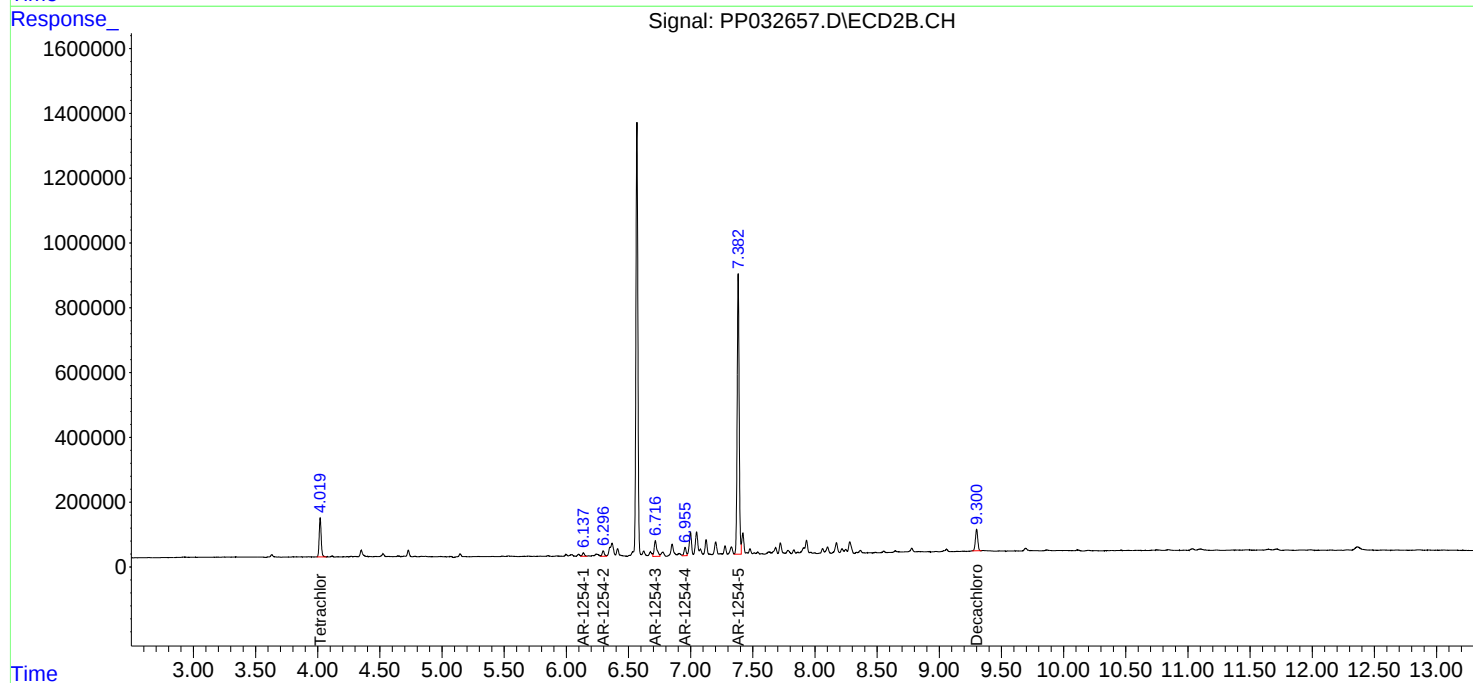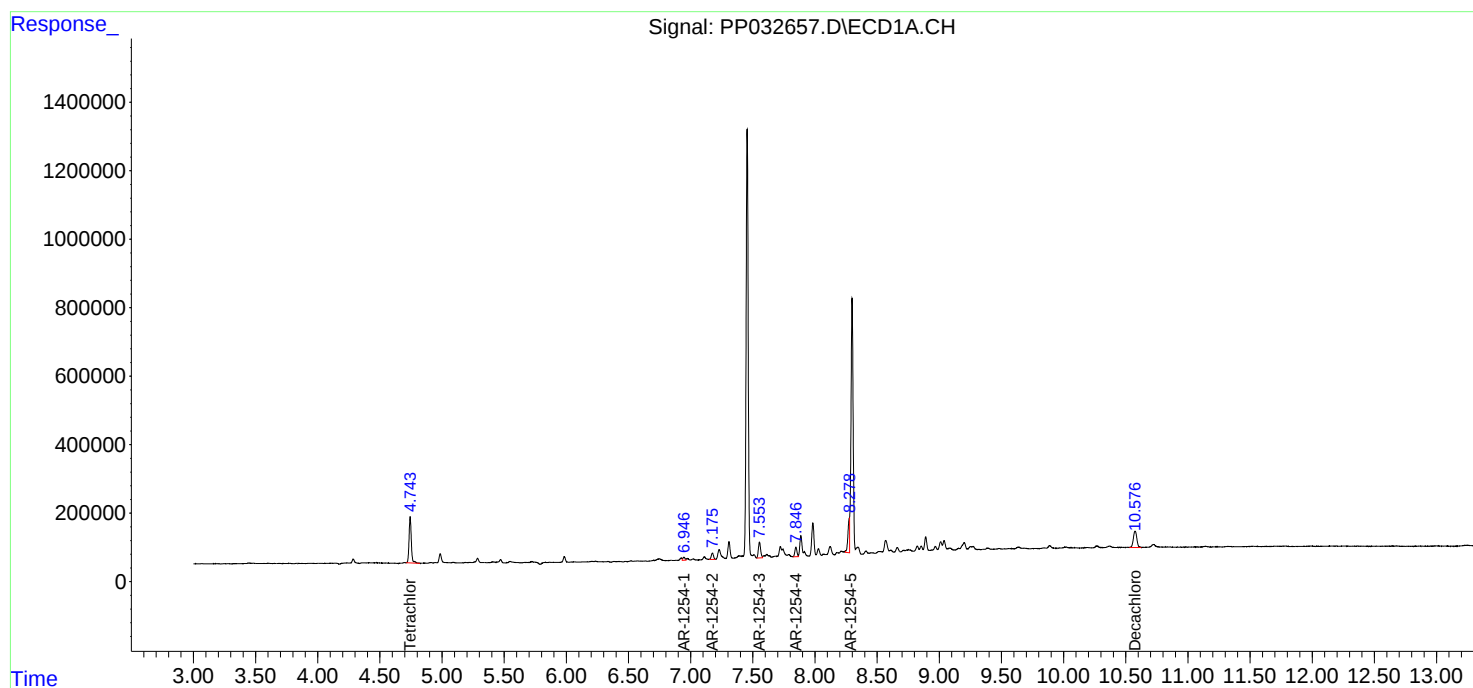

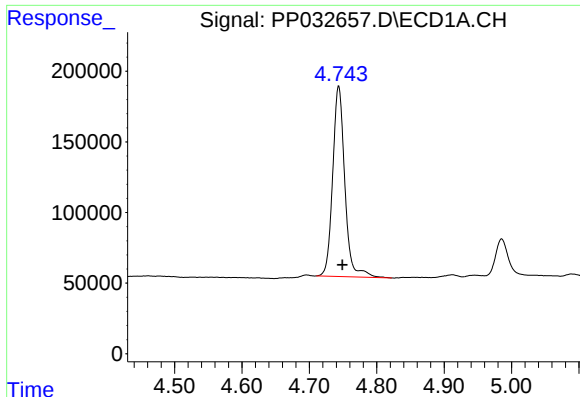


#1 Tetrachloro-m-xylene

R.T.: 4.744 min
Delta R.T.: -0.005 min
Response: 1689008
Conc: 30.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-5A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:56 PM

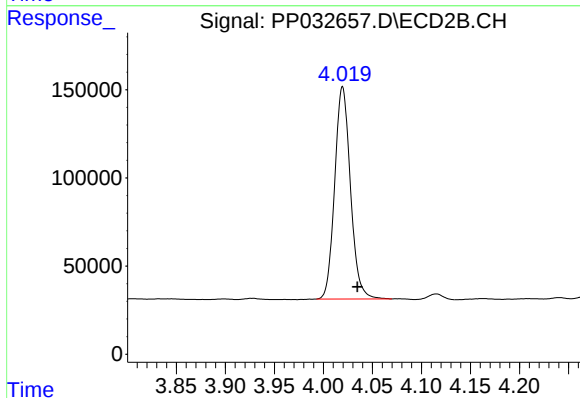


#1 Tetrachloro-m-xylene

R.T.: 4.020 min
Delta R.T.: -0.015 min
Response: 1348771
Conc: 27.87 ng/ml

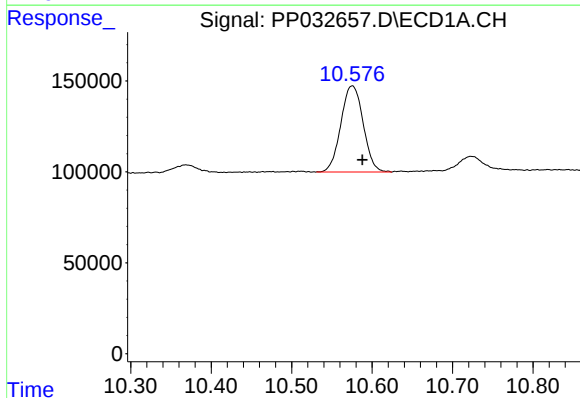


#2 Decachlorobiphenyl

R.T.: 10.575 min
Delta R.T.: -0.013 min
Response: 915150
Conc: 20.44 ng/ml

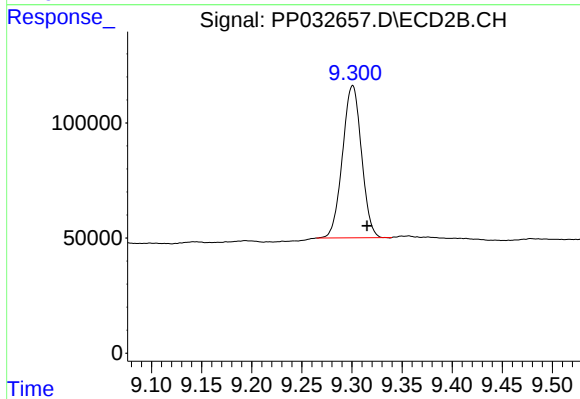

#2 Decachlorobiphenyl

R.T.: 9.301 min
Delta R.T.: -0.014 min
Response: 871309
Conc: 19.62 ng/ml

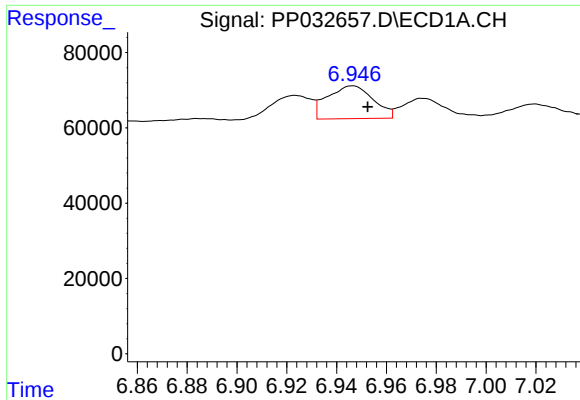


#26 AR-1254-1

R.T.: 6.946 min
Delta R.T.: -0.006 min
Response: 111689
Conc: 56.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-5A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:56 PM

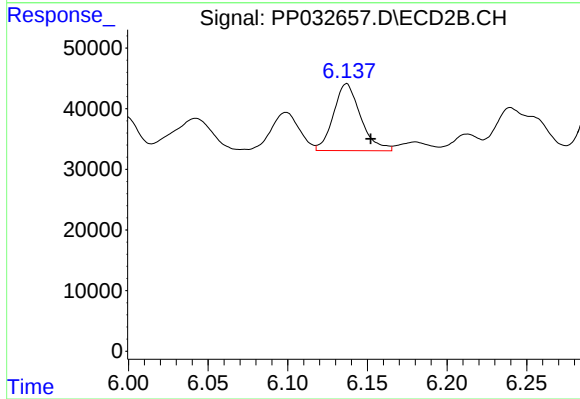


#26 AR-1254-1

R.T.: 6.137 min
Delta R.T.: -0.015 min
Response: 130827
Conc: 52.11 ng/ml

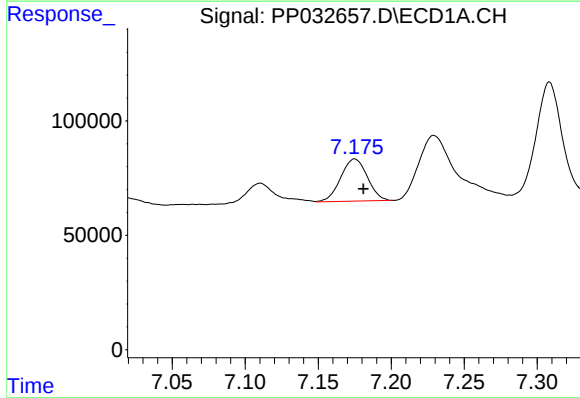


#27 AR-1254-2

R.T.: 7.175 min
Delta R.T.: -0.006 min
Response: 234668
Conc: 77.46 ng/ml

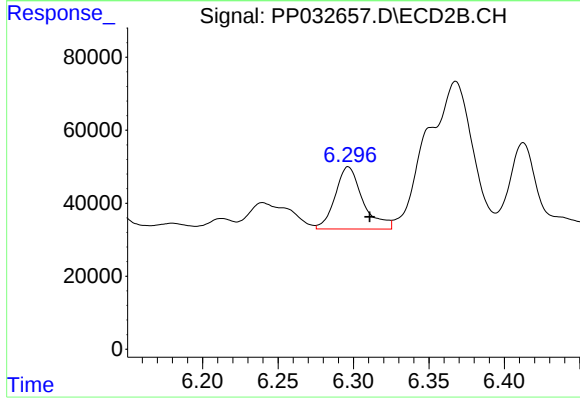

#27 AR-1254-2

R.T.: 6.297 min
Delta R.T.: -0.014 min
Response: 217505
Conc: 101.49 ng/ml

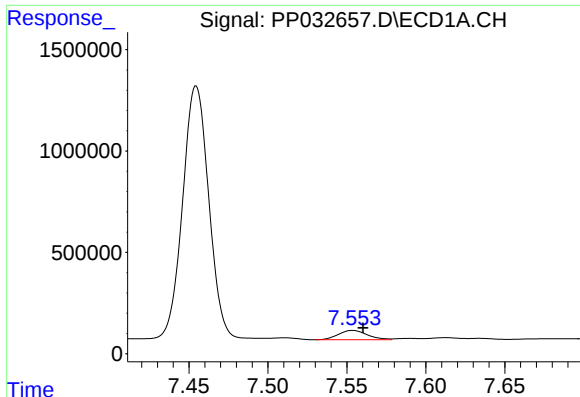


#28 AR-1254-3

R.T.: 7.554 min
Delta R.T.: -0.007 min
Response: 587380
Conc: 180.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-5A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:56 PM

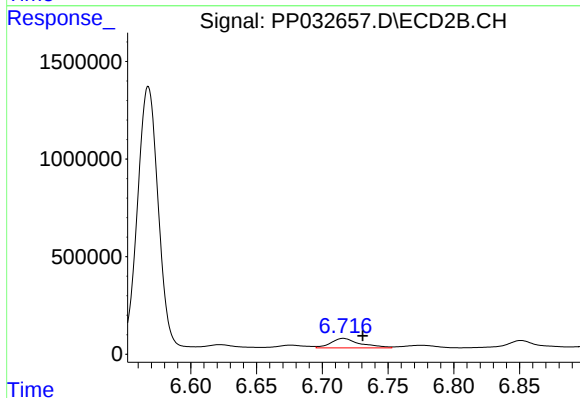


#28 AR-1254-3

R.T.: 6.716 min
Delta R.T.: -0.015 min
Response: 746905
Conc: 208.85 ng/ml

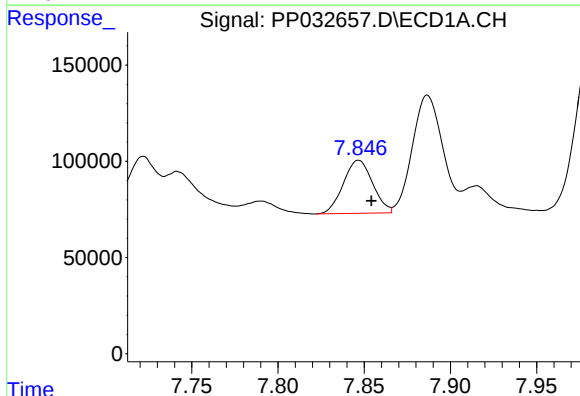


#29 AR-1254-4

R.T.: 7.847 min
Delta R.T.: -0.007 min
Response: 326600
Conc: 141.74 ng/ml

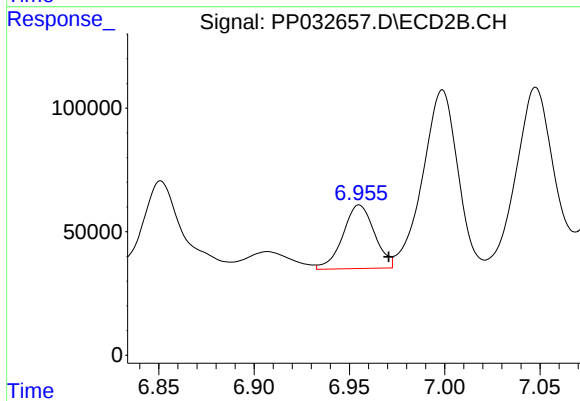

#29 AR-1254-4

R.T.: 6.955 min
Delta R.T.: -0.015 min
Response: 297067
Conc: 144.22 ng/ml

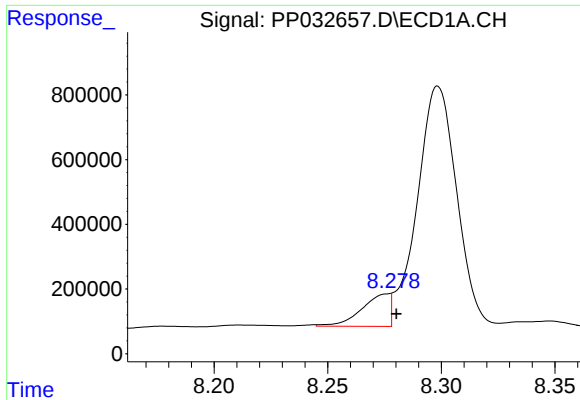


#30 AR-1254-5

R.T.: 8.278 min
Delta R.T.: -0.002 min
Response: 894245
Conc: 364.14 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-5A

Manual Integrations
APPROVED

Ankita
1/13/2021 3:37:56 PM

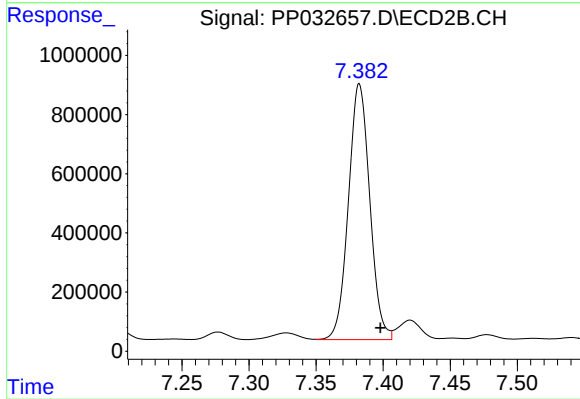

#30 AR-1254-5

R.T.: 7.382 min
Delta R.T.: -0.016 min
Response: 9571024
Conc: 3095.08 ng/ml