

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032661.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 21:42
 Operator : DD\AJ
 Sample : M1093-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-9A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:38:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:29:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.743	4.019f	886620	817995	16.212	16.900
2) SA Decachlor...	10.575	9.298f	443206	429265	9.900	9.668
Target Compounds						
26) L6 AR-1254-1	6.948	6.136f	22396	35818	11.243	14.266m#
27) L6 AR-1254-2	7.176	6.295f	67903	42113	22.414	19.651
28) L6 AR-1254-3	7.553	6.715f	112812	129385	34.626	36.179
29) L6 AR-1254-4	7.847	6.954f	97720	91461	42.410	44.402
30) L6 AR-1254-5	8.279	7.381f	167137	1308821	68.059m	423.246 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032661.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 21:42
Operator : DD\AJ
Sample : M1093-04
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
263K-9A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:29:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

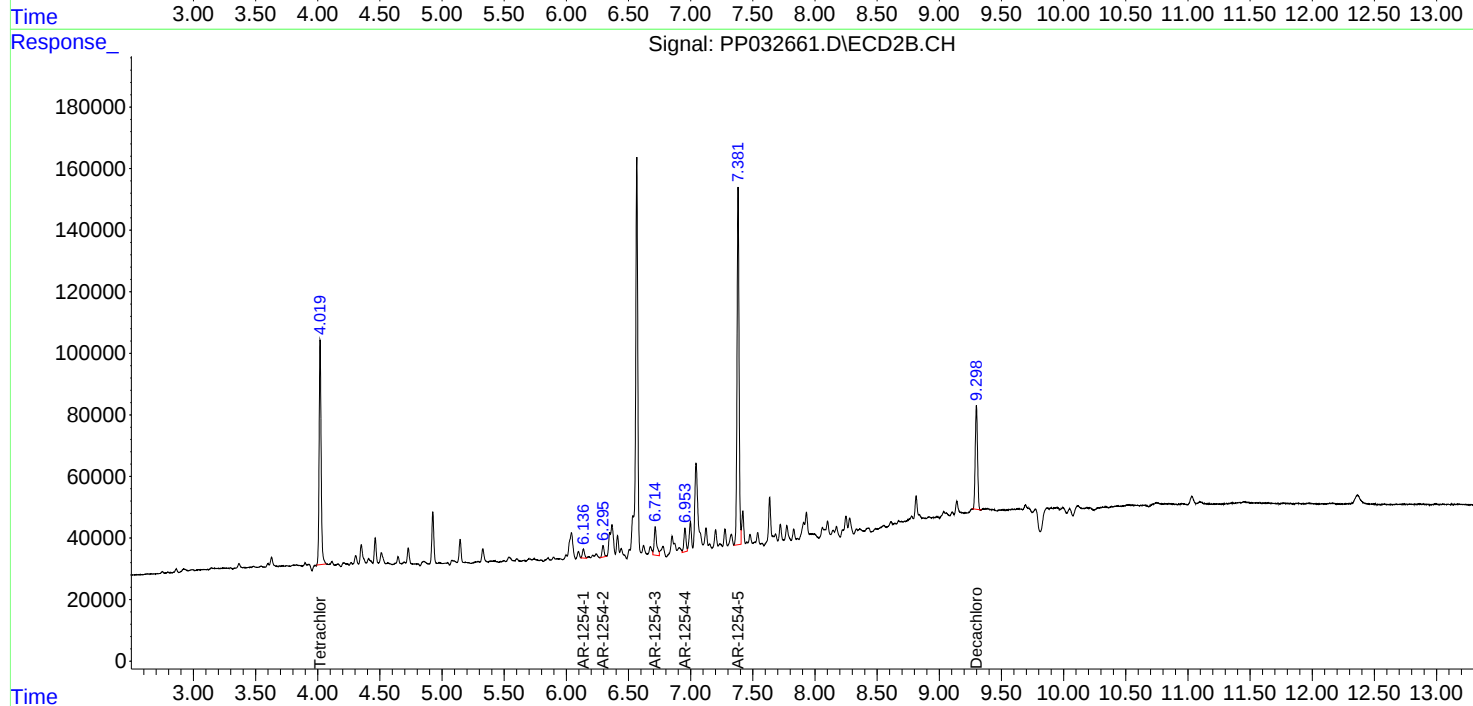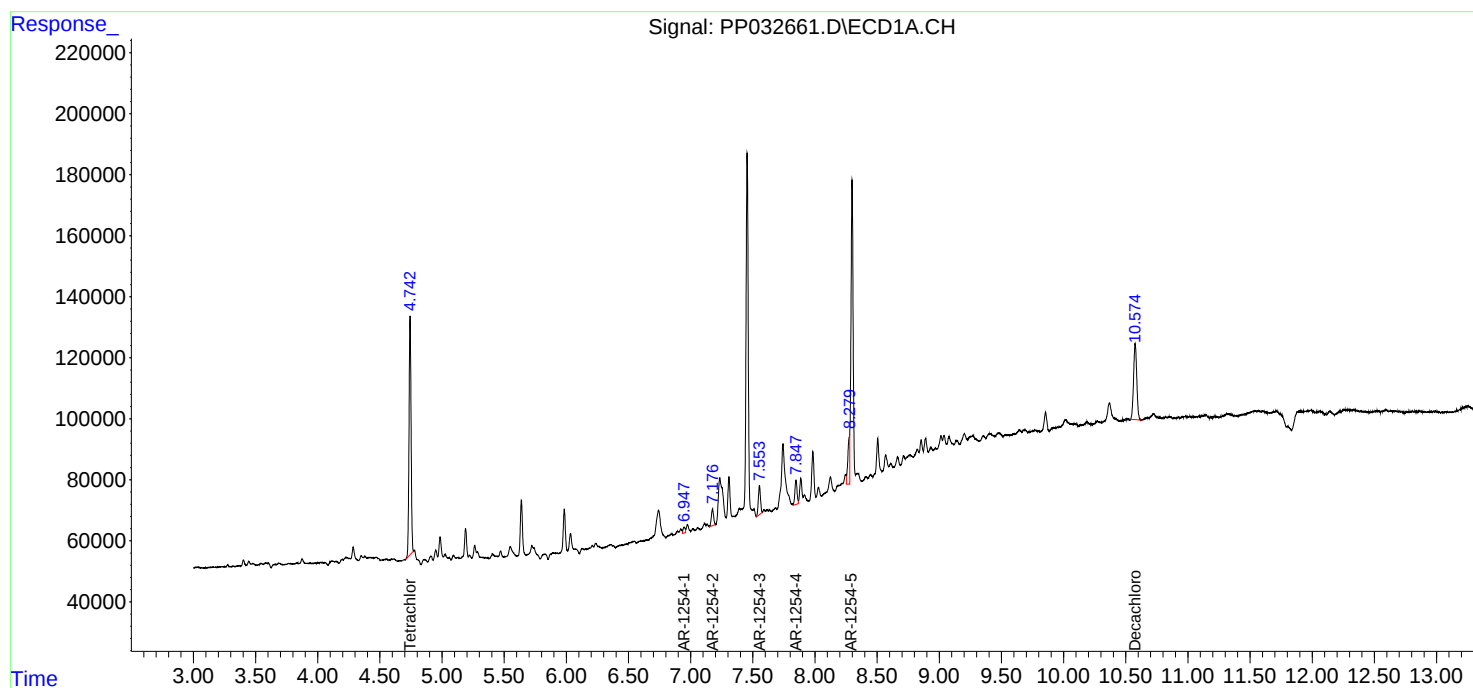

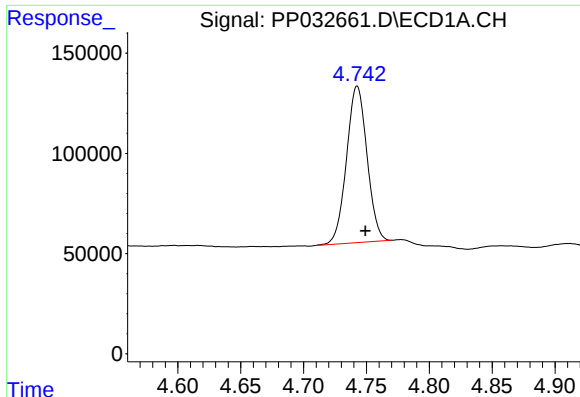


#1 Tetrachloro-m-xylene

R.T.: 4.743 min
Delta R.T.: -0.006 min
Response: 886620
Conc: 16.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-9A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:03 PM

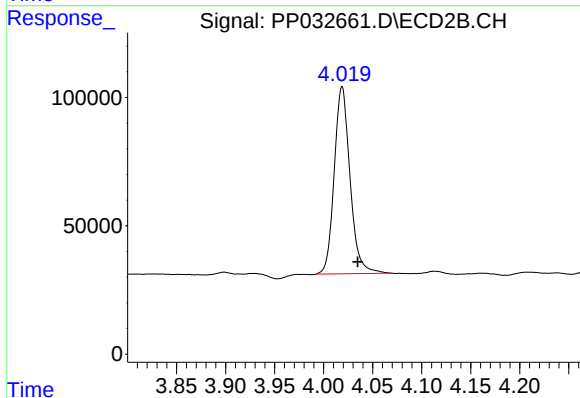


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.016 min
Response: 817995
Conc: 16.90 ng/ml

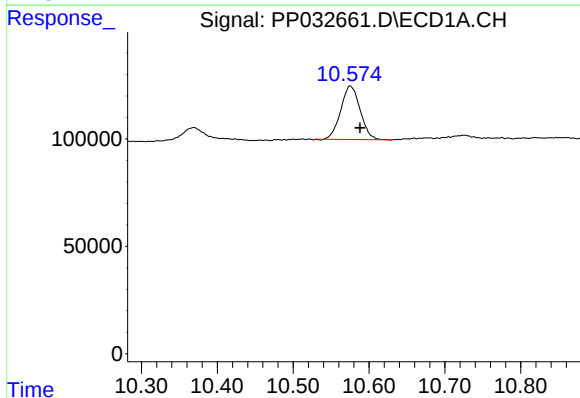


#2 Decachlorobiphenyl

R.T.: 10.575 min
Delta R.T.: -0.013 min
Response: 443206
Conc: 9.90 ng/ml

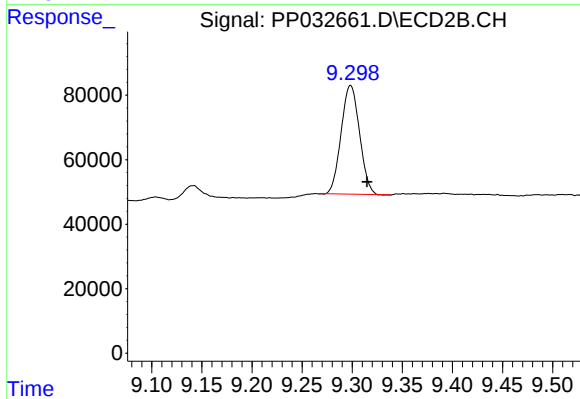

#2 Decachlorobiphenyl

R.T.: 9.298 min
Delta R.T.: -0.017 min
Response: 429265
Conc: 9.67 ng/ml

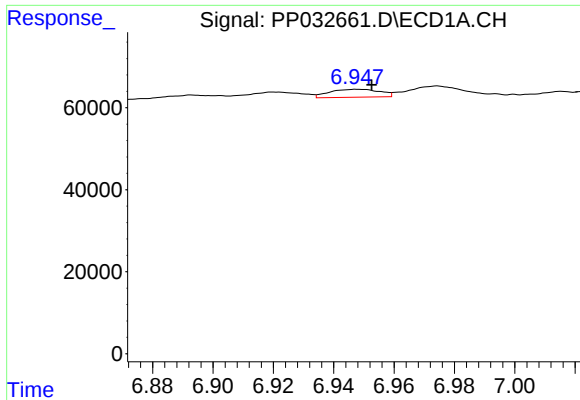


#26 AR-1254-1

R.T.: 6.948 min
Delta R.T.: -0.004 min
Response: 22396
Conc: 11.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-9A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:03 PM

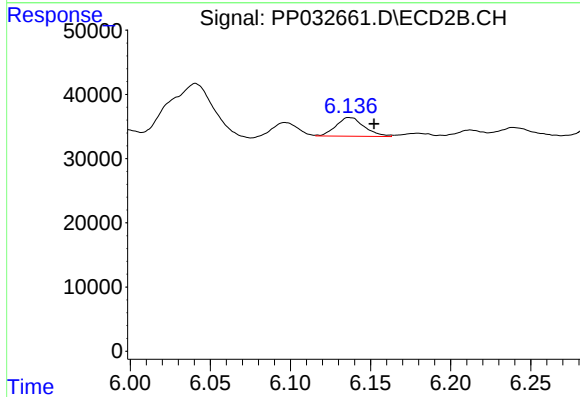


#26 AR-1254-1

R.T.: 6.136 min
Delta R.T.: -0.016 min
Response: 35818
Conc: 14.27 ng/ml m

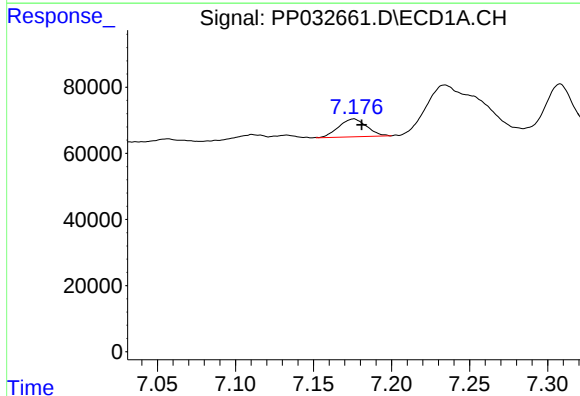


#27 AR-1254-2

R.T.: 7.176 min
Delta R.T.: -0.005 min
Response: 67903
Conc: 22.41 ng/ml

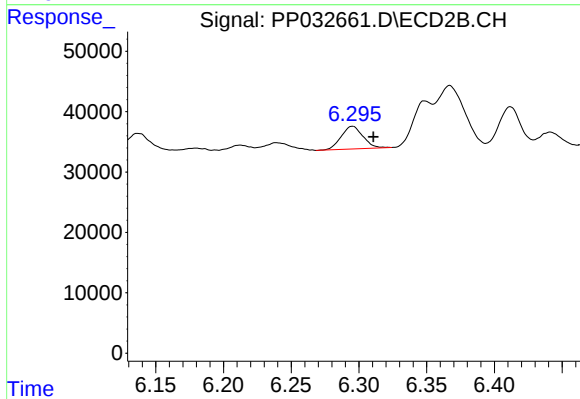

#27 AR-1254-2

R.T.: 6.295 min
Delta R.T.: -0.016 min
Response: 42113
Conc: 19.65 ng/ml

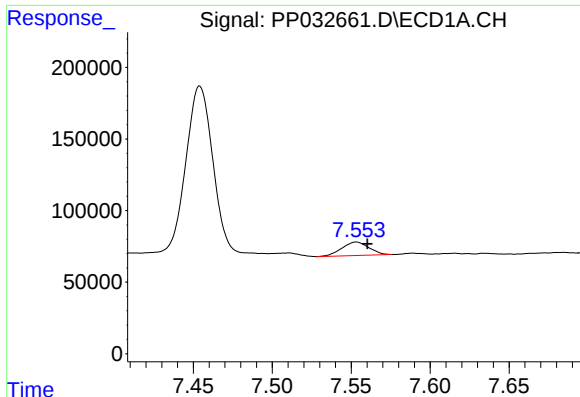


#28 AR-1254-3

R.T.: 7.553 min
Delta R.T.: -0.007 min
Response: 112812
Conc: 34.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-9A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:03 PM

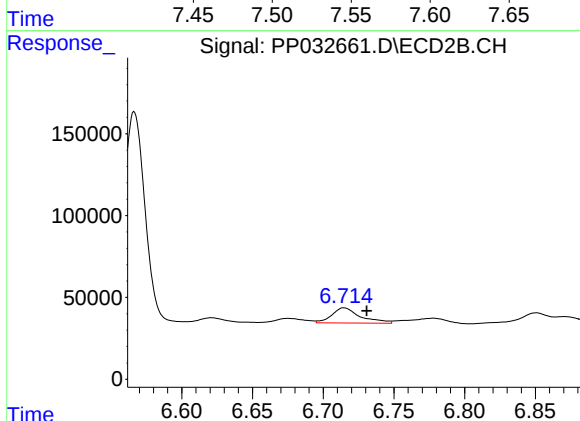


#28 AR-1254-3

R.T.: 6.715 min
Delta R.T.: -0.016 min
Response: 129385
Conc: 36.18 ng/ml

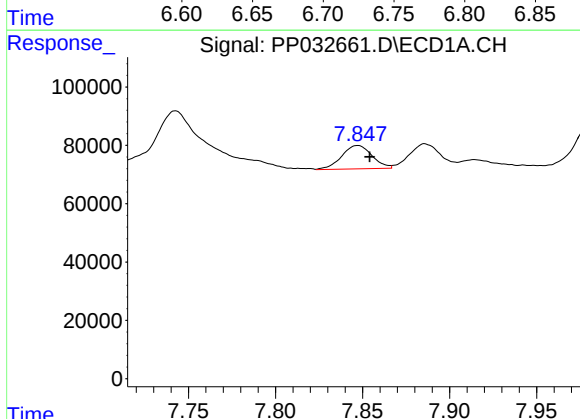


#29 AR-1254-4

R.T.: 7.847 min
Delta R.T.: -0.007 min
Response: 97720
Conc: 42.41 ng/ml

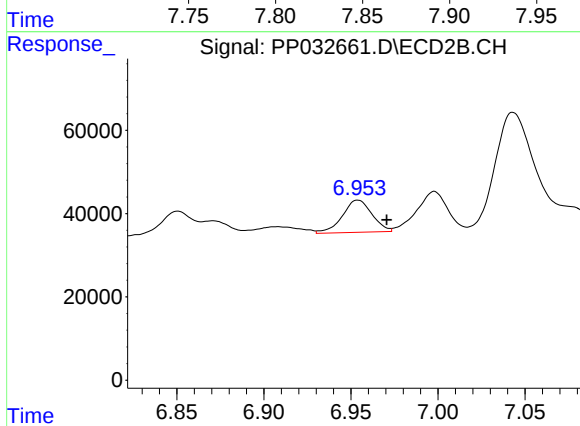

#29 AR-1254-4

R.T.: 6.954 min
Delta R.T.: -0.017 min
Response: 91461
Conc: 44.40 ng/ml

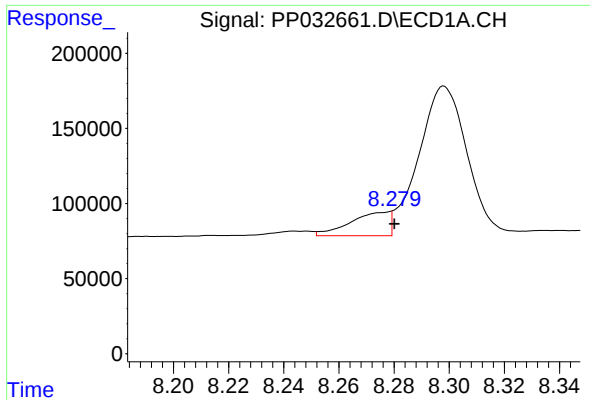


#30 AR-1254-5

R.T.: 8.279 min
Delta R.T.: 0.000 min
Response: 167137
Conc: 68.06 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-9A

Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:03 PM

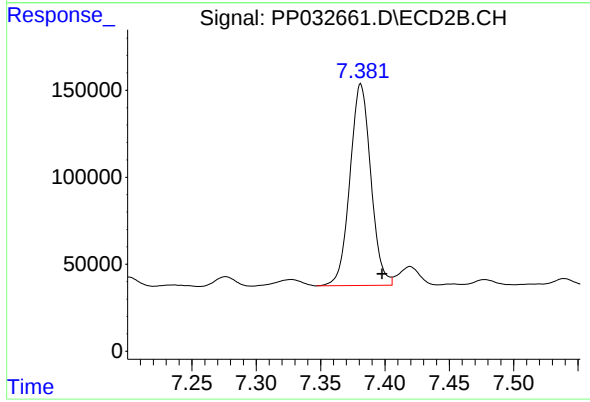

#30 AR-1254-5

R.T.: 7.381 min
Delta R.T.: -0.017 min
Response: 1308821
Conc: 423.25 ng/ml