

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032664.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 22:32
 Operator : DD\AJ
 Sample : M1093-13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-13A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:38:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:31:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.744	4.019f	1504484	1205309	27.510	24.902
2) SA Decachlor...	10.575	9.299f	696849	669437	15.566	15.077
Target Compounds						
26) L6 AR-1254-1	6.946	6.136f	141166	134847	70.865m	53.708
27) L6 AR-1254-2	7.174	6.295f	263888	195344	87.105	91.154
28) L6 AR-1254-3	7.553	6.715f	835054	972135	256.310	271.828
29) L6 AR-1254-4	7.847	6.955f	411799	344620	178.719	167.303
30) L6 AR-1254-5	8.275	7.382f	1307051	7661962	532.237	2477.724 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032664.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 22:32
Operator : DD\AJ
Sample : M1093-13
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
263K-13A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:31:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

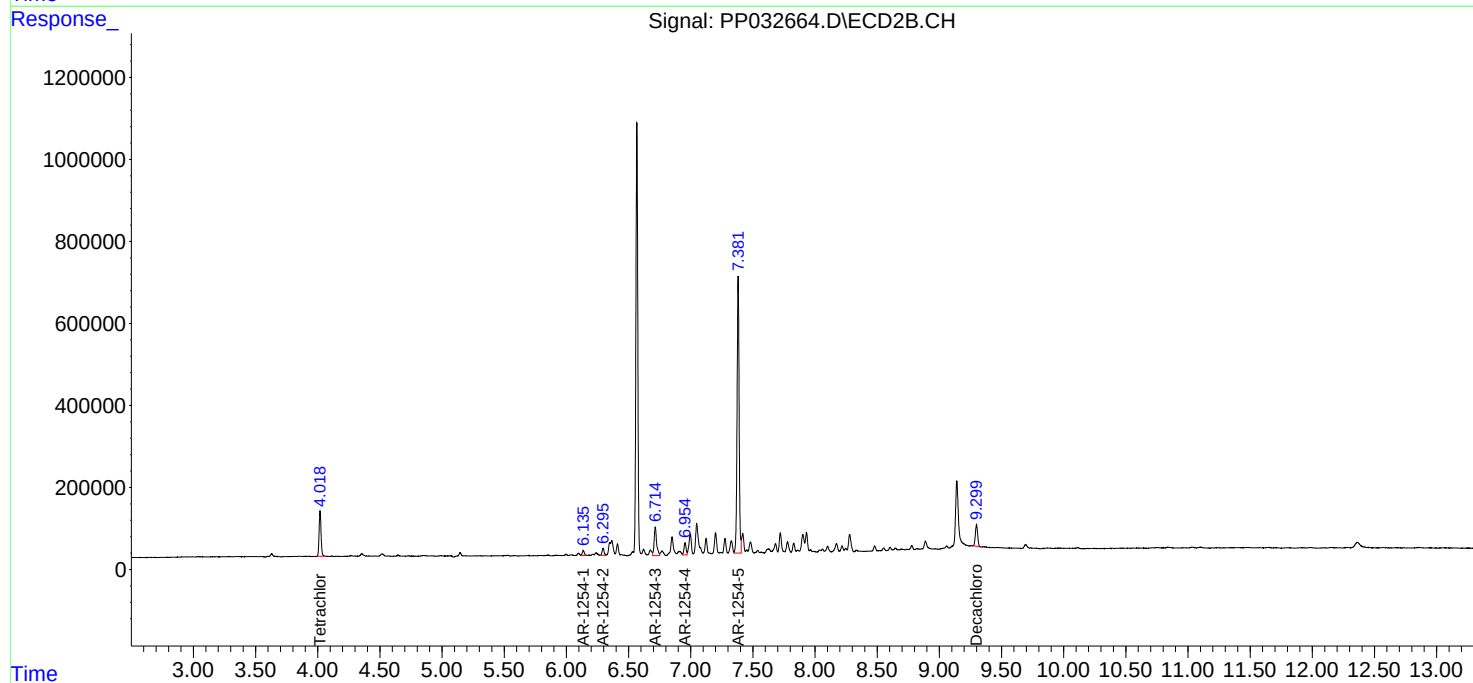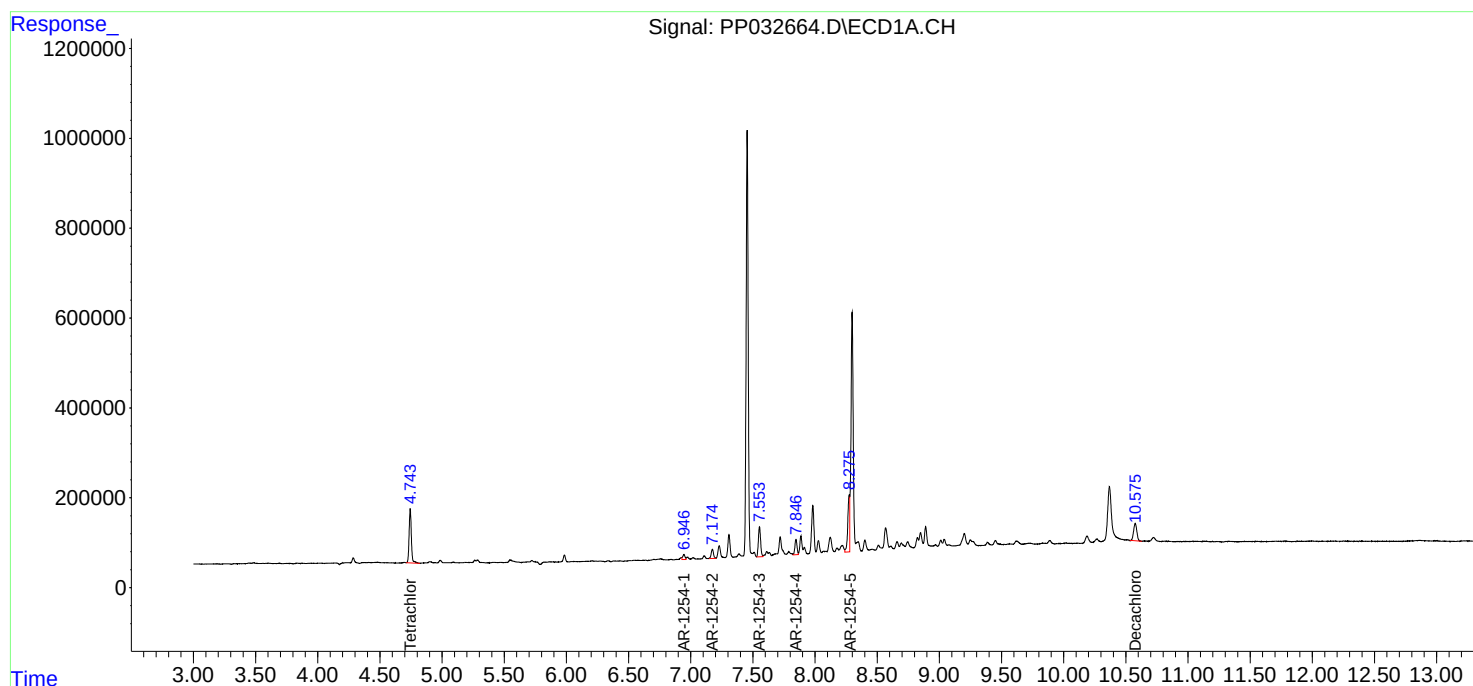

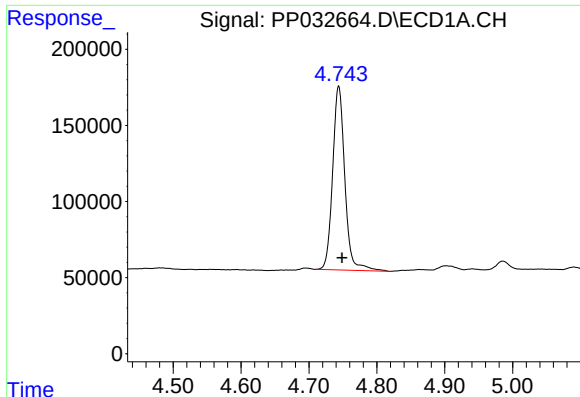


#1 Tetrachloro-m-xylene

R.T.: 4.744 min
Delta R.T.: -0.005 min
Response: 1504484
Conc: 27.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-13A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:09 PM

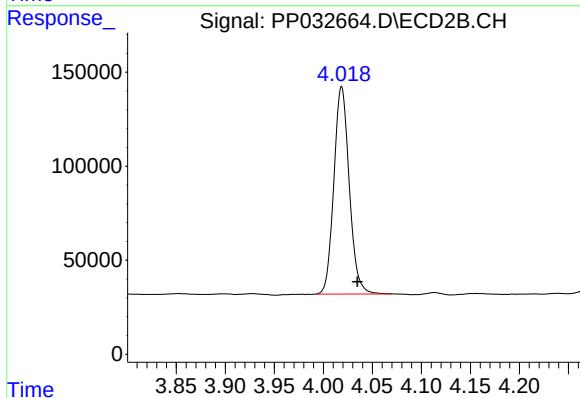


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.016 min
Response: 1205309
Conc: 24.90 ng/ml

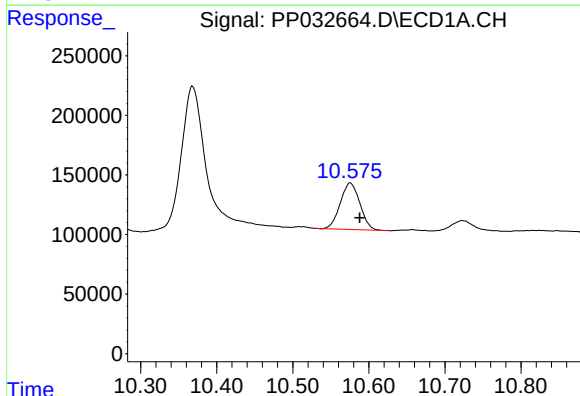


#2 Decachlorobiphenyl

R.T.: 10.575 min
Delta R.T.: -0.013 min
Response: 696849
Conc: 15.57 ng/ml

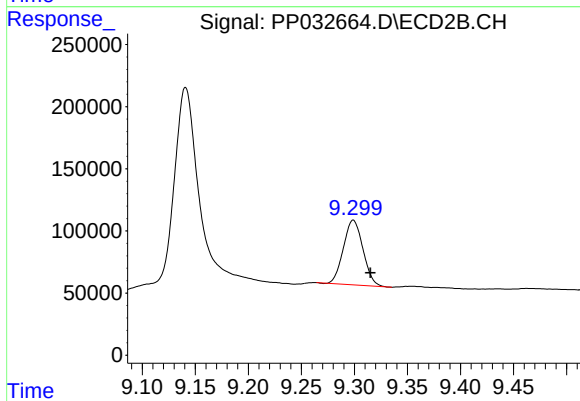

#2 Decachlorobiphenyl

R.T.: 9.299 min
Delta R.T.: -0.016 min
Response: 669437
Conc: 15.08 ng/ml

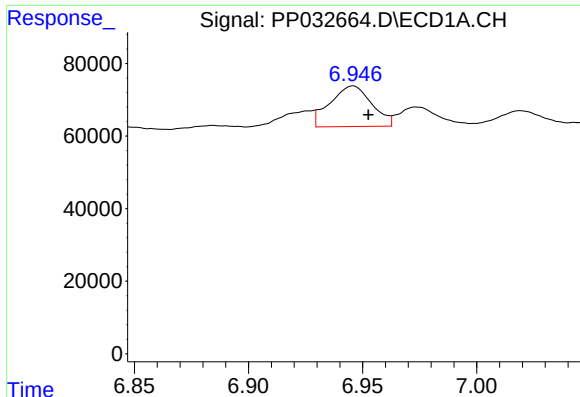


#26 AR-1254-1

R.T.: 6.946 min
Delta R.T.: -0.007 min
Response: 141166
Conc: 70.87 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-13A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:09 PM

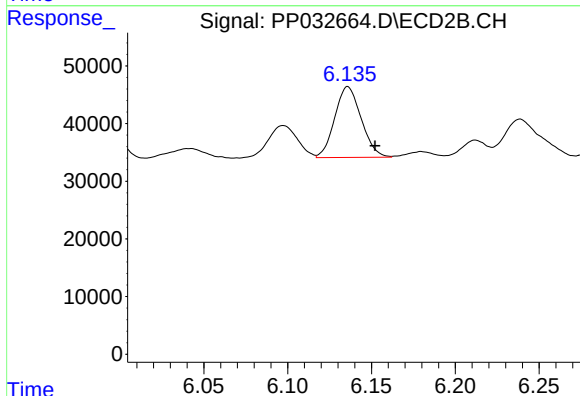


#26 AR-1254-1

R.T.: 6.136 min
Delta R.T.: -0.016 min
Response: 134847
Conc: 53.71 ng/ml

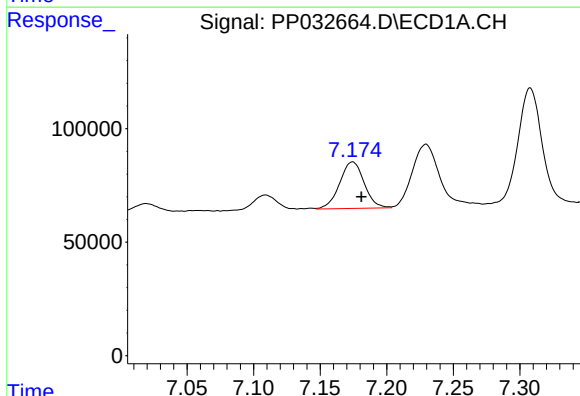


#27 AR-1254-2

R.T.: 7.174 min
Delta R.T.: -0.007 min
Response: 263888
Conc: 87.11 ng/ml

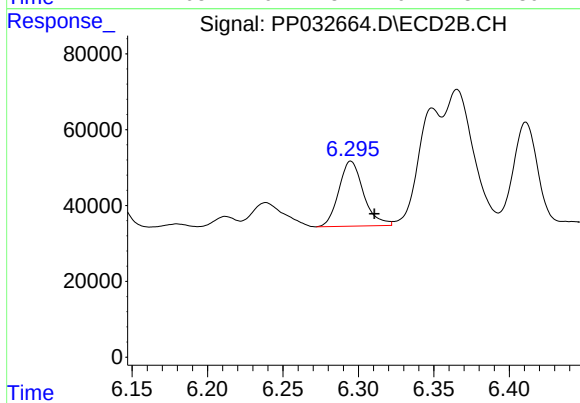

#27 AR-1254-2

R.T.: 6.295 min
Delta R.T.: -0.016 min
Response: 195344
Conc: 91.15 ng/ml

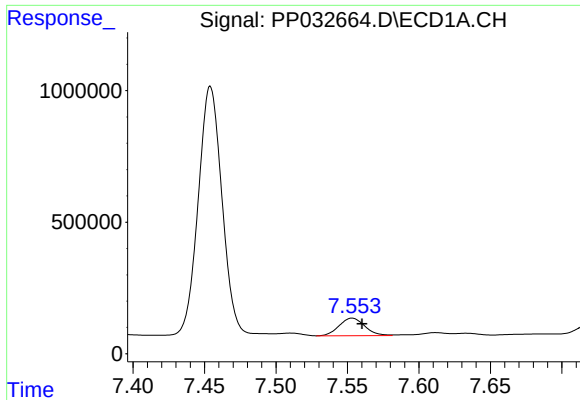


#28 AR-1254-3

R.T.: 7.553 min
Delta R.T.: -0.007 min
Response: 835054
Conc: 256.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-13A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:09 PM

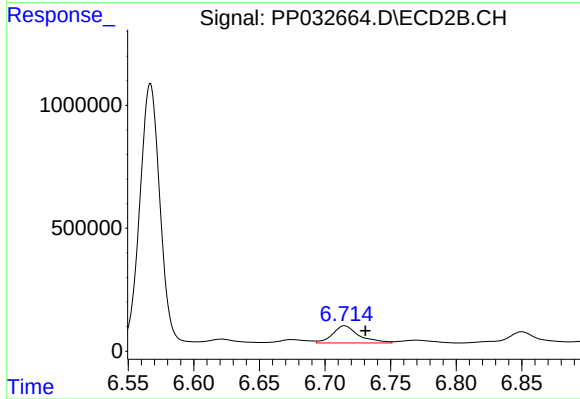


#28 AR-1254-3

R.T.: 6.715 min
Delta R.T.: -0.016 min
Response: 972135
Conc: 271.83 ng/ml

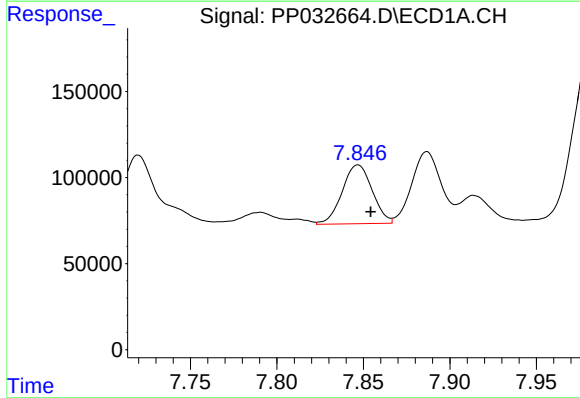


#29 AR-1254-4

R.T.: 7.847 min
Delta R.T.: -0.007 min
Response: 411799
Conc: 178.72 ng/ml

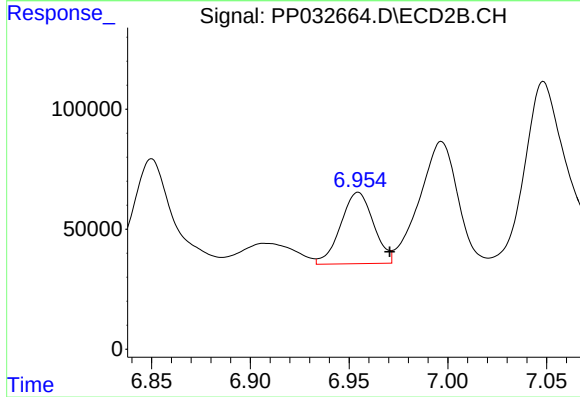

#29 AR-1254-4

R.T.: 6.955 min
Delta R.T.: -0.016 min
Response: 344620
Conc: 167.30 ng/ml

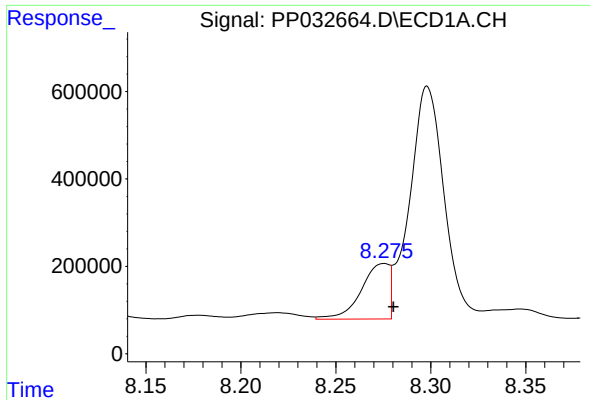


#30 AR-1254-5

R.T.: 8.275 min
Delta R.T.: -0.005 min
Response: 1307051
Conc: 532.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-13A

Manual Integrations
APPROVED

Ankita
1/13/2021 3:38:09 PM

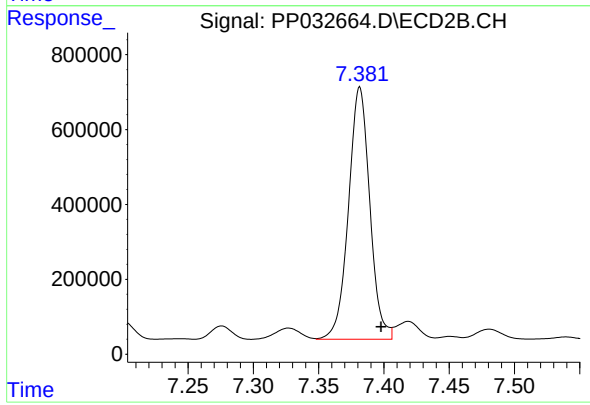

#30 AR-1254-5

R.T.: 7.382 min
Delta R.T.: -0.016 min
Response: 7661962
Conc: 2477.72 ng/ml