

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032680.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 3:16
 Operator : DD\AJ
 Sample : M1094-17
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-21A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:39:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 05:53:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.743	4.019f	1454912	1246304	26.604	25.749
2)	SA Decachlor...	10.575	9.298f	718936	659748	16.059	14.859
Target Compounds							
26)	L6 AR-1254-1	6.947	6.137f	59820	93979	30.029	37.431
27)	L6 AR-1254-2	7.176	6.295f	171676	103429	56.667	48.263
28)	L6 AR-1254-3	7.553	6.715f	419493	440676	128.758	123.222
29)	L6 AR-1254-4	7.847	6.955f	214215	151491	92.969	73.544
30)	L6 AR-1254-5	8.274	7.381f	645218	3838649	262.736m	1241.342 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032680.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 3:16
Operator : DD\AJ
Sample : M1094-17
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
263K-21A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 05:53:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

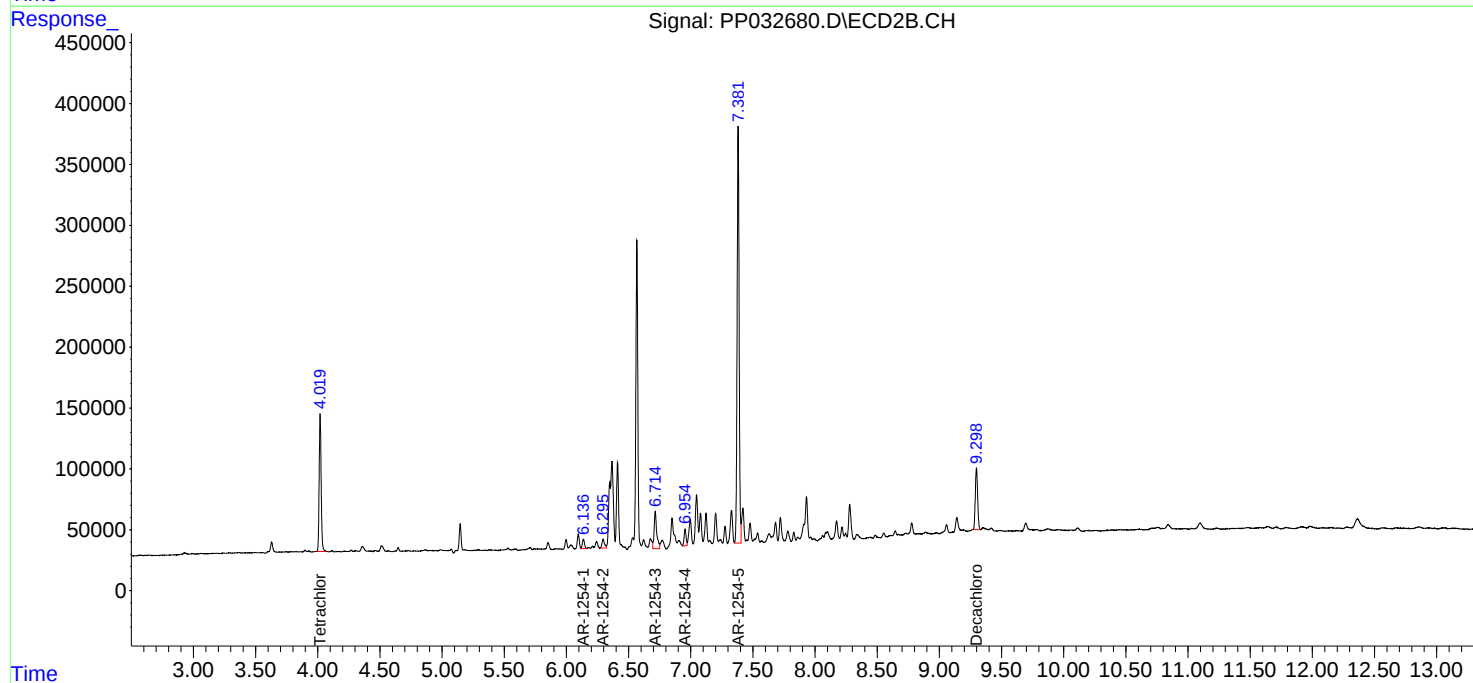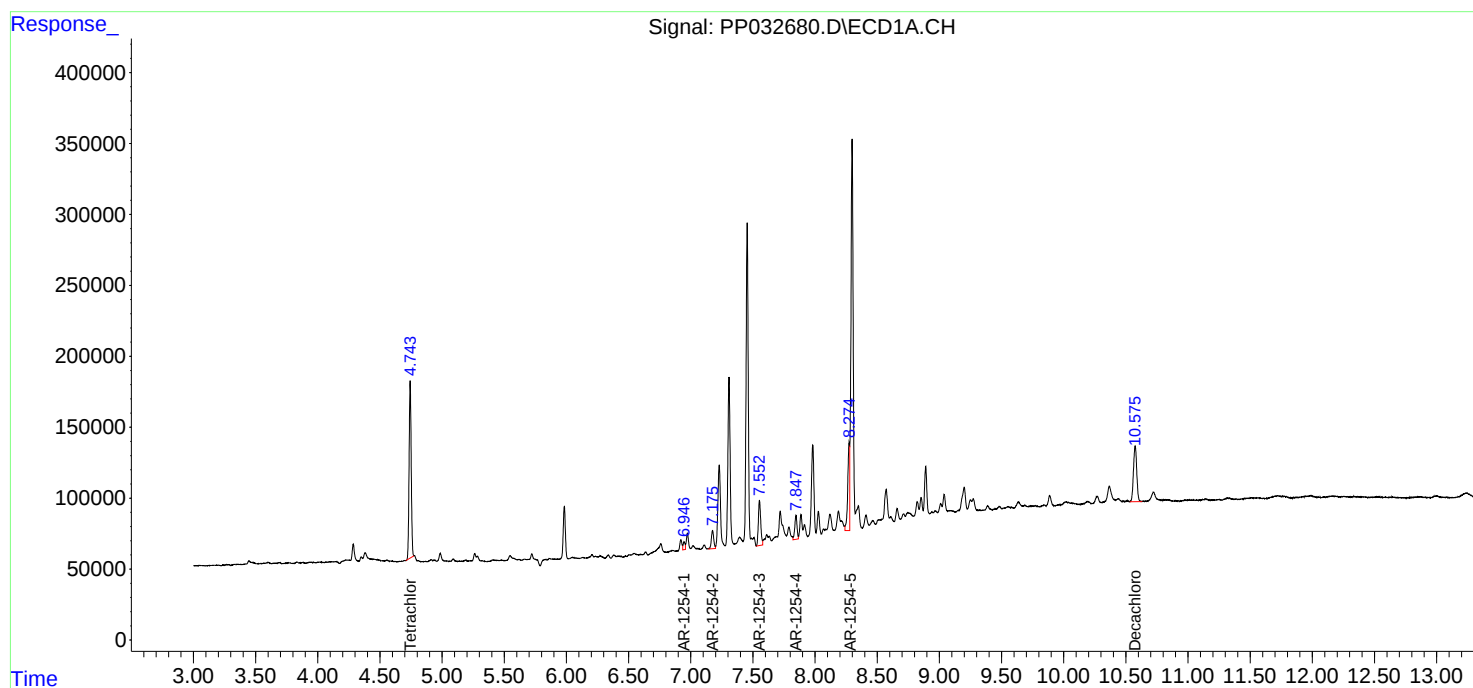

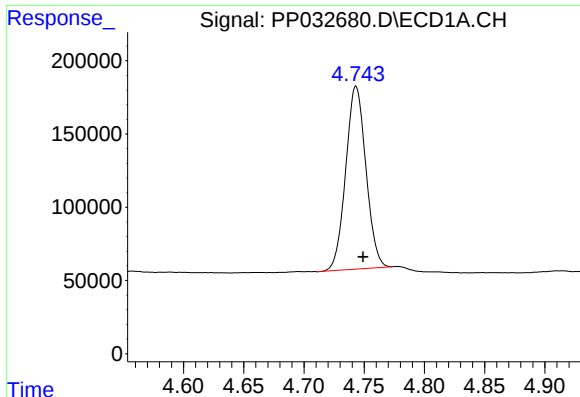


#1 Tetrachloro-m-xylene

R.T.: 4.743 min
Delta R.T.: -0.006 min
Response: 1454912
Conc: 26.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-21A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:27 PM

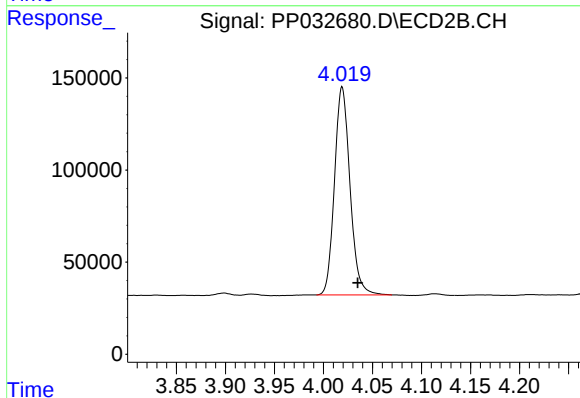


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.016 min
Response: 1246304
Conc: 25.75 ng/ml

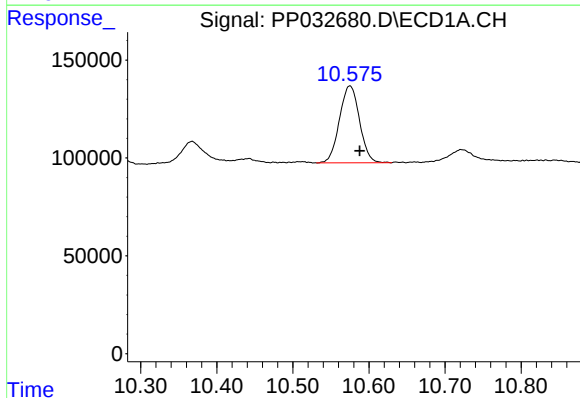


#2 Decachlorobiphenyl

R.T.: 10.575 min
Delta R.T.: -0.013 min
Response: 718936
Conc: 16.06 ng/ml

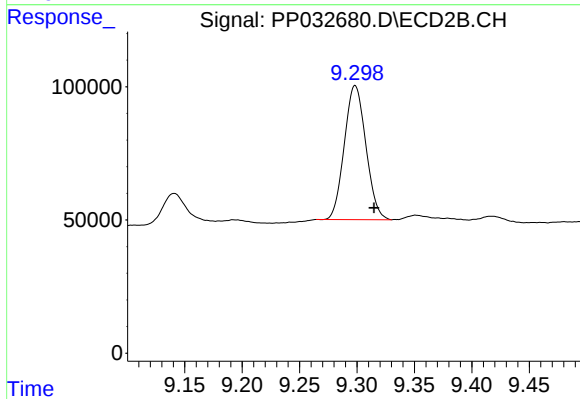

#2 Decachlorobiphenyl

R.T.: 9.298 min
Delta R.T.: -0.017 min
Response: 659748
Conc: 14.86 ng/ml

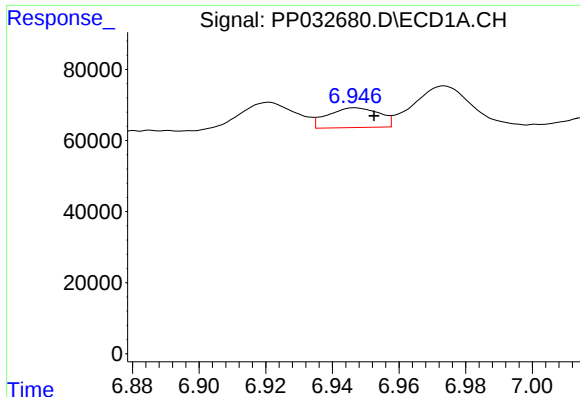


#26 AR-1254-1

R.T.: 6.947 min
Delta R.T.: -0.006 min
Response: 59820
Conc: 30.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-21A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:27 PM

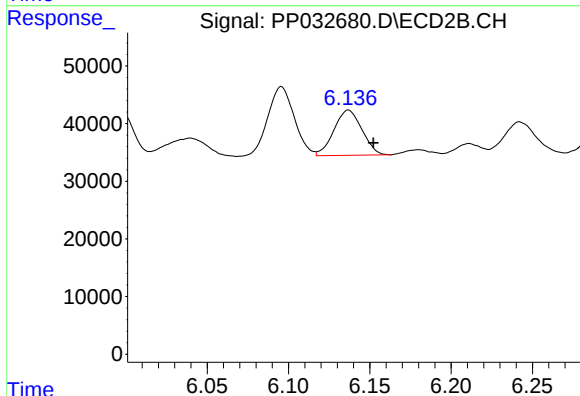


#26 AR-1254-1

R.T.: 6.137 min
Delta R.T.: -0.015 min
Response: 93979
Conc: 37.43 ng/ml

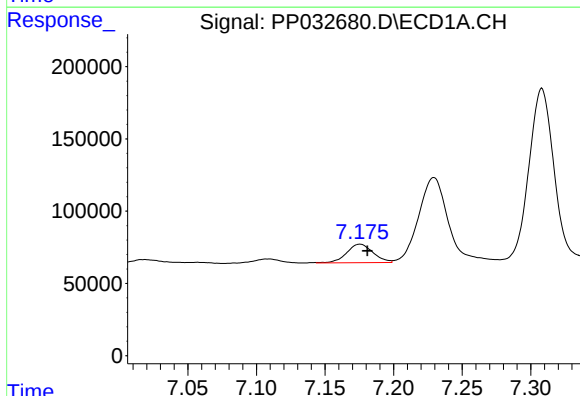


#27 AR-1254-2

R.T.: 7.176 min
Delta R.T.: -0.005 min
Response: 171676
Conc: 56.67 ng/ml

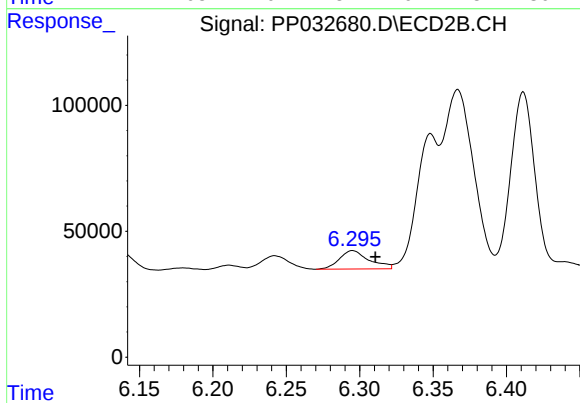

#27 AR-1254-2

R.T.: 6.295 min
Delta R.T.: -0.016 min
Response: 103429
Conc: 48.26 ng/ml

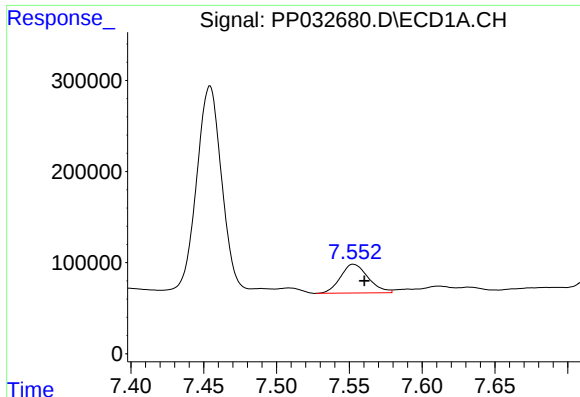


#28 AR-1254-3

R.T.: 7.553 min
Delta R.T.: -0.007 min
Response: 419493
Conc: 128.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-21A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:27 PM

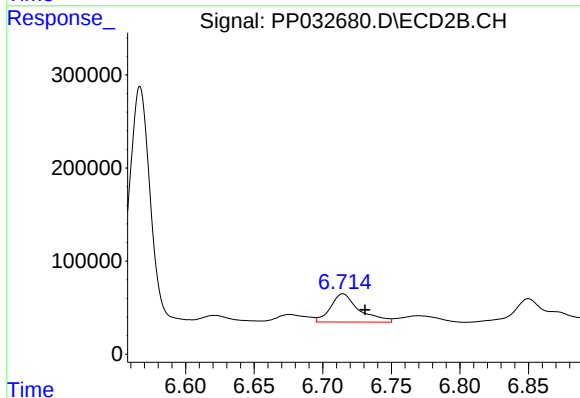


#28 AR-1254-3

R.T.: 6.715 min
Delta R.T.: -0.016 min
Response: 440676
Conc: 123.22 ng/ml

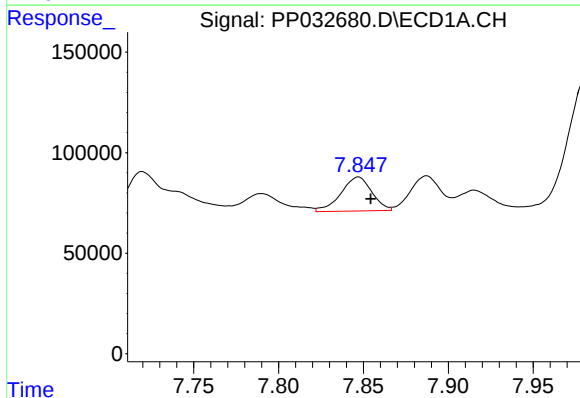


#29 AR-1254-4

R.T.: 7.847 min
Delta R.T.: -0.007 min
Response: 214215
Conc: 92.97 ng/ml

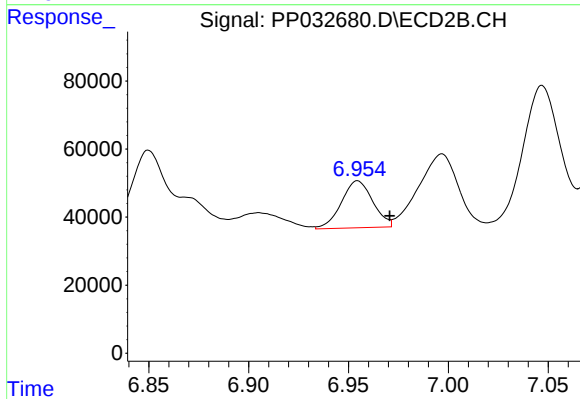

#29 AR-1254-4

R.T.: 6.955 min
Delta R.T.: -0.016 min
Response: 151491
Conc: 73.54 ng/ml

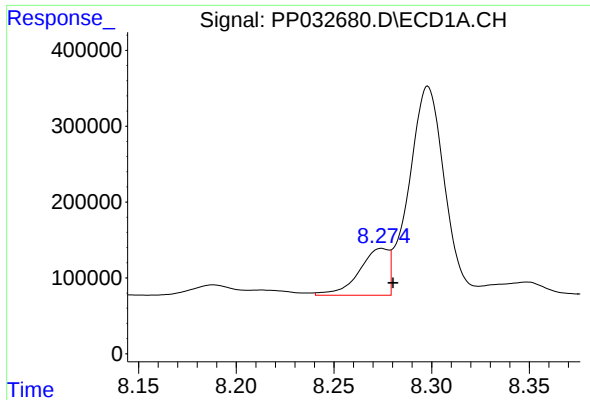


#30 AR-1254-5

R.T.: 8.274 min
Delta R.T.: -0.006 min
Response: 645218
Conc: 262.74 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-21A

Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:27 PM

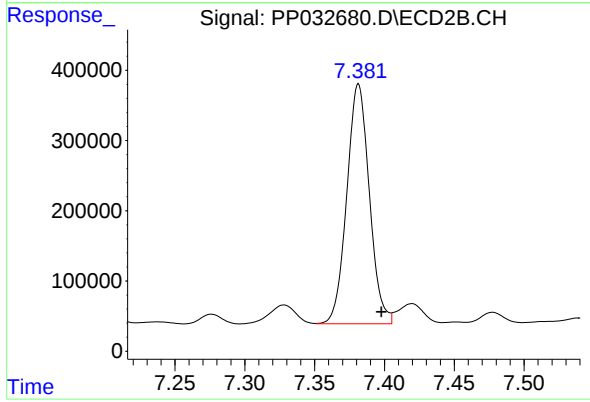

#30 AR-1254-5

R.T.: 7.381 min
Delta R.T.: -0.016 min
Response: 3838649
Conc: 1241.34 ng/ml