

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032683.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 4:06
 Operator : DD\AJ
 Sample : M1095-06
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-24A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 05:54:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.744	4.019f	1378344	1184701	25.204	24.476
2) SA Decachlor...	10.576	9.299f	860586	786341	19.223	17.710

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032683.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 4:06
Operator : DD\AJ
Sample : M1095-06
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
263K-24A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 05:54:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

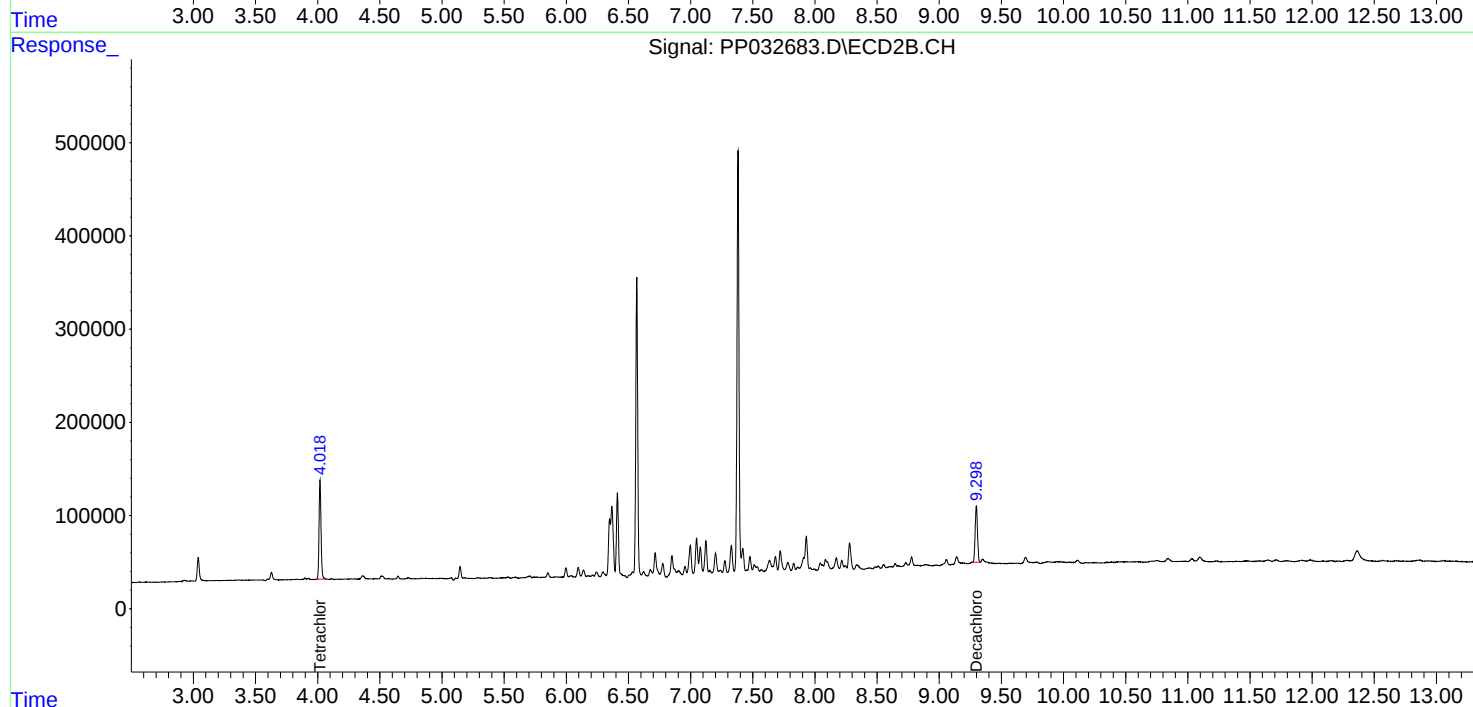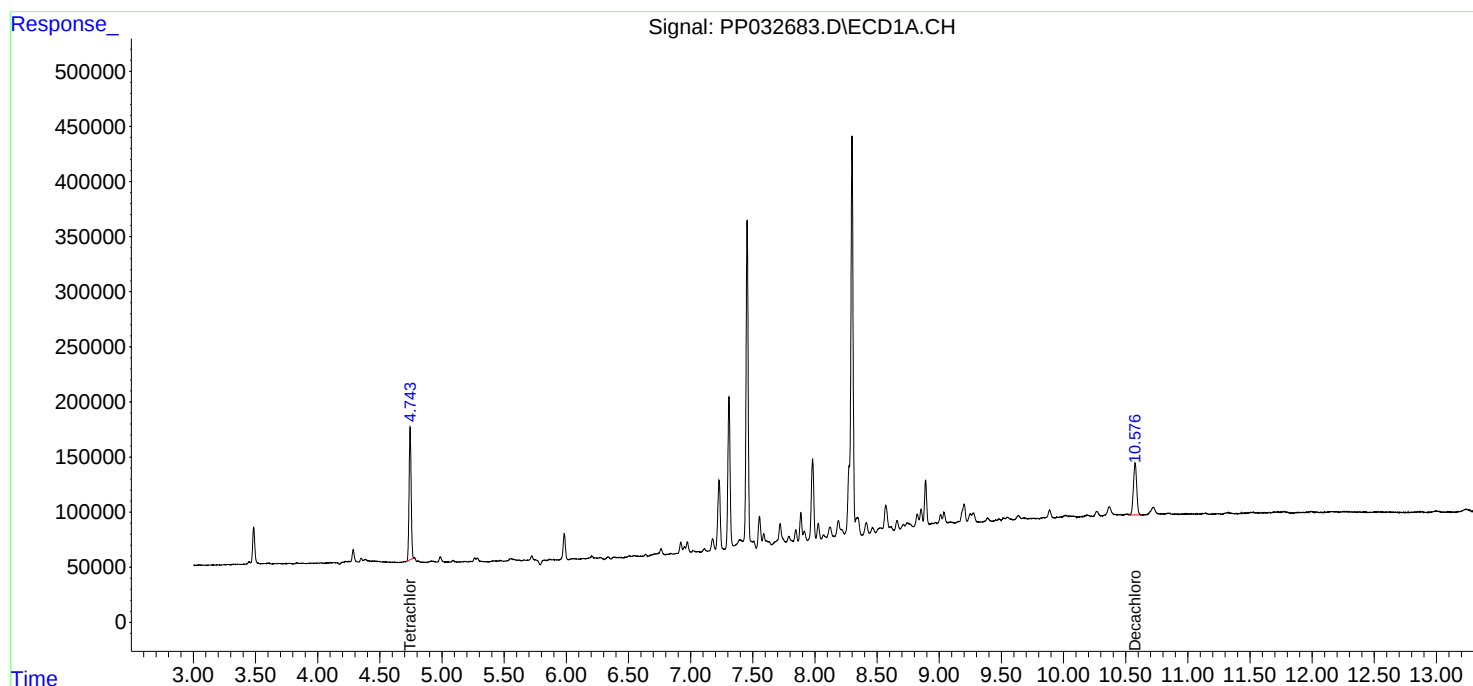


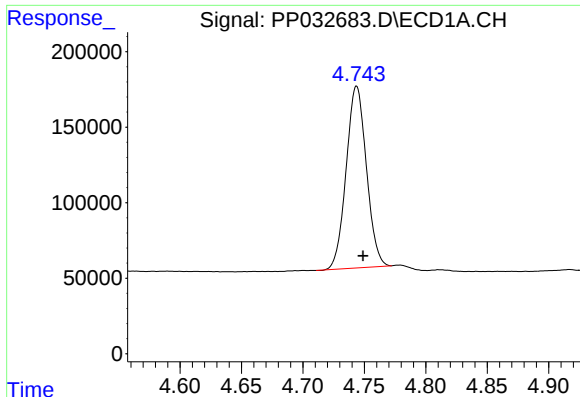

#1 Tetrachloro-m-xylene


R.T.: 4.744 min
Delta R.T.: -0.005 min
Response: 1378344
Conc: 25.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-24A

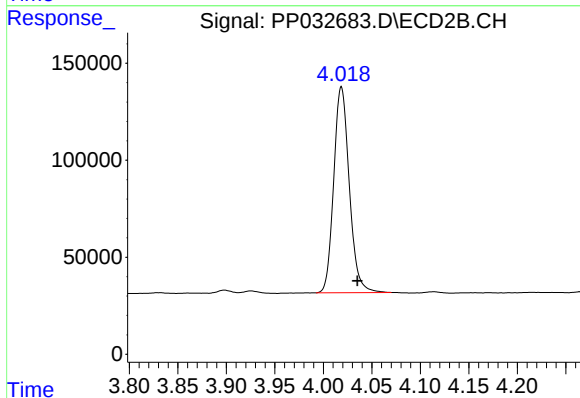


#1 Tetrachloro-m-xylene

R.T.: 4.019 min
Delta R.T.: -0.016 min
Response: 1184701
Conc: 24.48 ng/ml

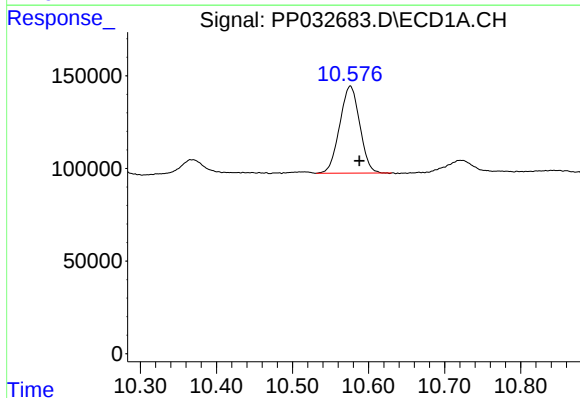

#2 Decachlorobiphenyl

R.T.: 10.576 min
Delta R.T.: -0.012 min
Response: 860586
Conc: 19.22 ng/ml

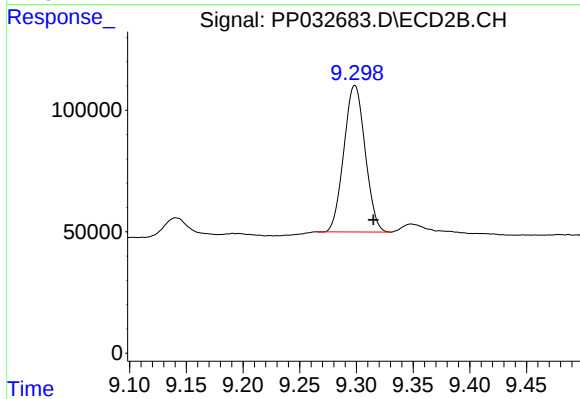

#2 Decachlorobiphenyl

R.T.: 9.299 min
Delta R.T.: -0.016 min
Response: 786341
Conc: 17.71 ng/ml