

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
 Data File : PP032684.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 4:23
 Operator : DD\AJ
 Sample : M1095-09
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-25A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 3:39:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 05:55:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 07:49:02 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.744	4.018f	1692913	1376906	30.956	28.447
2) SA Decachlor...	10.575	9.298f	1091014	1039749	24.370	23.417
Target Compounds						
26) L6 AR-1254-1	6.947	6.136f	73743	98293	37.019	39.149
27) L6 AR-1254-2	7.176	6.294f	193844	95522	63.985	44.574 #
28) L6 AR-1254-3	7.553	6.715f	361232	424693	110.876	118.752
29) L6 AR-1254-4	7.847	6.954f	197521	151069	85.724	73.340
30) L6 AR-1254-5	8.277	7.381f	568020	5287792	231.301m	1709.965 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011321\
Data File : PP032684.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 4:23
Operator : DD\AJ
Sample : M1095-09
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
263K-25A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 05:55:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 07:49:02 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

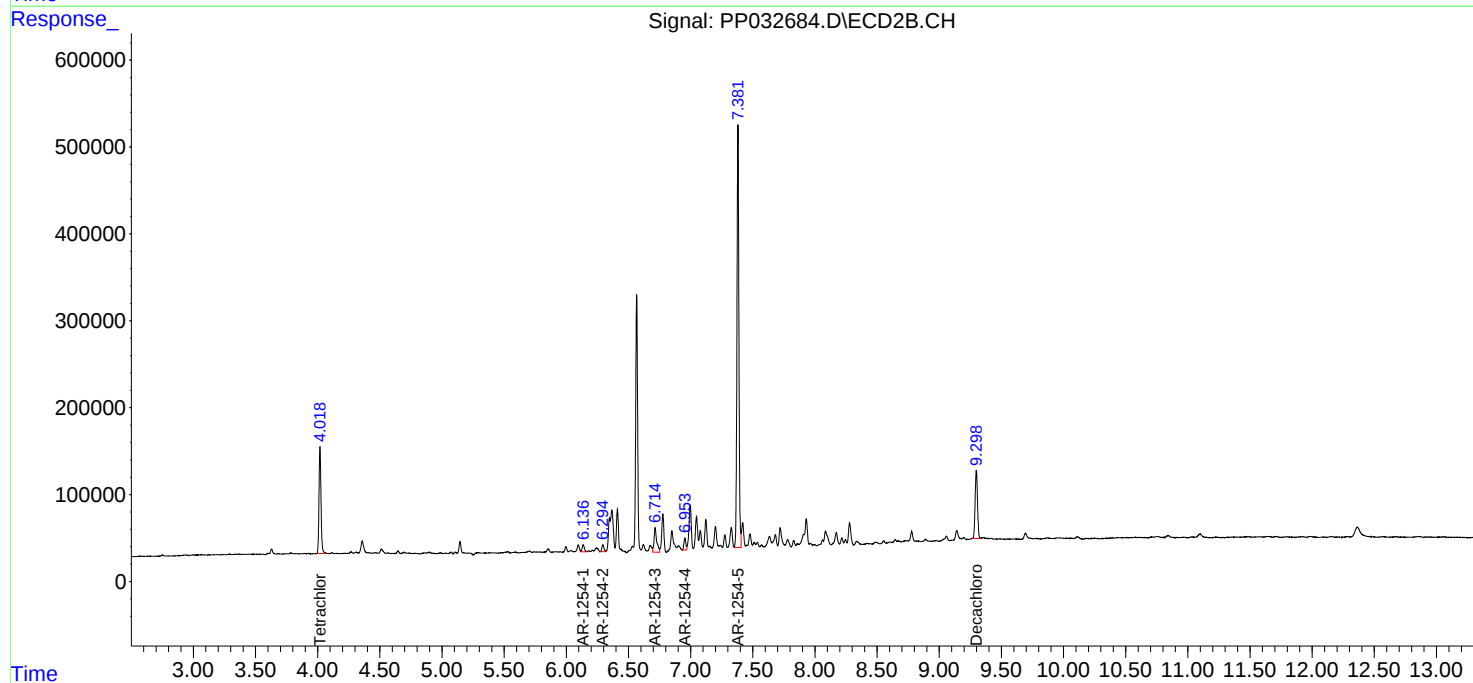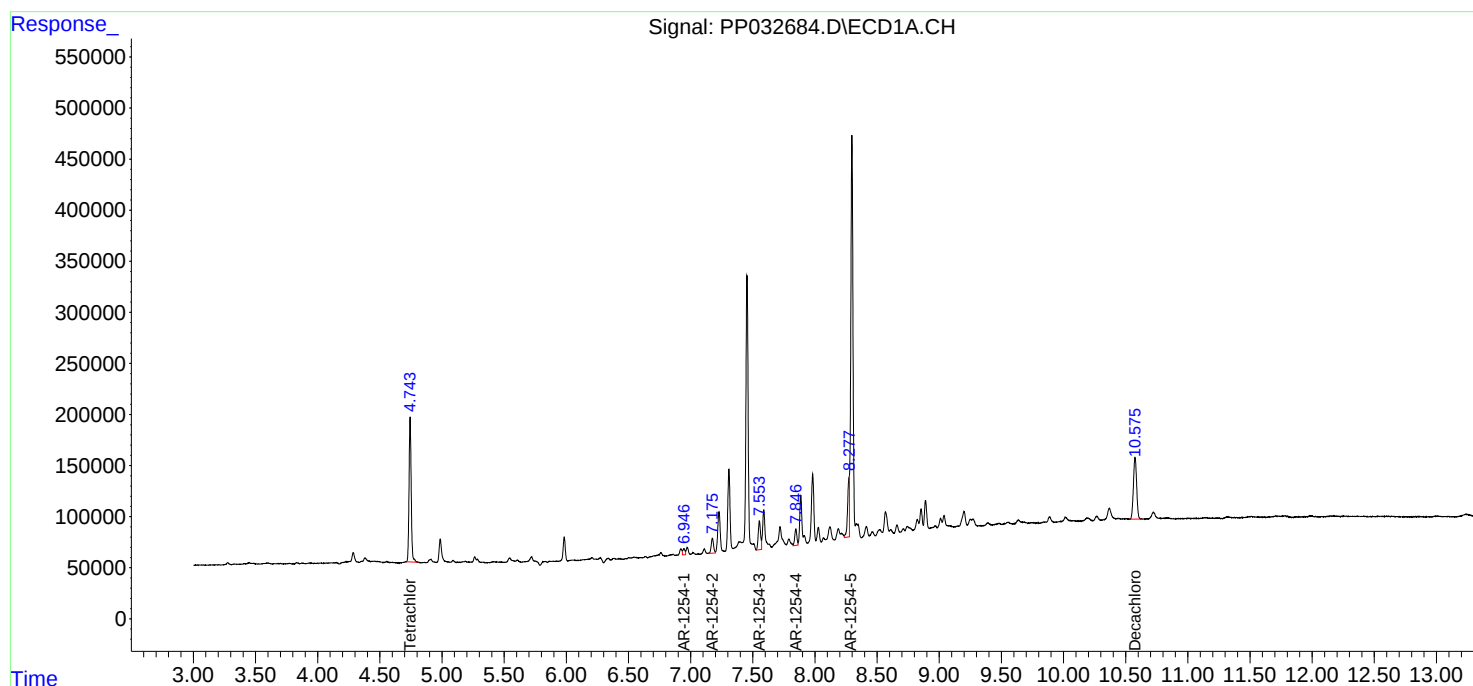

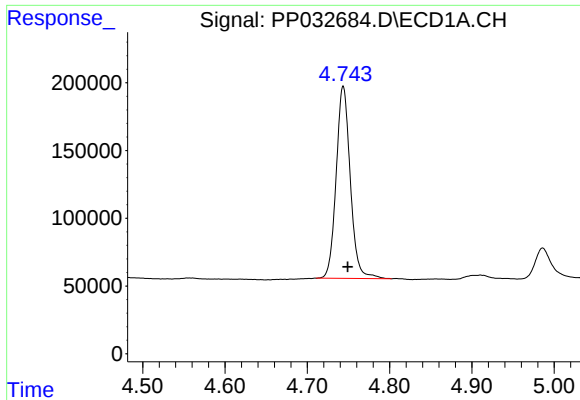


#1 Tetrachloro-m-xylene

R.T.: 4.744 min
Delta R.T.: -0.005 min
Response: 1692913
Conc: 30.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-25A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:30 PM

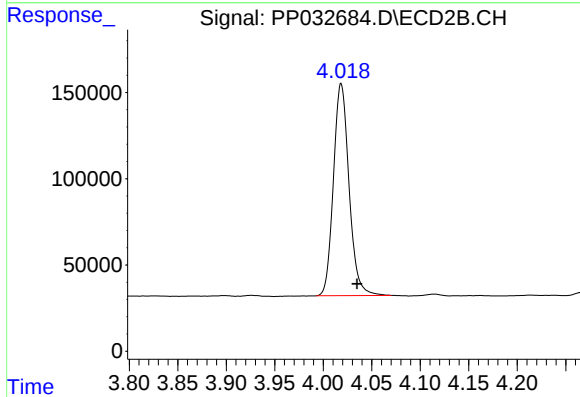


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: -0.016 min
Response: 1376906
Conc: 28.45 ng/ml

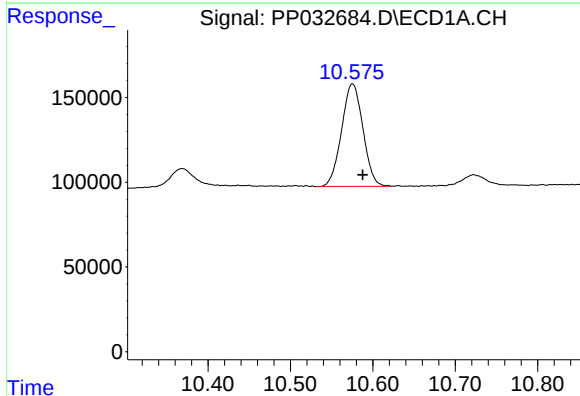


#2 Decachlorobiphenyl

R.T.: 10.575 min
Delta R.T.: -0.013 min
Response: 1091014
Conc: 24.37 ng/ml

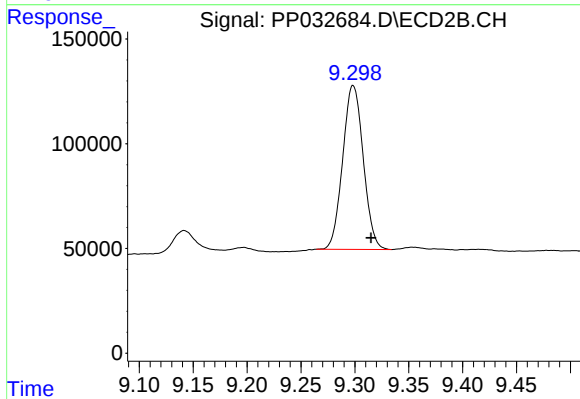

#2 Decachlorobiphenyl

R.T.: 9.298 min
Delta R.T.: -0.017 min
Response: 1039749
Conc: 23.42 ng/ml

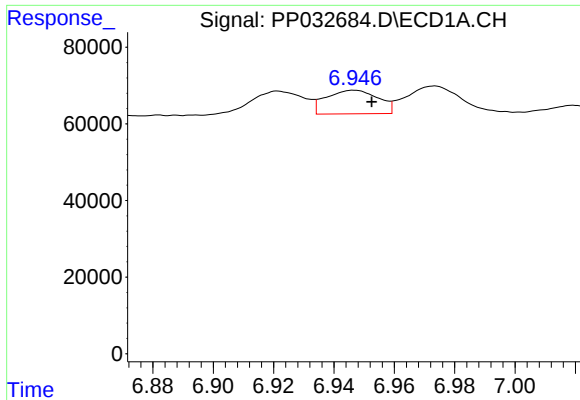


#26 AR-1254-1

R.T.: 6.947 min
Delta R.T.: -0.006 min
Response: 73743
Conc: 37.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-25A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:30 PM

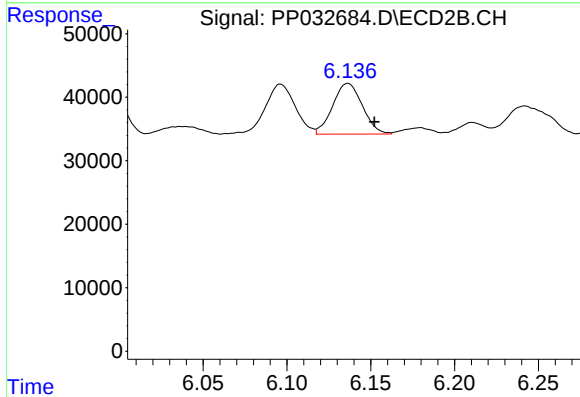


#26 AR-1254-1

R.T.: 6.136 min
Delta R.T.: -0.016 min
Response: 98293
Conc: 39.15 ng/ml

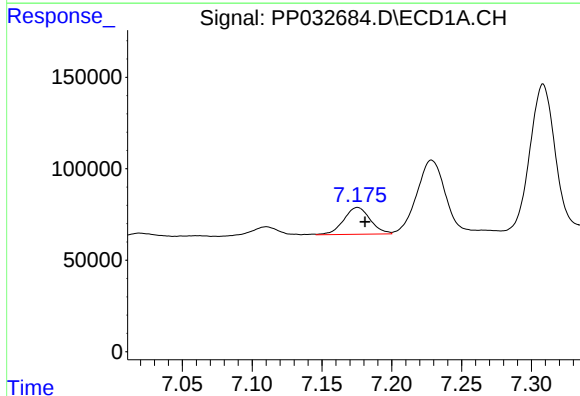


#27 AR-1254-2

R.T.: 7.176 min
Delta R.T.: -0.005 min
Response: 193844
Conc: 63.98 ng/ml

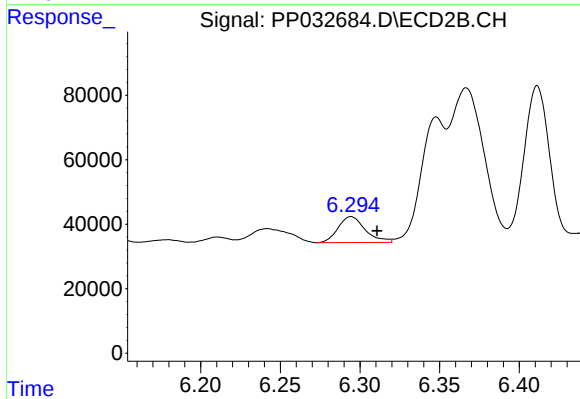

#27 AR-1254-2

R.T.: 6.294 min
Delta R.T.: -0.016 min
Response: 95522
Conc: 44.57 ng/ml

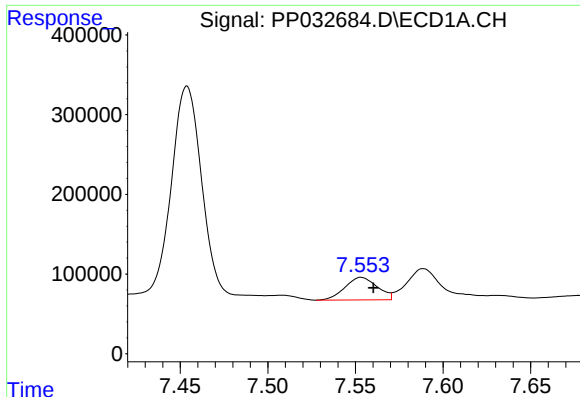


#28 AR-1254-3

R.T.: 7.553 min
Delta R.T.: -0.007 min
Response: 361232
Conc: 110.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-25A


Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:30 PM

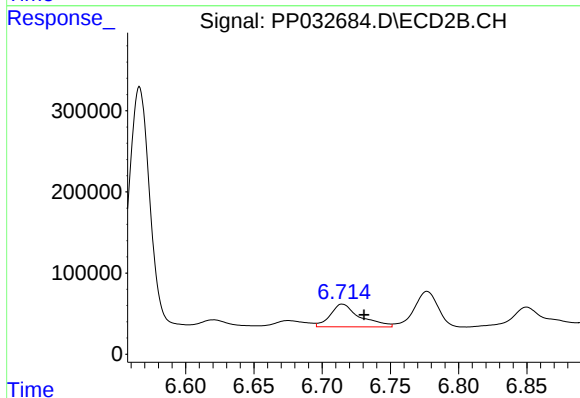


#28 AR-1254-3

R.T.: 6.715 min
Delta R.T.: -0.016 min
Response: 424693
Conc: 118.75 ng/ml

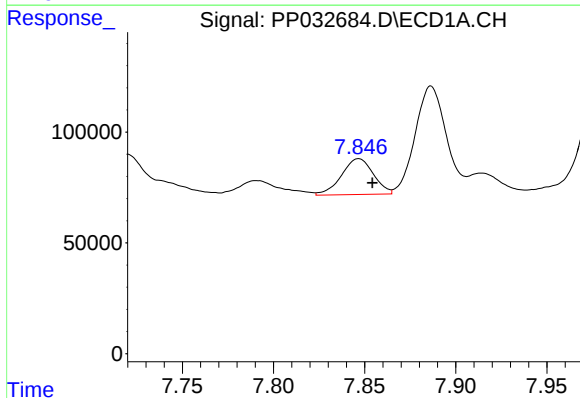


#29 AR-1254-4

R.T.: 7.847 min
Delta R.T.: -0.007 min
Response: 197521
Conc: 85.72 ng/ml

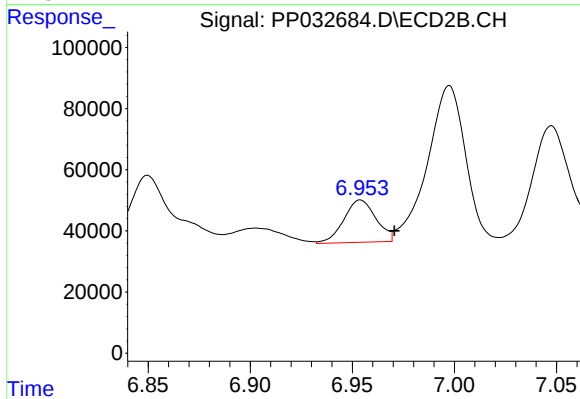

#29 AR-1254-4

R.T.: 6.954 min
Delta R.T.: -0.017 min
Response: 151069
Conc: 73.34 ng/ml

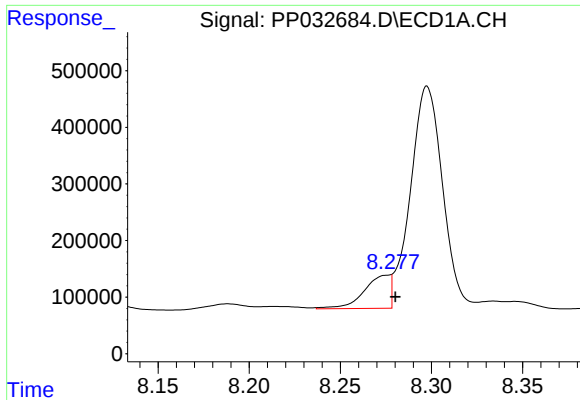


#30 AR-1254-5

R.T.: 8.277 min
Delta R.T.: -0.003 min
Response: 568020
Conc: 231.30 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-25A

Manual Integrations
APPROVED

Ankita
1/13/2021 3:39:30 PM

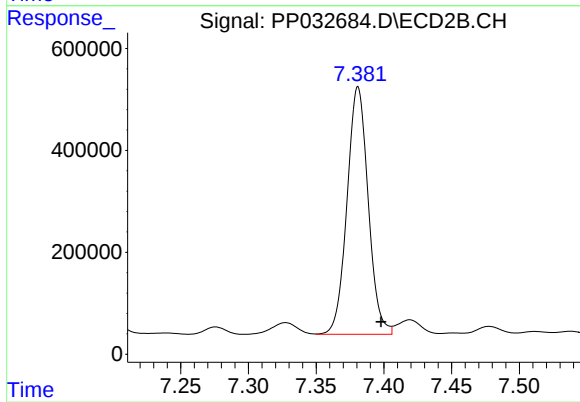

#30 AR-1254-5

R.T.: 7.381 min
Delta R.T.: -0.017 min
Response: 5287792
Conc: 1709.97 ng/ml