Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
Data File : PP042841.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2022 10:19
Operator : AJ\MA
Sample : PB141958BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 17:40:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 01:54:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	
	System Monitoring Compounds							
1)	SA Tetrachlo...	4.875	4.045	458566	521331	19.380	20.873	
2)	SA Decachlor...	10.805	9.381	270783	432438	18.523	22.169	
	Target Compounds							
8)	L2 AR-1221-1	5.114	0.000	2027	0	7.613	N.D.	#
9)	L2 AR-1221-2	5.216	4.378f	2135	6628	10.566	27.241	#
33)	L7 AR-1260-3	8.515f	0.000	6522	0	8.645	N.D.	#
34)	L7 AR-1260-4	8.747f	0.000	9096	0	10.678	N.D.	#
35)	L7 AR-1260-5	9.049	0.000	8558	0	5.201	N.D.	#
36)	L8 AR-1262-1	8.515f	0.000	6522	0	6.177	N.D.	#
37)	L8 AR-1262-2	9.049	0.000	8558	0	4.944	N.D.	#
45)	L9 AR-1268-5	10.492f	0.000	24934	0	4.679	N.D.	#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (Not Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
Data File : PP042841.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2022 10:19
Operator : AJ\MA
Sample : PB141958BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 17:40:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 01:54:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

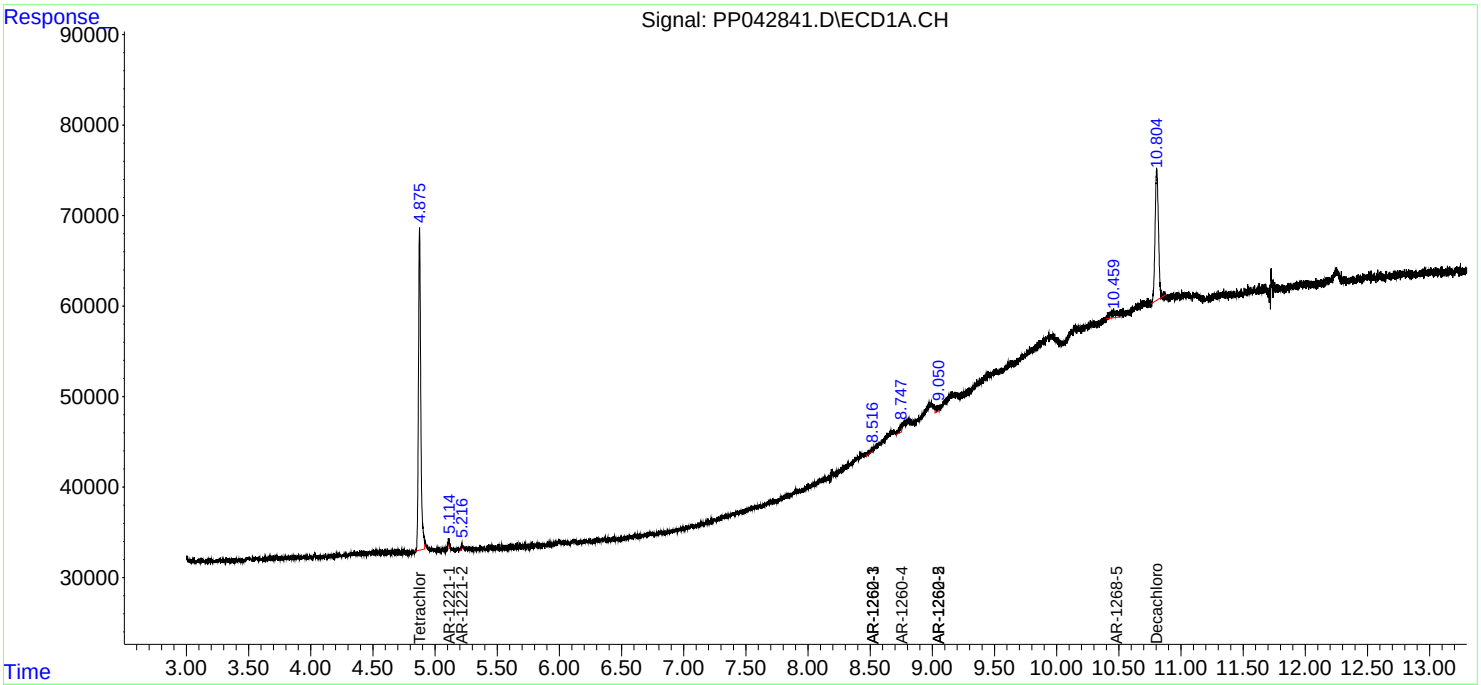

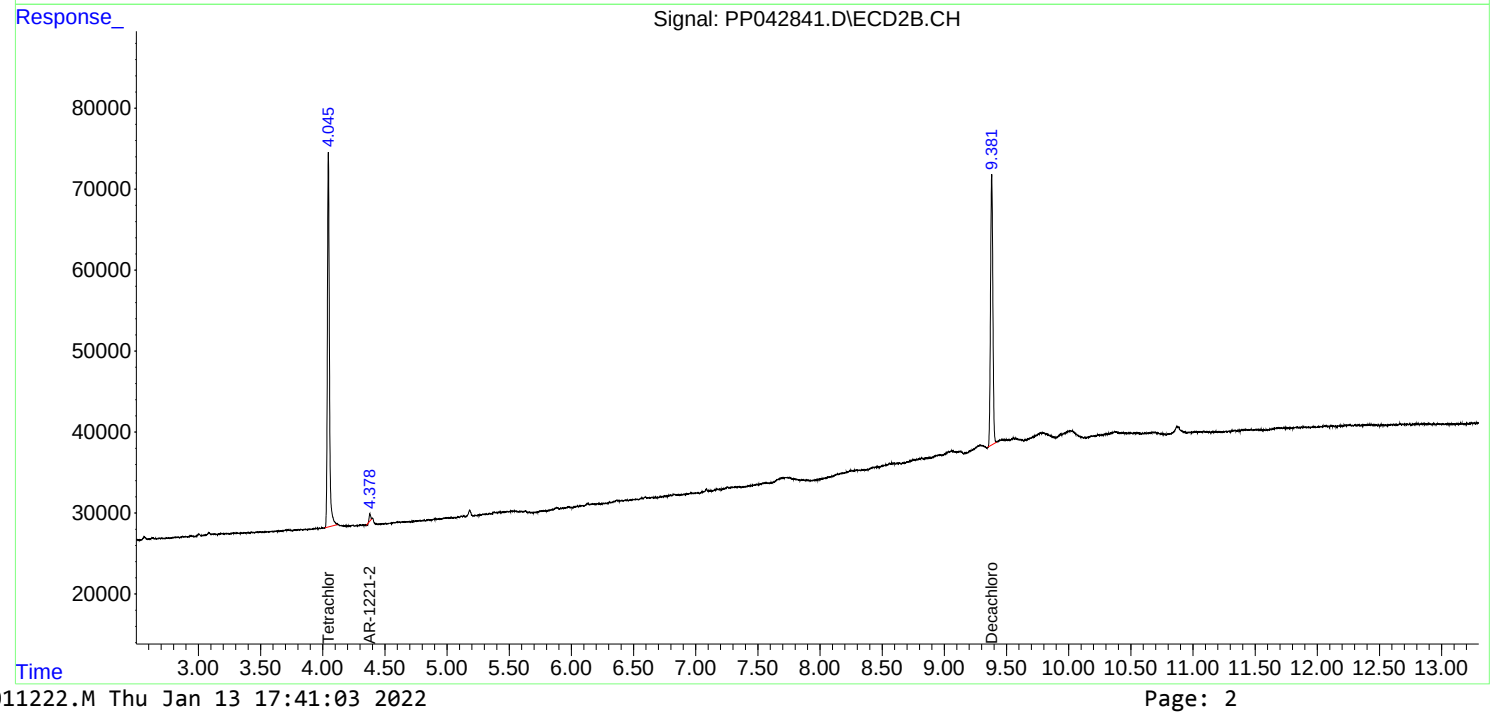

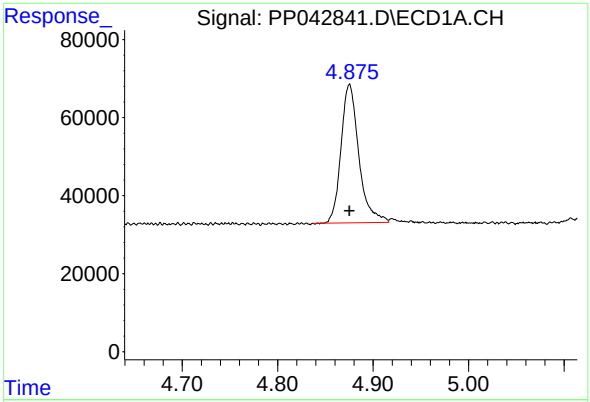

#1 Tetrachloro-m-xylene

R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 458566
Conc: 19.38 ng/ml

Instrument :
ECD_P
ClientSampleId :

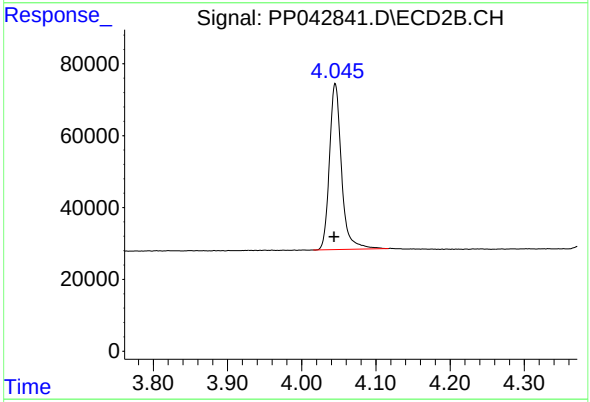

#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.002 min
Response: 521331
Conc: 20.87 ng/ml

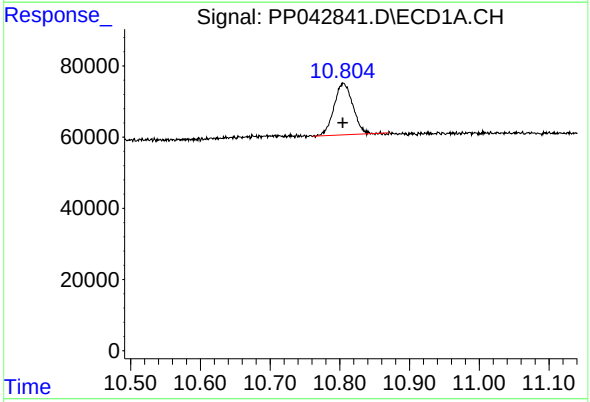

#2 Decachlorobiphenyl

R.T.: 10.805 min
Delta R.T.: 0.000 min
Response: 270783
Conc: 18.52 ng/ml

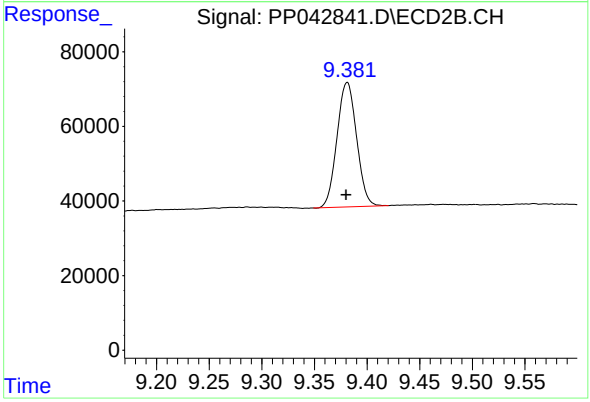

#2 Decachlorobiphenyl

R.T.: 9.381 min
Delta R.T.: 0.001 min
Response: 432438
Conc: 22.17 ng/ml

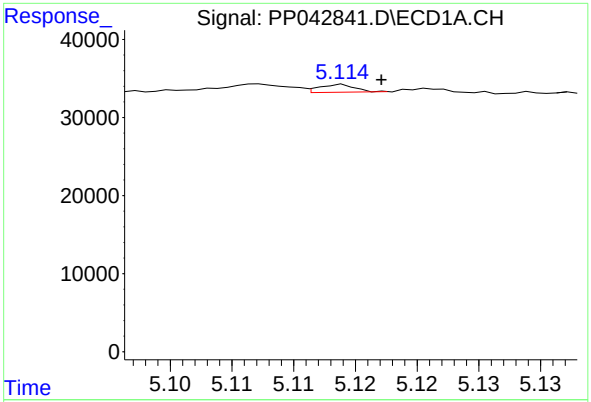

#8 AR-1221-1

R.T.: 5.114 min
Delta R.T.: -0.003 min
Response: 2027
Conc: 7.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

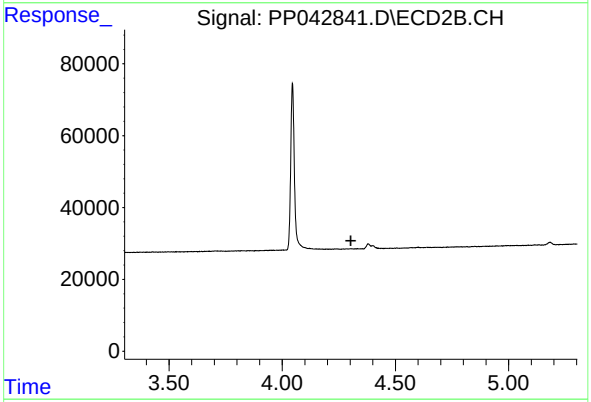

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.303 min
Response: 0
Conc: N.D.

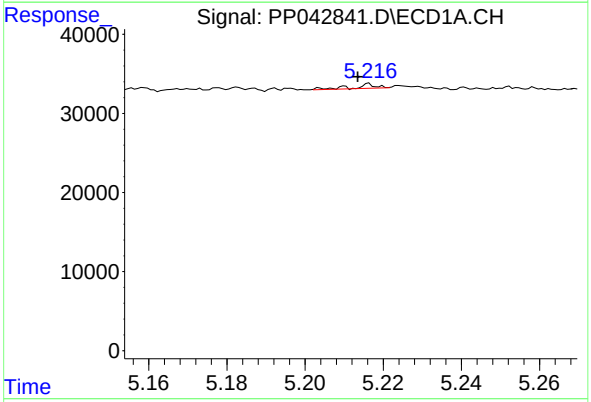

#9 AR-1221-2

R.T.: 5.216 min
Delta R.T.: 0.003 min
Response: 2135
Conc: 10.57 ng/ml

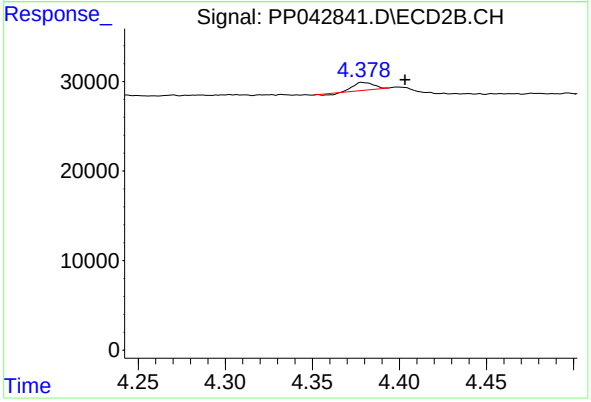

#9 AR-1221-2

R.T.: 4.378 min
Delta R.T.: -0.025 min
Response: 6628
Conc: 27.24 ng/ml

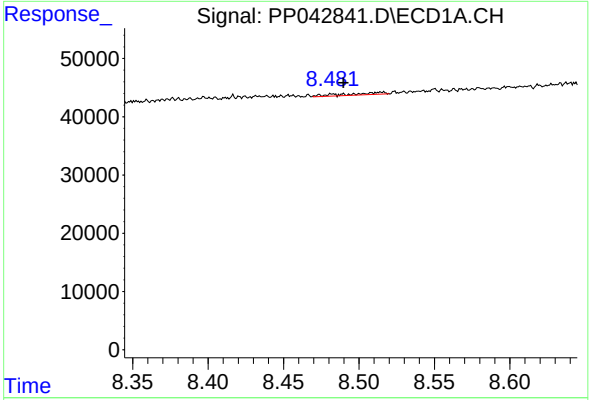

#33 AR-1260-3

R.T.: 8.515 min
Delta R.T.: 0.025 min
Response: 6522
Conc: 8.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

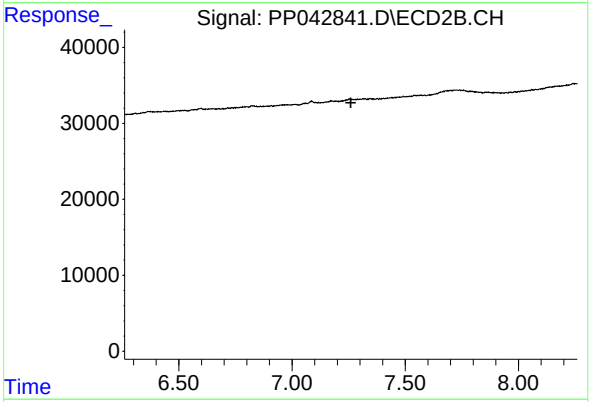

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 7.260 min
Response: 0
Conc: N.D.

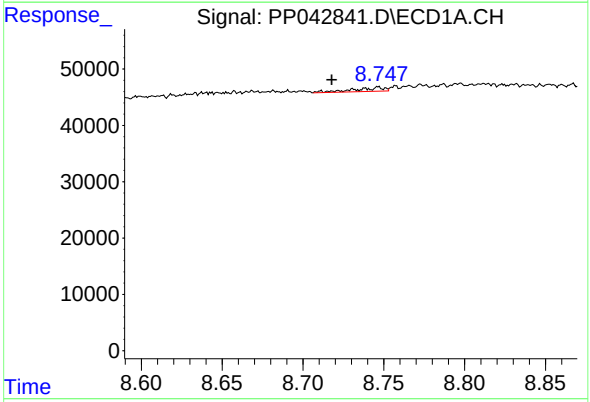

#34 AR-1260-4

R.T.: 8.747 min
Delta R.T.: 0.029 min
Response: 9096
Conc: 10.68 ng/ml

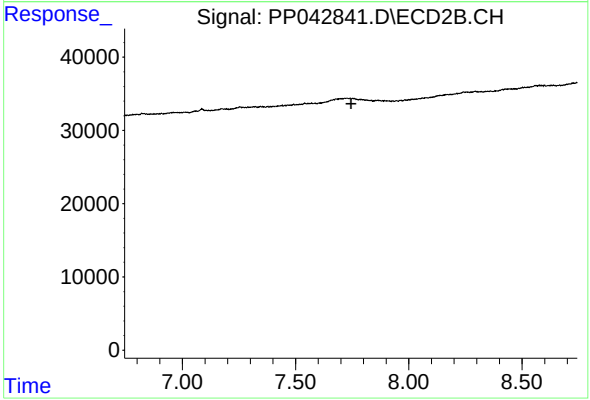

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.745 min
Response: 0
Conc: N.D.

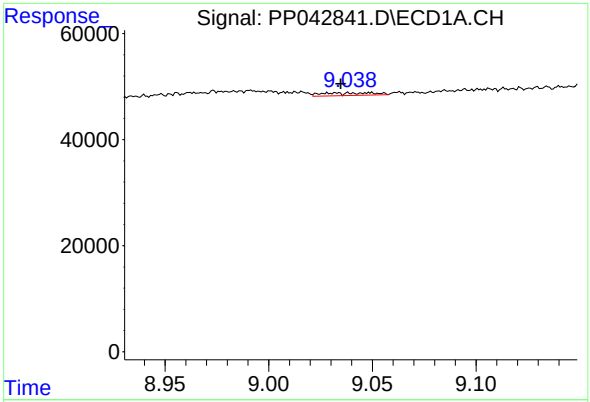

#35 AR-1260-5

R.T.: 9.049 min
Delta R.T.: 0.014 min
Response: 8558
Conc: 5.20 ng/ml

Instrument :
ECD_P
ClientSampleId :

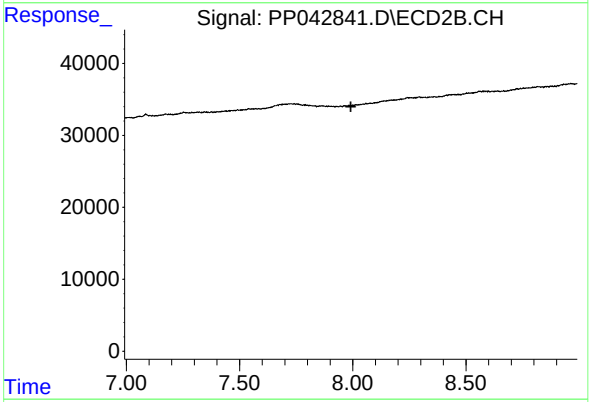

#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

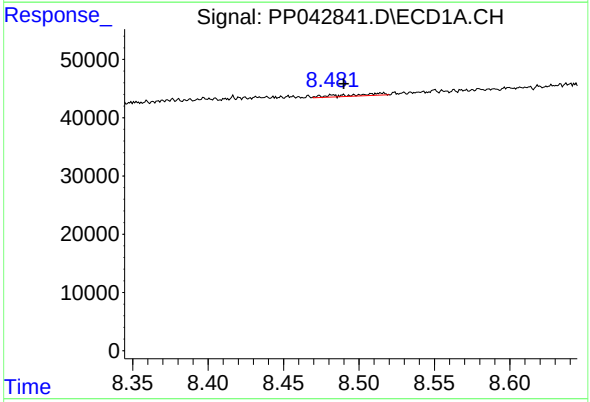

#36 AR-1262-1

R.T.: 8.515 min
Delta R.T.: 0.025 min
Response: 6522
Conc: 6.18 ng/ml

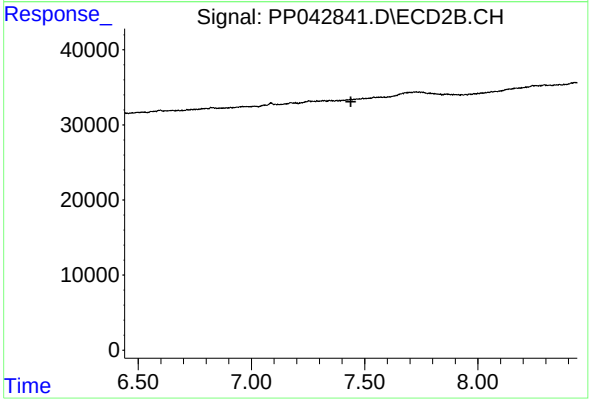

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.439 min
Response: 0
Conc: N.D.

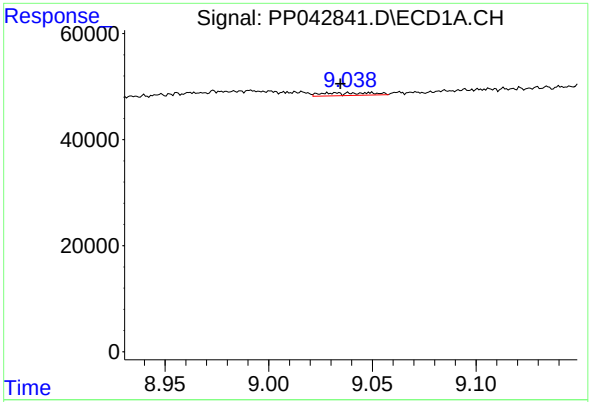

#37 AR-1262-2

R.T.: 9.049 min
Delta R.T.: 0.014 min
Response: 8558
Conc: 4.94 ng/ml

Instrument :
ECD_P
ClientSampleId :

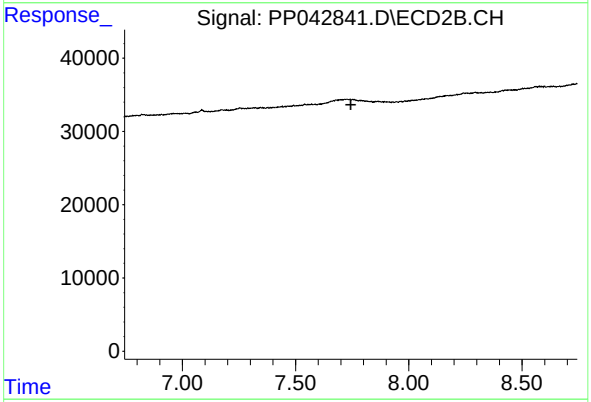

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

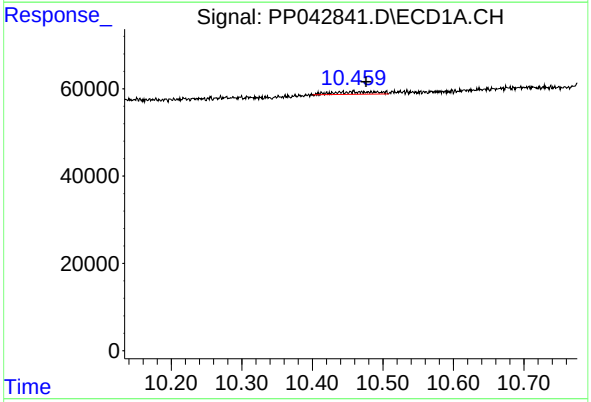

#45 AR-1268-5

R.T.: 10.492 min
Delta R.T.: 0.016 min
Response: 24934
Conc: 4.68 ng/ml

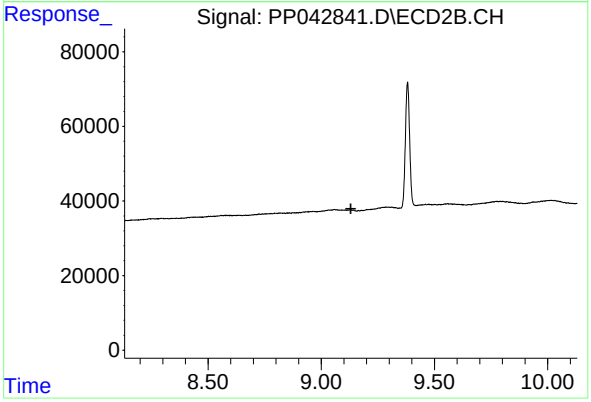

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.131 min
Response: 0
Conc: N.D.