

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
 Data File : PP042854.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2022 14:09
 Operator : AJ\MA
 Sample : PB141959BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 17:43:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 01:54:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.873	4.043	466322	538939	19.708	21.578
2)	SA Decachlor...	10.805	9.380	307669	449319	21.047	23.034
Target Compounds							
8)	L2 AR-1221-1	5.109	0.000	3012	0	11.316	N.D. #
9)	L2 AR-1221-2	0.000	4.378f	0	8518	N.D.	35.009 #
29)	L6 AR-1254-4	7.976	0.000	3484	0	3.986	N.D. #
33)	L7 AR-1260-3	8.519f	0.000	12256	0	16.244	N.D. #
36)	L8 AR-1262-1	8.519f	0.000	12256	0	11.607	N.D. #
39)	L8 AR-1262-4	9.454f	0.000	19929	0	36.944	N.D. #
42)	L9 AR-1268-2	9.454f	0.000	19929	0	10.434	N.D. #
43)	L9 AR-1268-3	9.660	0.000	25272	0	15.001	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
Data File : PP042854.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2022 14:09
Operator : AJ\MA
Sample : PB141959BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 17:43:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 01:54:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

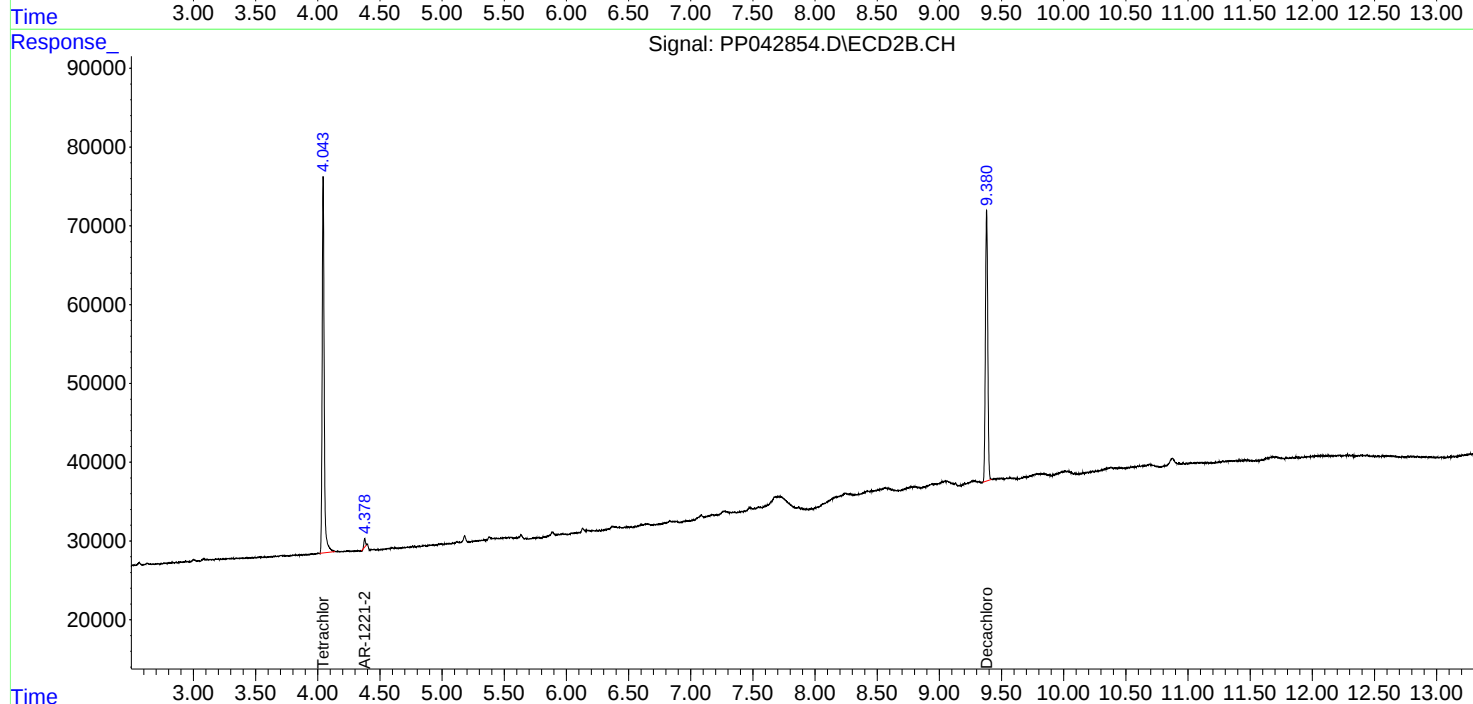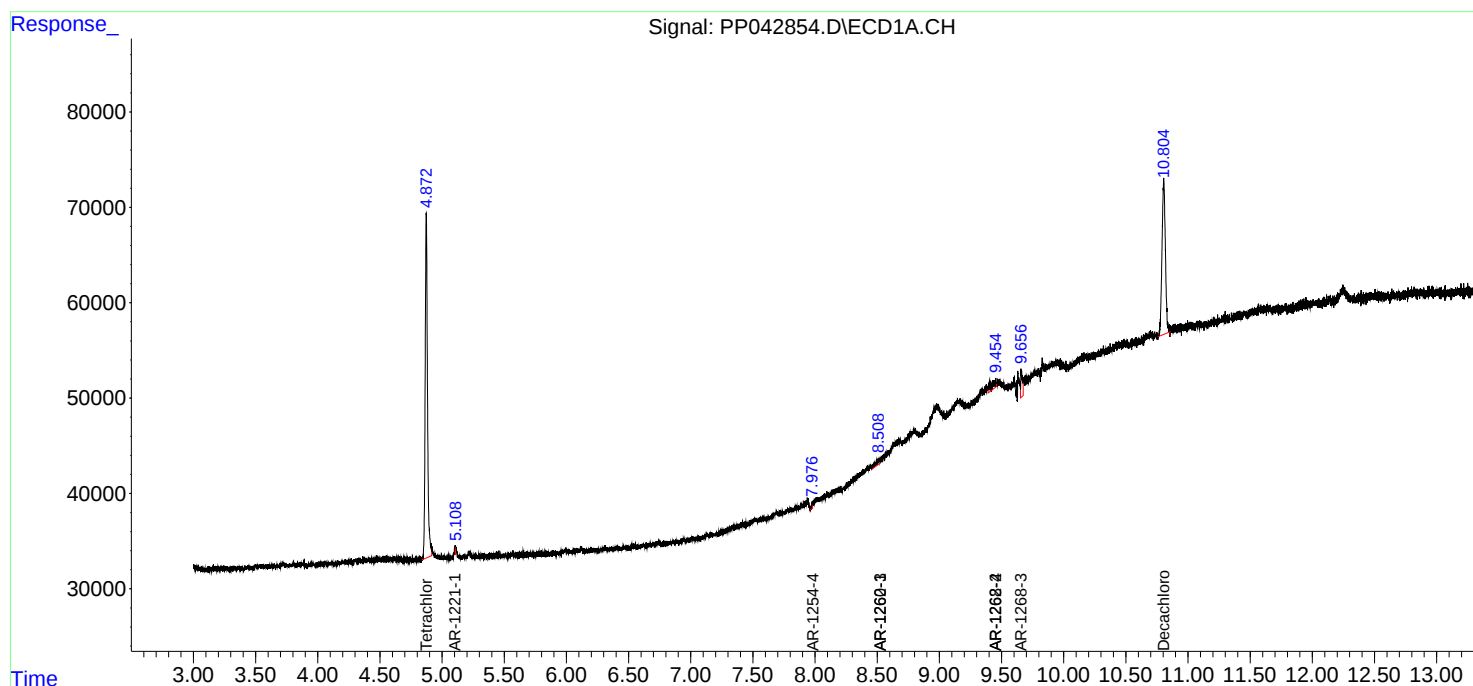


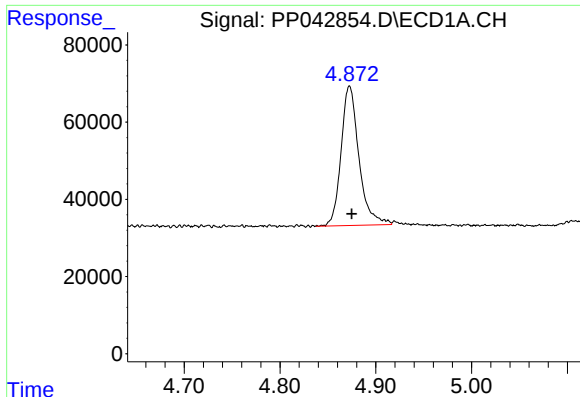

#1 Tetrachloro-m-xylene


R.T.: 4.873 min
Delta R.T.: -0.002 min
Response: 466322
Conc: 19.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

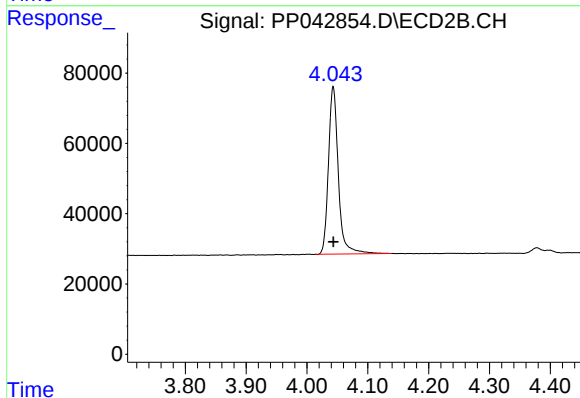


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 538939
Conc: 21.58 ng/ml

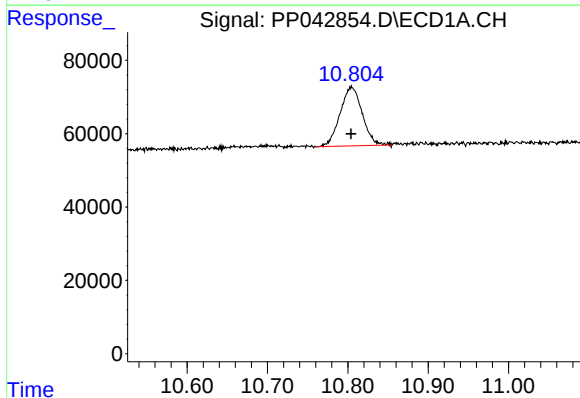


#2 Decachlorobiphenyl

R.T.: 10.805 min
Delta R.T.: 0.000 min
Response: 307669
Conc: 21.05 ng/ml

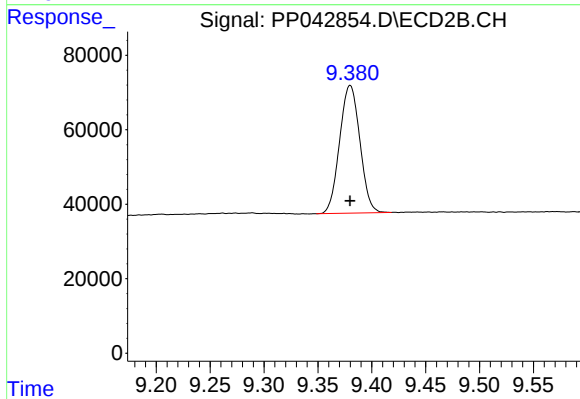

#2 Decachlorobiphenyl


R.T.: 9.380 min
Delta R.T.: 0.000 min
Response: 449319
Conc: 23.03 ng/ml

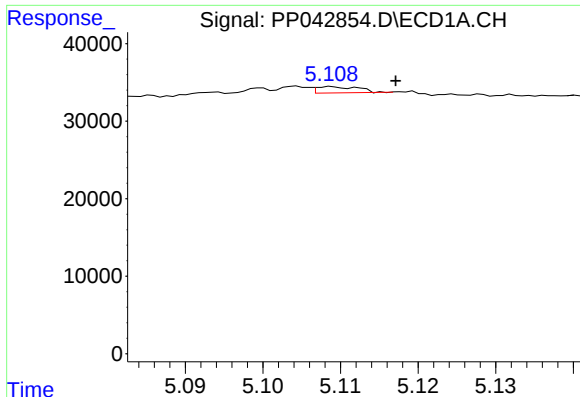

#8 AR-1221-1


R.T.: 5.109 min
Delta R.T.: -0.008 min
Response: 3012
Conc: 11.32 ng/ml

Instrument :
ECD_P
ClientSampleId :

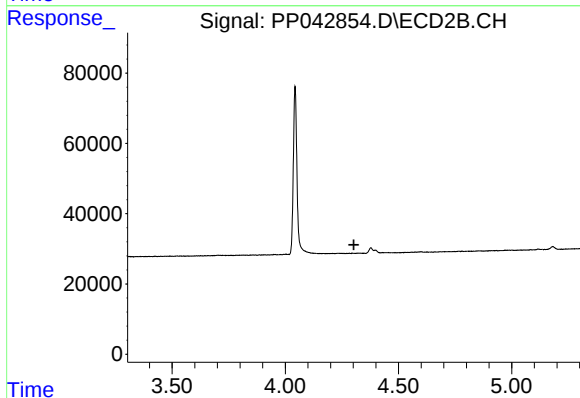


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.303 min
Response: 0
Conc: N.D.

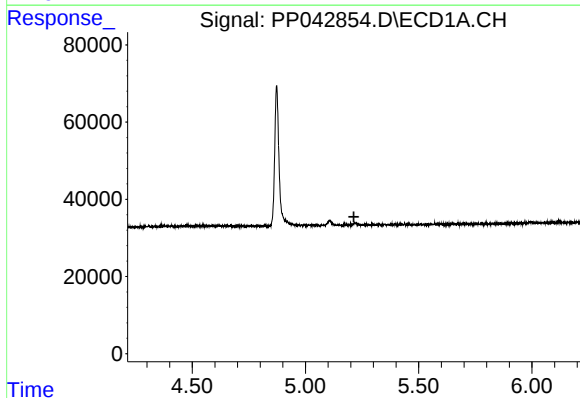


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

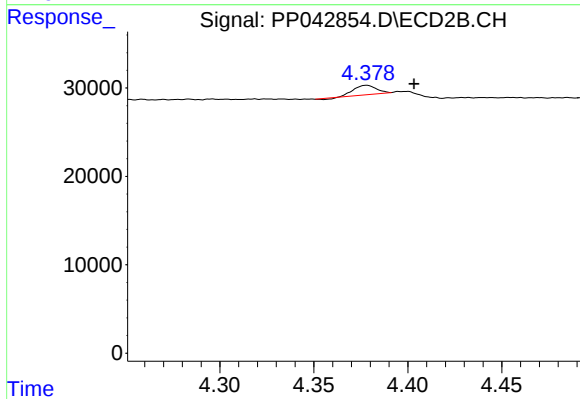

#9 AR-1221-2


R.T.: 4.378 min
Delta R.T.: -0.025 min
Response: 8518
Conc: 35.01 ng/ml

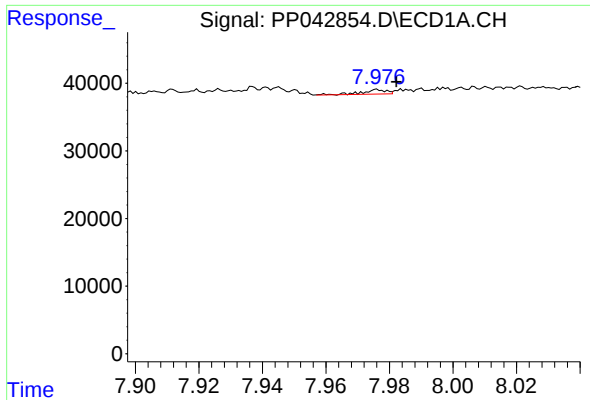

#29 AR-1254-4


R.T.: 7.976 min
Delta R.T.: -0.006 min
Response: 3484
Conc: 3.99 ng/ml

Instrument :
ECD_P
ClientSampleId :

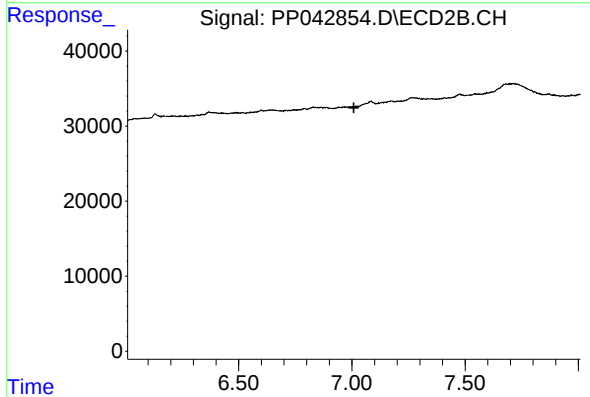


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

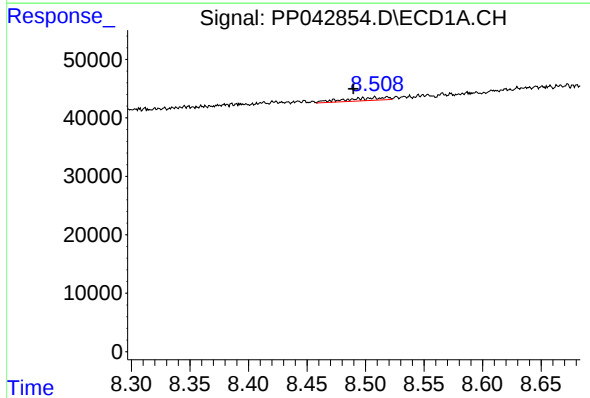


#33 AR-1260-3

R.T.: 8.519 min
Delta R.T.: 0.029 min
Response: 12256
Conc: 16.24 ng/ml

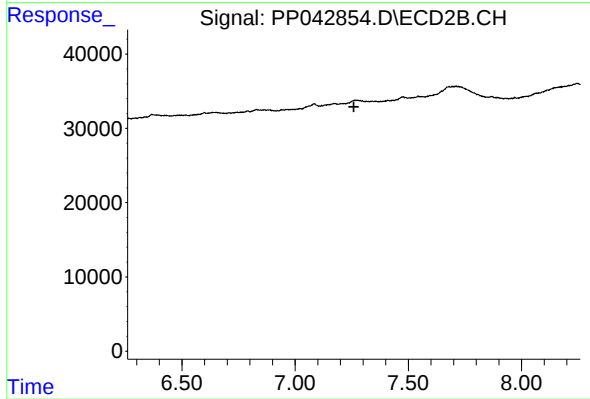

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.260 min
Response: 0
Conc: N.D.

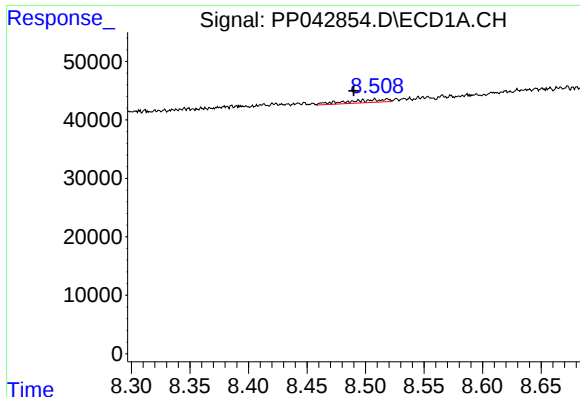

#36 AR-1262-1


R.T.: 8.519 min
Delta R.T.: 0.029 min
Response: 12256
Conc: 11.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

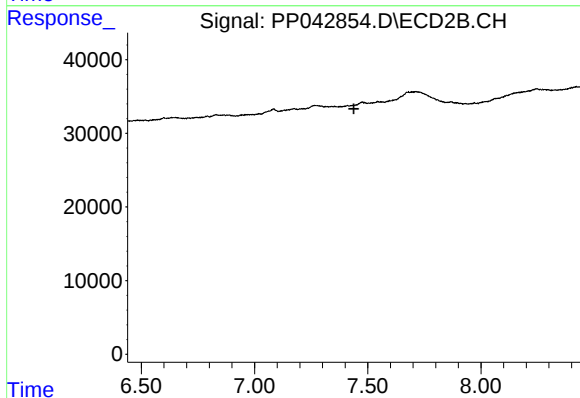


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.439 min
Response: 0
Conc: N.D.

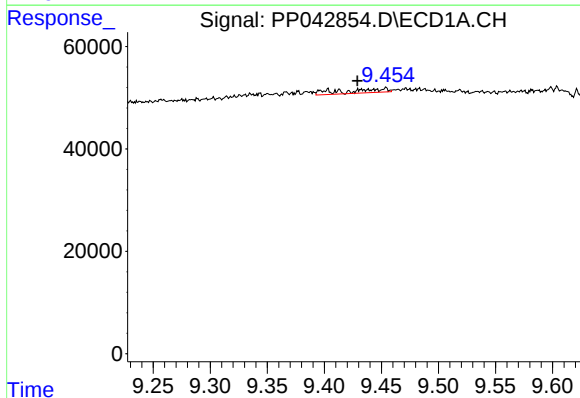


#39 AR-1262-4

R.T.: 9.454 min
Delta R.T.: 0.025 min
Response: 19929
Conc: 36.94 ng/ml

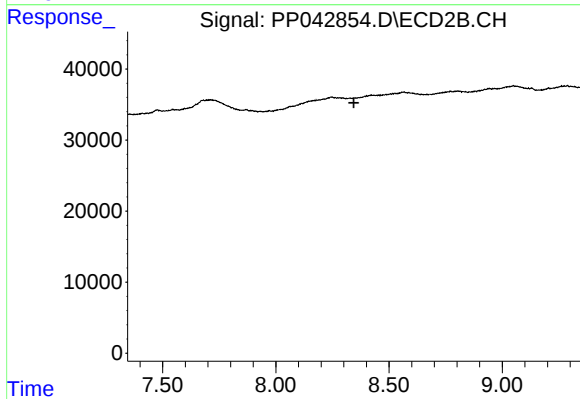

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

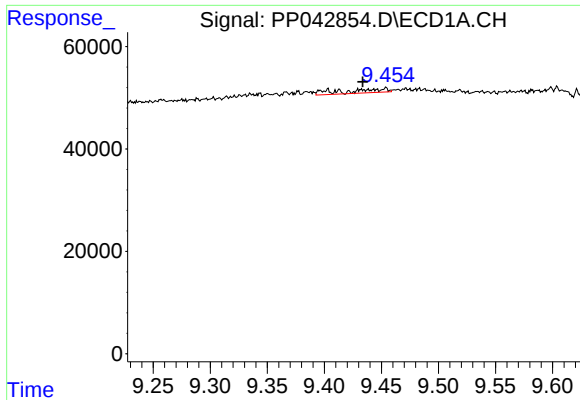

#42 AR-1268-2


R.T.: 9.454 min
Delta R.T.: 0.020 min
Response: 19929
Conc: 10.43 ng/ml

Instrument :
ECD_P
ClientSampleId :

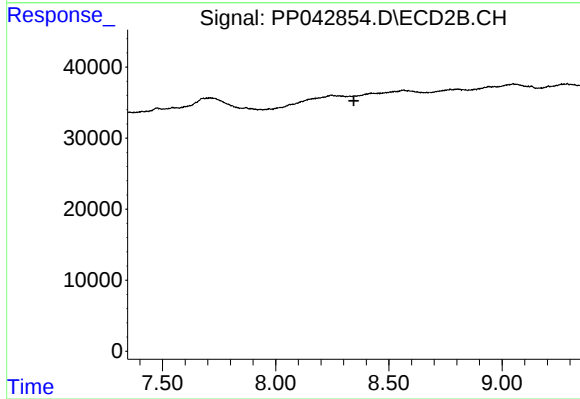


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

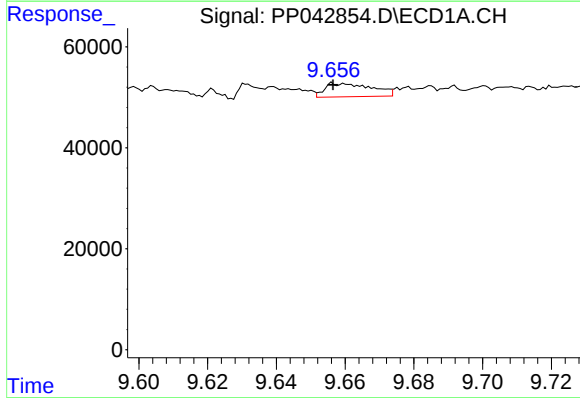

#43 AR-1268-3

R.T.: 9.660 min
Delta R.T.: 0.003 min
Response: 25272
Conc: 15.00 ng/ml

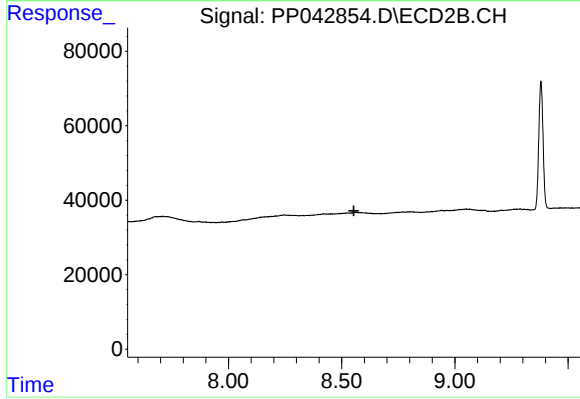

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.554 min
Response: 0
Conc: N.D.