

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
 Data File : PP042886.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2022 23:41
 Operator : AJ\MA
 Sample : N1095-30 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 00:23:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.875	4.046	41098	53835	1.737	2.155
2) SA Decachlor...	10.811	9.382	32623	45865	2.232	2.351
Target Compounds						
28) L6 AR-1254-3	7.692	0.000	5844	0	4.504	N.D. #
31) L7 AR-1260-1	7.857	0.000	3954	0	4.146	N.D. #
32) L7 AR-1260-2	0.000	7.084f	0	671	N.D.	0.430 #
33) L7 AR-1260-3	8.501	0.000	5889	0	7.805	N.D. #
35) L7 AR-1260-5	0.000	7.993	0	10441	N.D.	4.163 #
36) L8 AR-1262-1	8.501	0.000	5889	0	5.577	N.D. #
39) L8 AR-1262-4	9.447f	0.000	45728	0	83.166	N.D. #
42) L9 AR-1268-2	9.447	0.000	45728	0	23.942	N.D. #
43) L9 AR-1268-3	9.637f	0.000	6647	0	3.946	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
Data File : PP042886.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2022 23:41
Operator : AJ\MA
Sample : N1095-30 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 00:23:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

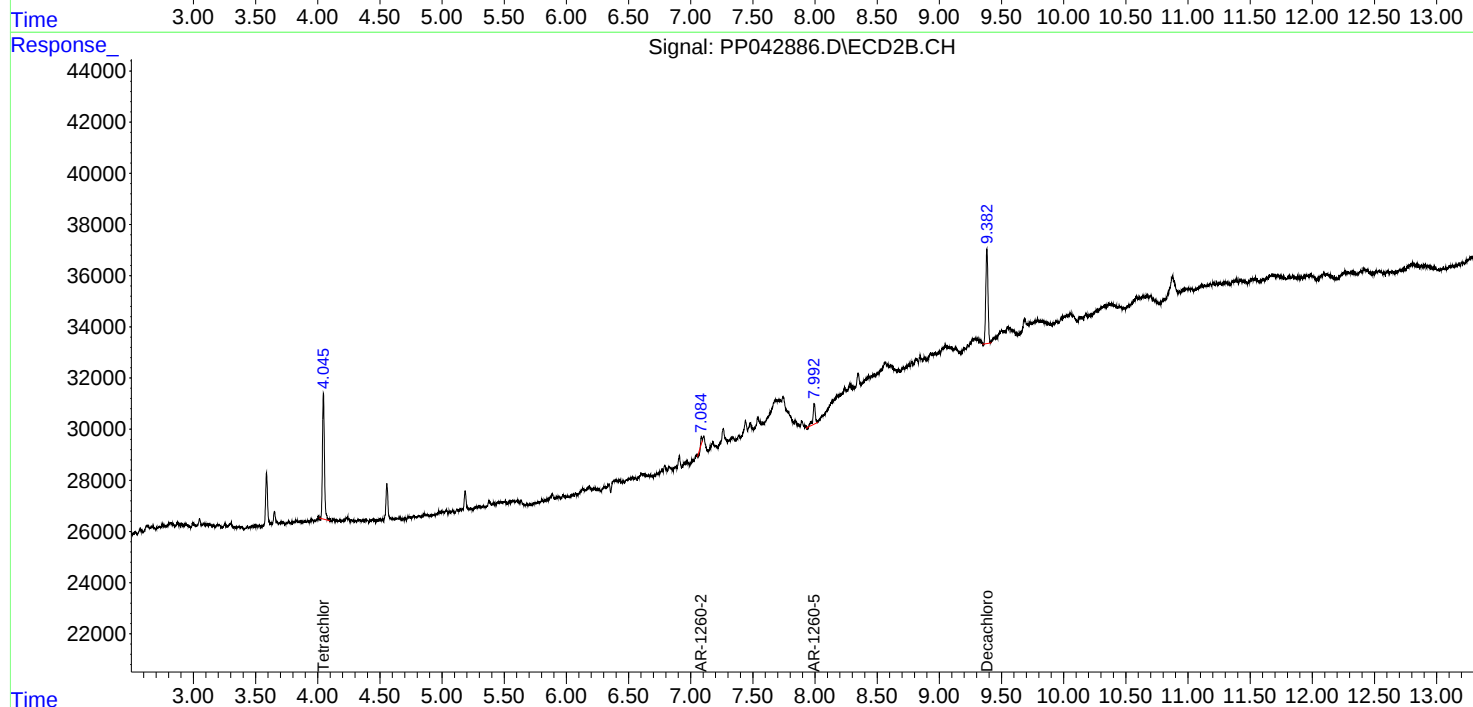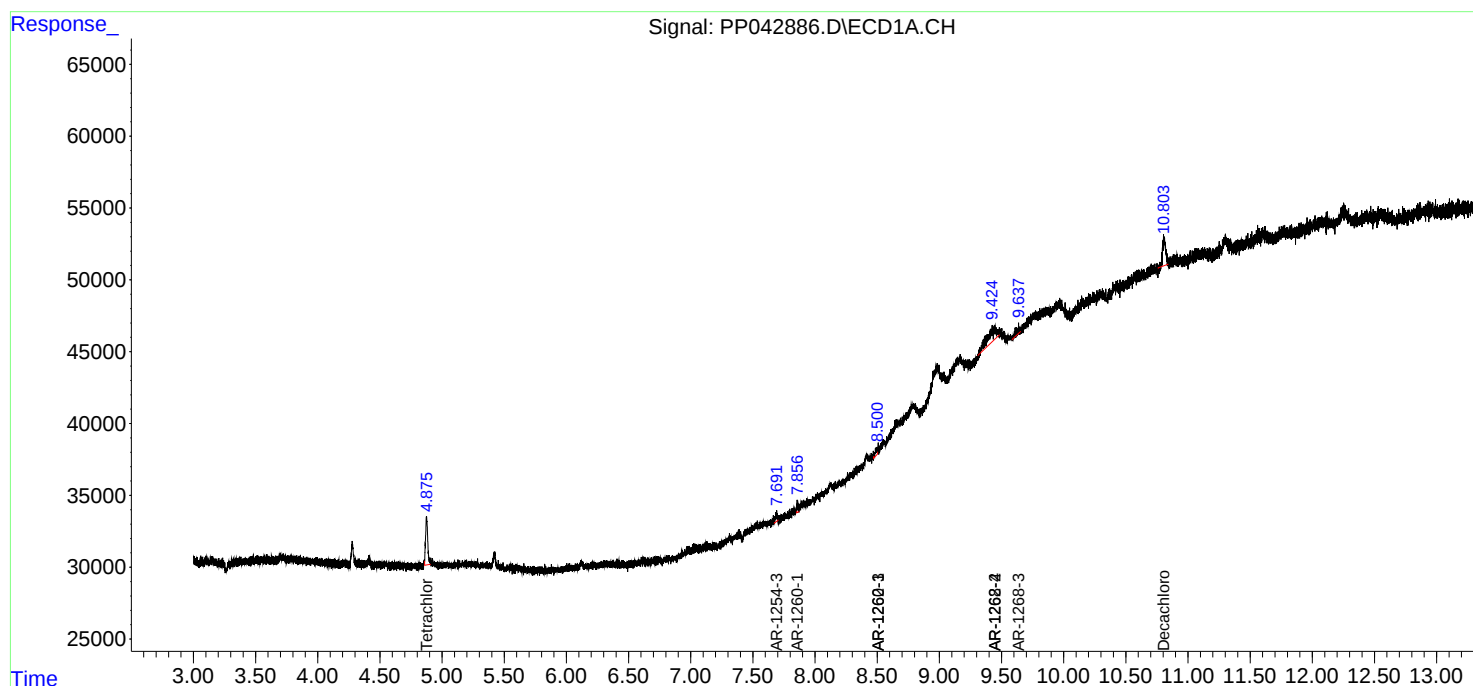


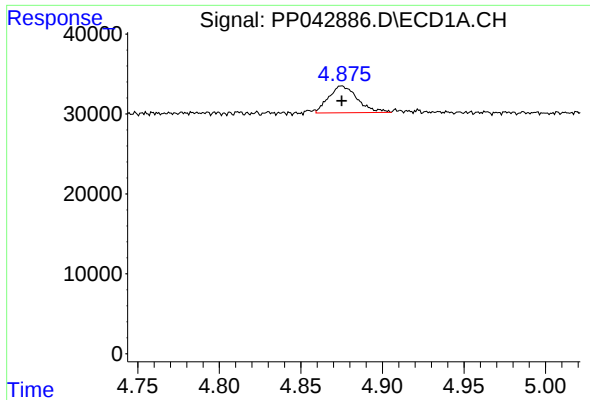

#1 Tetrachloro-m-xylene


R.T.: 4.875 min
Delta R.T.: 0.000 min
Response: 41098
Conc: 1.74 ng/ml

Instrument :
ECD_P
ClientSampleId :

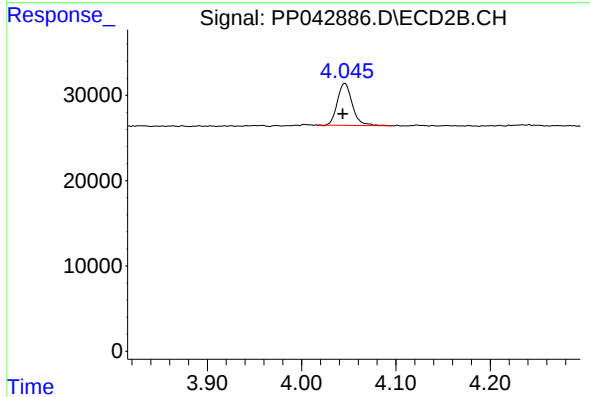


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.002 min
Response: 53835
Conc: 2.16 ng/ml

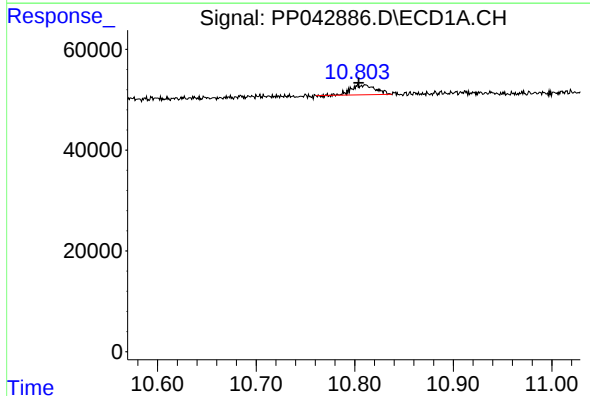


#2 Decachlorobiphenyl

R.T.: 10.811 min
Delta R.T.: 0.007 min
Response: 32623
Conc: 2.23 ng/ml

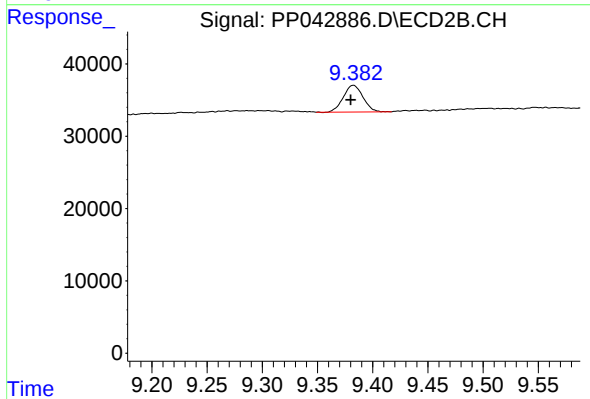

#2 Decachlorobiphenyl


R.T.: 9.382 min
Delta R.T.: 0.002 min
Response: 45865
Conc: 2.35 ng/ml

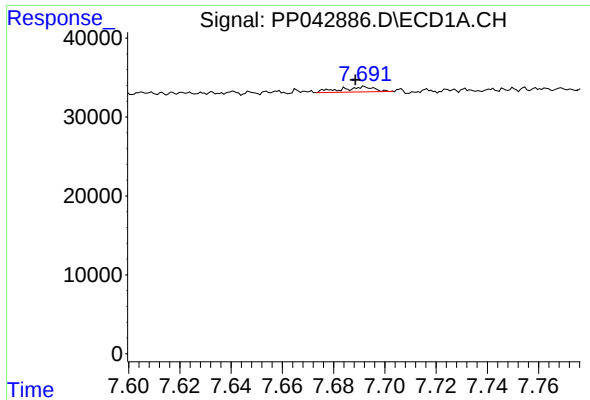

#28 AR-1254-3


R.T.: 7.692 min
Delta R.T.: 0.004 min
Response: 5844
Conc: 4.50 ng/ml

Instrument :
ECD_P
ClientSampleId :

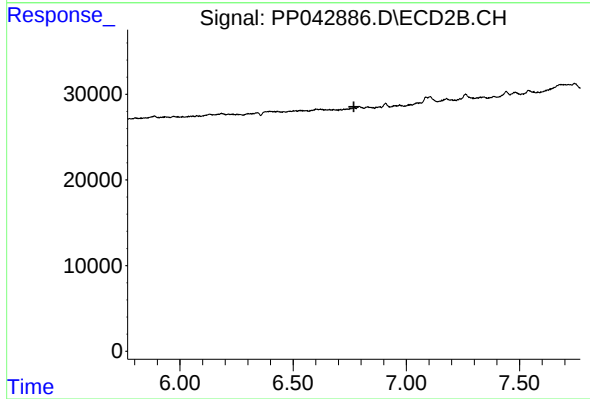


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

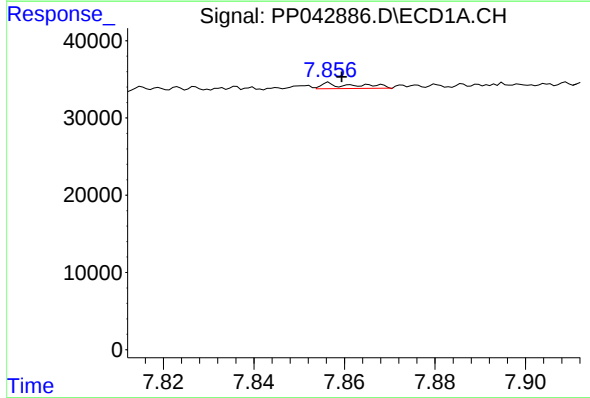


#31 AR-1260-1

R.T.: 7.857 min
Delta R.T.: -0.003 min
Response: 3954
Conc: 4.15 ng/ml

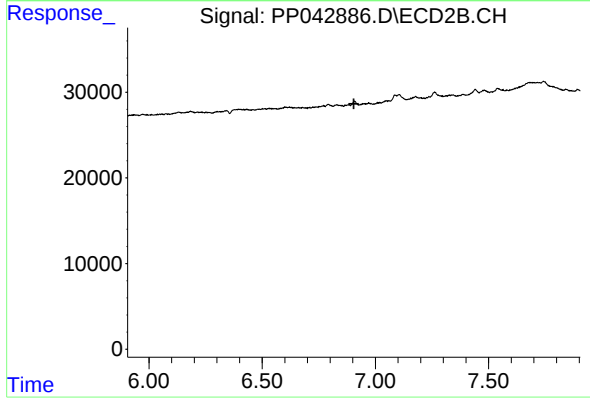

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.905 min
Response: 0
Conc: N.D.

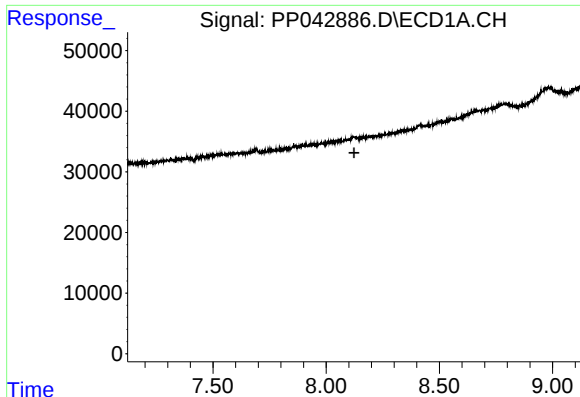

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

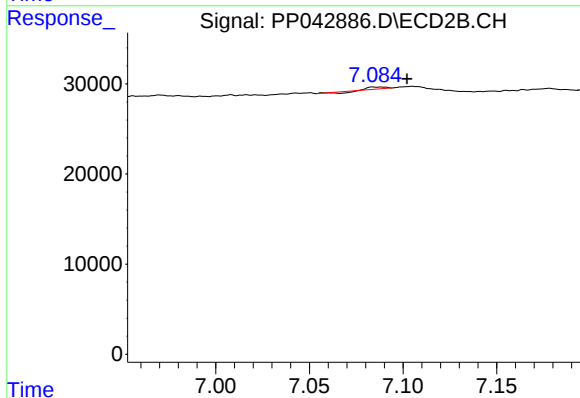


#32 AR-1260-2

R.T.: 7.084 min
Delta R.T.: -0.018 min
Response: 671
Conc: 0.43 ng/ml

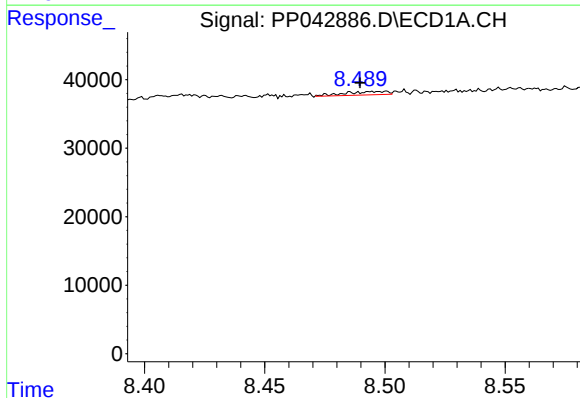


#33 AR-1260-3

R.T.: 8.501 min
Delta R.T.: 0.011 min
Response: 5889
Conc: 7.80 ng/ml

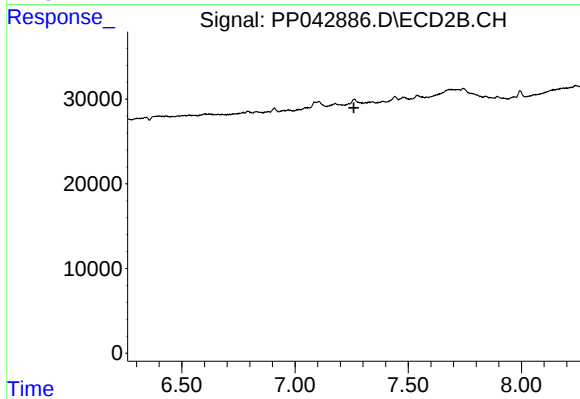

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.260 min
Response: 0
Conc: N.D.

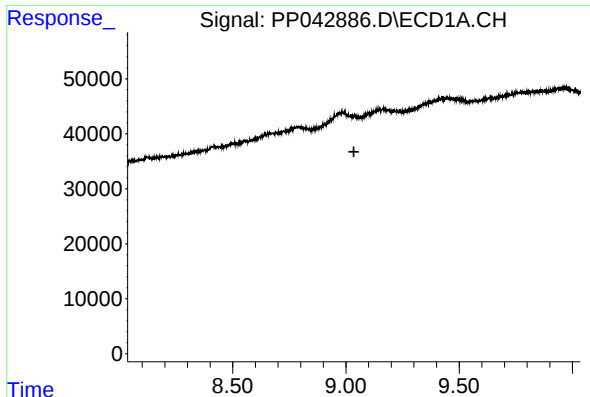

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

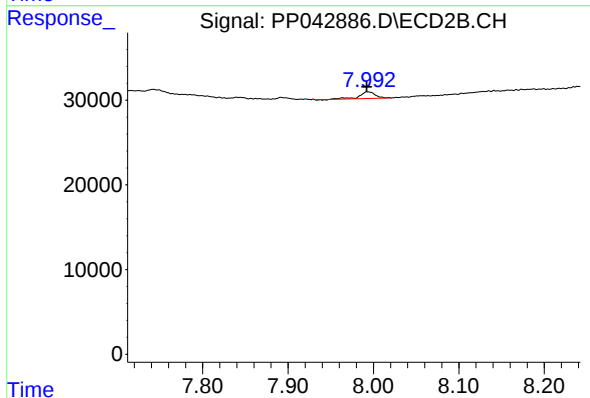


#35 AR-1260-5

R.T.: 7.993 min
Delta R.T.: 0.001 min
Response: 10441
Conc: 4.16 ng/ml

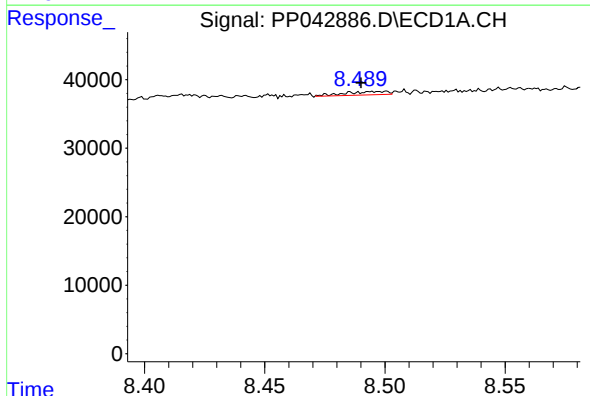


#36 AR-1262-1

R.T.: 8.501 min
Delta R.T.: 0.011 min
Response: 5889
Conc: 5.58 ng/ml

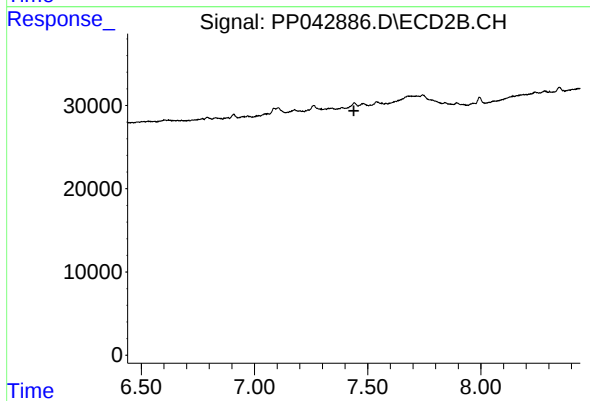

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.439 min
Response: 0
Conc: N.D.

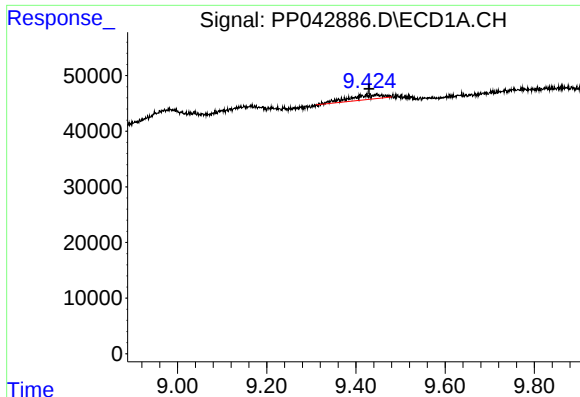

#39 AR-1262-4


R.T.: 9.447 min
Delta R.T.: 0.018 min
Response: 45728
Conc: 83.17 ng/ml

Instrument :
ECD_P
ClientSampleId :

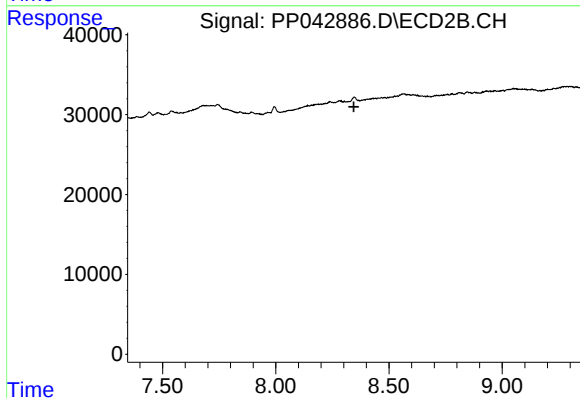


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

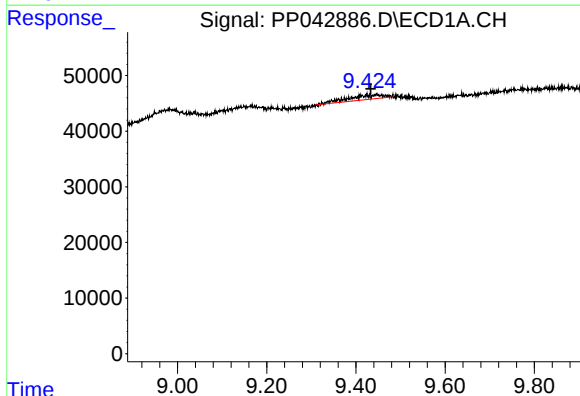


#42 AR-1268-2

R.T.: 9.447 min
Delta R.T.: 0.013 min
Response: 45728
Conc: 23.94 ng/ml

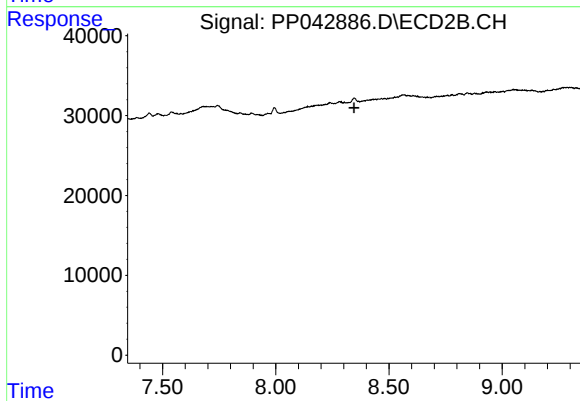

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

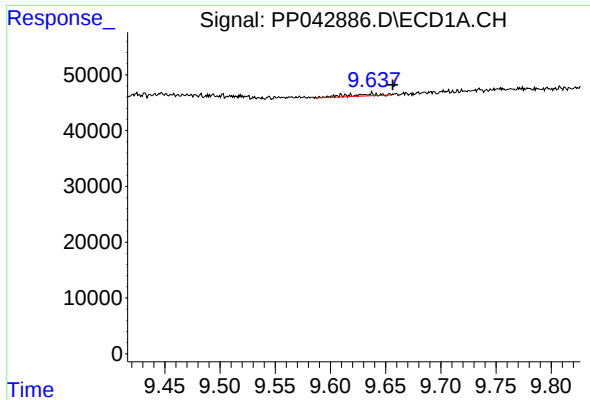

#43 AR-1268-3

R.T.: 9.637 min
Delta R.T.: -0.019 min
Response: 6647
Conc: 3.95 ng/ml

Instrument :
ECD_P
ClientSampleId :

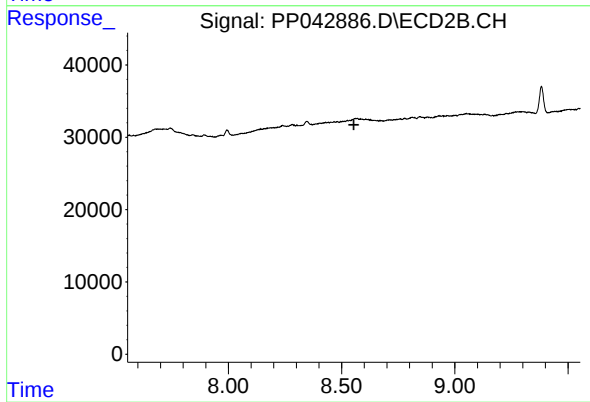

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.554 min
Response: 0
Conc: N.D.