

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
 Data File : PP042850.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2022 12:49
 Operator : AJ\MA
 Sample : N1095-08 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IRV-2022-5A

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
 Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 17:42:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 01:54:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.872	4.043	40539	54600	1.713	2.186 #
2) SA Decachlor...	10.803	9.379	42977	34837	2.940	1.786 #
Target Compounds						
26) L6 AR-1254-1	7.081	6.186	16527	45195	21.062	29.145 #
27) L6 AR-1254-2	7.311	6.345	40574	45373	32.238	33.423
28) L6 AR-1254-3	7.689	6.769	88517	56160	68.227	26.256m#
29) L6 AR-1254-4	7.982	7.009	24929	38629	28.522m	30.963
30) L6 AR-1254-5	8.408	7.439	11984	52737	12.791	30.928 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
Data File : PP042850.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2022 12:49
Operator : AJ\MA
Sample : N1095-08 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
IRV-2022-5A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 17:42:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 01:54:06 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

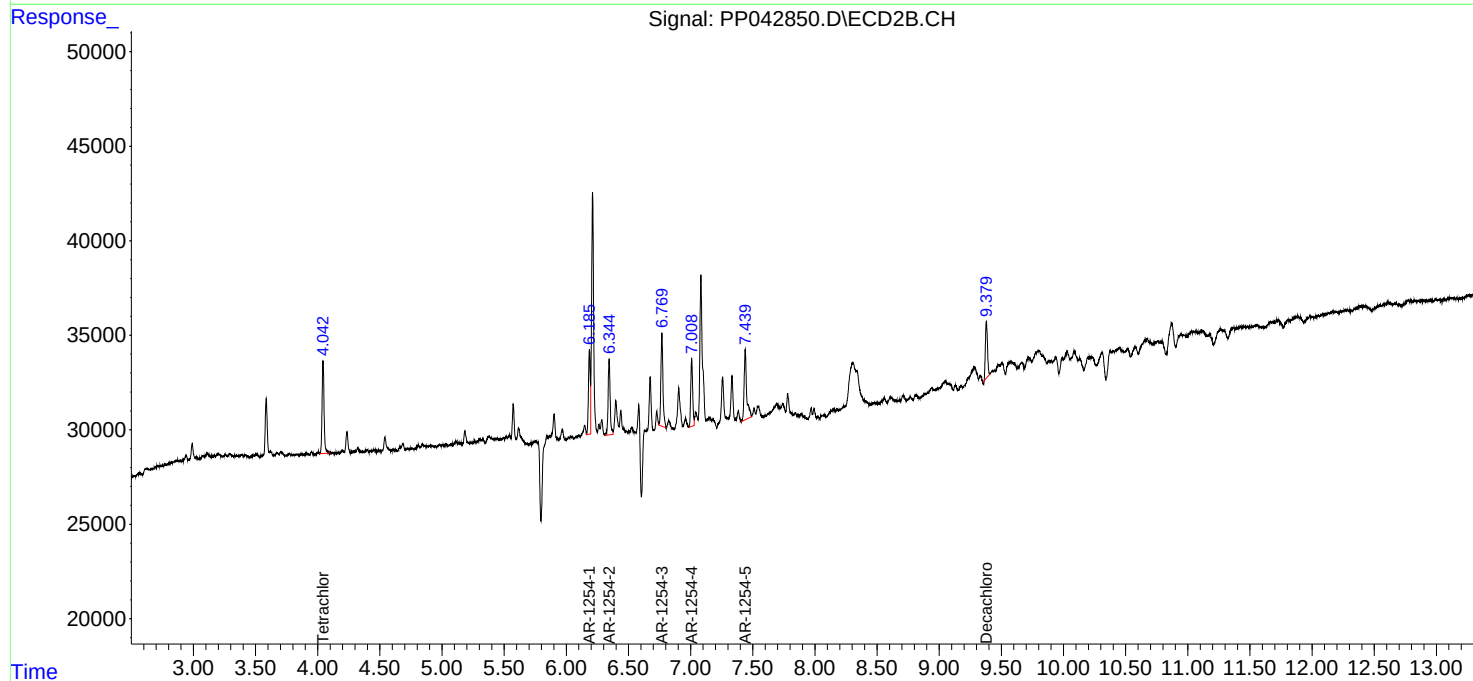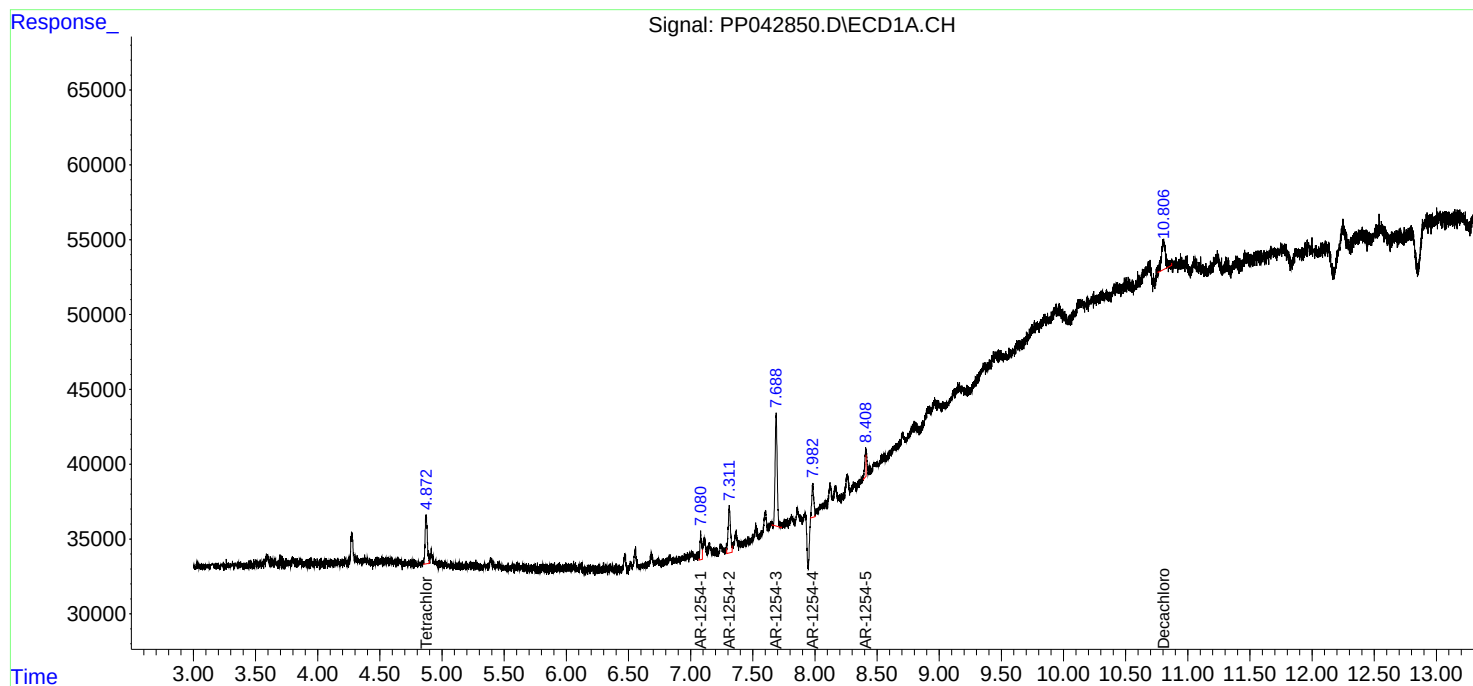

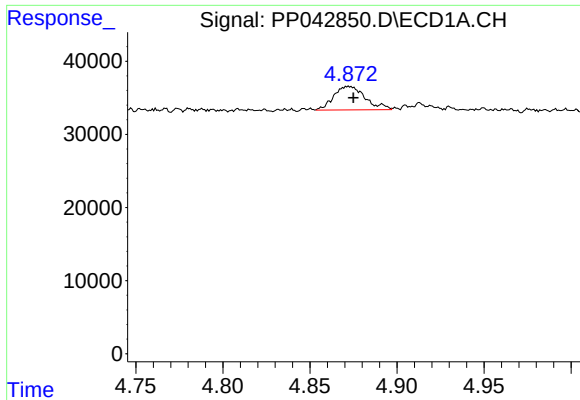


#1 Tetrachloro-m-xylene

R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 40539
Conc: 1.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-5A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

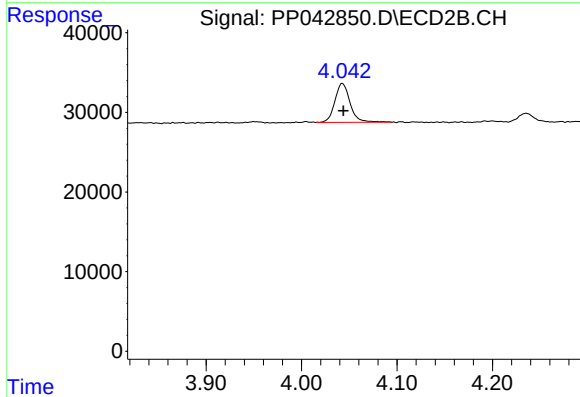


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 54600
Conc: 2.19 ng/ml

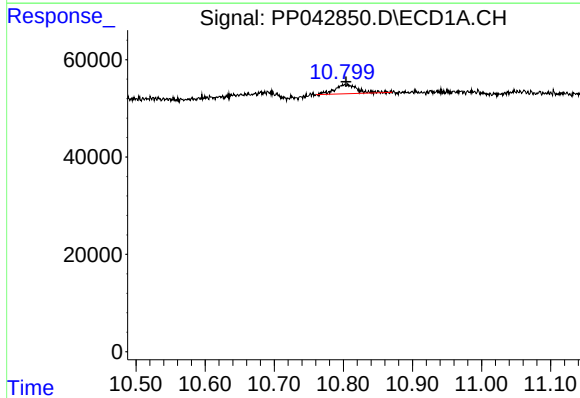


#2 Decachlorobiphenyl

R.T.: 10.803 min
Delta R.T.: -0.002 min
Response: 42977
Conc: 2.94 ng/ml

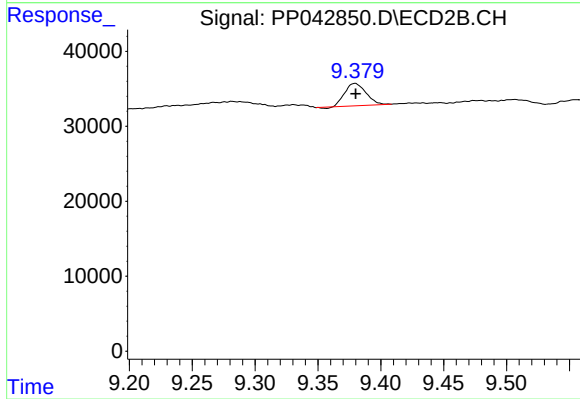

#2 Decachlorobiphenyl

R.T.: 9.379 min
Delta R.T.: 0.000 min
Response: 34837
Conc: 1.79 ng/ml

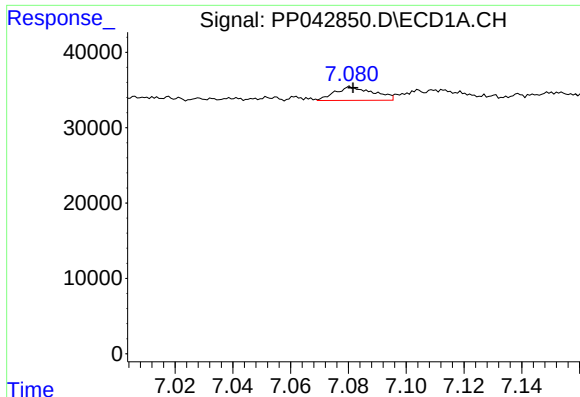


#26 AR-1254-1

R.T.: 7.081 min
Delta R.T.: 0.000 min
Response: 16527
Conc: 21.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-5A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

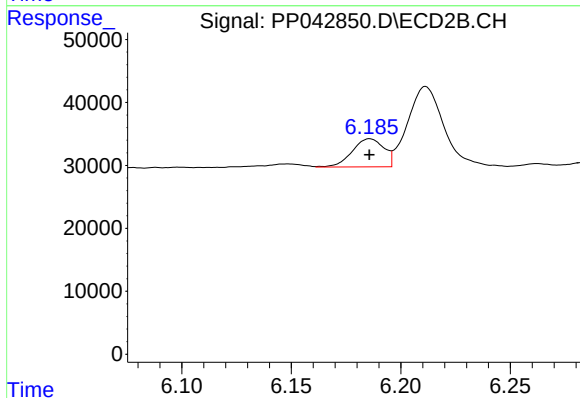


#26 AR-1254-1

R.T.: 6.186 min
Delta R.T.: 0.000 min
Response: 45195
Conc: 29.14 ng/ml

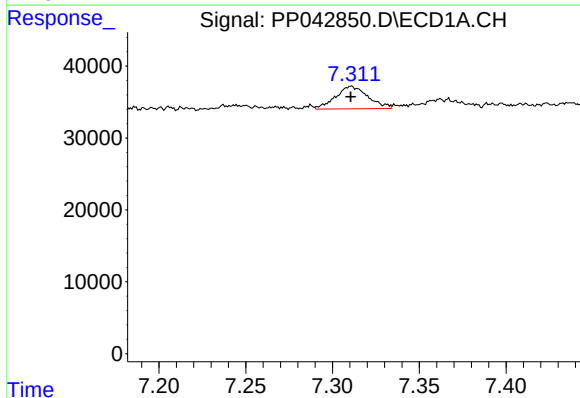


#27 AR-1254-2

R.T.: 7.311 min
Delta R.T.: 0.000 min
Response: 40574
Conc: 32.24 ng/ml

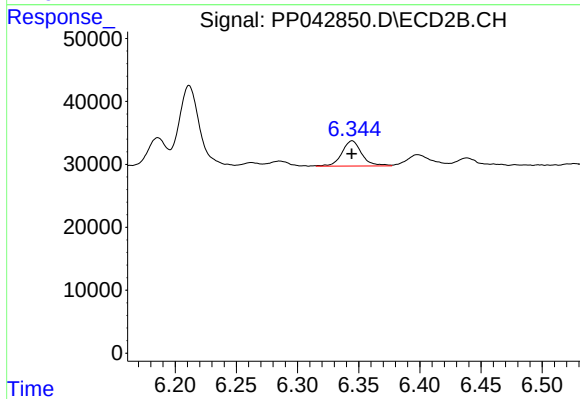

#27 AR-1254-2

R.T.: 6.345 min
Delta R.T.: 0.000 min
Response: 45373
Conc: 33.42 ng/ml

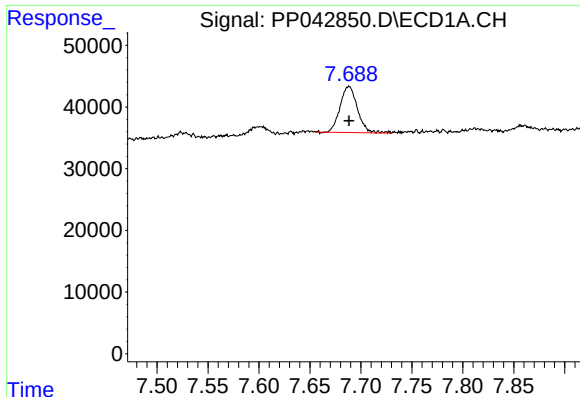


#28 AR-1254-3

R.T.: 7.689 min
Delta R.T.: 0.000 min
Response: 88517
Conc: 68.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-5A


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

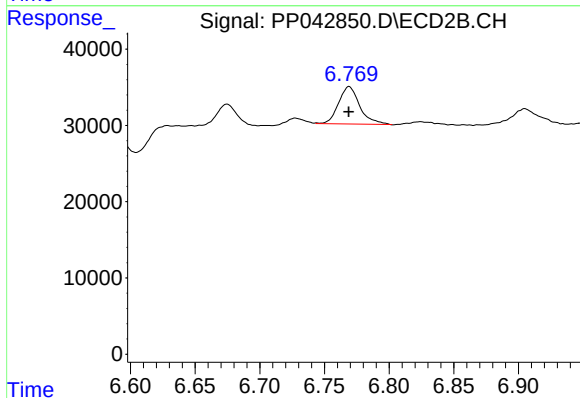


#28 AR-1254-3

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 56160
Conc: 26.26 ng/ml m

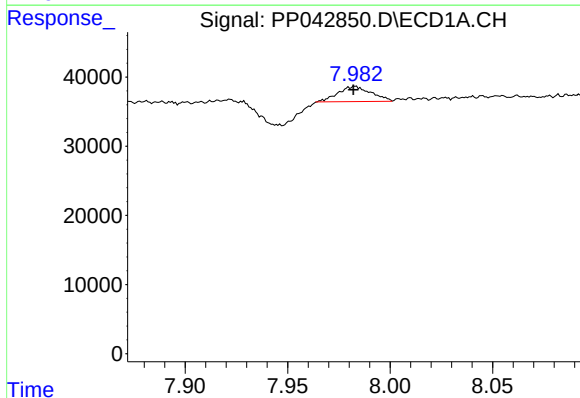


#29 AR-1254-4

R.T.: 7.982 min
Delta R.T.: 0.000 min
Response: 24929
Conc: 28.52 ng/ml m

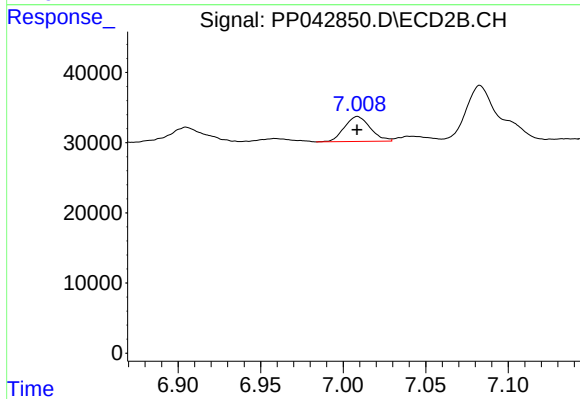

#29 AR-1254-4

R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 38629
Conc: 30.96 ng/ml

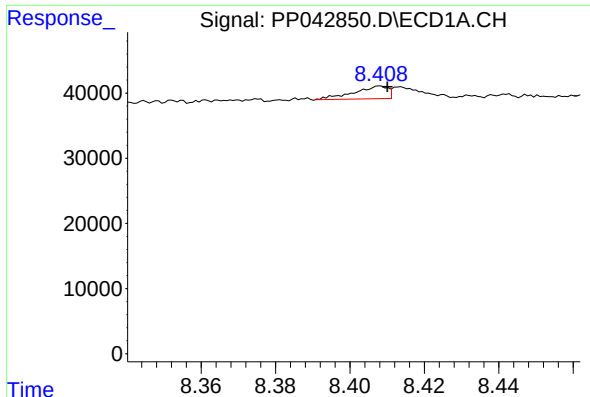


#30 AR-1254-5

R.T.: 8.408 min
Delta R.T.: -0.002 min
Response: 11984
Conc: 12.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-5A

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

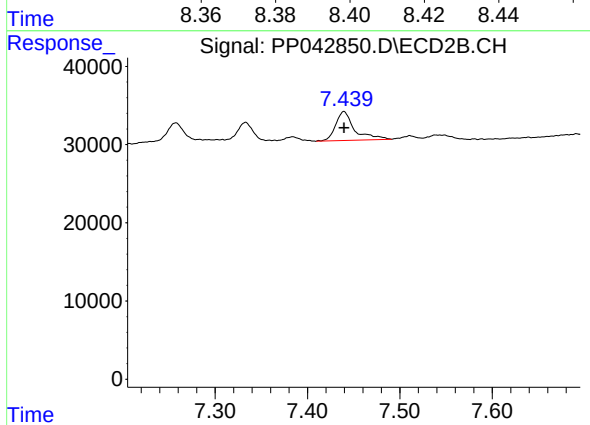

#30 AR-1254-5

R.T.: 7.439 min
Delta R.T.: 0.000 min
Response: 52737
Conc: 30.93 ng/ml