

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP011322\  
 Data File : PP042890.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 14 Jan 2022 00:48  
 Operator : AJ\MA  
 Sample : N1105-03 10X  
 Misc :  
 ALS Vial : 43 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 IRV-2022-21A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 14 00:52:59 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP011222.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Jan 13 19:45:07 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml |
|-----------------------------|--------|-------|--------|--------|-------|-------|
| -----                       |        |       |        |        |       |       |
| System Monitoring Compounds |        |       |        |        |       |       |
| 1) SA Tetrachlo...          | 4.873  | 4.044 | 39298  | 44095  | 1.661 | 1.765 |
| 2) SA Decachlor...          | 10.808 | 9.381 | 28087  | 29335  | 1.921 | 1.504 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP011322\  
Data File : PP042890.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 14 Jan 2022 00:48  
Operator : AJ\MA  
Sample : N1105-03 10X  
Misc :  
ALS Vial : 43 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
IRV-2022-21A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 14 00:52:59 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP011222.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Jan 13 19:45:07 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

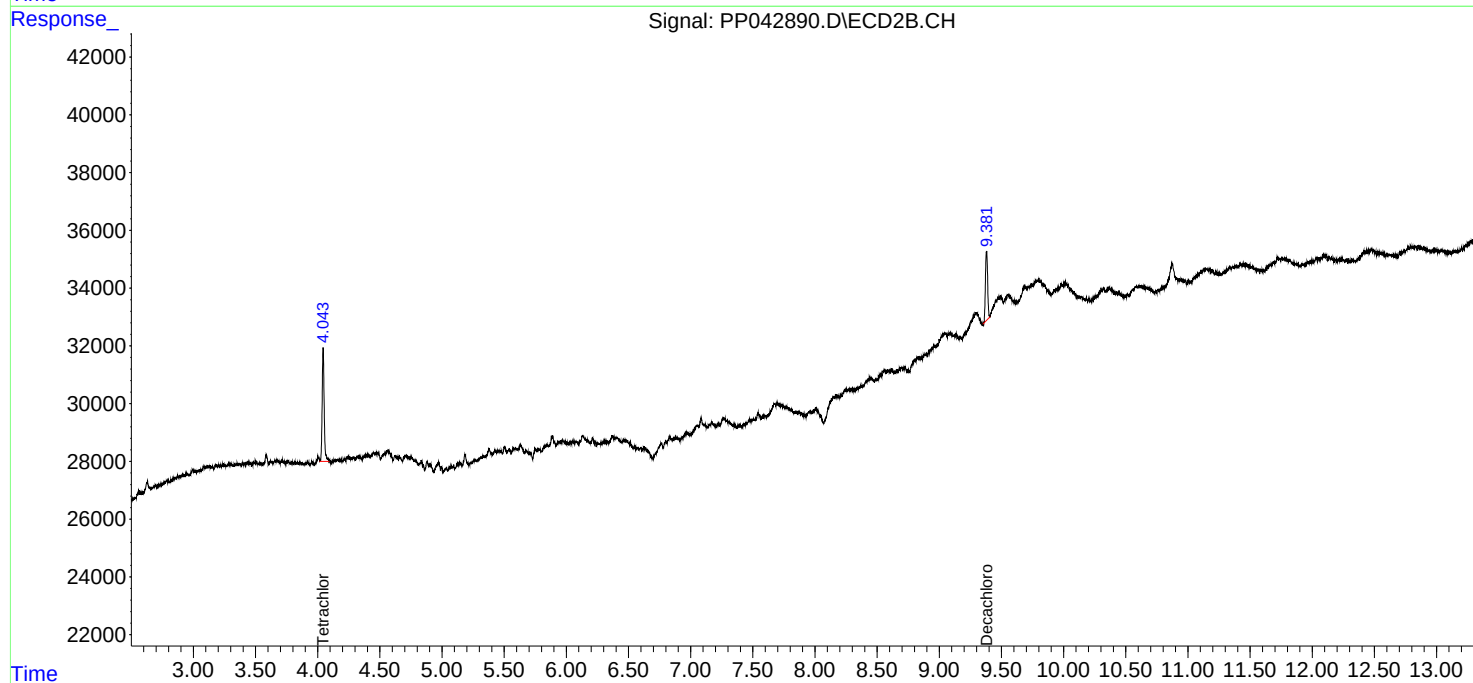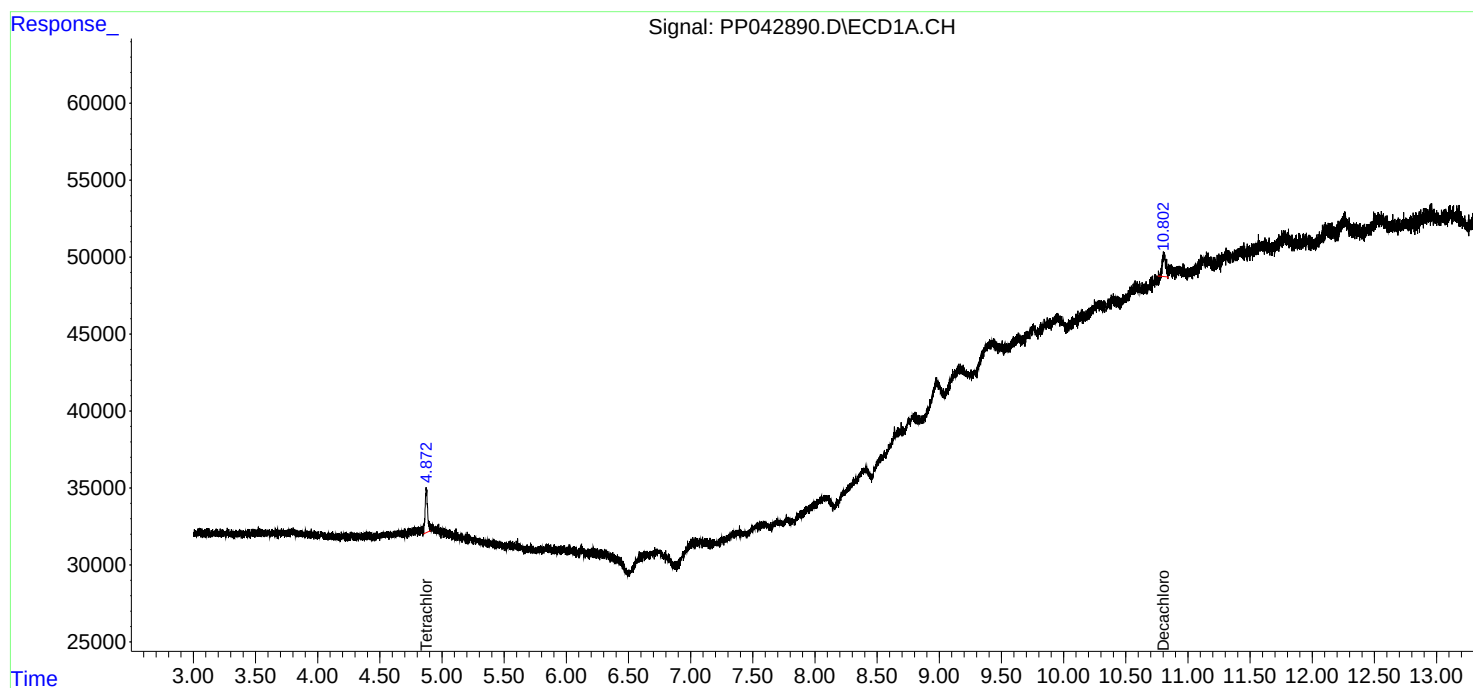


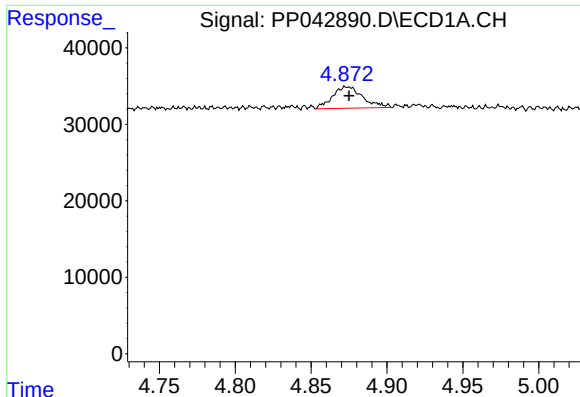

#1 Tetrachloro-m-xylene


R.T.: 4.873 min  
Delta R.T.: -0.002 min  
Response: 39298  
Conc: 1.66 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
IRV-2022-21A

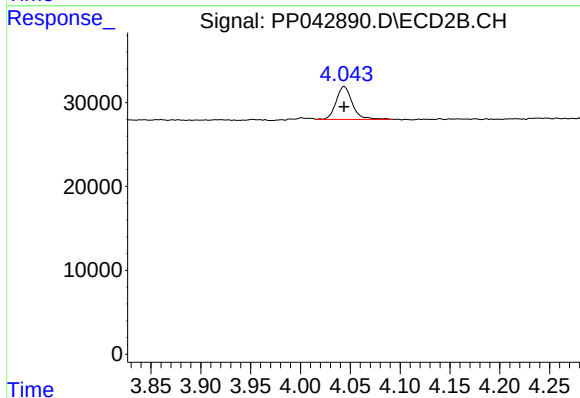


#1 Tetrachloro-m-xylene

R.T.: 4.044 min  
Delta R.T.: 0.000 min  
Response: 44095  
Conc: 1.77 ng/ml

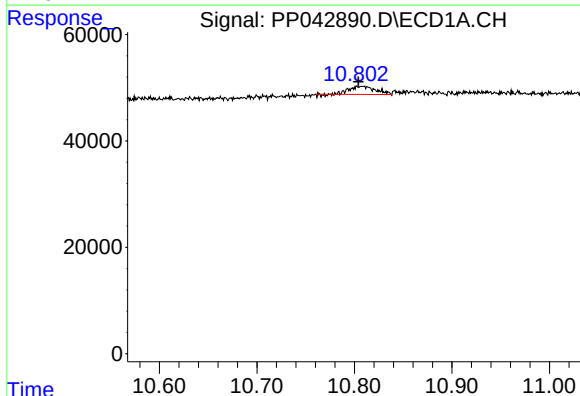

#2 Decachlorobiphenyl

R.T.: 10.808 min  
Delta R.T.: 0.004 min  
Response: 28087  
Conc: 1.92 ng/ml

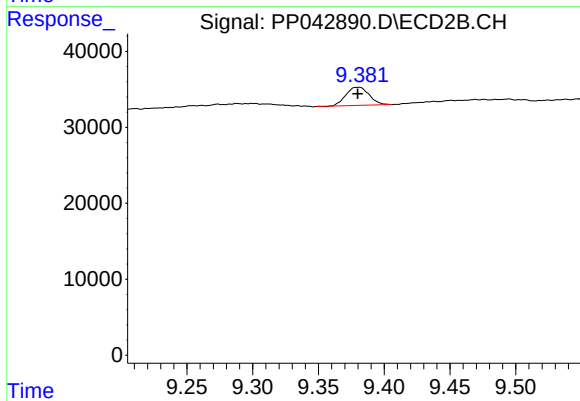

#2 Decachlorobiphenyl

R.T.: 9.381 min  
Delta R.T.: 0.001 min  
Response: 29335  
Conc: 1.50 ng/ml