

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
 Data File : PP042894.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 2:22
 Operator : AJ\MA
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
 Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 02:19:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.874	4.044	1226971	1323380	51.856	52.986
2)	SA Decachlor...	10.806	9.380	779414	1001037	53.317	51.318
Target Compounds							
26)	L6 AR-1254-1	7.083	6.186	357295	777578	455.345	501.434
27)	L6 AR-1254-2	7.311	6.345	592037	679921	470.397m	500.843
28)	L6 AR-1254-3	7.690	6.770	624316	1054349	481.205m	492.931
29)	L6 AR-1254-4	7.983	7.009	455479	638244	521.125	511.579
30)	L6 AR-1254-5	8.412	7.441	452816	835377	483.305	489.908

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
Data File : PP042894.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 2:22
Operator : AJ\MA
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 02:19:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

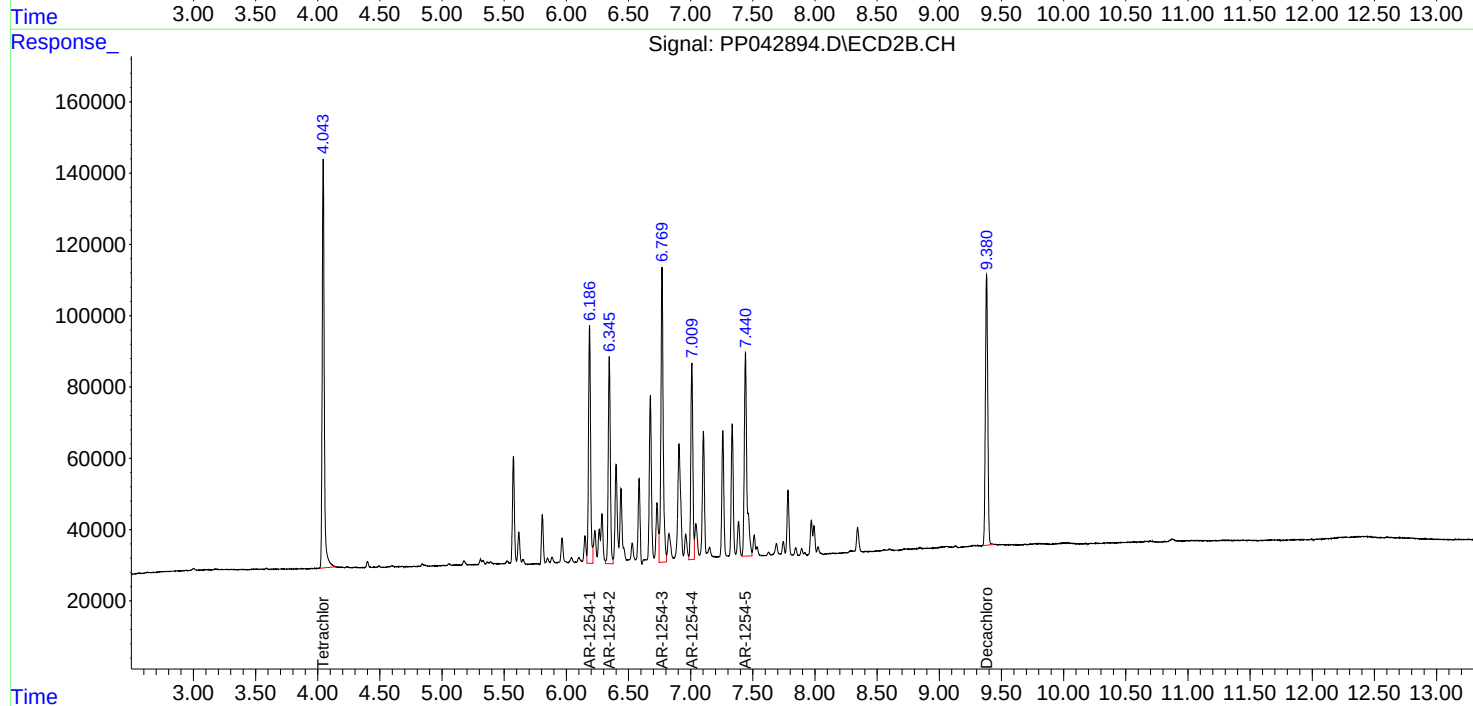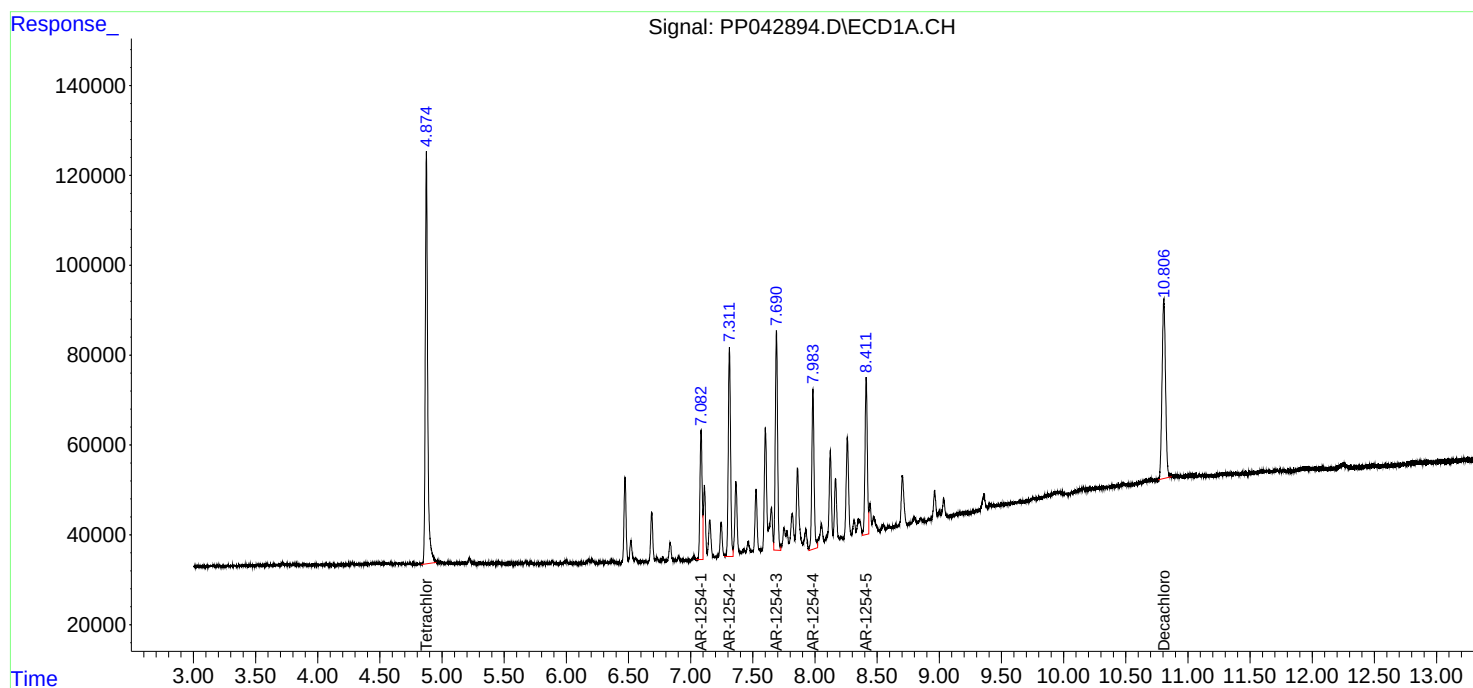

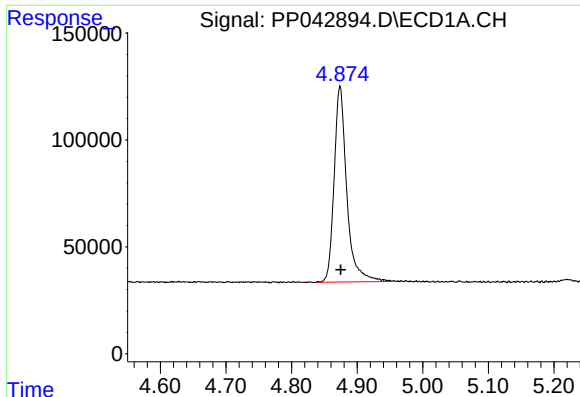


#1 Tetrachloro-m-xylene

R.T.: 4.874 min
Delta R.T.: -0.001 min
Response: 1226971
Conc: 51.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

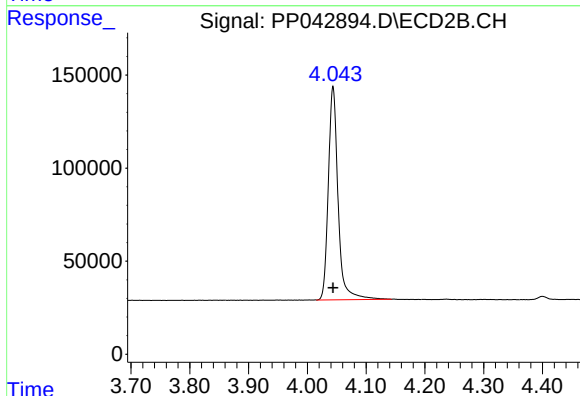


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 1323380
Conc: 52.99 ng/ml

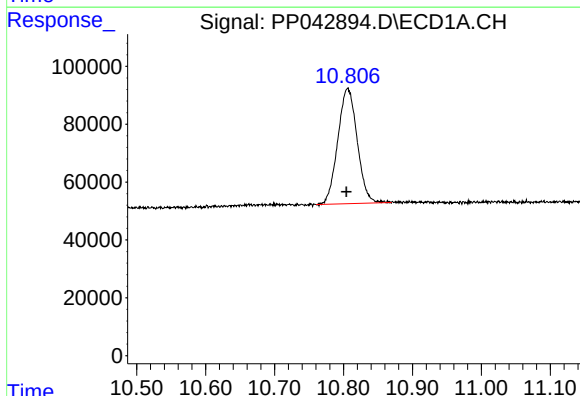


#2 Decachlorobiphenyl

R.T.: 10.806 min
Delta R.T.: 0.002 min
Response: 779414
Conc: 53.32 ng/ml

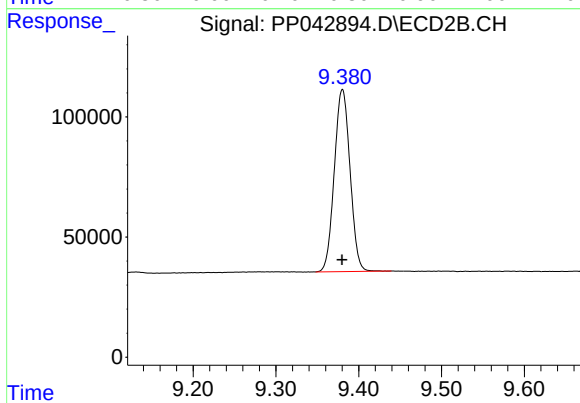

#2 Decachlorobiphenyl

R.T.: 9.380 min
Delta R.T.: 0.000 min
Response: 1001037
Conc: 51.32 ng/ml

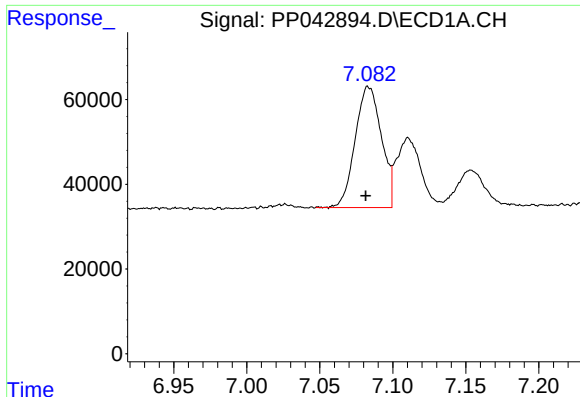


#26 AR-1254-1

R.T.: 7.083 min
Delta R.T.: 0.001 min
Response: 357295
Conc: 455.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

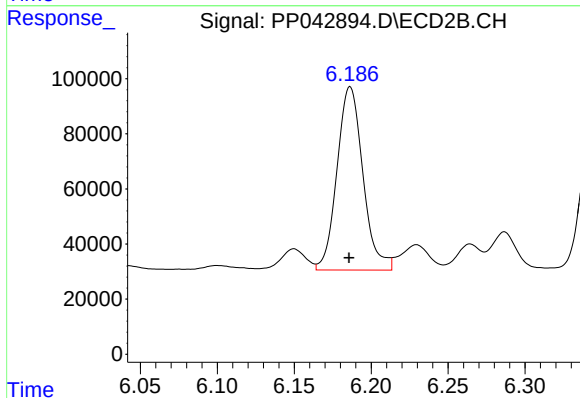


#26 AR-1254-1

R.T.: 6.186 min
Delta R.T.: 0.000 min
Response: 777578
Conc: 501.43 ng/ml

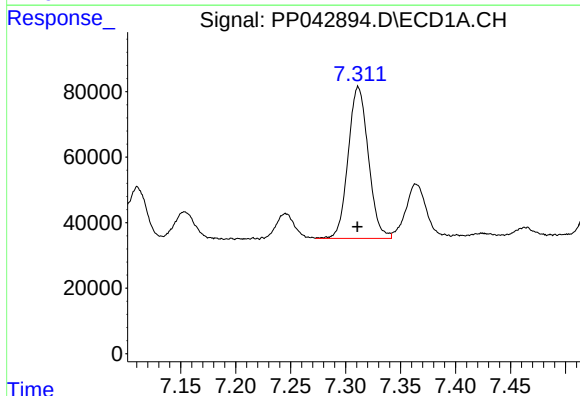


#27 AR-1254-2

R.T.: 7.311 min
Delta R.T.: 0.000 min
Response: 592037
Conc: 470.40 ng/ml m

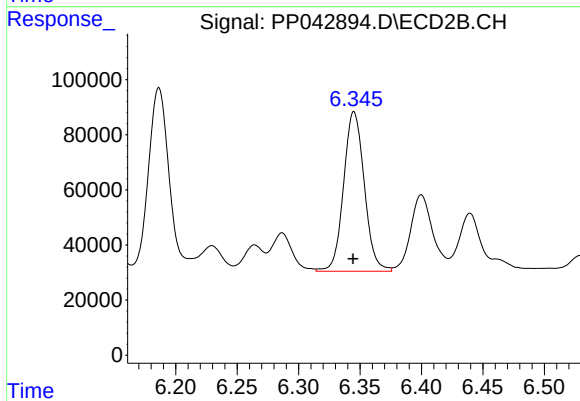

#27 AR-1254-2

R.T.: 6.345 min
Delta R.T.: 0.000 min
Response: 679921
Conc: 500.84 ng/ml

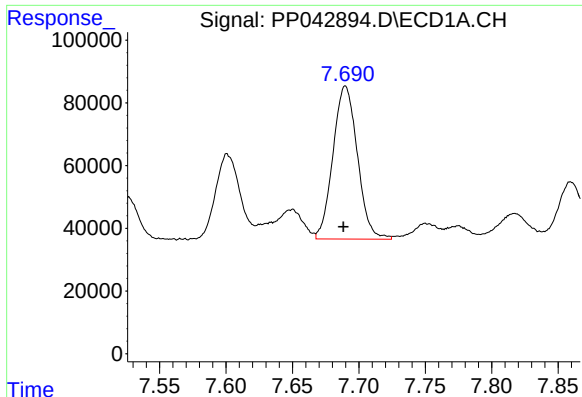


#28 AR-1254-3

R.T.: 7.690 min
Delta R.T.: 0.001 min
Response: 624316
Conc: 481.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

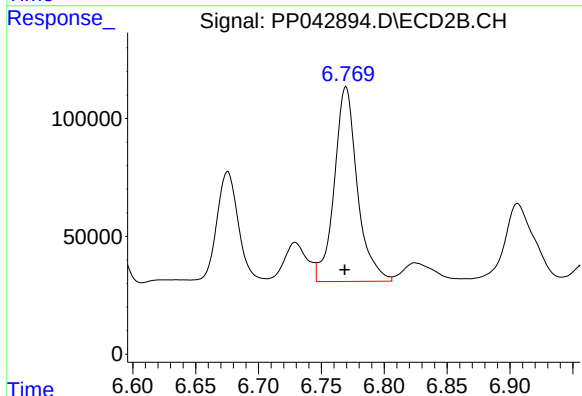


#28 AR-1254-3

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 1054349
Conc: 492.93 ng/ml

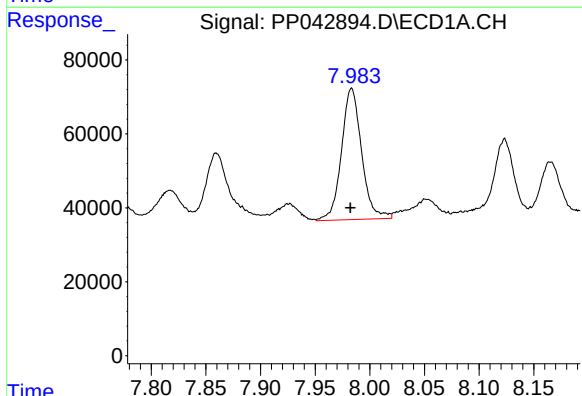


#29 AR-1254-4

R.T.: 7.983 min
Delta R.T.: 0.001 min
Response: 455479
Conc: 521.12 ng/ml

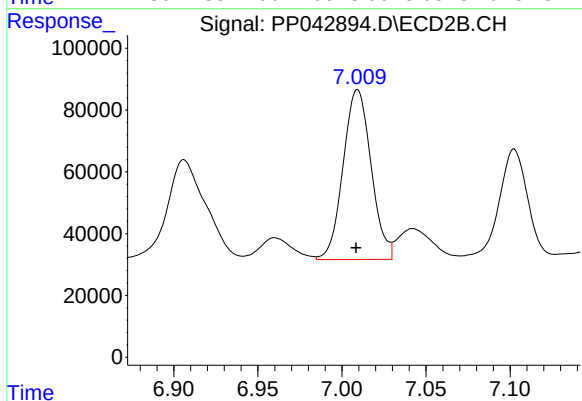

#29 AR-1254-4

R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 638244
Conc: 511.58 ng/ml

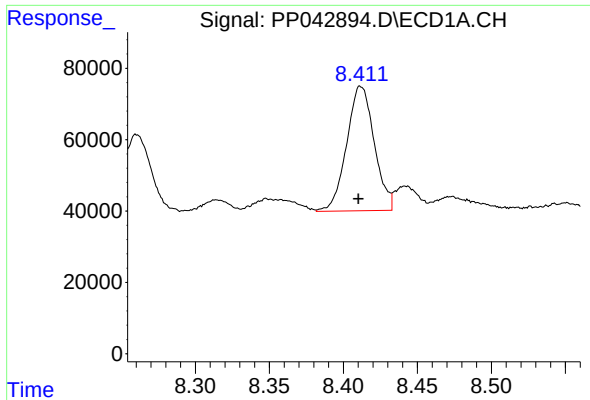


#30 AR-1254-5

R.T.: 8.412 min
Delta R.T.: 0.002 min
Response: 452816
Conc: 483.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/14/2022
Supervised By :mohammad ahmed 01/14/2022

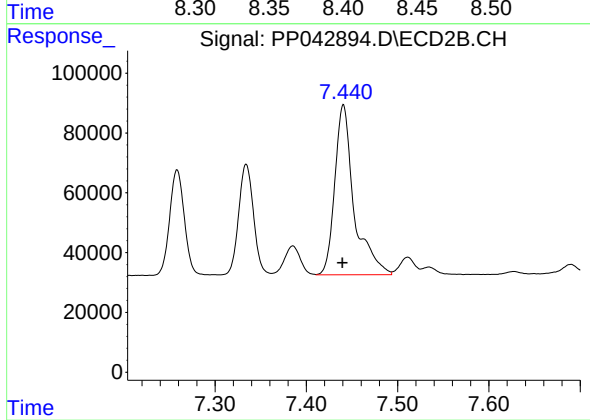

#30 AR-1254-5

R.T.: 7.441 min
Delta R.T.: 0.000 min
Response: 835377
Conc: 489.91 ng/ml