

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP011322\  
 Data File : PP042904.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 14 Jan 2022 5:07  
 Operator : AJ\MA  
 Sample : N1105-15 10X  
 Misc :  
 ALS Vial : 54 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 IRV-2022-33A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 14 08:52:42 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP011222.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Jan 13 19:45:07 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml   |
|-----------------------------|--------|-------|--------|--------|-------|---------|
| -----                       |        |       |        |        |       |         |
| System Monitoring Compounds |        |       |        |        |       |         |
| 1) SA Tetrachlo...          | 4.874  | 4.044 | 43161  | 44764  | 1.824 | 1.792   |
| 2) SA Decachlor...          | 10.812 | 9.383 | 33305  | 30902  | 2.278 | 1.584 # |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP011322\  
Data File : PP042904.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 14 Jan 2022 5:07  
Operator : AJ\MA  
Sample : N1105-15 10X  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
IRV-2022-33A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 14 08:52:42 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP011222.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Jan 13 19:45:07 2022  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

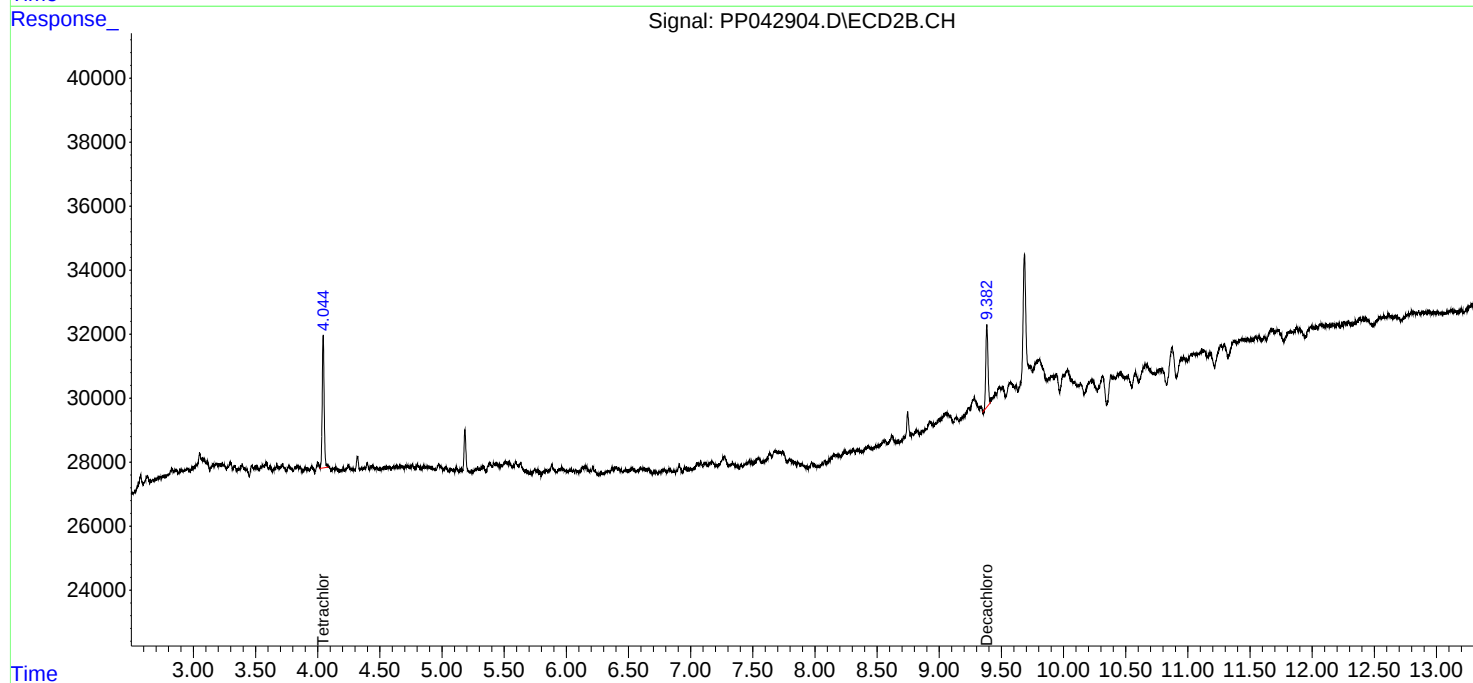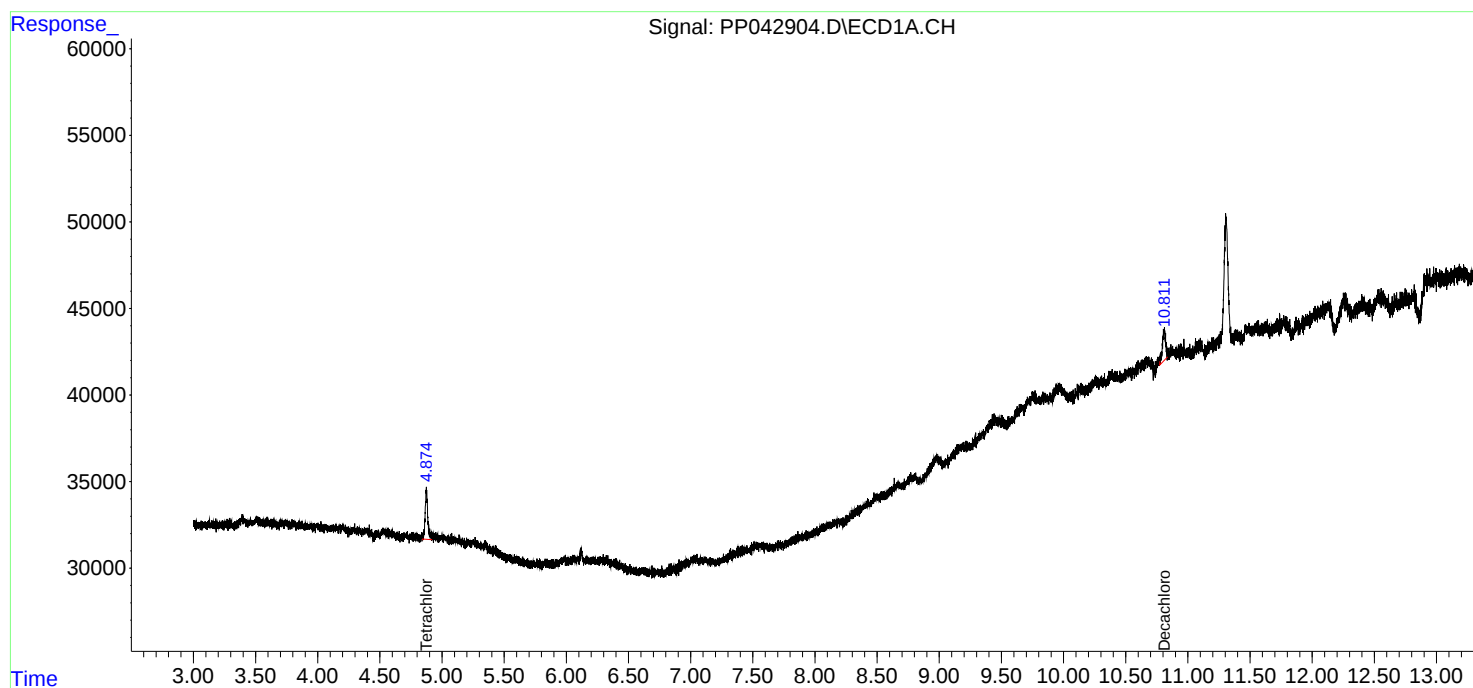


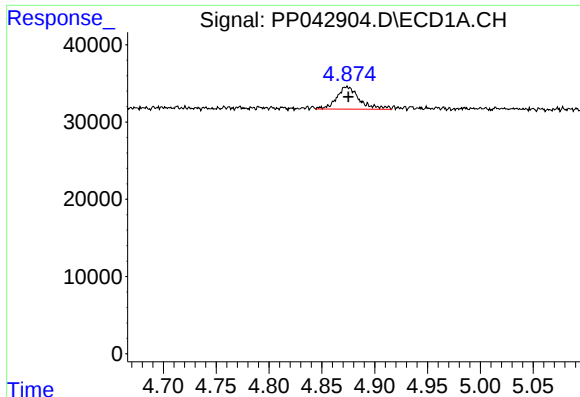

#1 Tetrachloro-m-xylene


R.T.: 4.874 min  
Delta R.T.: -0.001 min  
Response: 43161  
Conc: 1.82 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
IRV-2022-33A

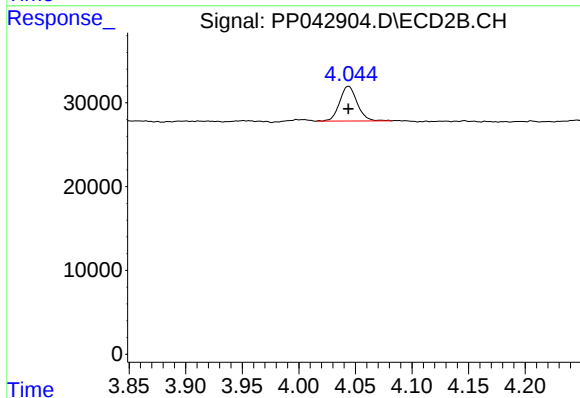


#1 Tetrachloro-m-xylene

R.T.: 4.044 min  
Delta R.T.: 0.000 min  
Response: 44764  
Conc: 1.79 ng/ml

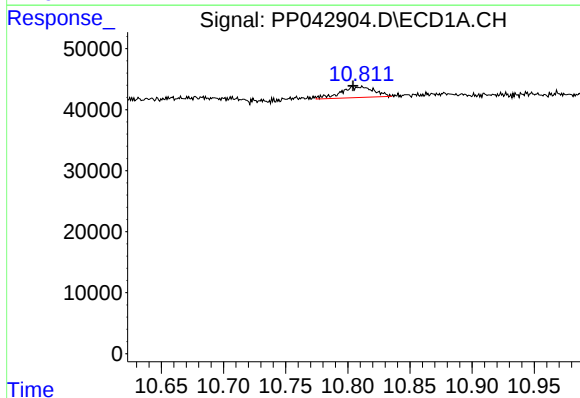

#2 Decachlorobiphenyl

R.T.: 10.812 min  
Delta R.T.: 0.007 min  
Response: 33305  
Conc: 2.28 ng/ml

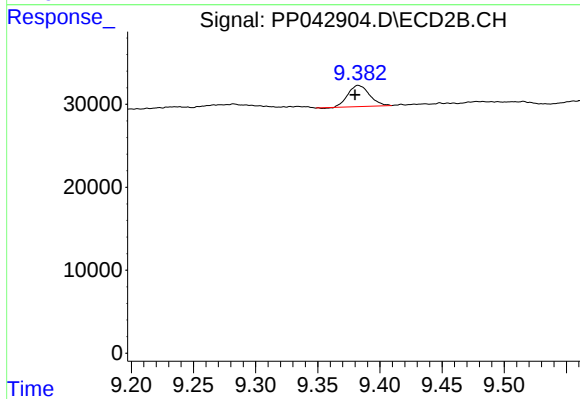

#2 Decachlorobiphenyl

R.T.: 9.383 min  
Delta R.T.: 0.003 min  
Response: 30902  
Conc: 1.58 ng/ml