

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
 Data File : PP042917.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 9:38
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 09:34:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.873	4.044	521305	588324	22.032	23.555
2)	SA Decachlor...	10.804	9.379	344091	461021	23.538	23.634
Target Compounds							
9)	L2 AR-1221-2	5.221	0.000	7942	0	39.300	N.D. #
20)	L4 AR-1242-5	0.000	6.211f	0	63348	N.D.	88.036 #
25)	L5 AR-1248-5	0.000	6.211f	0	63348	N.D.	66.354 #
26)	L6 AR-1254-1	0.000	6.211f	0	63348	N.D.	40.851 #
28)	L6 AR-1254-3	7.688	0.000	24224	0	18.671	N.D. #
29)	L6 AR-1254-4	7.980	0.000	7531	0	8.617	N.D. #
32)	L7 AR-1260-2	0.000	7.083f	0	35926	N.D.	23.001 #
38)	L8 AR-1262-3	0.000	8.300f	0	4884	N.D.	4.377 #
41)	L9 AR-1268-1	0.000	8.300f	0	4884	N.D.	1.584 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011322\
Data File : PP042917.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 9:38
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 09:34:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

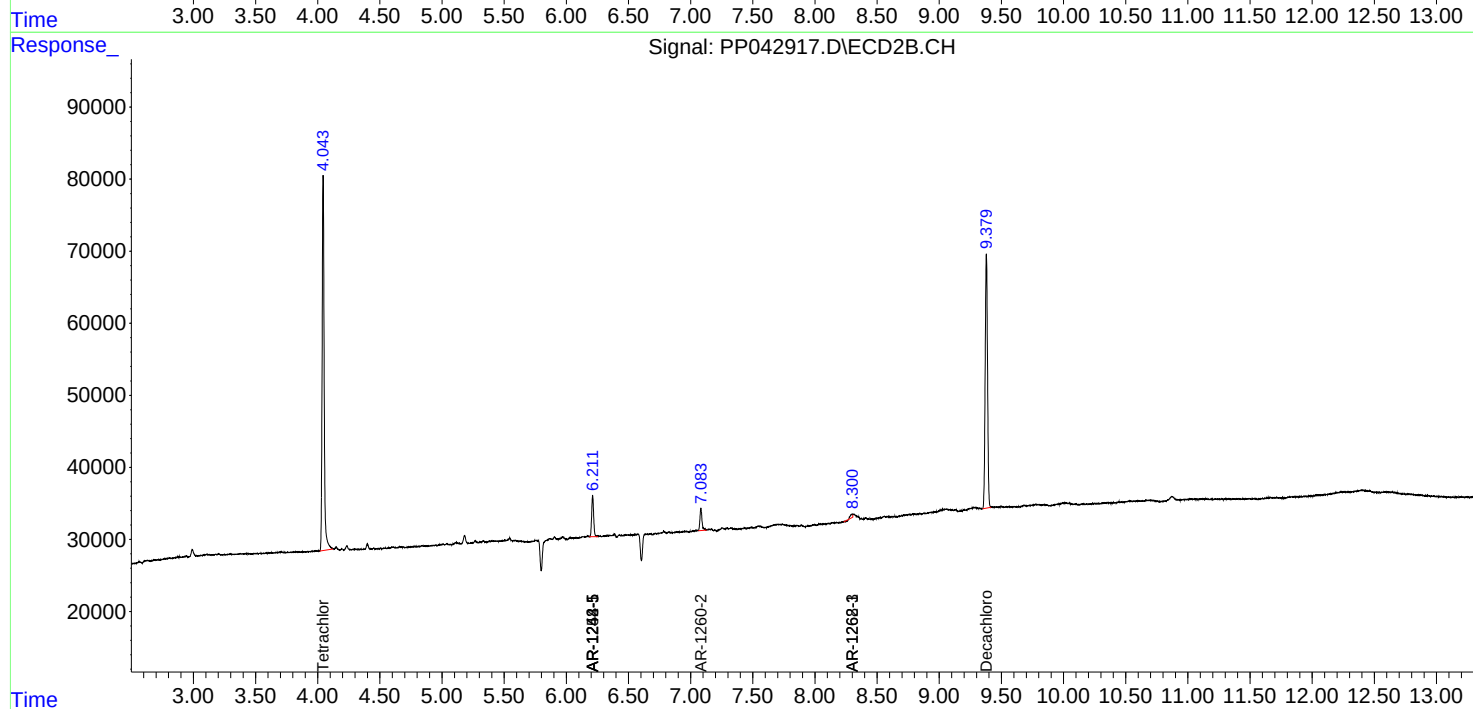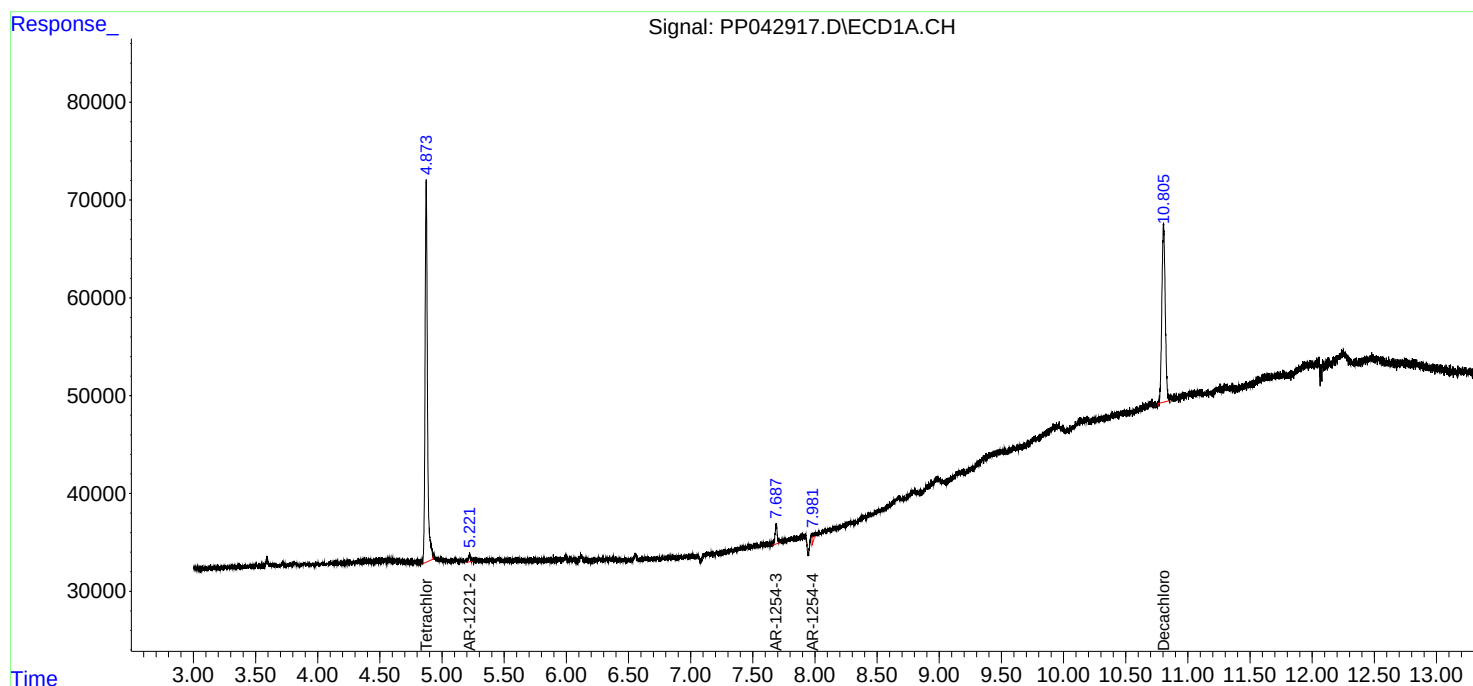


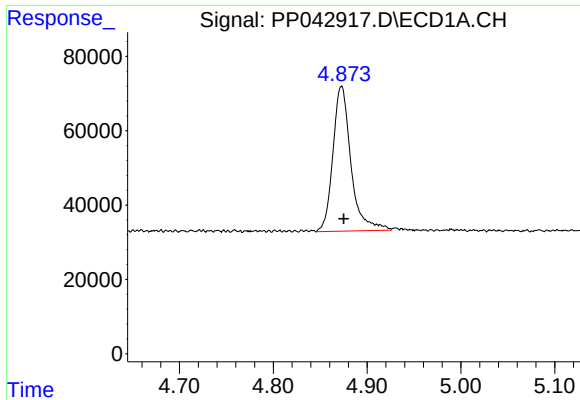

#1 Tetrachloro-m-xylene


R.T.: 4.873 min
Delta R.T.: -0.002 min
Response: 521305
Conc: 22.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

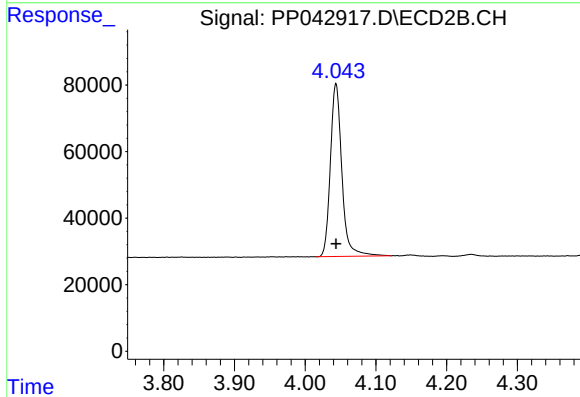


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 588324
Conc: 23.56 ng/ml

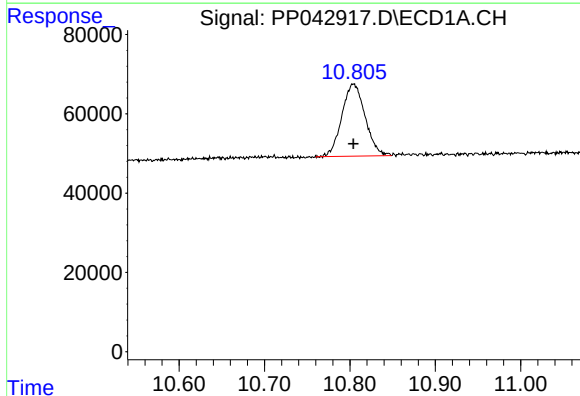


#2 Decachlorobiphenyl

R.T.: 10.804 min
Delta R.T.: 0.000 min
Response: 344091
Conc: 23.54 ng/ml

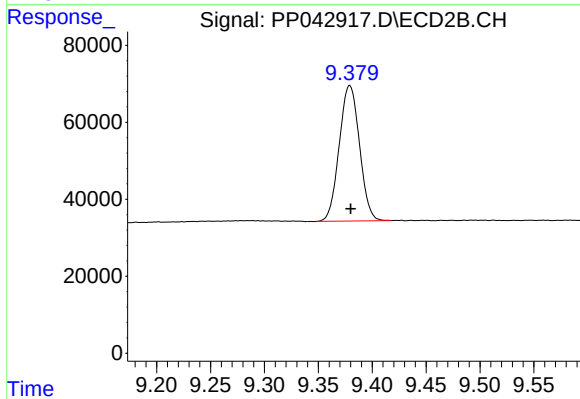

#2 Decachlorobiphenyl


R.T.: 9.379 min
Delta R.T.: 0.000 min
Response: 461021
Conc: 23.63 ng/ml

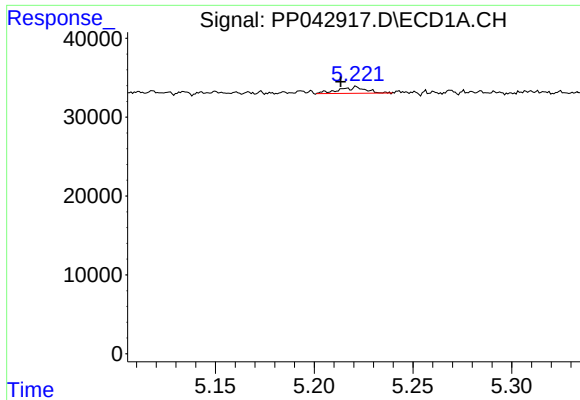

#9 AR-1221-2


R.T.: 5.221 min
Delta R.T.: 0.008 min
Response: 7942
Conc: 39.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

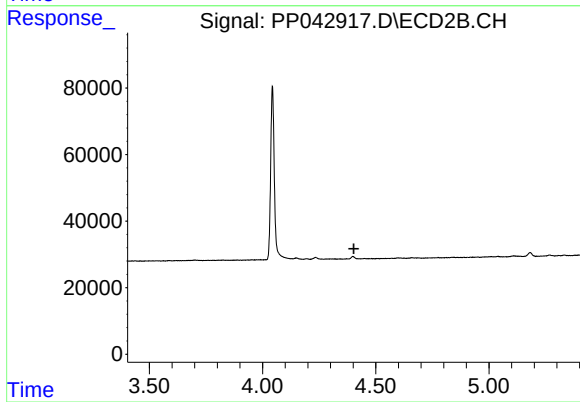


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.403 min
Response: 0
Conc: N.D.

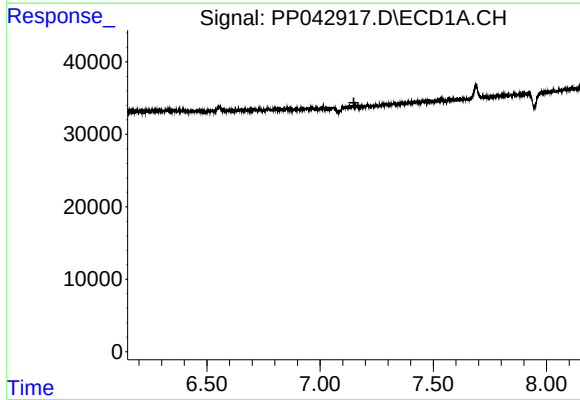


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

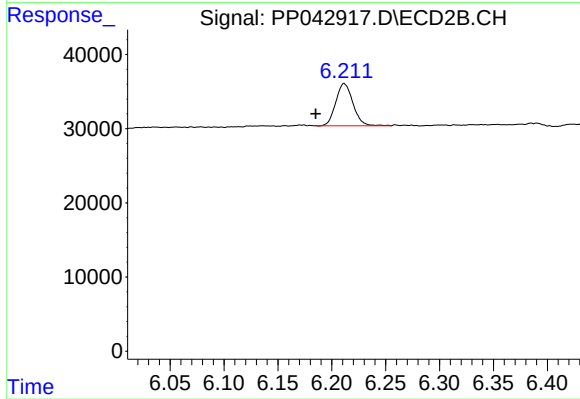

#20 AR-1242-5


R.T.: 6.211 min
Delta R.T.: 0.026 min
Response: 63348
Conc: 88.04 ng/ml

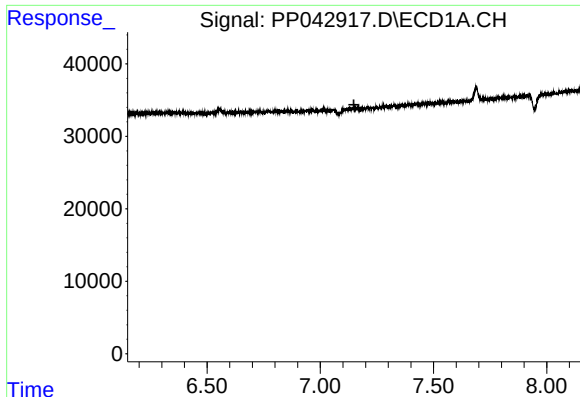

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

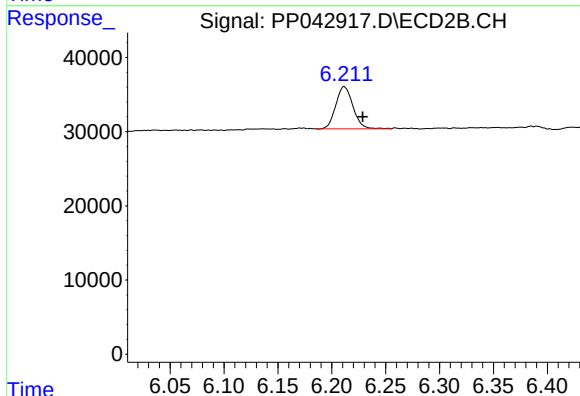


#25 AR-1248-5

R.T.: 6.211 min
Delta R.T.: -0.017 min
Response: 63348
Conc: 66.35 ng/ml

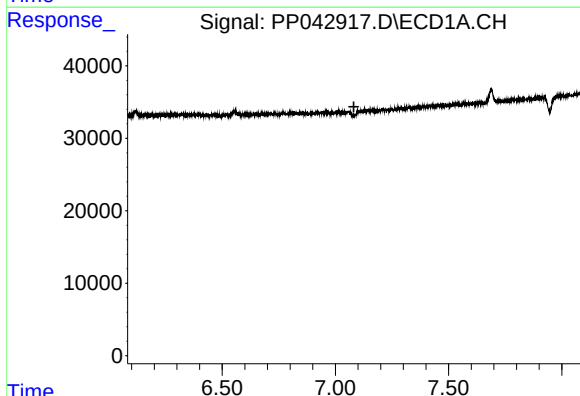


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.082 min
Response: 0
Conc: N.D.

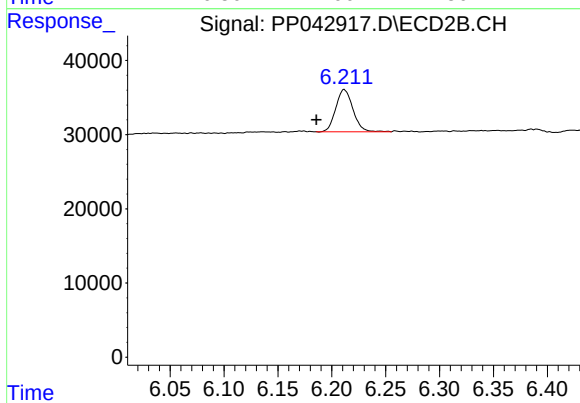

#26 AR-1254-1


R.T.: 6.211 min
Delta R.T.: 0.026 min
Response: 63348
Conc: 40.85 ng/ml

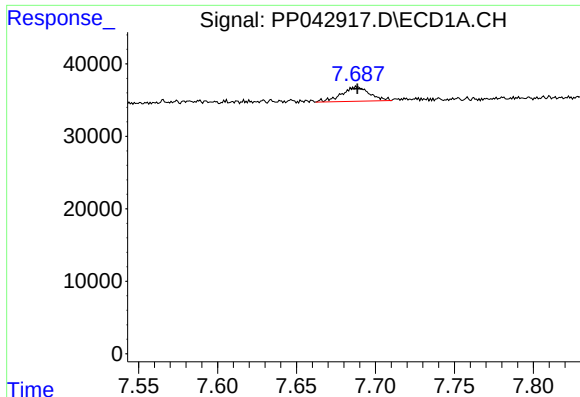

#28 AR-1254-3


R.T.: 7.688 min
Delta R.T.: 0.000 min
Response: 24224
Conc: 18.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

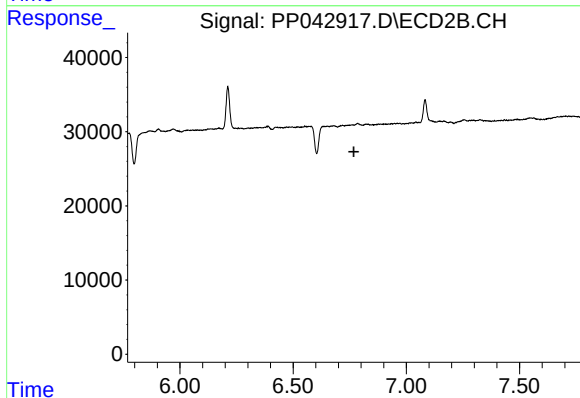


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

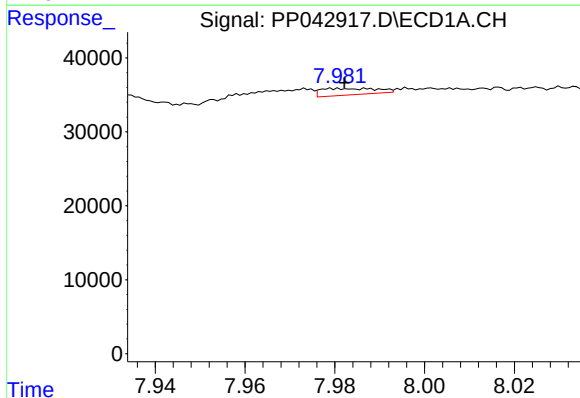


#29 AR-1254-4

R.T.: 7.980 min
Delta R.T.: -0.002 min
Response: 7531
Conc: 8.62 ng/ml

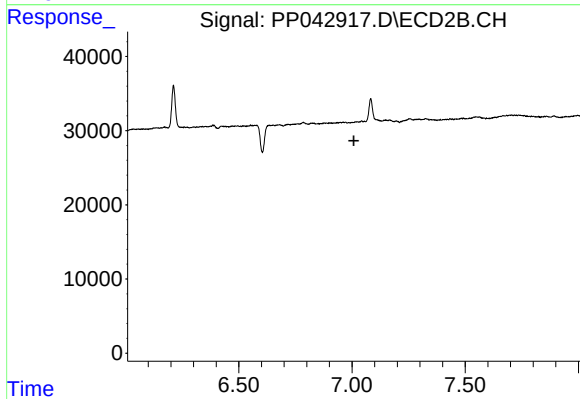

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

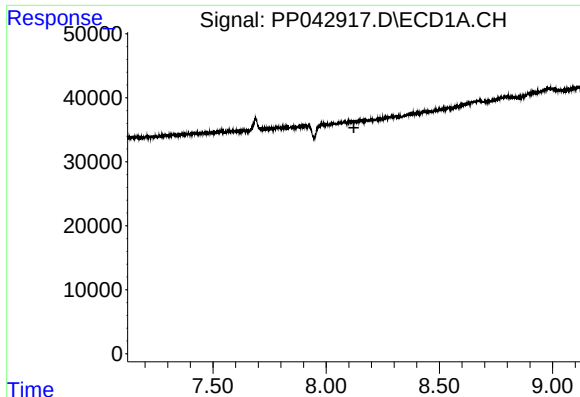

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

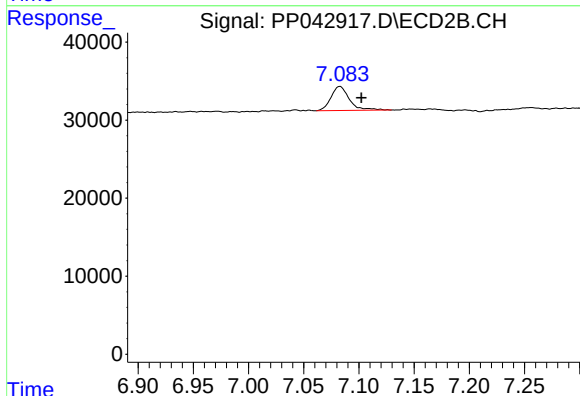


#32 AR-1260-2

R.T.: 7.083 min
Delta R.T.: -0.019 min
Response: 35926
Conc: 23.00 ng/ml

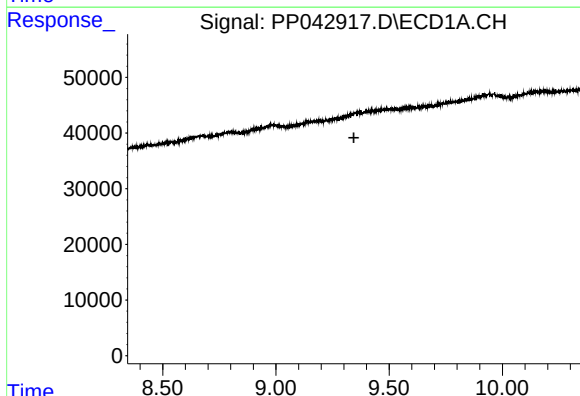


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.344 min
Response: 0
Conc: N.D.

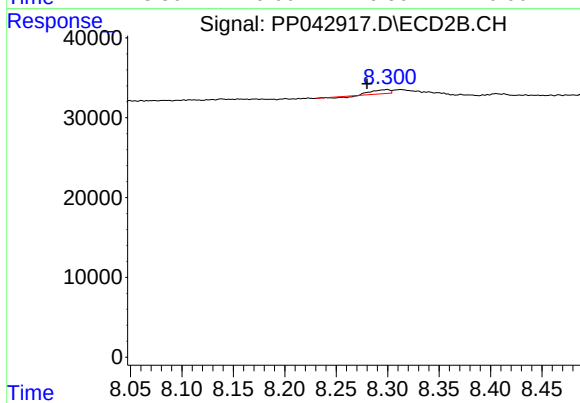

#38 AR-1262-3


R.T.: 8.300 min
Delta R.T.: 0.020 min
Response: 4884
Conc: 4.38 ng/ml

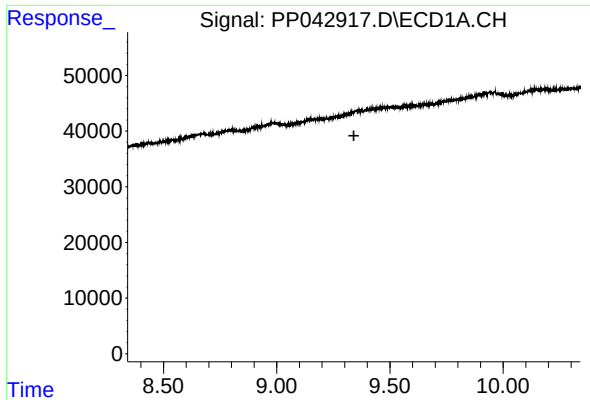

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

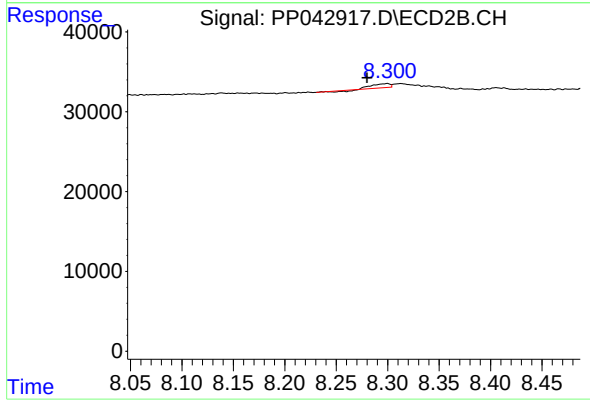

#41 AR-1268-1

R.T.: 8.300 min
Delta R.T.: 0.020 min
Response: 4884
Conc: 1.58 ng/ml