

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011325\
 Data File : PP069077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2025 11:55
 Operator : YP\AJ
 Sample : Q1064-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-25-0003

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/14/2025
 Supervised By :Ankita Jodhani 01/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 12:07:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.672	3.985	13507593	10117409	9.709	10.364
2) SA Decachlor...	10.518	9.104	12331850	16995787	11.045	14.148m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011325\
Data File : PP069077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2025 11:55
Operator : YP\AJ
Sample : Q1064-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LAW-25-0003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/14/2025
Supervised By :Ankita Jodhani 01/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 12:07:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

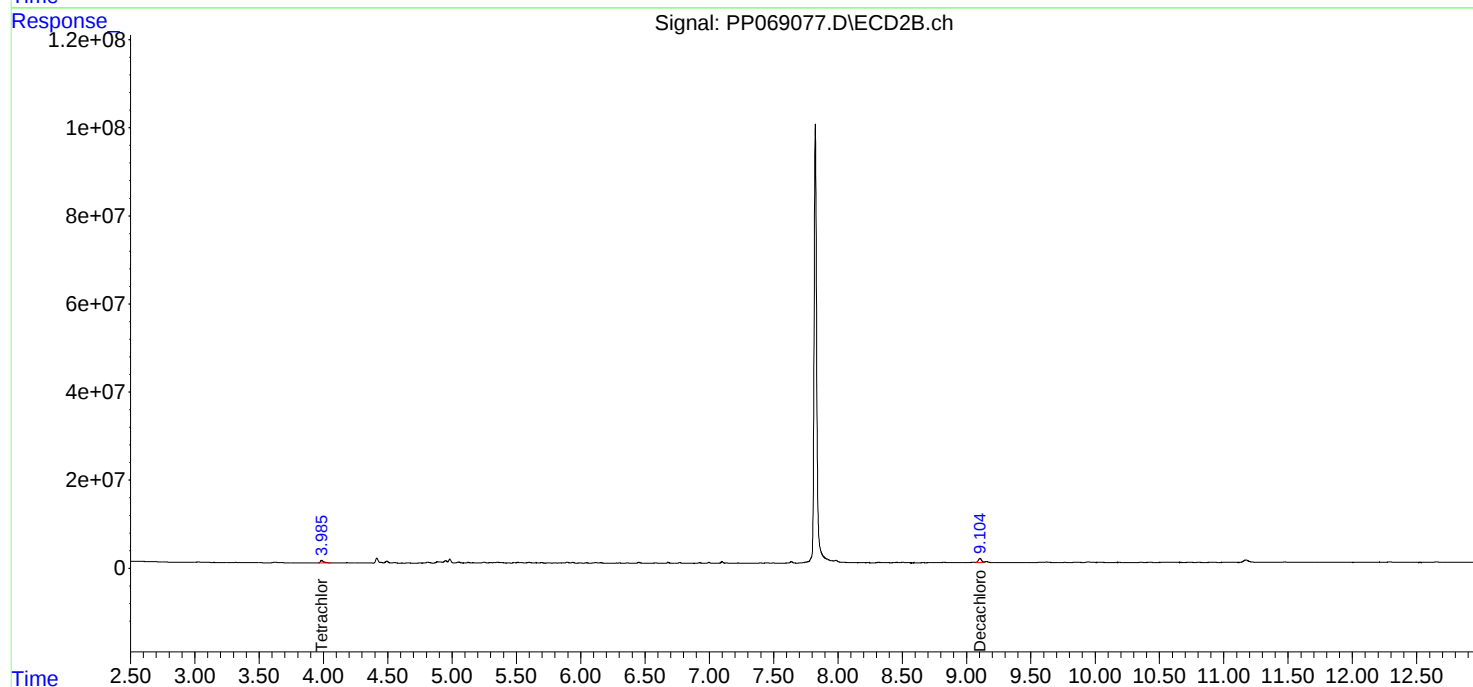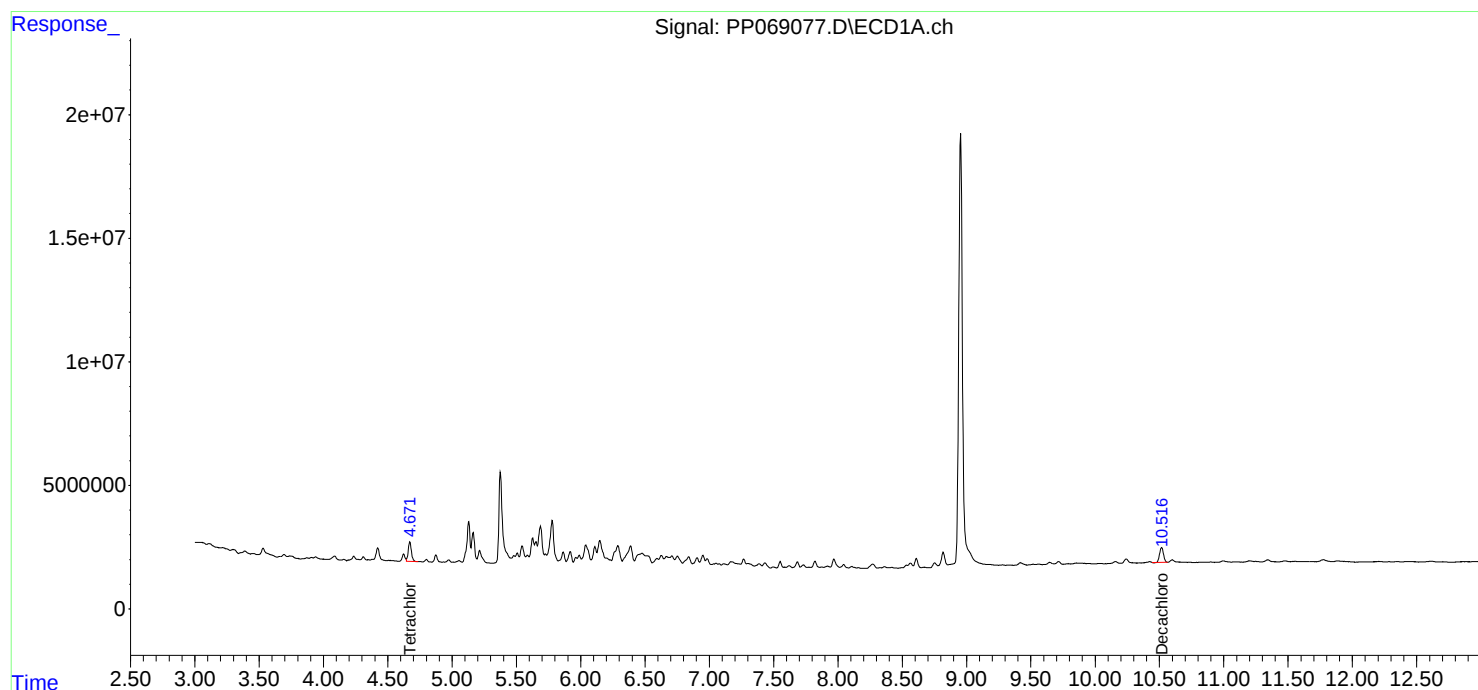

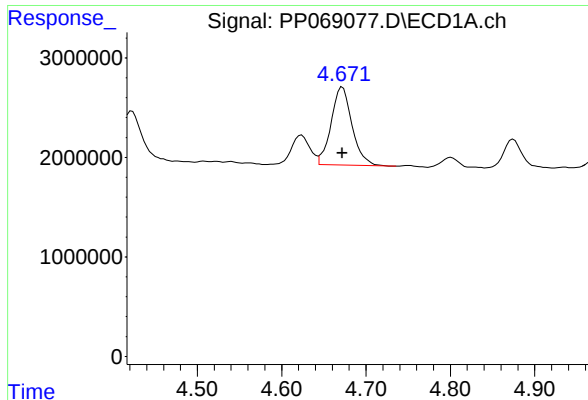


#1 Tetrachloro-m-xylene

R.T.: 4.672 min
Delta R.T.: 0.000 min
Response: 13507593
Conc: 9.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LAW-25-0003


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/14/2025
Supervised By :Ankita Jodhani 01/14/2025

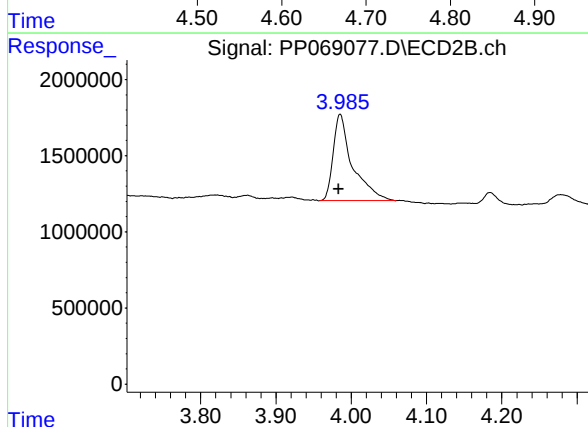


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.002 min
Response: 10117409
Conc: 10.36 ng/ml

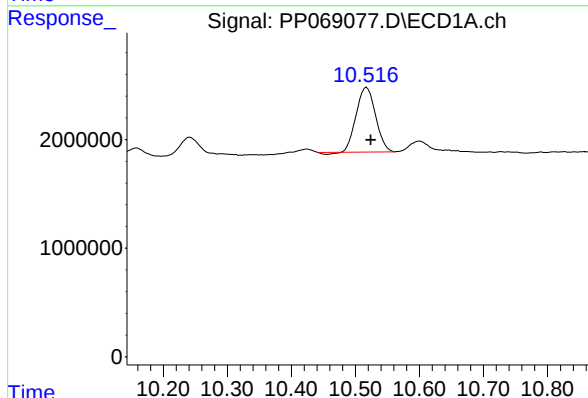

#2 Decachlorobiphenyl

R.T.: 10.518 min
Delta R.T.: -0.007 min
Response: 12331850
Conc: 11.05 ng/ml

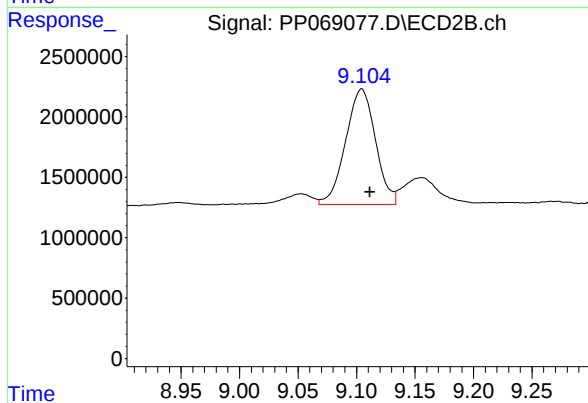

#2 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: -0.007 min
Response: 16995787
Conc: 14.15 ng/ml m