

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011421\
 Data File : PP032708.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 20:38
 Operator : DD\AJ
 Sample : M1113-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 S11-01-B

Manual Integrations
 APPROVED

Ankita
 1/14/2021 4:38:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 11:42:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.741	4.011	1083554	846081	18.656	17.986
2) SA Decachlor...	10.576	9.294	1198788	1127810	30.385	30.105
Target Compounds						
41) L9 AR-1268-1	9.183	8.211	3226242	2751354	487.322	487.953
42) L9 AR-1268-2	9.273	8.276	1987196	1833004	329.883	338.123
43) L9 AR-1268-3	9.483	8.480	2780011	2457377	519.342	517.544
44) L9 AR-1268-4	9.888	8.773	469014	436968	228.693	241.596
45) L9 AR-1268-5	10.268	9.053	7006413	6754531	463.499	466.530

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011421\
Data File : PP032708.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 20:38
Operator : DD\AJ
Sample : M1113-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
S11-01-B


Manual Integrations
APPROVED

Ankita
1/14/2021 4:38:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 11:42:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

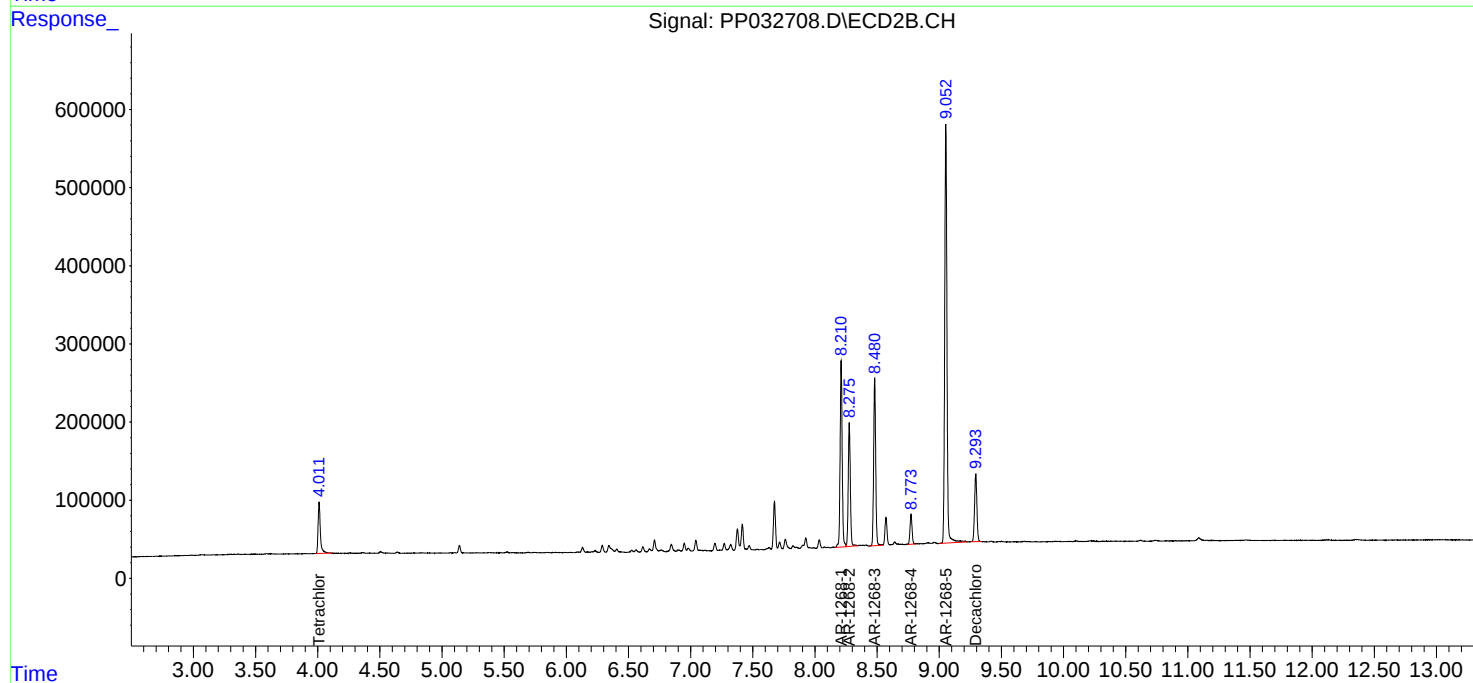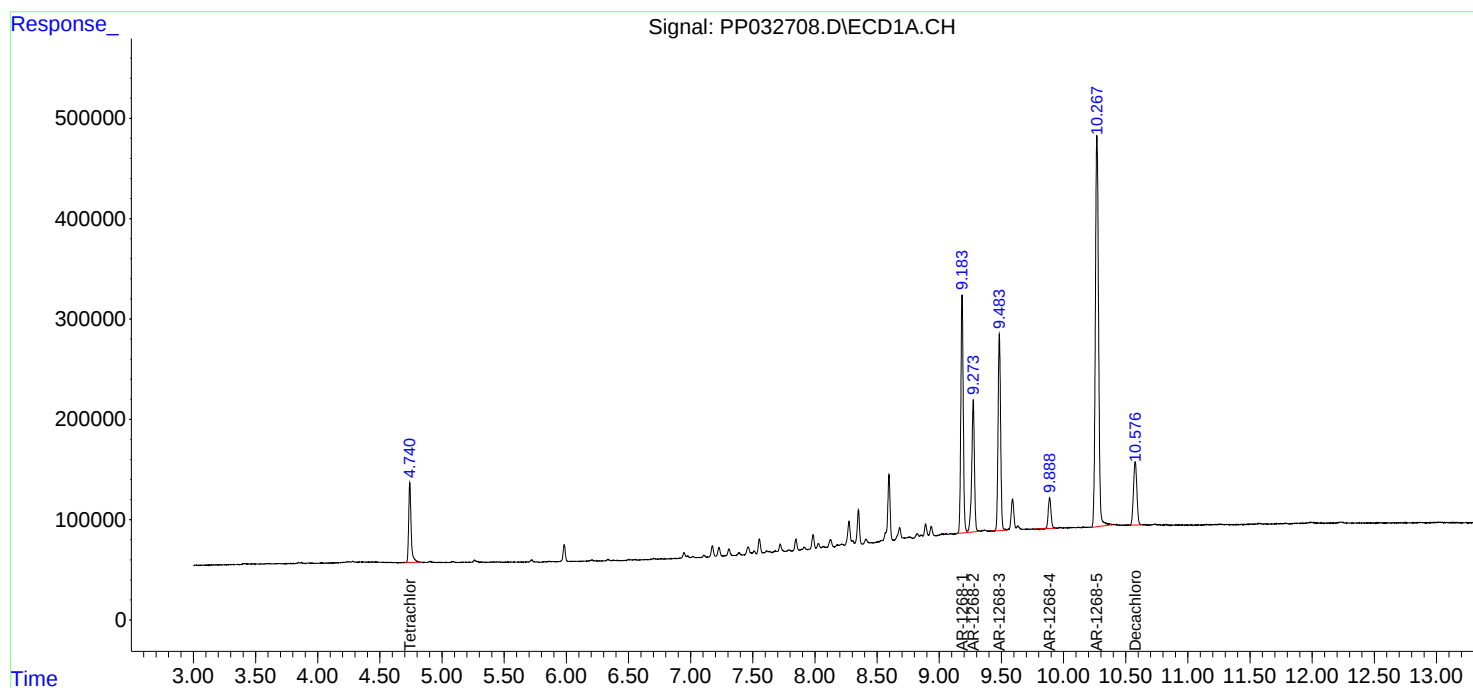

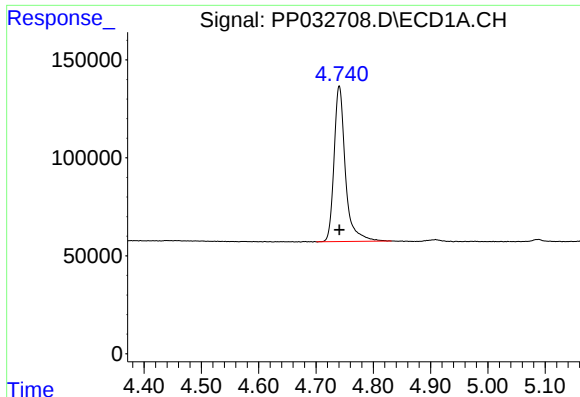


#1 Tetrachloro-m-xylene

R.T.: 4.741 min
Delta R.T.: 0.000 min
Response: 1083554
Conc: 18.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
S11-01-B


Manual Integrations
APPROVED

Ankita
1/14/2021 4:38:53 PM

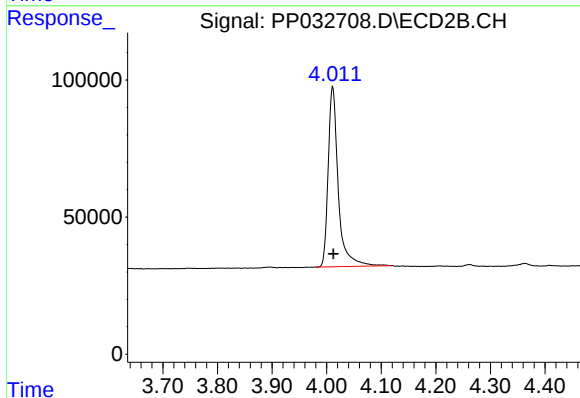


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.002 min
Response: 846081
Conc: 17.99 ng/ml

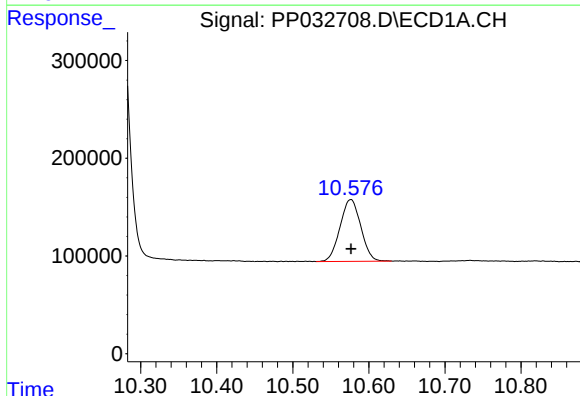


#2 Decachlorobiphenyl

R.T.: 10.576 min
Delta R.T.: 0.000 min
Response: 1198788
Conc: 30.38 ng/ml

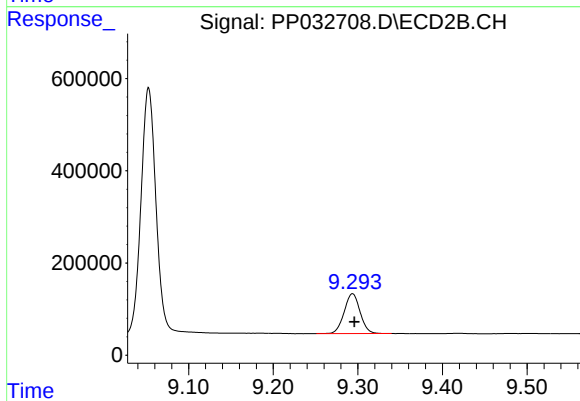

#2 Decachlorobiphenyl

R.T.: 9.294 min
Delta R.T.: -0.002 min
Response: 1127810
Conc: 30.11 ng/ml

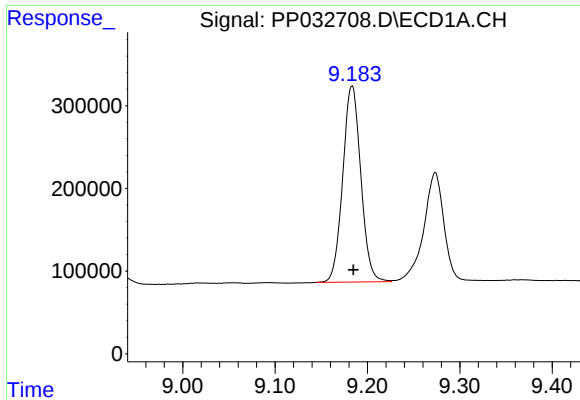


#41 AR-1268-1

R.T.: 9.183 min
Delta R.T.: -0.001 min
Response: 3226242
Conc: 487.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
S11-01-B


Manual Integrations
APPROVED

Ankita
1/14/2021 4:38:53 PM

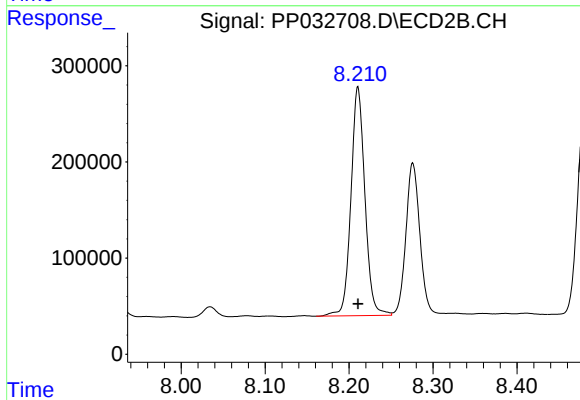


#41 AR-1268-1

R.T.: 8.211 min
Delta R.T.: 0.000 min
Response: 2751354
Conc: 487.95 ng/ml

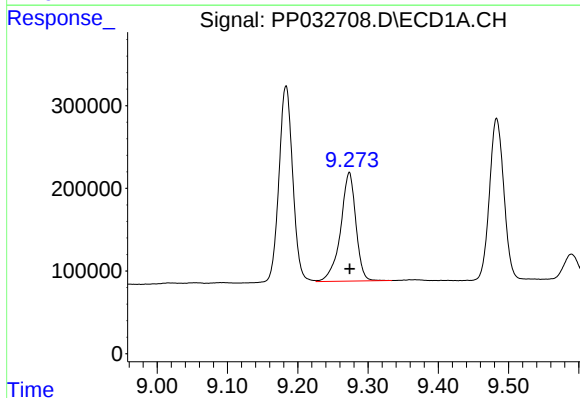


#42 AR-1268-2

R.T.: 9.273 min
Delta R.T.: 0.000 min
Response: 1987196
Conc: 329.88 ng/ml

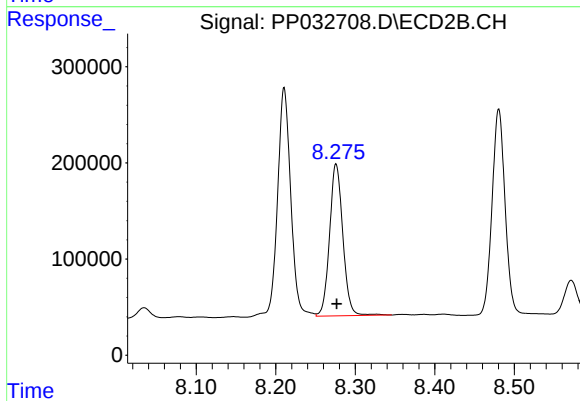

#42 AR-1268-2

R.T.: 8.276 min
Delta R.T.: 0.000 min
Response: 1833004
Conc: 338.12 ng/ml

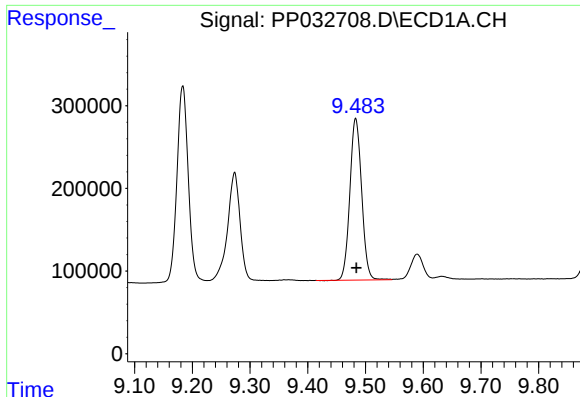


#43 AR-1268-3

R.T.: 9.483 min
Delta R.T.: -0.001 min
Response: 2780011
Conc: 519.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
S11-01-B


Manual Integrations
APPROVED

Ankita
1/14/2021 4:38:53 PM

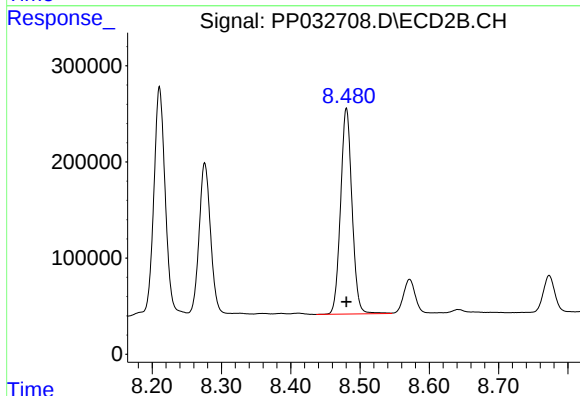


#43 AR-1268-3

R.T.: 8.480 min
Delta R.T.: 0.000 min
Response: 2457377
Conc: 517.54 ng/ml

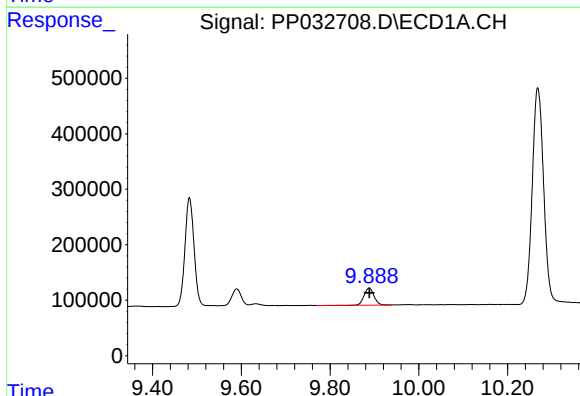


#44 AR-1268-4

R.T.: 9.888 min
Delta R.T.: -0.001 min
Response: 469014
Conc: 228.69 ng/ml

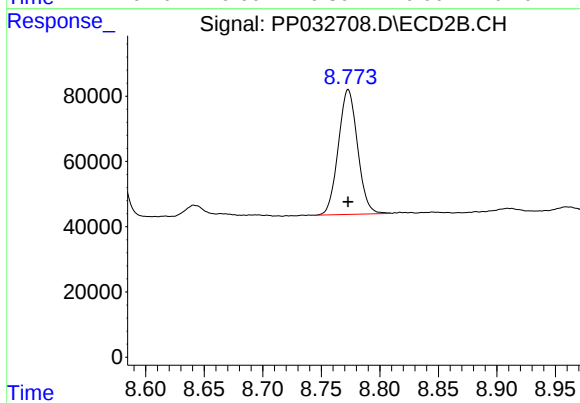

#44 AR-1268-4

R.T.: 8.773 min
Delta R.T.: 0.000 min
Response: 436968
Conc: 241.60 ng/ml

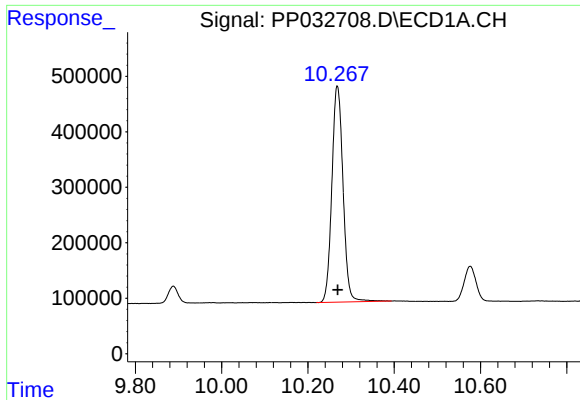


#45 AR-1268-5

R.T.: 10.268 min
Delta R.T.: -0.002 min
Response: 7006413
Conc: 463.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
S11-01-B

Manual Integrations
APPROVED

Ankita
1/14/2021 4:38:53 PM

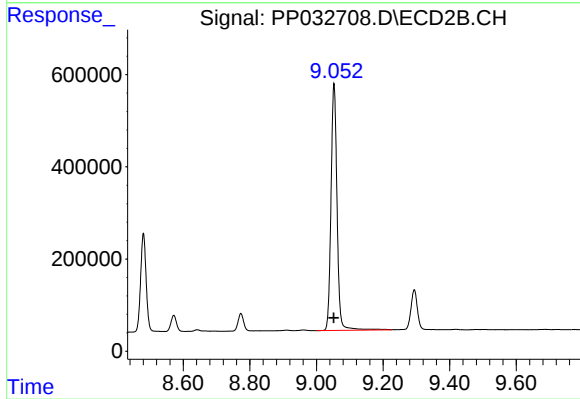

#45 AR-1268-5

R.T.: 9.053 min
Delta R.T.: 0.000 min
Response: 6754531
Conc: 466.53 ng/ml