

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
 Data File : PP042924.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 12:12
 Operator : AJ\MA
 Sample : PB142027BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:25:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.872	4.042	453852	526539	19.181	21.082
2)	SA Decachlor...	10.805	9.378	324260	422649	22.182	21.667
Target Compounds							
8)	L2 AR-1221-1	5.107	0.000	129641	0	486.985	N.D. #
9)	L2 AR-1221-2	0.000	4.376f	0	145751	N.D.	599.049 #
38)	L8 AR-1262-3	9.361f	0.000	7941	0	8.615	N.D. #
39)	L8 AR-1262-4	9.413f	0.000	10348	0	19.183	N.D. #
41)	L9 AR-1268-1	9.361f	0.000	7941	0	3.852	N.D. #
42)	L9 AR-1268-2	9.446	0.000	14744	0	7.720	N.D. #
45)	L9 AR-1268-5	10.470	0.000	18646	0	3.499	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
Data File : PP042924.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 12:12
Operator : AJ\MA
Sample : PB142027BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:25:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

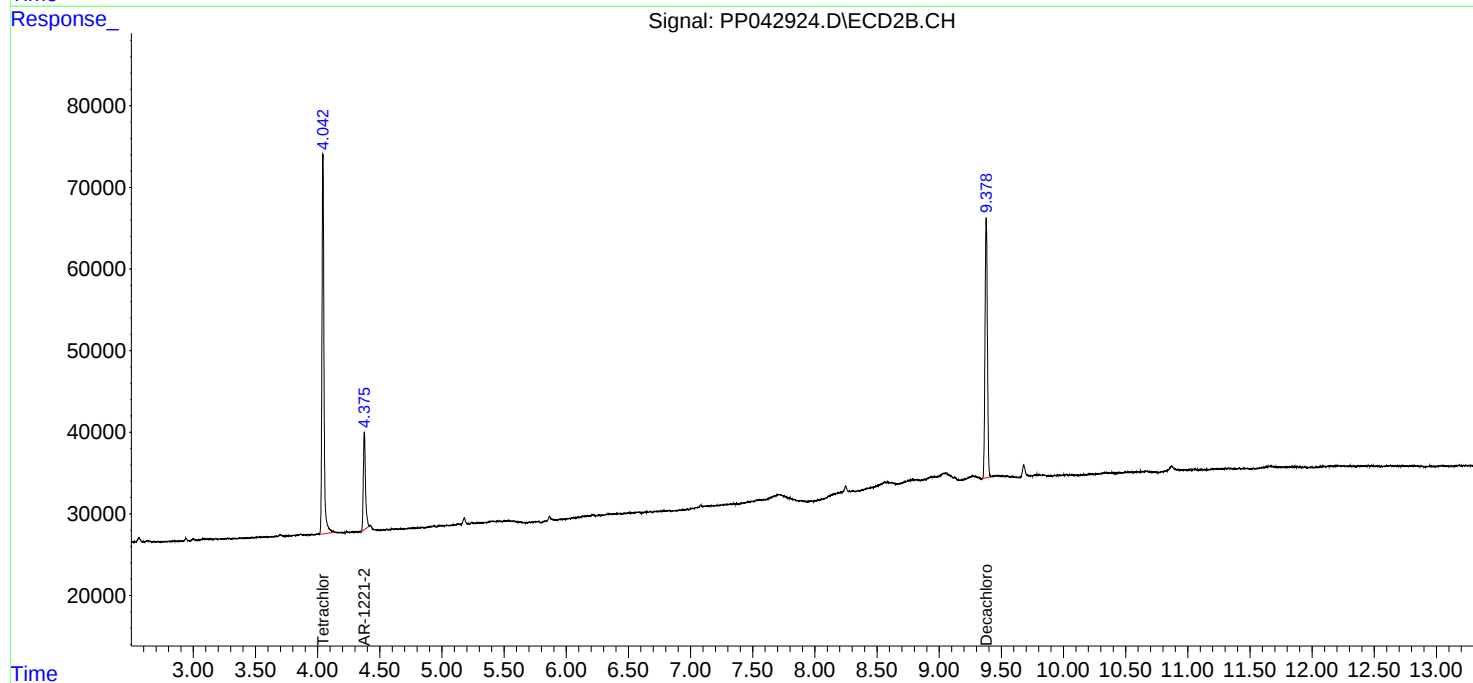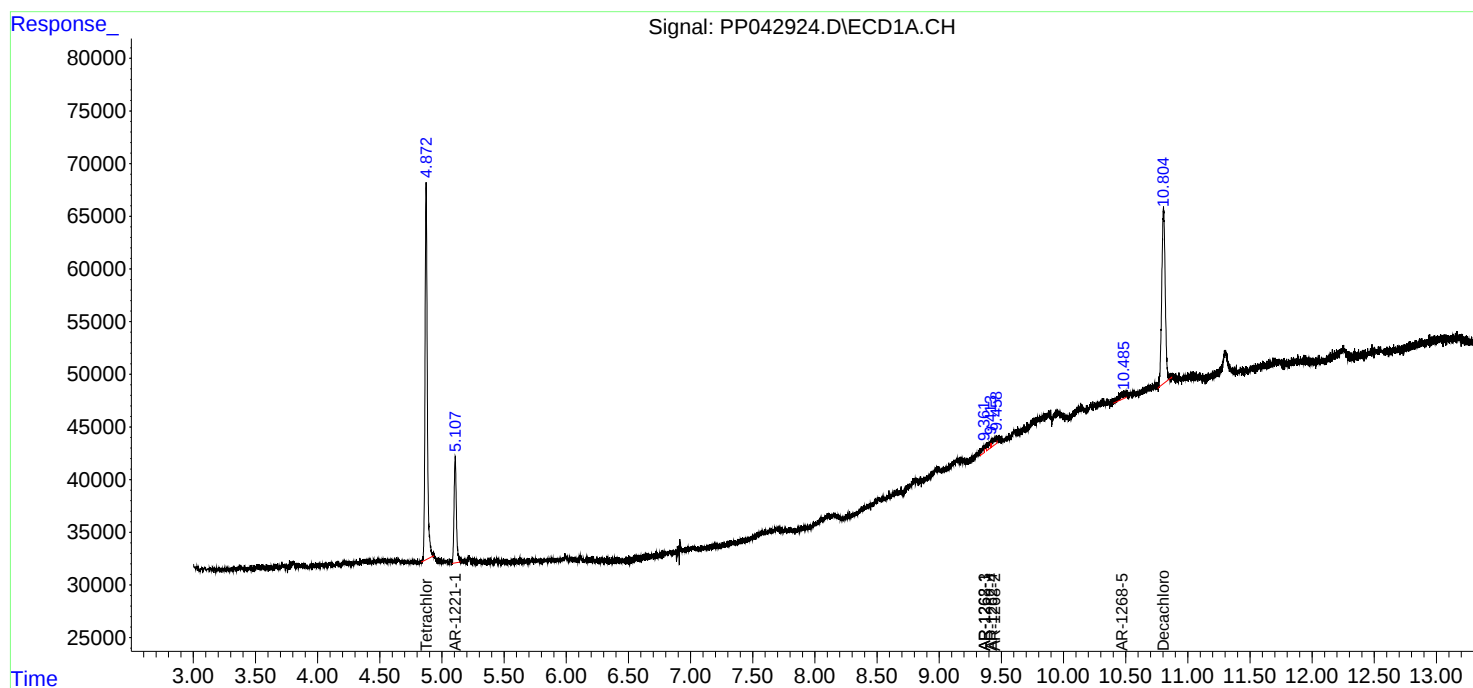


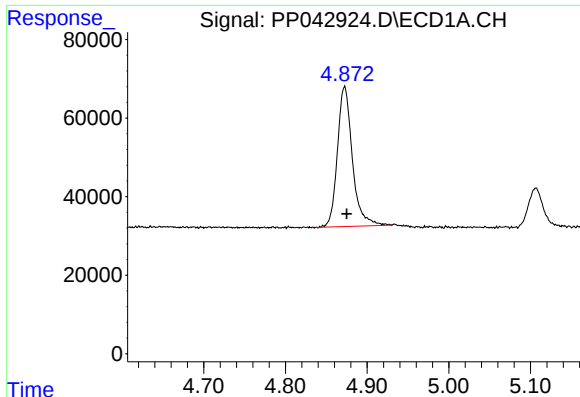

#1 Tetrachloro-m-xylene


R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 453852
Conc: 19.18 ng/ml

Instrument :
ECD_P
ClientSampleId :

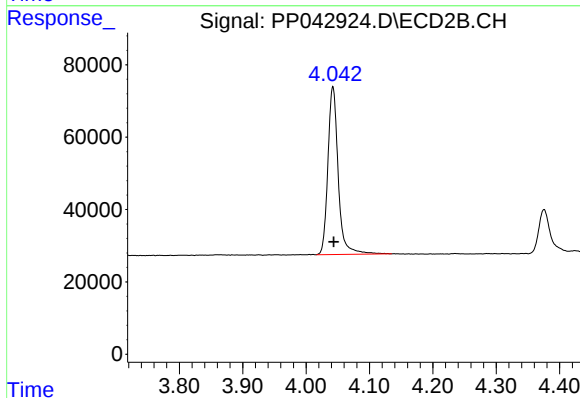


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.001 min
Response: 526539
Conc: 21.08 ng/ml

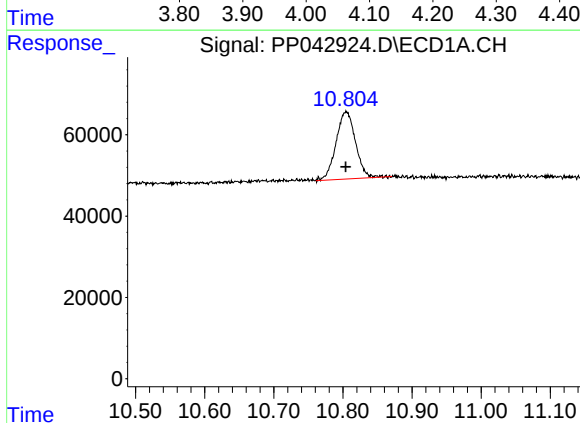


#2 Decachlorobiphenyl

R.T.: 10.805 min
Delta R.T.: 0.000 min
Response: 324260
Conc: 22.18 ng/ml

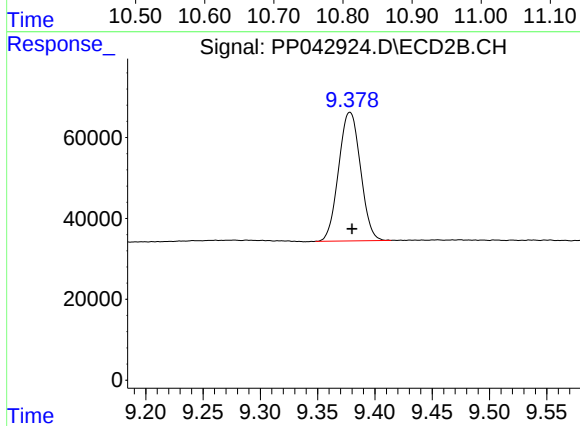

#2 Decachlorobiphenyl


R.T.: 9.378 min
Delta R.T.: -0.002 min
Response: 422649
Conc: 21.67 ng/ml

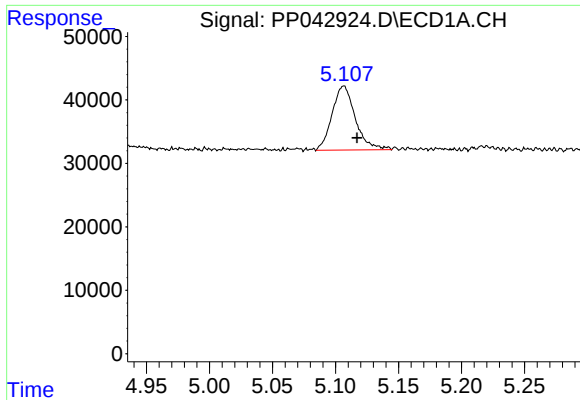

#8 AR-1221-1


R.T.: 5.107 min
Delta R.T.: -0.010 min
Response: 129641
Conc: 486.99 ng/ml

Instrument :
ECD_P
ClientSampleId :

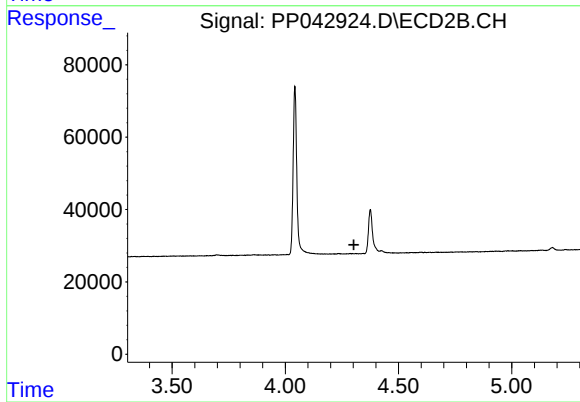


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.303 min
Response: 0
Conc: N.D.

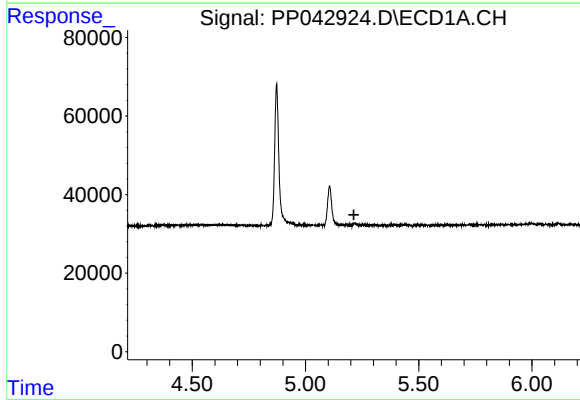


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

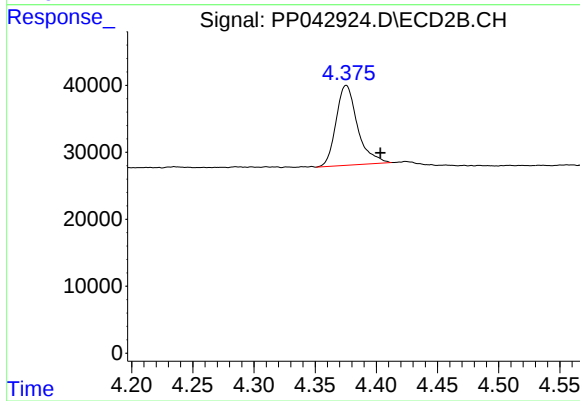

#9 AR-1221-2


R.T.: 4.376 min
Delta R.T.: -0.028 min
Response: 145751
Conc: 599.05 ng/ml

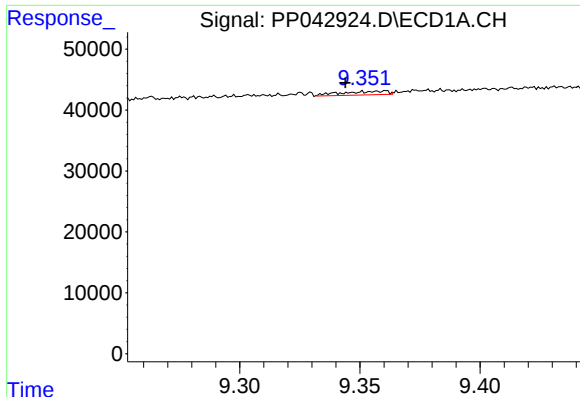

#38 AR-1262-3


R.T.: 9.361 min
Delta R.T.: 0.017 min
Response: 7941
Conc: 8.61 ng/ml

Instrument :
ECD_P
ClientSampleId :

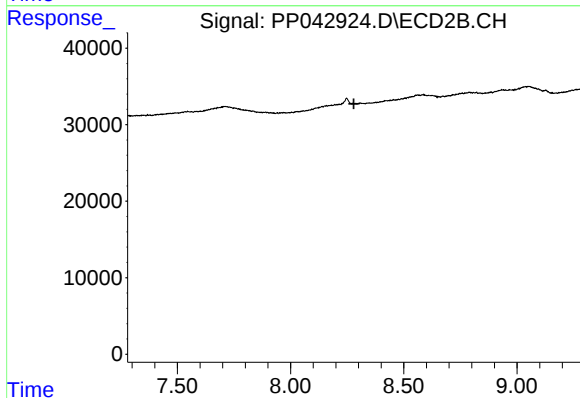


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.280 min
Response: 0
Conc: N.D.

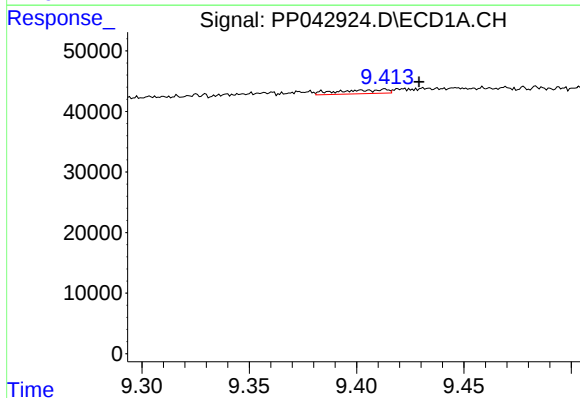


#39 AR-1262-4

R.T.: 9.413 min
Delta R.T.: -0.016 min
Response: 10348
Conc: 19.18 ng/ml

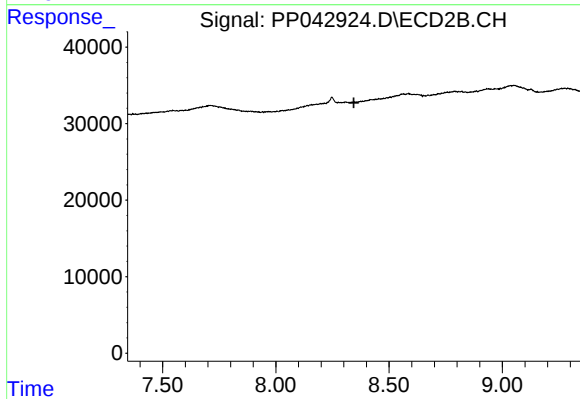

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

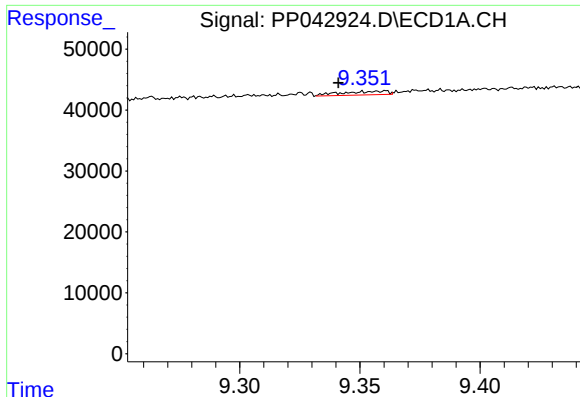

#41 AR-1268-1


R.T.: 9.361 min
Delta R.T.: 0.020 min
Response: 7941
Conc: 3.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

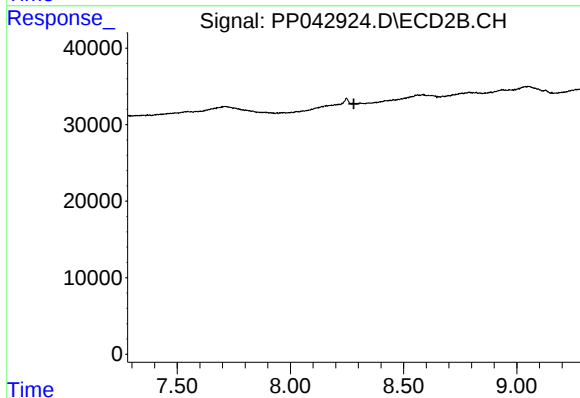


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.280 min
Response: 0
Conc: N.D.

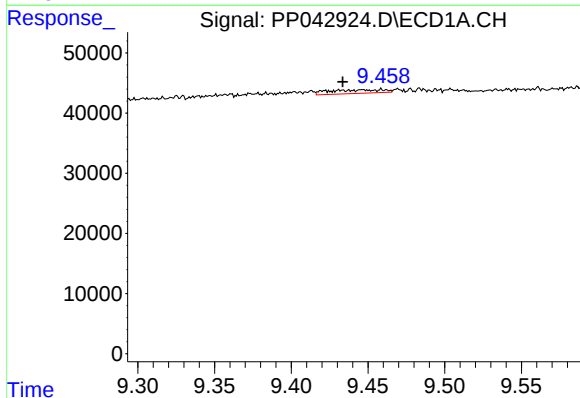


#42 AR-1268-2

R.T.: 9.446 min
Delta R.T.: 0.013 min
Response: 14744
Conc: 7.72 ng/ml

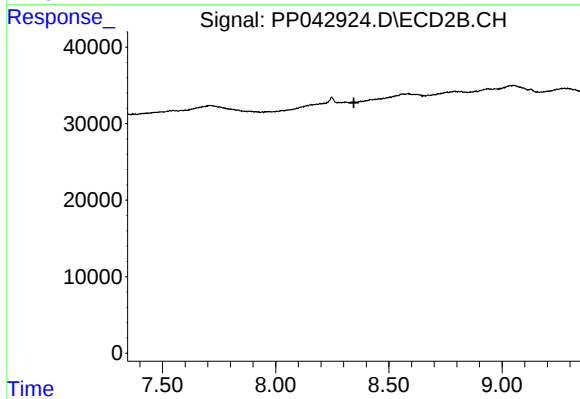

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

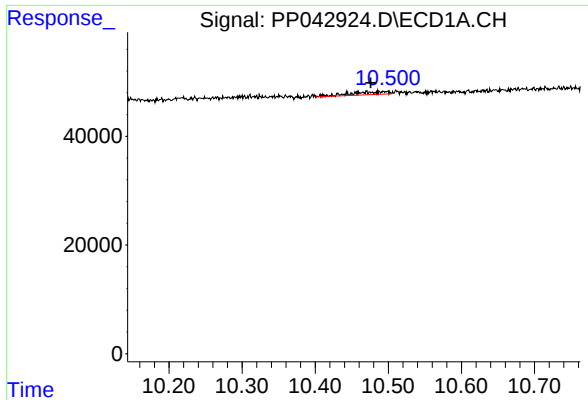

#45 AR-1268-5

R.T.: 10.470 min
Delta R.T.: -0.006 min
Response: 18646
Conc: 3.50 ng/ml

Instrument :
ECD_P
ClientSampleId :

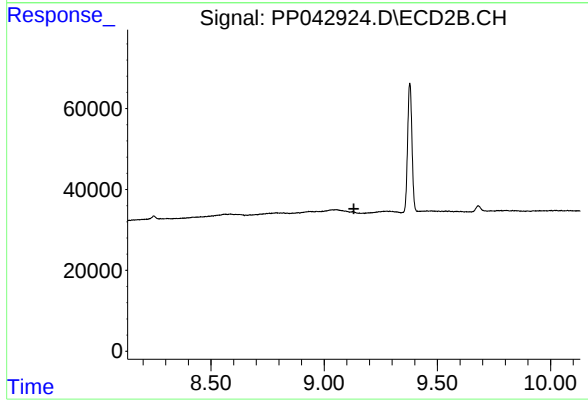

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.131 min
Response: 0
Conc: N.D.