

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
 Data File : PP042923.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 11:20
 Operator : AJ\MA
 Sample : N1105-10DL 20X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 IRV-2022-30BDL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
 Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:24:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.872	4.043	12640	21112	0.534	0.845 #
2) SA Decachlor...	10.808	9.377	11962	19185	0.818m	0.984m
Target Compounds						
26) L6 AR-1254-1	7.082	6.185	457423	877354	582.950	565.777
27) L6 AR-1254-2	7.310	6.343	695213	759483	552.375	559.449
28) L6 AR-1254-3	7.689	6.768	669092	1093648	515.717	511.304
29) L6 AR-1254-4	7.982	7.008	483471	658718	553.152	527.990
30) L6 AR-1254-5	8.411	7.439	567936	978297	606.177	573.724

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
Data File : PP042923.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 11:20
Operator : AJ\MA
Sample : N1105-10DL 20X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
IRV-2022-30BDL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:24:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

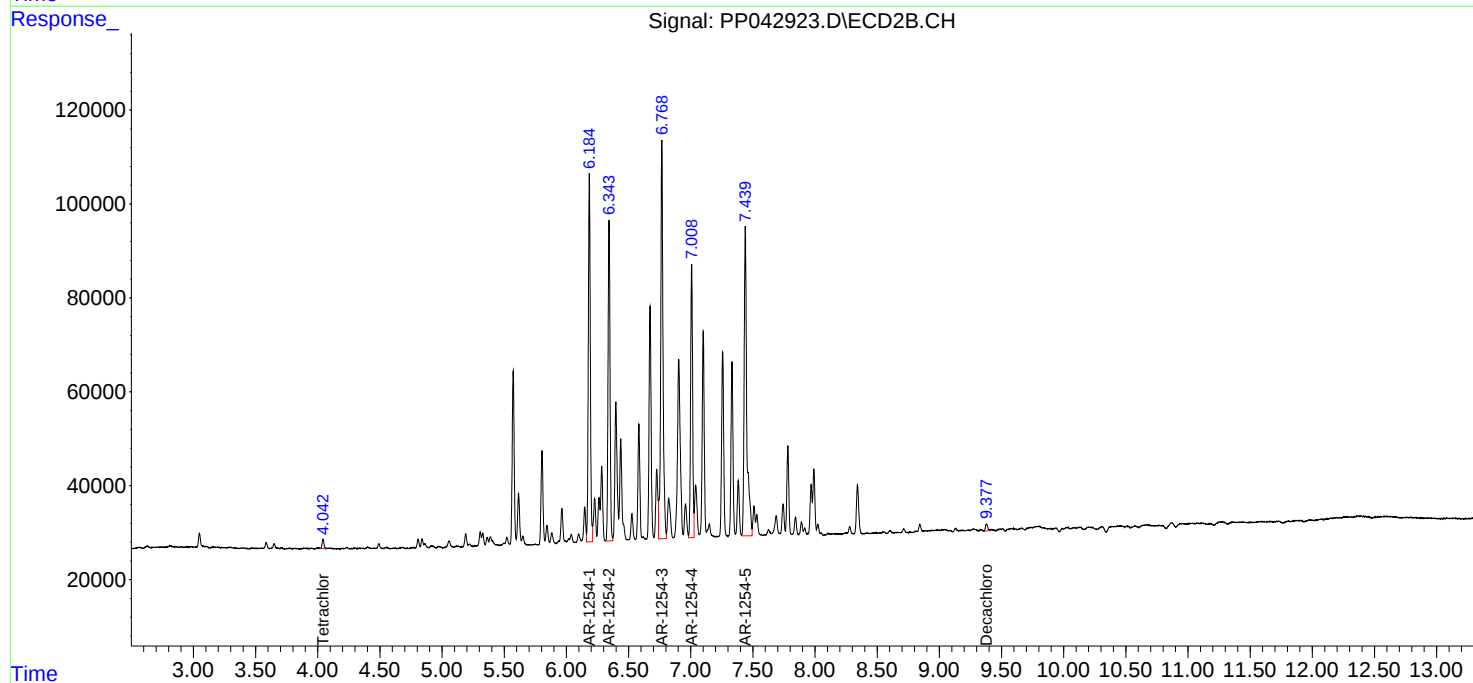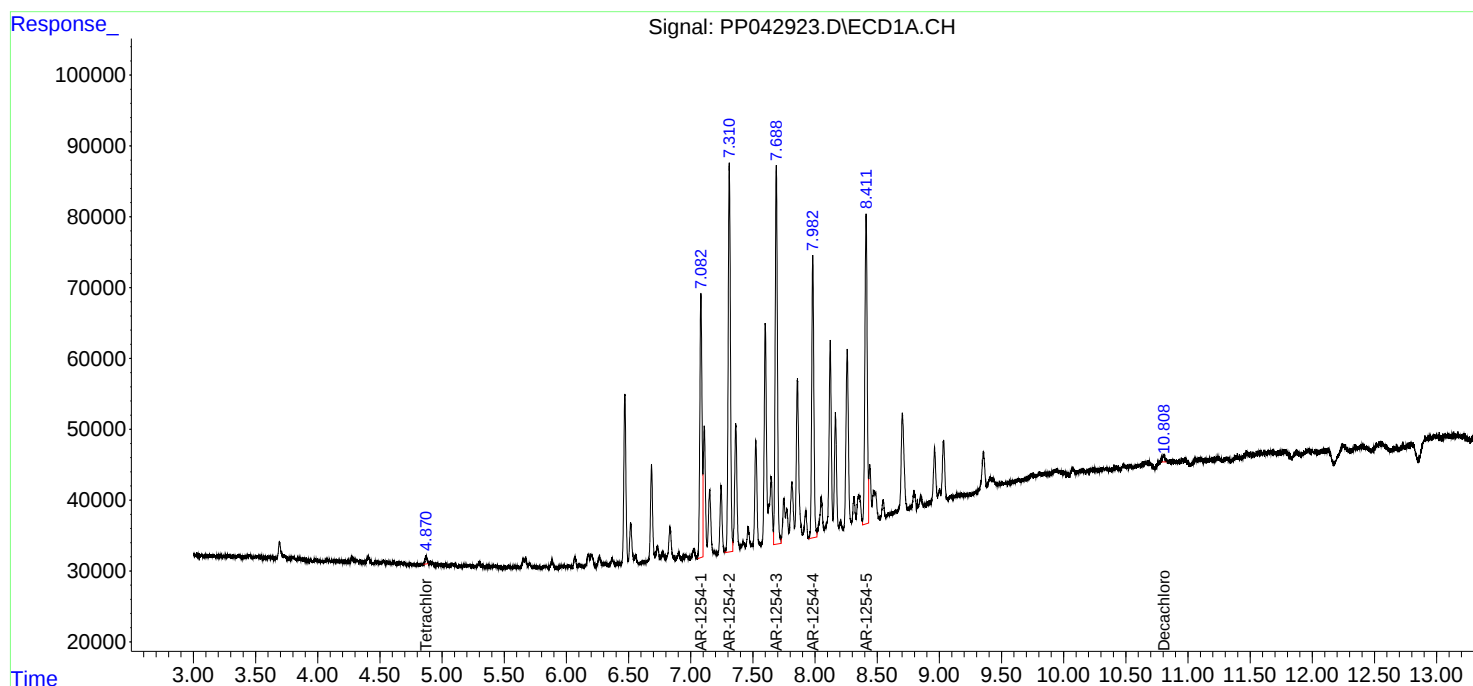

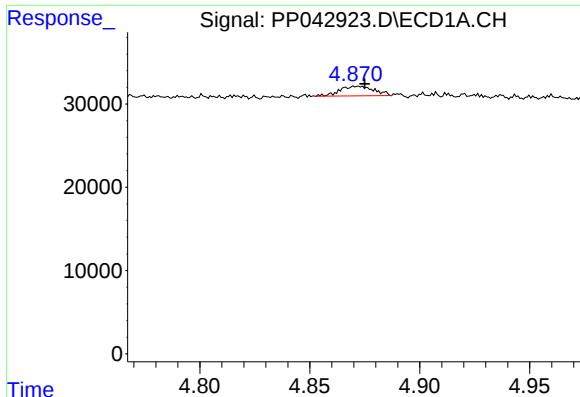


#1 Tetrachloro-m-xylene

R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 12640
Conc: 0.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-30BDL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

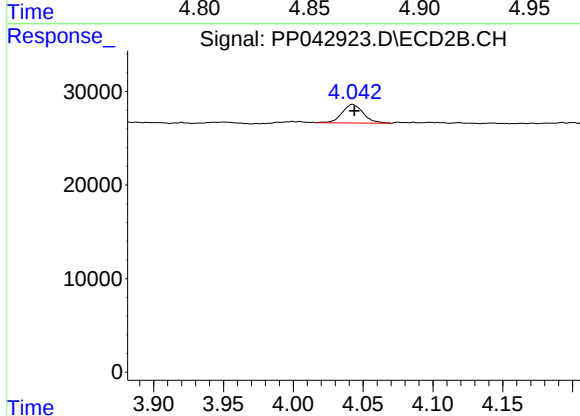


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: -0.001 min
Response: 21112
Conc: 0.85 ng/ml

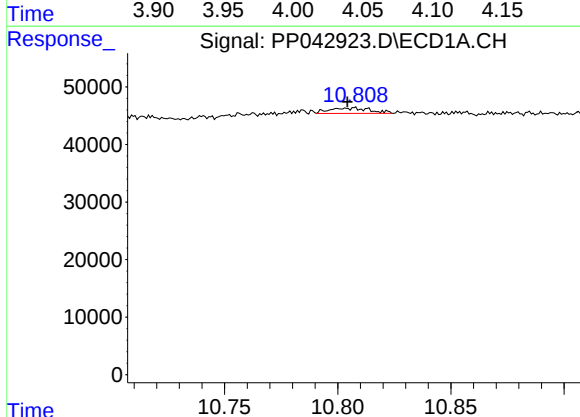


#2 Decachlorobiphenyl

R.T.: 10.808 min
Delta R.T.: 0.004 min
Response: 11962
Conc: 0.82 ng/ml m

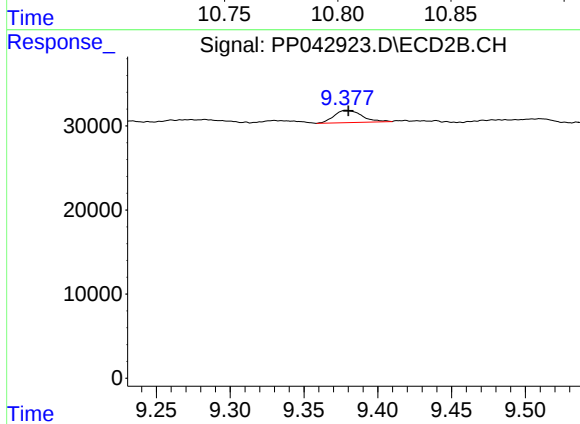

#2 Decachlorobiphenyl

R.T.: 9.377 min
Delta R.T.: -0.003 min
Response: 19185
Conc: 0.98 ng/ml m

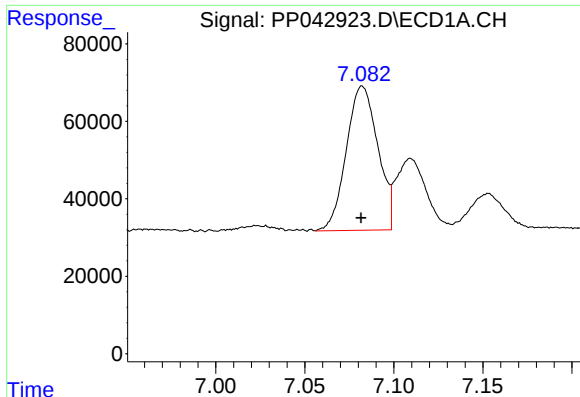


#26 AR-1254-1

R.T.: 7.082 min
Delta R.T.: 0.000 min
Response: 457423
Conc: 582.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-30BDL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

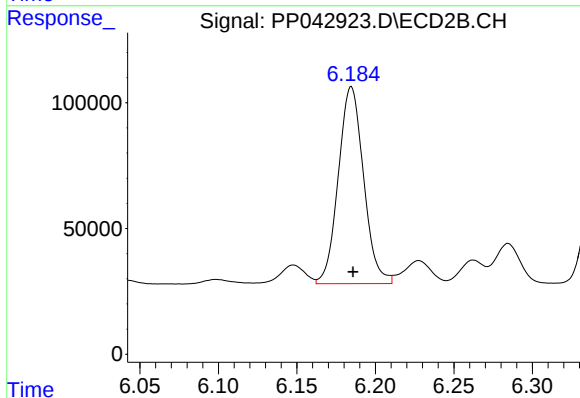


#26 AR-1254-1

R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 877354
Conc: 565.78 ng/ml

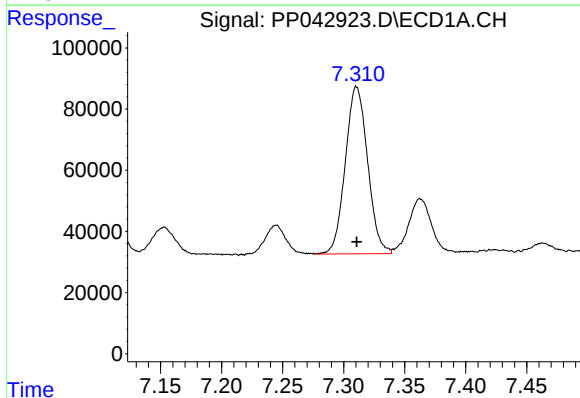


#27 AR-1254-2

R.T.: 7.310 min
Delta R.T.: 0.000 min
Response: 695213
Conc: 552.37 ng/ml

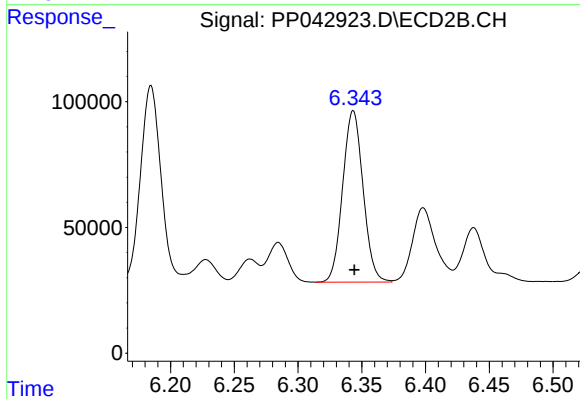

#27 AR-1254-2

R.T.: 6.343 min
Delta R.T.: 0.000 min
Response: 759483
Conc: 559.45 ng/ml

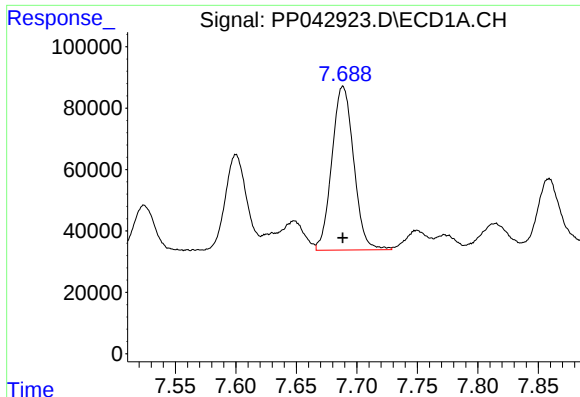


#28 AR-1254-3

R.T.: 7.689 min
Delta R.T.: 0.000 min
Response: 669092
Conc: 515.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-30BDL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

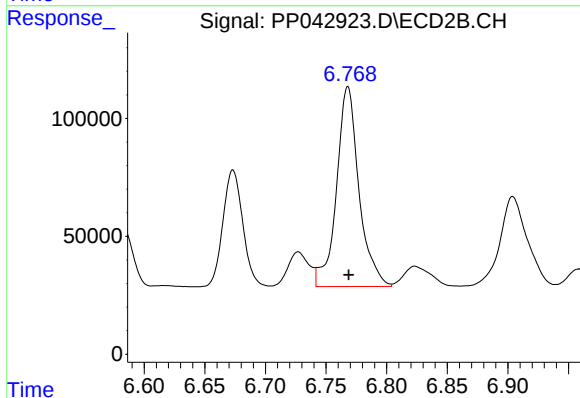


#28 AR-1254-3

R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 1093648
Conc: 511.30 ng/ml

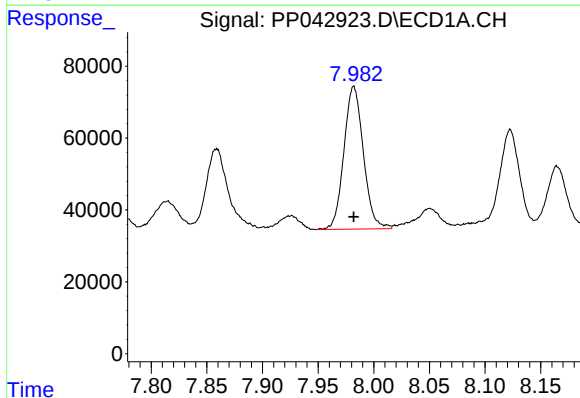


#29 AR-1254-4

R.T.: 7.982 min
Delta R.T.: 0.000 min
Response: 483471
Conc: 553.15 ng/ml

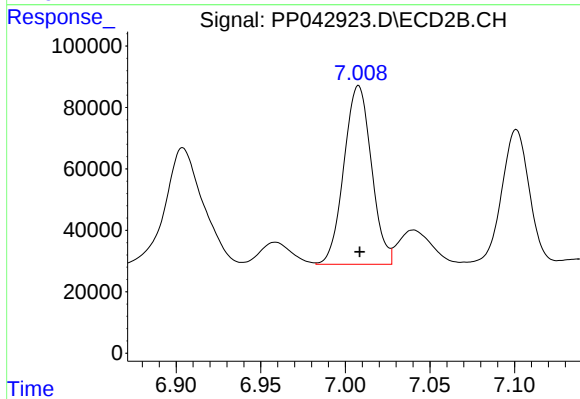

#29 AR-1254-4

R.T.: 7.008 min
Delta R.T.: 0.000 min
Response: 658718
Conc: 527.99 ng/ml

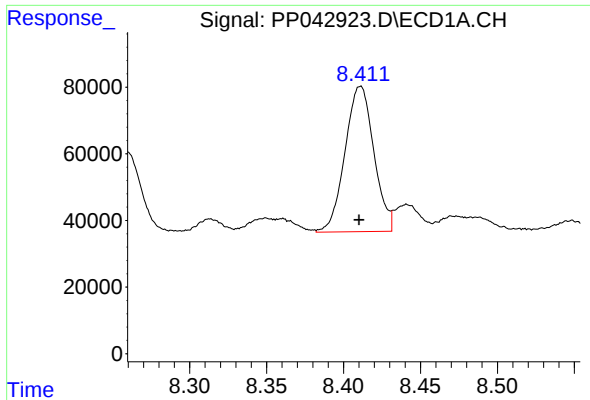


#30 AR-1254-5

R.T.: 8.411 min
Delta R.T.: 0.000 min
Response: 567936
Conc: 606.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2022-30BDL

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

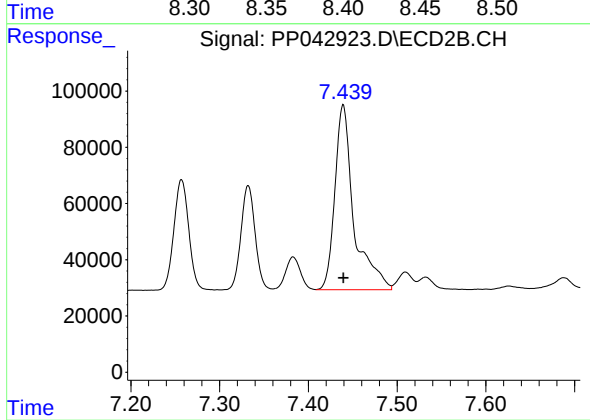

#30 AR-1254-5

R.T.: 7.439 min
Delta R.T.: 0.000 min
Response: 978297
Conc: 573.72 ng/ml