

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
 Data File : PP042935.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 16:31
 Operator : AJ\MA
 Sample : AR1254CCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254CCC500

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
 Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:30:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.872	4.042	1145330	1295432	48.405	51.867
2) SA Decachlor...	10.803	9.378	752516	997726	51.477m	51.148
Target Compounds						
26) L6 AR-1254-1	7.081	6.184	377858	738663	481.550	476.339
27) L6 AR-1254-2	7.311	6.343	549673	649722	436.737	478.597
28) L6 AR-1254-3	7.688	6.767	576481	1020883	444.335	477.286
29) L6 AR-1254-4	7.982	7.007	398545	619526	455.985	496.576
30) L6 AR-1254-5	8.411	7.439	418147	827389	446.301	485.224

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
Data File : PP042935.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 16:31
Operator : AJ\MA
Sample : AR1254CCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:30:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

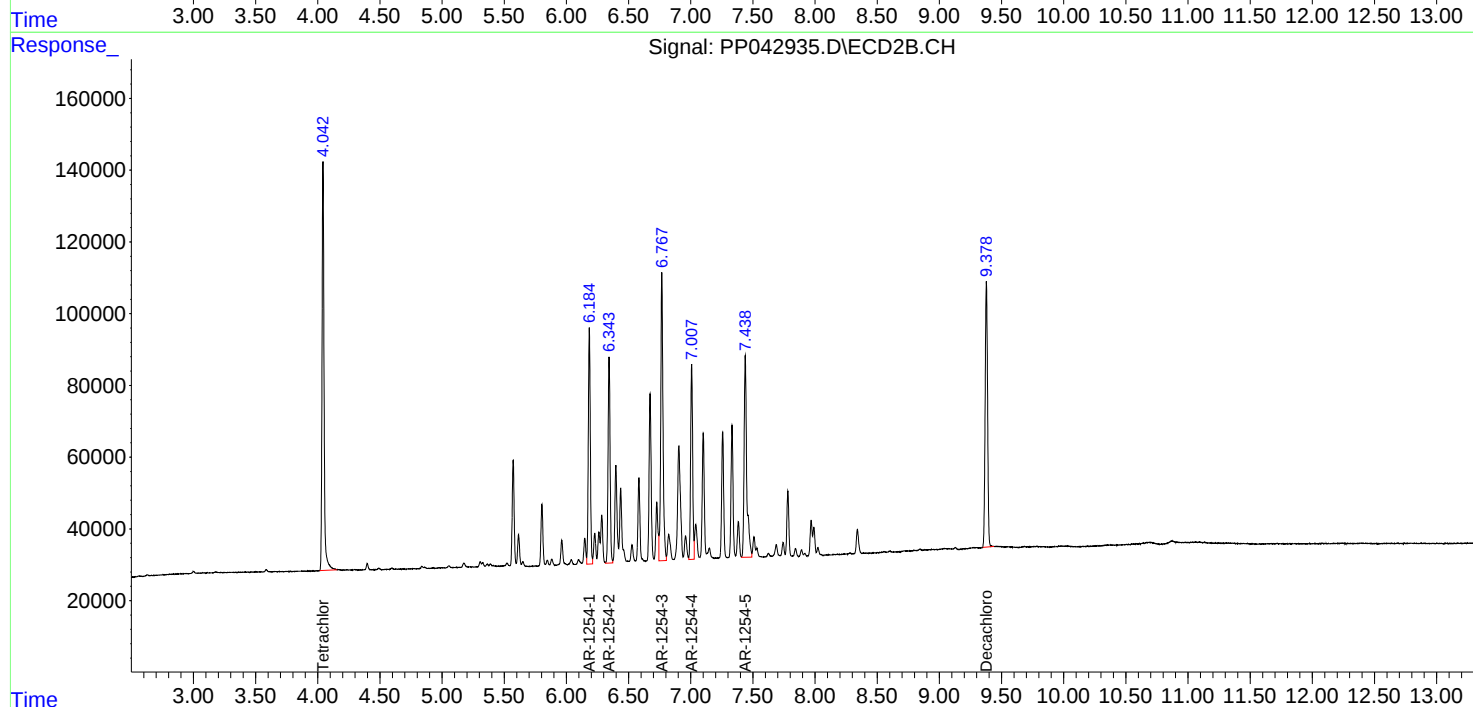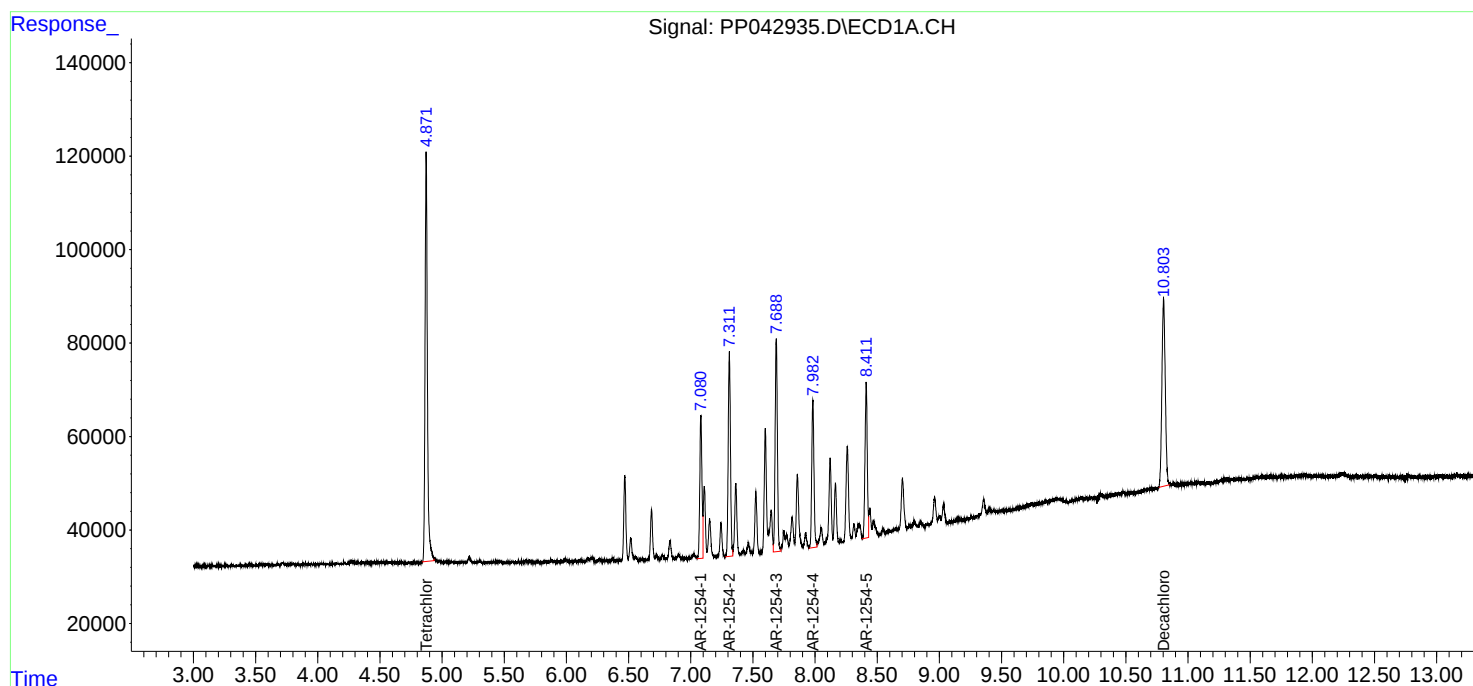

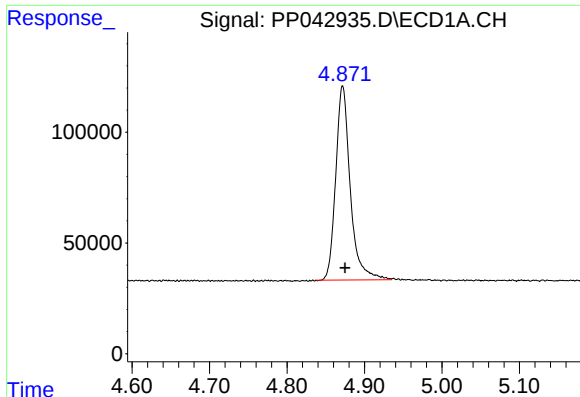


#1 Tetrachloro-m-xylene

R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 1145330
Conc: 48.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

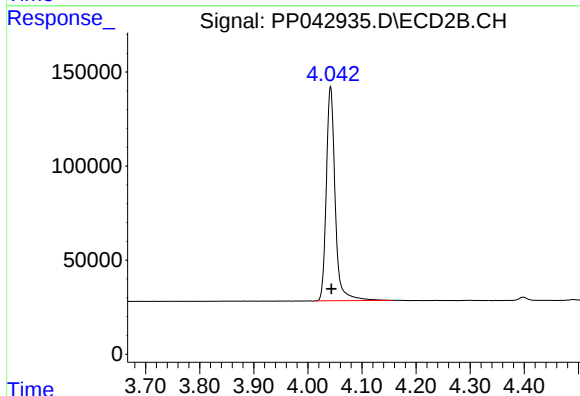


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.002 min
Response: 1295432
Conc: 51.87 ng/ml

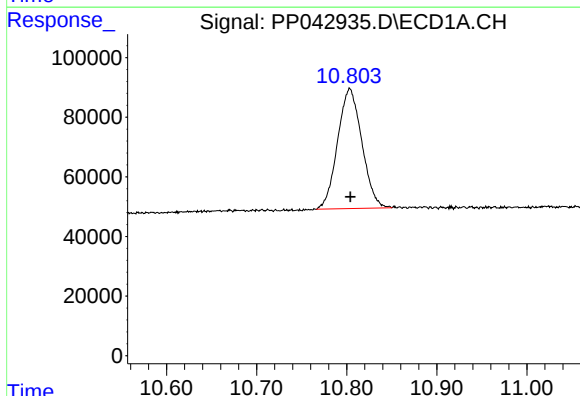


#2 Decachlorobiphenyl

R.T.: 10.803 min
Delta R.T.: -0.001 min
Response: 752516
Conc: 51.48 ng/ml m

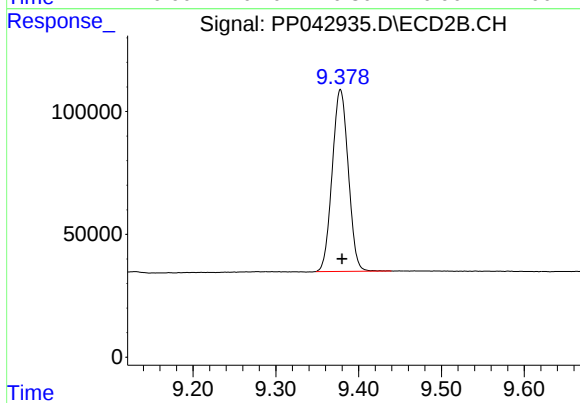

#2 Decachlorobiphenyl

R.T.: 9.378 min
Delta R.T.: -0.002 min
Response: 997726
Conc: 51.15 ng/ml

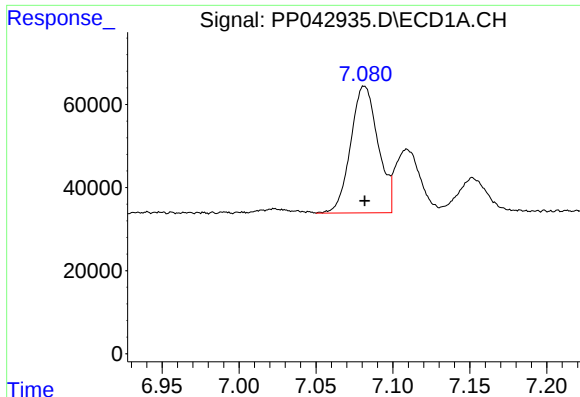


#26 AR-1254-1

R.T.: 7.081 min
Delta R.T.: 0.000 min
Response: 377858
Conc: 481.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

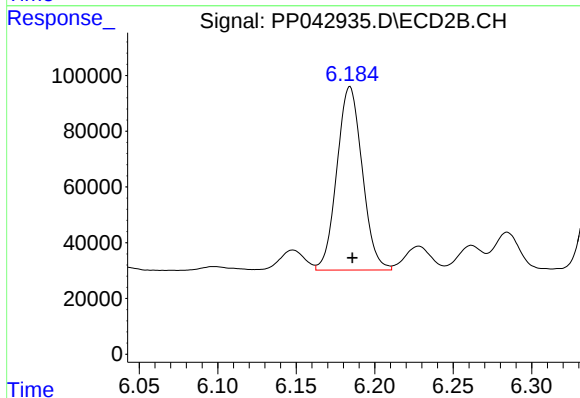


#26 AR-1254-1

R.T.: 6.184 min
Delta R.T.: -0.001 min
Response: 738663
Conc: 476.34 ng/ml

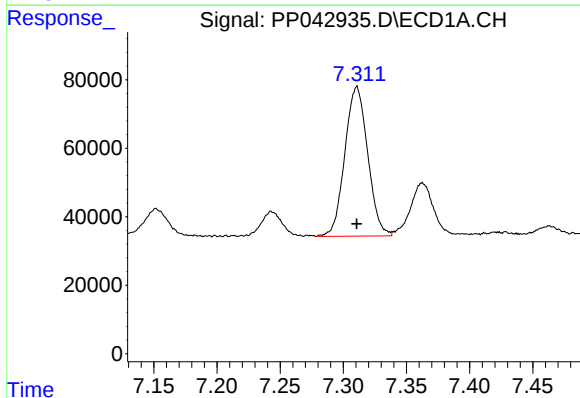


#27 AR-1254-2

R.T.: 7.311 min
Delta R.T.: 0.000 min
Response: 549673
Conc: 436.74 ng/ml

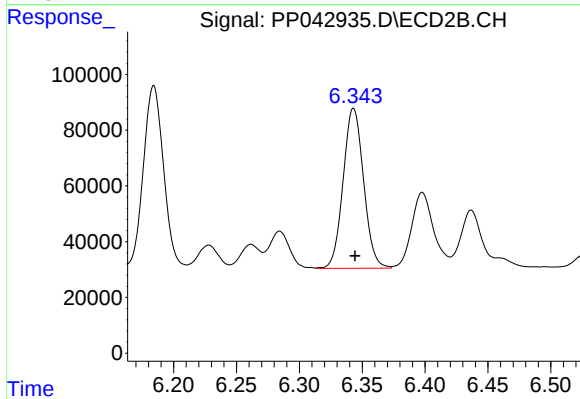

#27 AR-1254-2

R.T.: 6.343 min
Delta R.T.: -0.001 min
Response: 649722
Conc: 478.60 ng/ml

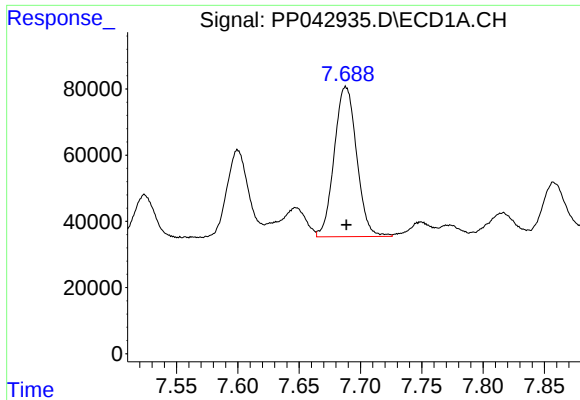


#28 AR-1254-3

R.T.: 7.688 min
Delta R.T.: 0.000 min
Response: 576481
Conc: 444.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

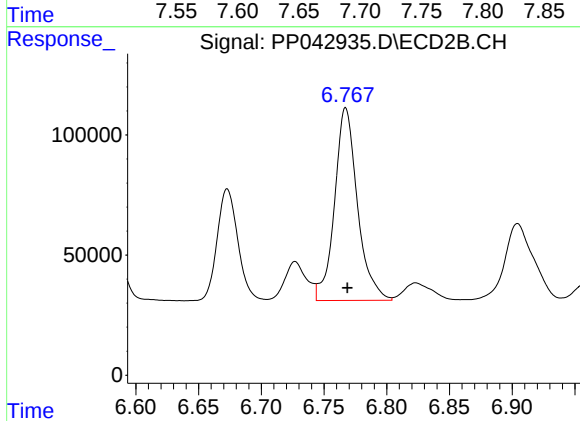


#28 AR-1254-3

R.T.: 6.767 min
Delta R.T.: -0.001 min
Response: 1020883
Conc: 477.29 ng/ml

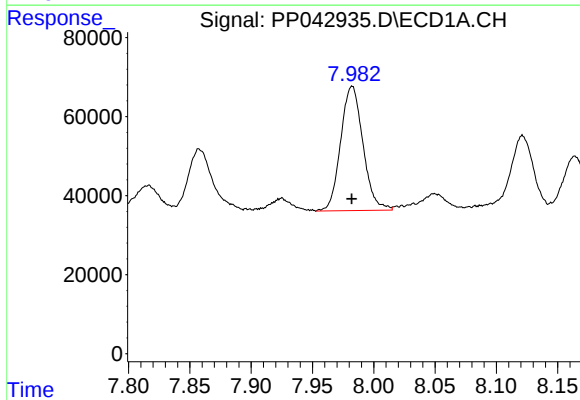


#29 AR-1254-4

R.T.: 7.982 min
Delta R.T.: 0.000 min
Response: 398545
Conc: 455.99 ng/ml

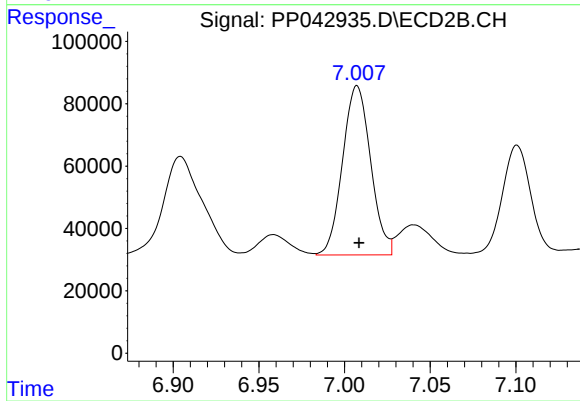

#29 AR-1254-4

R.T.: 7.007 min
Delta R.T.: -0.001 min
Response: 619526
Conc: 496.58 ng/ml

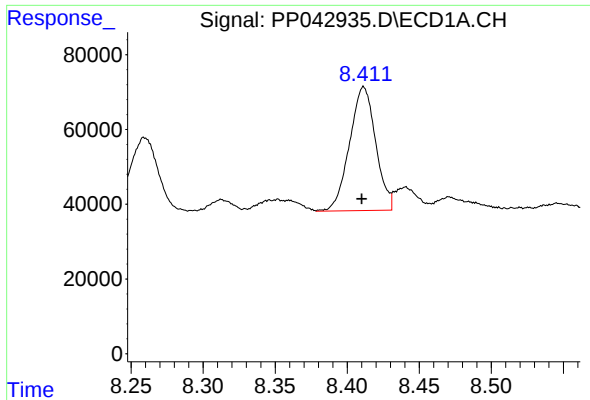


#30 AR-1254-5

R.T.: 8.411 min
Delta R.T.: 0.001 min
Response: 418147
Conc: 446.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1254CCC500

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

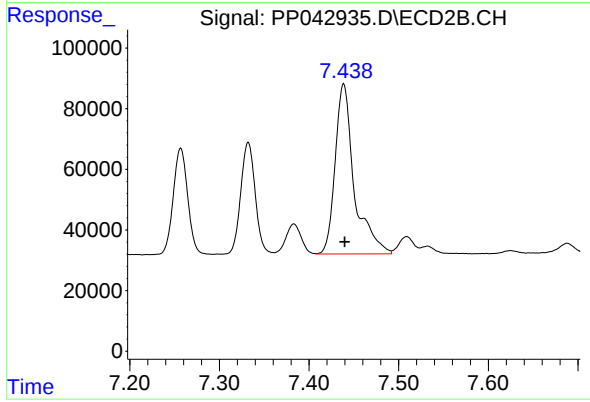

#30 AR-1254-5

R.T.: 7.439 min
Delta R.T.: -0.001 min
Response: 827389
Conc: 485.22 ng/ml