

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
 Data File : PP042948.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 20:47
 Operator : AJ\MA
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
 Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:34:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.872	4.043	1178210	1261464	49.795	50.507
2) SA Decachlor...	10.804	9.378	793090	1028459	54.253m	52.724
Target Compounds						
16) L4 AR-1242-1	6.175	5.307	290633	414142	490.546	516.783
17) L4 AR-1242-2	6.198	5.328	428484	560074	480.270	494.636
18) L4 AR-1242-3	6.264	5.521	272002	317011	490.223	497.189
19) L4 AR-1242-4	6.369	5.617	219364	299370	482.140	487.370
20) L4 AR-1242-5	7.148	6.185	218482	370781	487.074	515.284

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
Data File : PP042948.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 20:47
Operator : AJ\MA
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:34:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

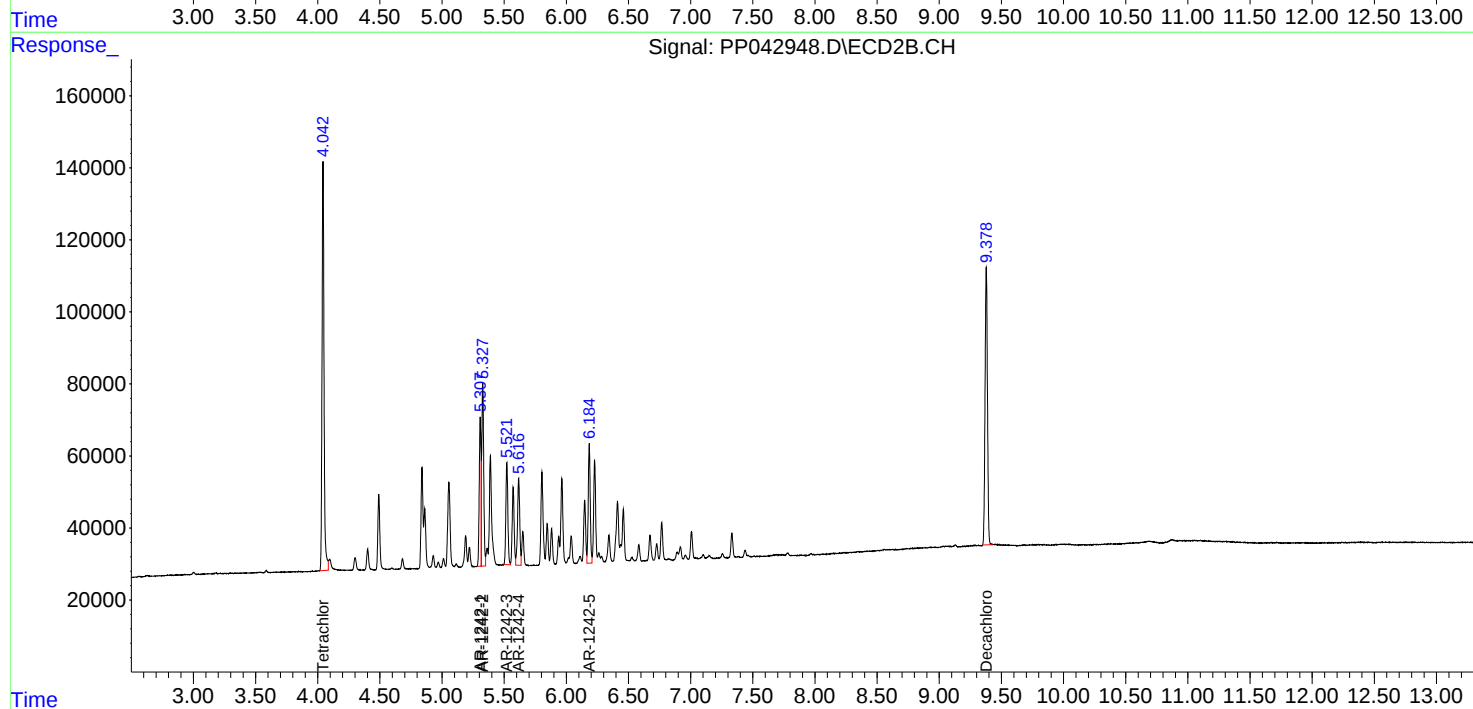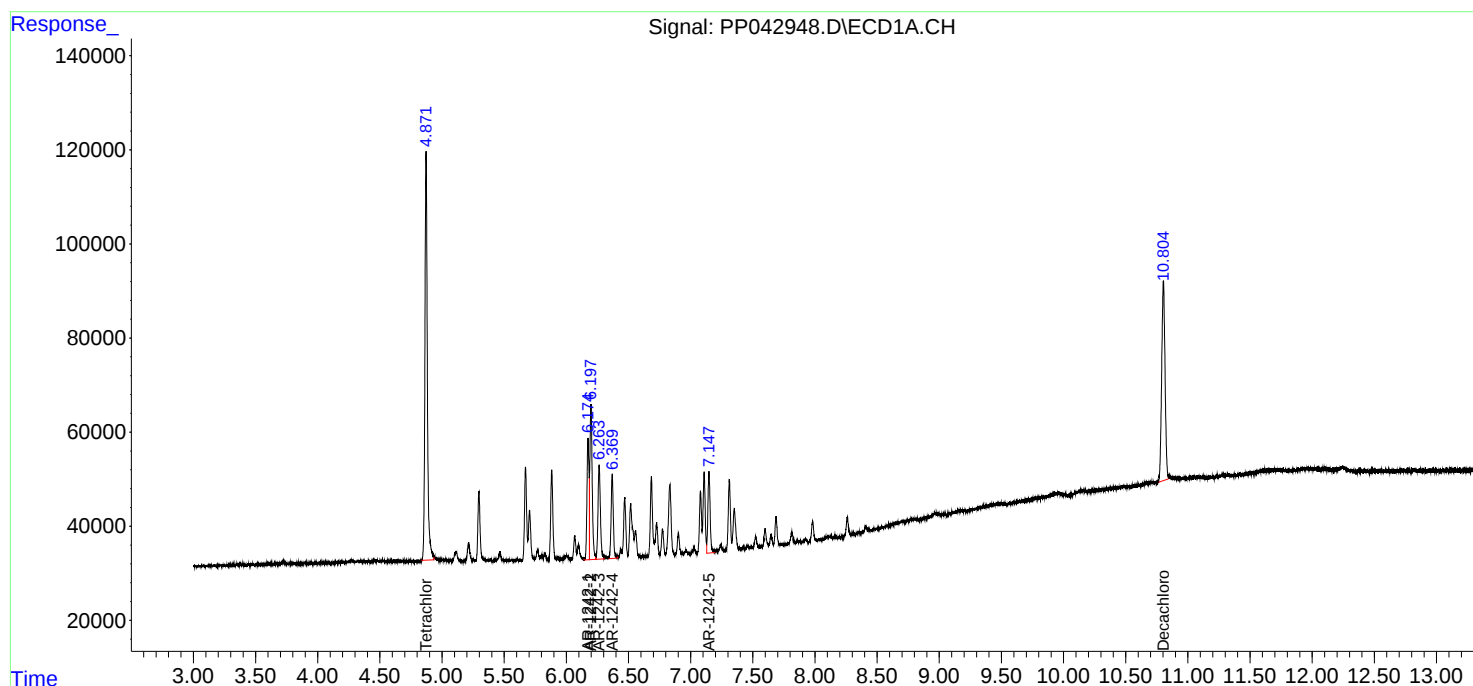

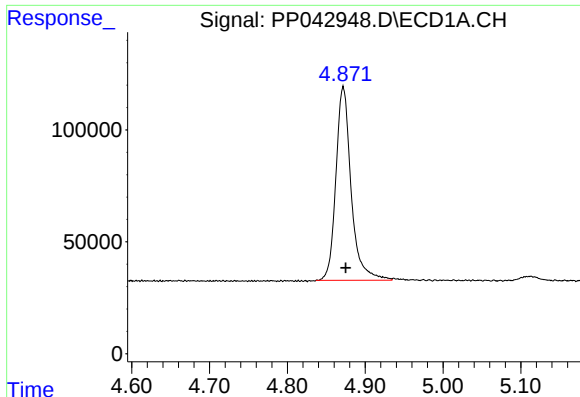


#1 Tetrachloro-m-xylene

R.T.: 4.872 min
Delta R.T.: -0.003 min
Response: 1178210
Conc: 49.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

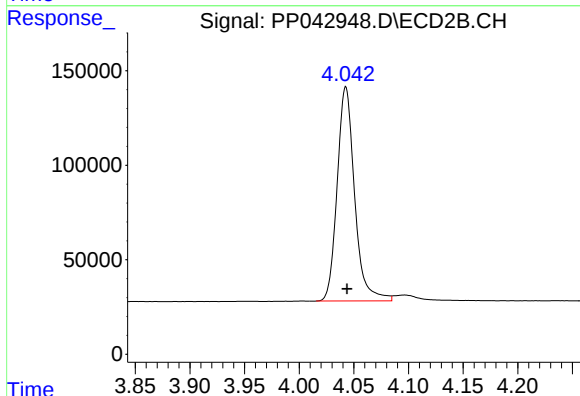


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 1261464
Conc: 50.51 ng/ml

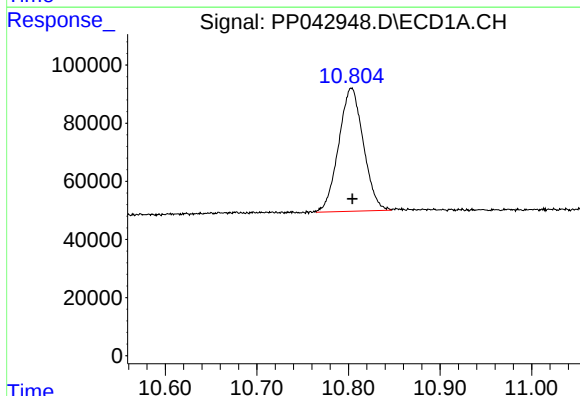


#2 Decachlorobiphenyl

R.T.: 10.804 min
Delta R.T.: 0.000 min
Response: 793090
Conc: 54.25 ng/ml m

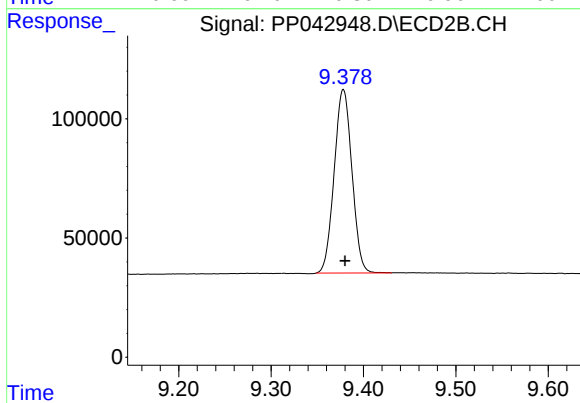

#2 Decachlorobiphenyl

R.T.: 9.378 min
Delta R.T.: -0.002 min
Response: 1028459
Conc: 52.72 ng/ml

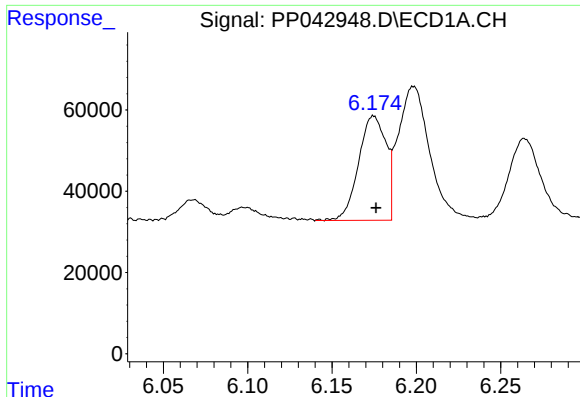


#16 AR-1242-1

R.T.: 6.175 min
Delta R.T.: -0.001 min
Response: 290633
Conc: 490.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

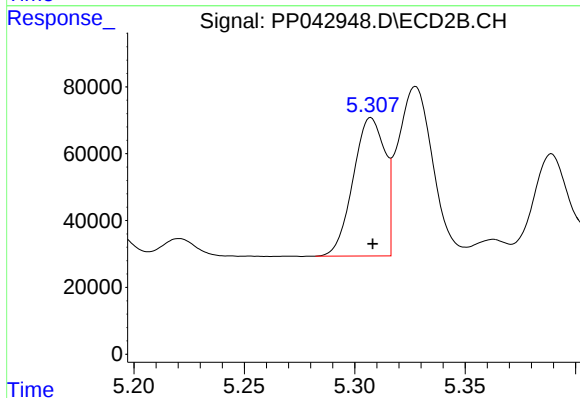


#16 AR-1242-1

R.T.: 5.307 min
Delta R.T.: 0.000 min
Response: 414142
Conc: 516.78 ng/ml

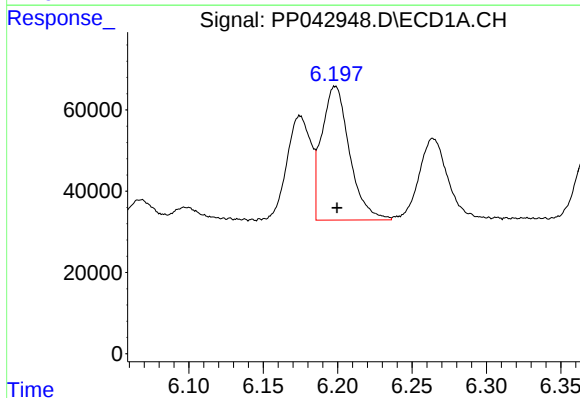


#17 AR-1242-2

R.T.: 6.198 min
Delta R.T.: -0.001 min
Response: 428484
Conc: 480.27 ng/ml

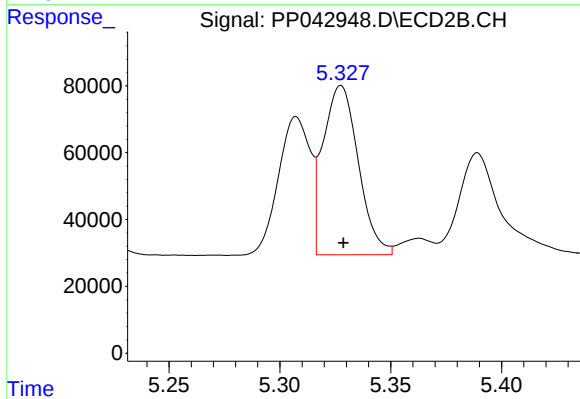

#17 AR-1242-2

R.T.: 5.328 min
Delta R.T.: -0.001 min
Response: 560074
Conc: 494.64 ng/ml

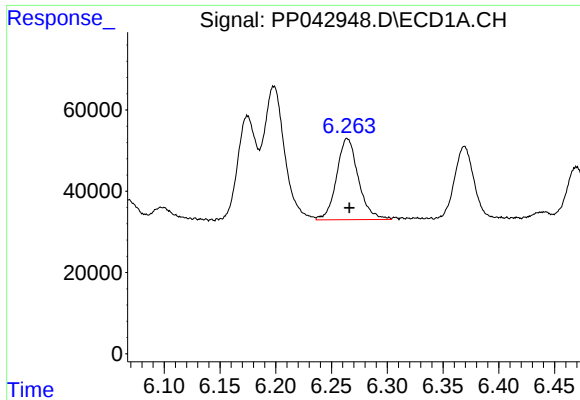


#18 AR-1242-3

R.T.: 6.264 min
Delta R.T.: -0.002 min
Response: 272002
Conc: 490.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

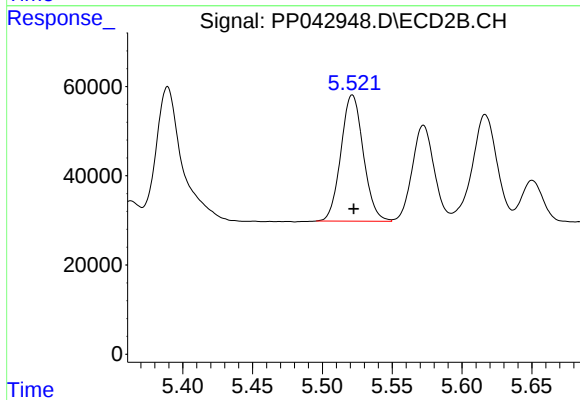


#18 AR-1242-3

R.T.: 5.521 min
Delta R.T.: -0.001 min
Response: 317011
Conc: 497.19 ng/ml

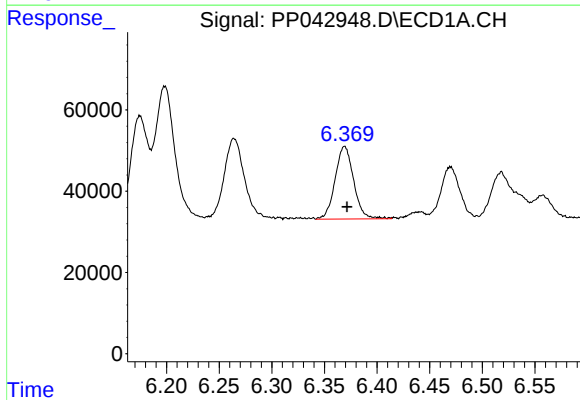


#19 AR-1242-4

R.T.: 6.369 min
Delta R.T.: -0.002 min
Response: 219364
Conc: 482.14 ng/ml

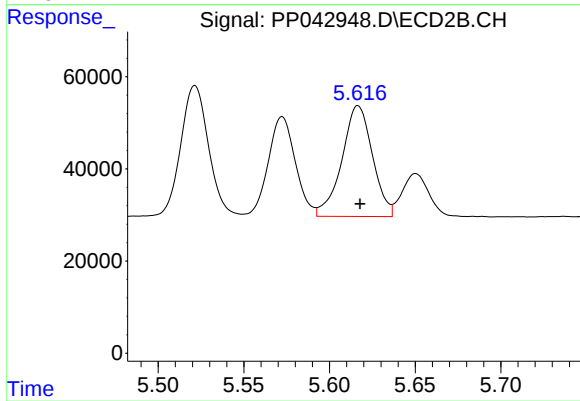

#19 AR-1242-4

R.T.: 5.617 min
Delta R.T.: -0.001 min
Response: 299370
Conc: 487.37 ng/ml

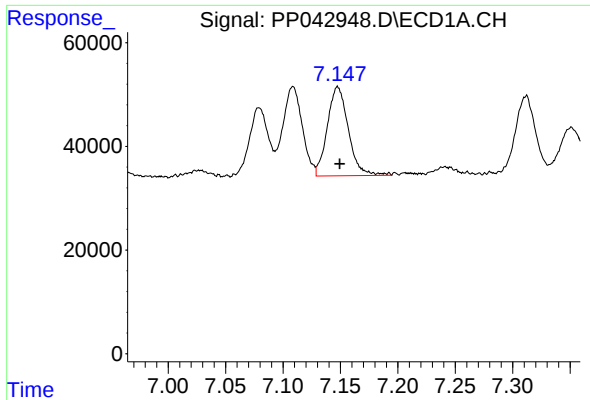


#20 AR-1242-5

R.T.: 7.148 min
Delta R.T.: -0.002 min
Response: 218482
Conc: 487.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

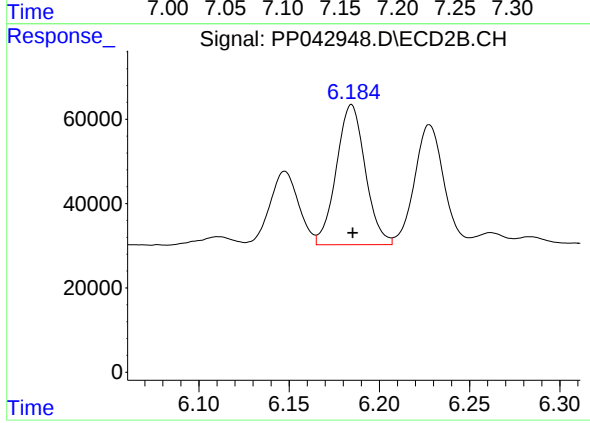

#20 AR-1242-5

R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 370781
Conc: 515.28 ng/ml