

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
 Data File : PP042956.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2022 23:00
 Operator : AJ\MA
 Sample : N1143-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WEST-BOILER-ROOM-SOUTH-SIDEWALL

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
 Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:37:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.873	4.046	366868	891084	15.505m	35.677m#
2) SA Decachlor...	10.802	9.378	332751	407119	22.762m	20.871

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011422\
Data File : PP042956.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2022 23:00
Operator : AJ\MA
Sample : N1143-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WEST-BOILER-ROOM-SOUTH-SIDEWALL


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/17/2022
Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:37:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

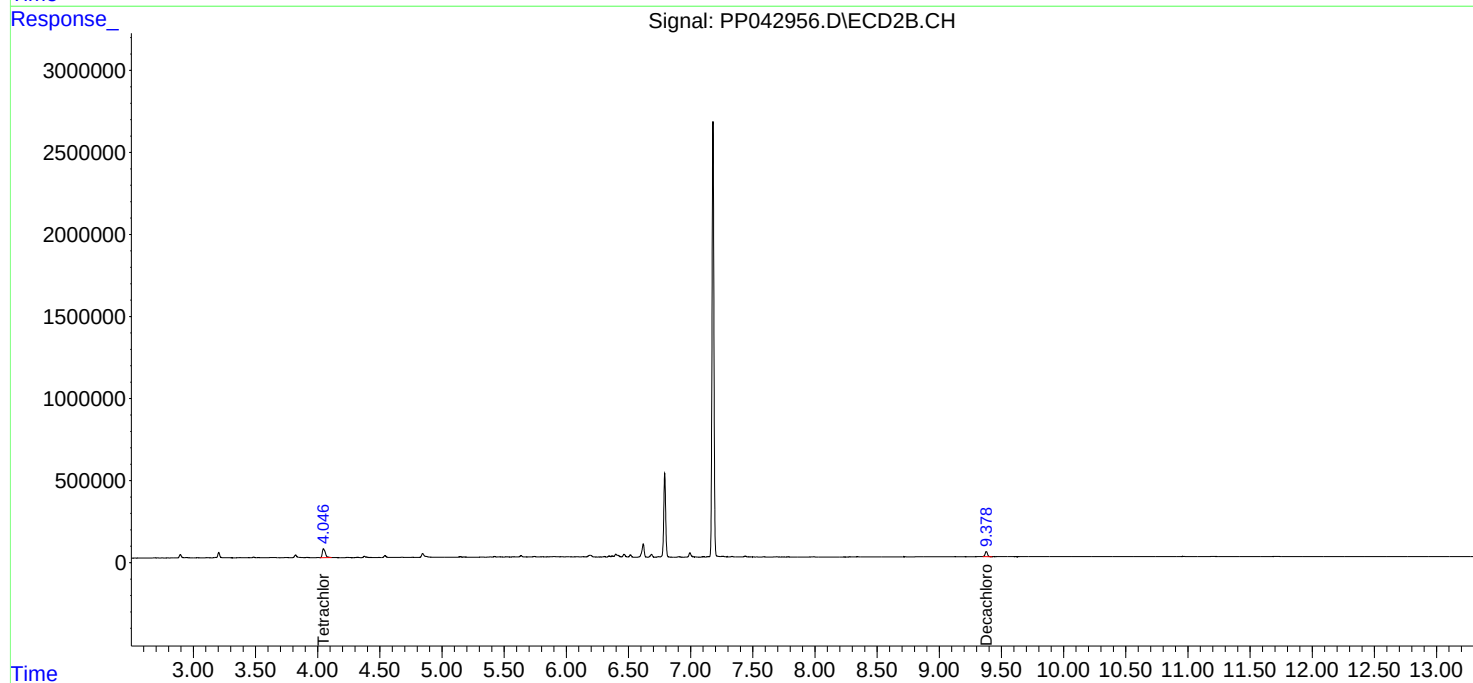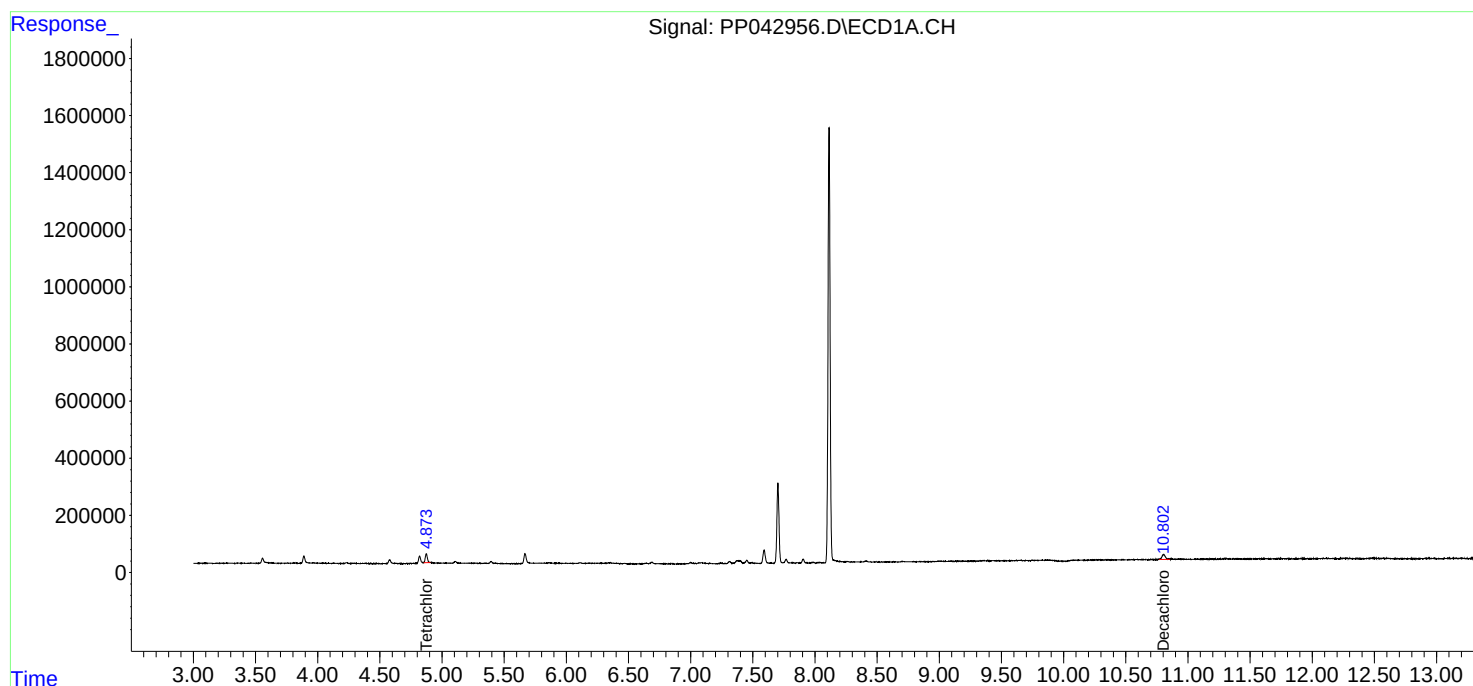

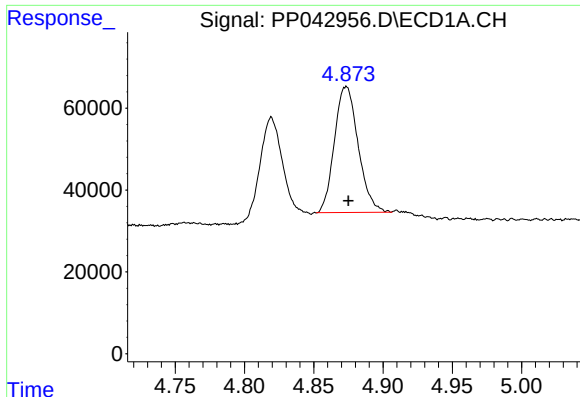

#1 Tetrachloro-m-xylene

R.T.: 4.873 min
Delta R.T.: -0.002 min
Response: 366868
Conc: 15.50 ng/ml

Instrument :

ECD_P

ClientSampleId :


WEST-BOILER-ROOM-SOUTH-SIDEWALL

Manual Integrations

APPROVED


Reviewed By :Ankita Jodhani 01/17/2022

Supervised By :Yogesh Patel 01/18/2022

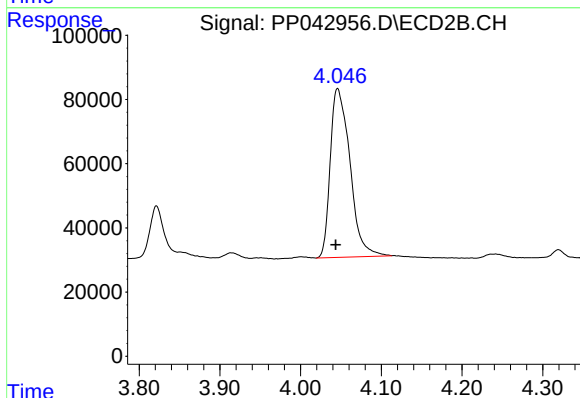


#1 Tetrachloro-m-xylene

R.T.: 4.046 min
Delta R.T.: 0.002 min
Response: 891084
Conc: 35.68 ng/ml m

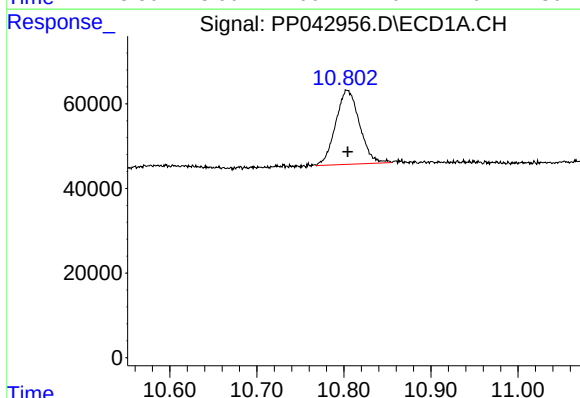

#2 Decachlorobiphenyl

R.T.: 10.802 min
Delta R.T.: -0.002 min
Response: 332751
Conc: 22.76 ng/ml m

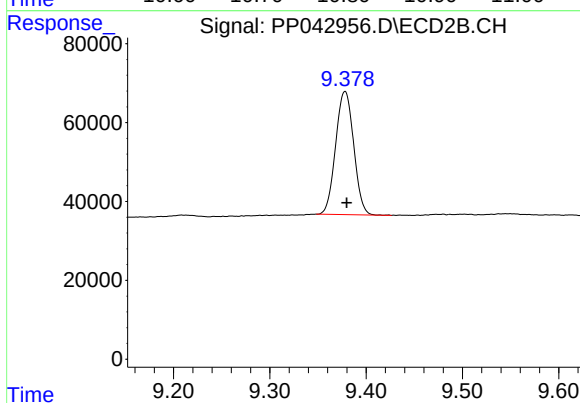

#2 Decachlorobiphenyl

R.T.: 9.378 min
Delta R.T.: -0.002 min
Response: 407119
Conc: 20.87 ng/ml