

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011425\
 Data File : PP069116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jan 2025 13:39
 Operator : YP\AJ
 Sample : Q1077-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-05-01132025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/15/2025
 Supervised By :Ankita Jodhani 01/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 00:52:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.668	3.979	21768997	18608594	15.647m	19.063m
2) SA Decachlor...	10.514	9.103	19749089	21660825	17.689	18.031

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011425\
Data File : PP069116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jan 2025 13:39
Operator : YP\AJ
Sample : Q1077-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TR-05-01132025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/15/2025
Supervised By :Ankita Jodhani 01/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 00:52:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

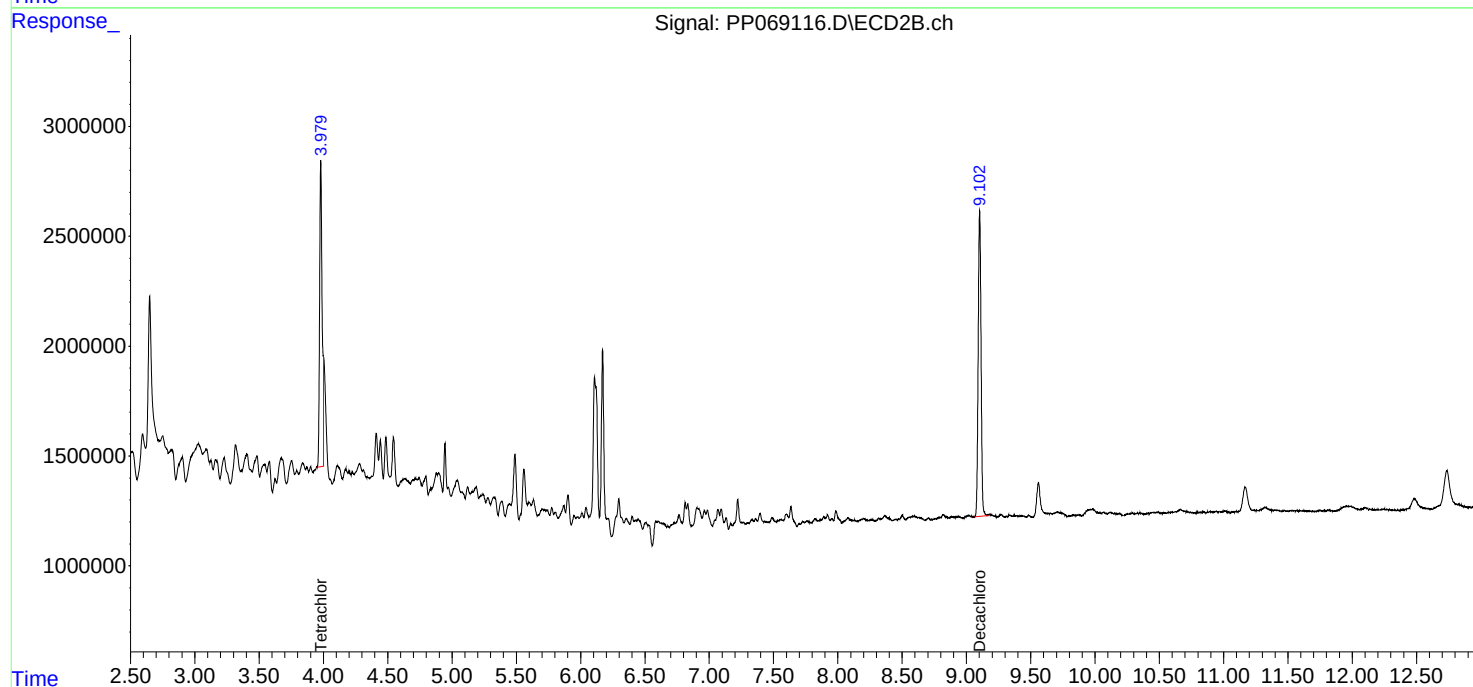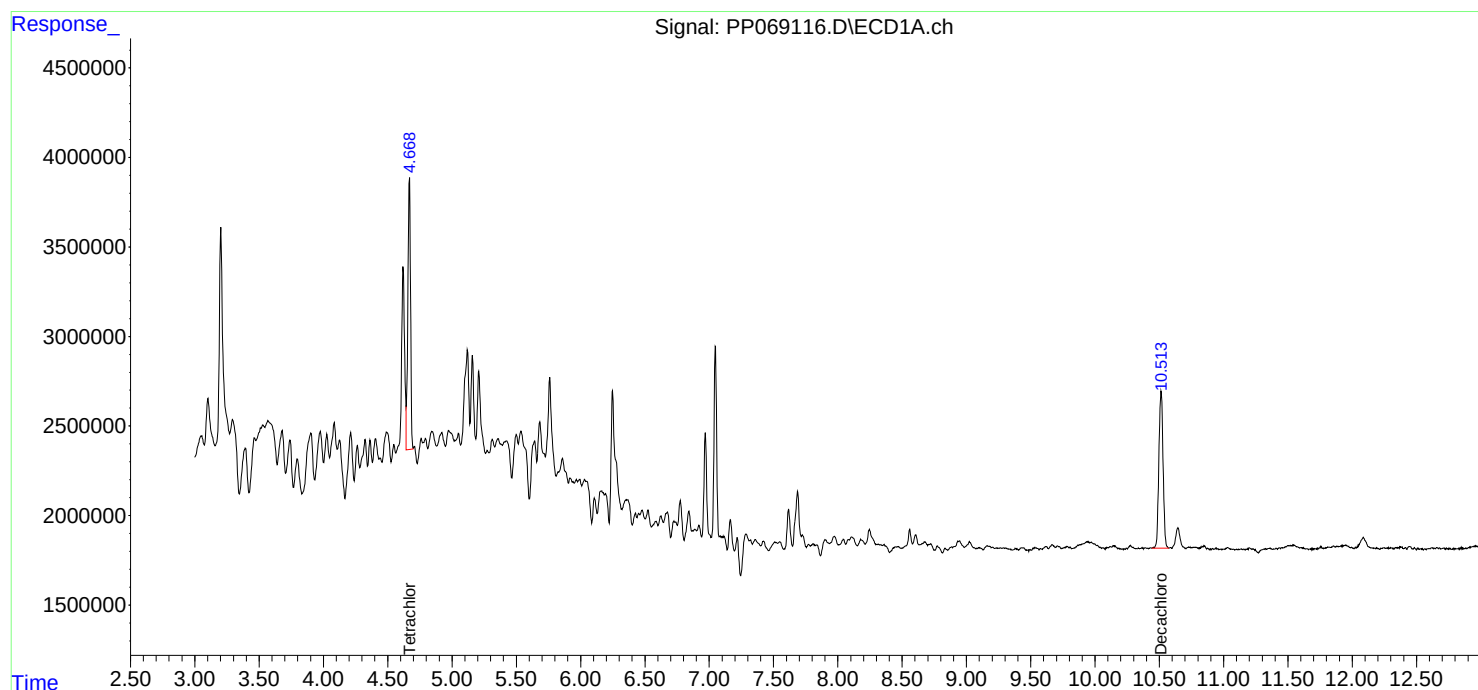

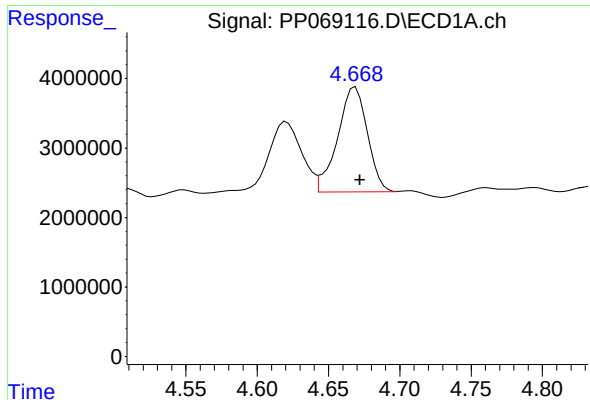


#1 Tetrachloro-m-xylene

R.T.: 4.668 min
Delta R.T.: -0.004 min
Response: 21768997
Conc: 15.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-05-01132025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/15/2025
Supervised By :Ankita Jodhani 01/15/2025

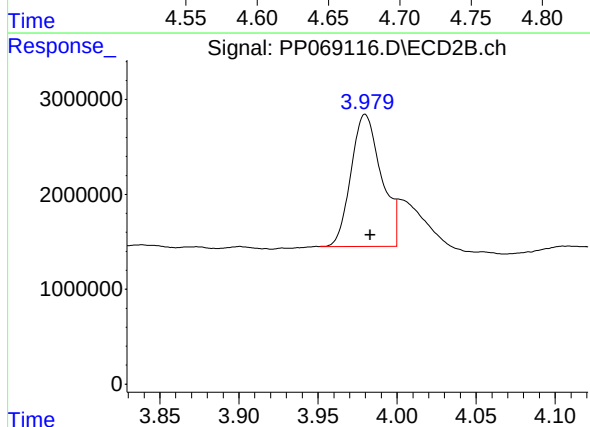


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.004 min
Response: 18608594
Conc: 19.06 ng/ml

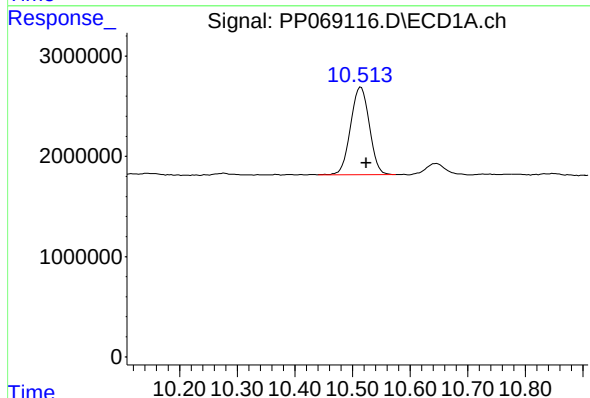

#2 Decachlorobiphenyl

R.T.: 10.514 min
Delta R.T.: -0.010 min
Response: 19749089
Conc: 17.69 ng/ml

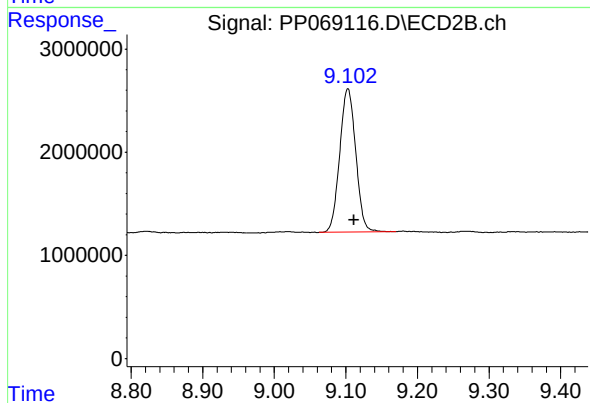

#2 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: -0.009 min
Response: 21660825
Conc: 18.03 ng/ml