

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011521\
 Data File : PP032776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2021 21:34
 Operator : DD\AJ
 Sample : M1096-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 263K-35A

Manual Integrations
 APPROVED

Ankita
 1/15/2021 1:49:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 01:36:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.740	4.011	1280270	903459	22.043	19.206
2) SA Decachlor...	10.575	9.288	668108	671152	16.934	17.915
Target Compounds						
26) L6 AR-1254-1	6.972f	6.129	1625449	150853	978.681	73.683 #
27) L6 AR-1254-2	7.176	6.287	230101	156555	91.493	89.142
28) L6 AR-1254-3	7.553	6.707	428987	468668	159.219	163.188
29) L6 AR-1254-4	7.846	6.947	175649	161904	89.170	97.773
30) L6 AR-1254-5	8.276	7.373	420702	5694800	201.733m	2354.318 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011521\
Data File : PP032776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2021 21:34
Operator : DD\AJ
Sample : M1096-17
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:49:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 01:36:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

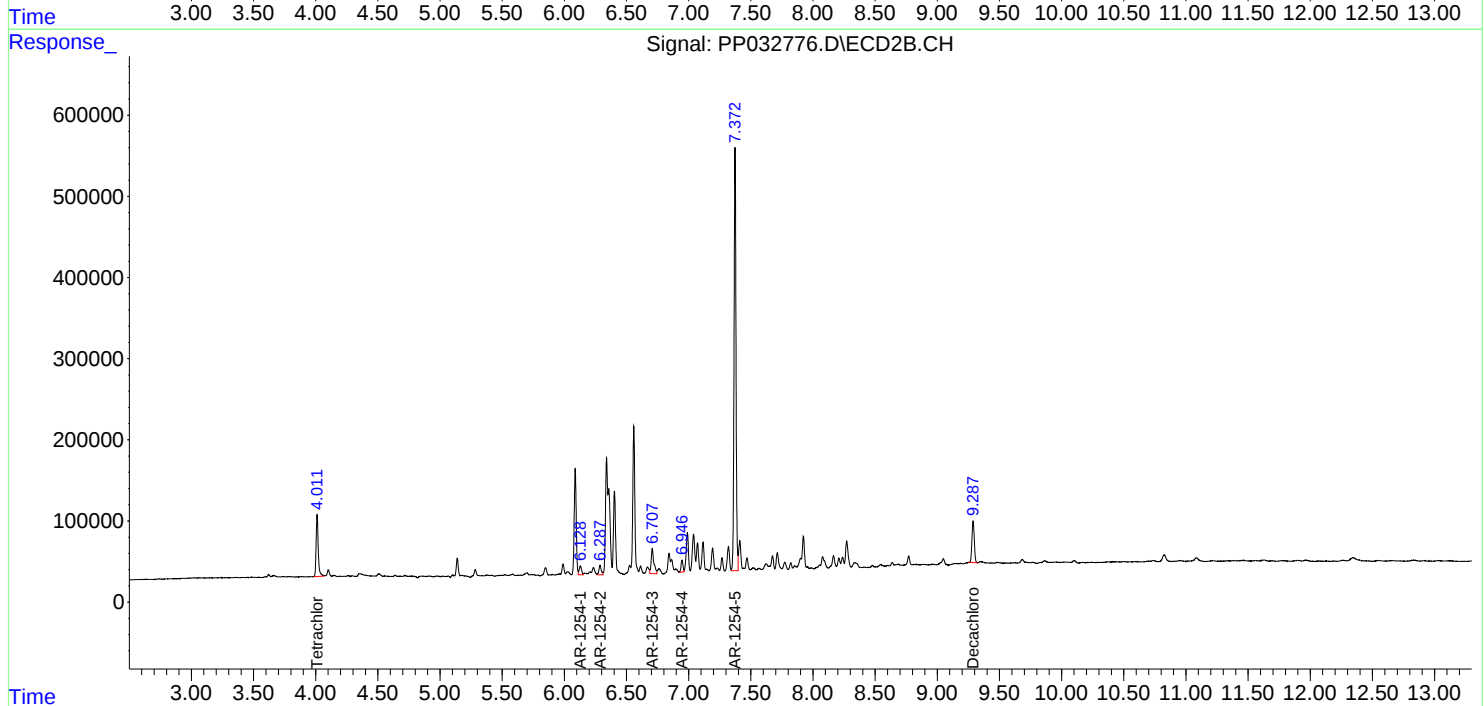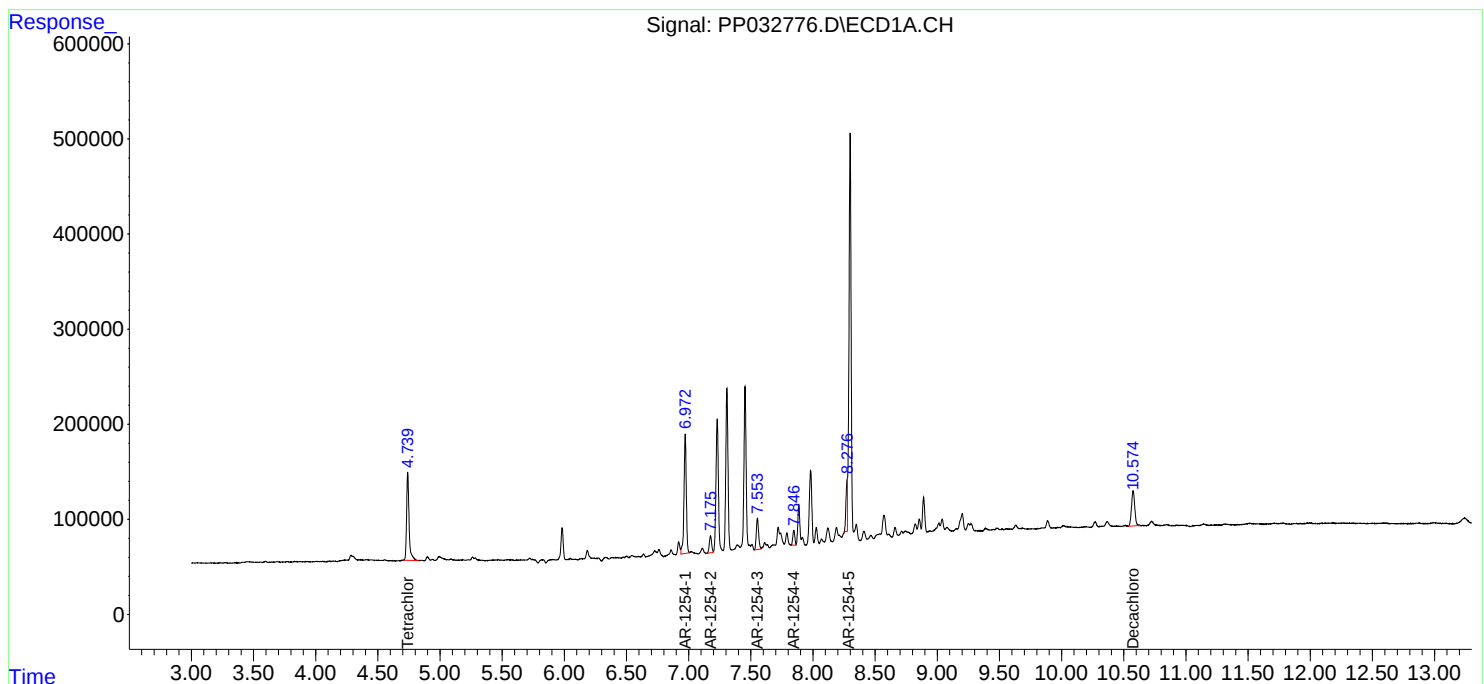

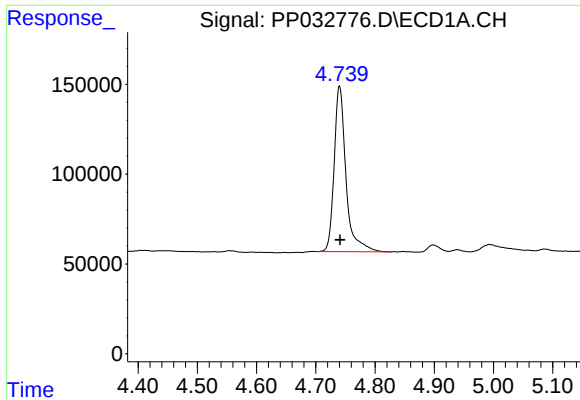


#1 Tetrachloro-m-xylene

R.T.: 4.740 min
Delta R.T.: -0.001 min
Response: 1280270
Conc: 22.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:49:00 PM

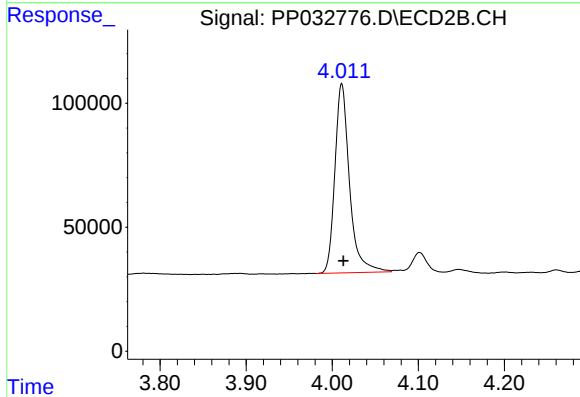


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: -0.002 min
Response: 903459
Conc: 19.21 ng/ml

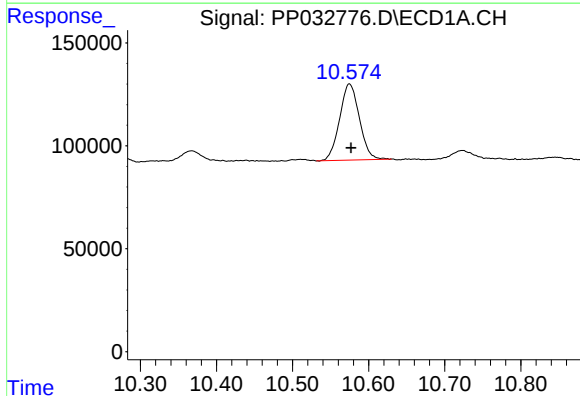


#2 Decachlorobiphenyl

R.T.: 10.575 min
Delta R.T.: -0.002 min
Response: 668108
Conc: 16.93 ng/ml

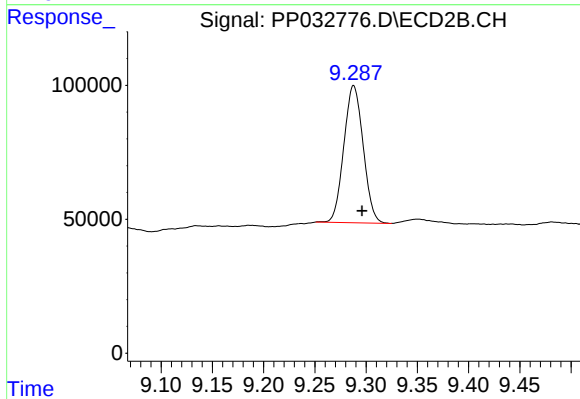

#2 Decachlorobiphenyl

R.T.: 9.288 min
Delta R.T.: -0.008 min
Response: 671152
Conc: 17.92 ng/ml

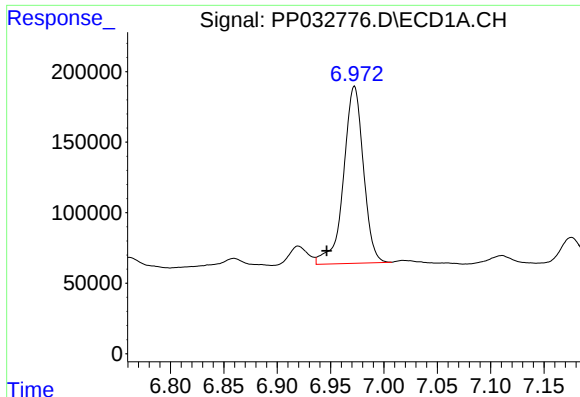


#26 AR-1254-1

R.T.: 6.972 min
Delta R.T.: 0.026 min
Response: 1625449
Conc: 978.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:49:00 PM

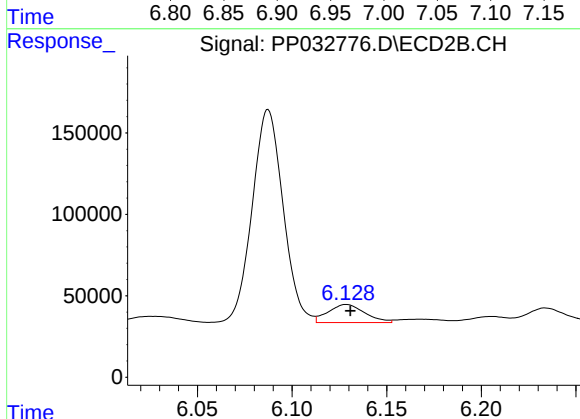


#26 AR-1254-1

R.T.: 6.129 min
Delta R.T.: -0.002 min
Response: 150853
Conc: 73.68 ng/ml

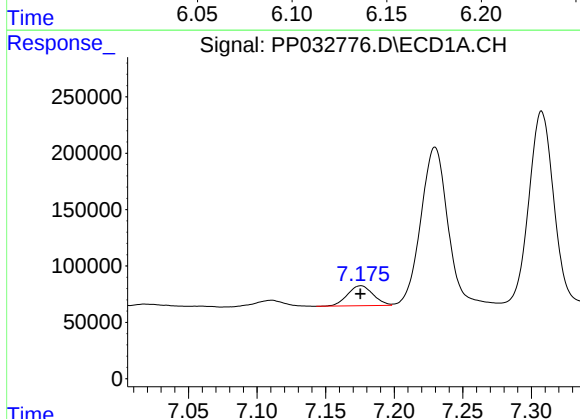


#27 AR-1254-2

R.T.: 7.176 min
Delta R.T.: 0.000 min
Response: 230101
Conc: 91.49 ng/ml

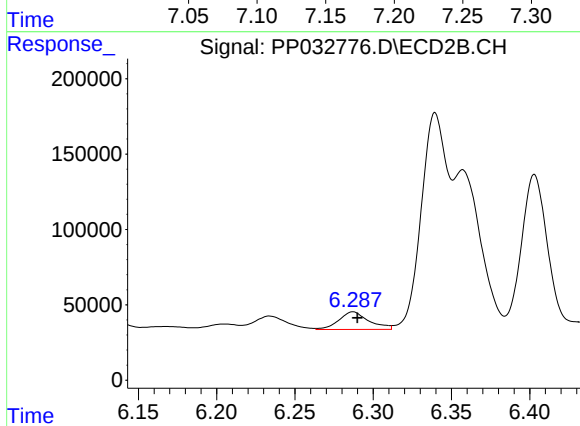

#27 AR-1254-2

R.T.: 6.287 min
Delta R.T.: -0.003 min
Response: 156555
Conc: 89.14 ng/ml

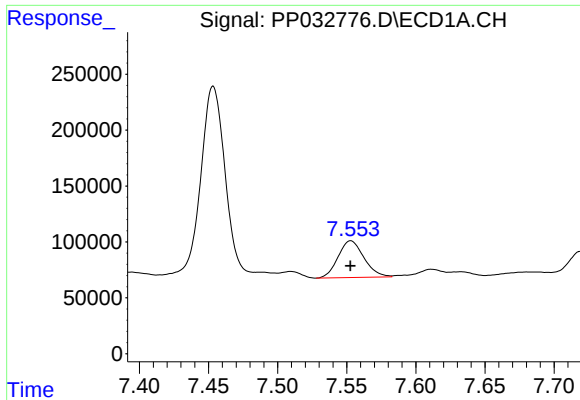


#28 AR-1254-3

R.T.: 7.553 min
Delta R.T.: 0.000 min
Response: 428987
Conc: 159.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
263K-35A


Manual Integrations
APPROVED

Ankita
1/15/2021 1:49:00 PM

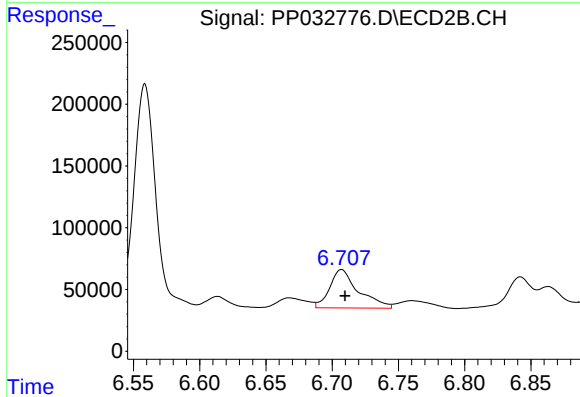


#28 AR-1254-3

R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 468668
Conc: 163.19 ng/ml

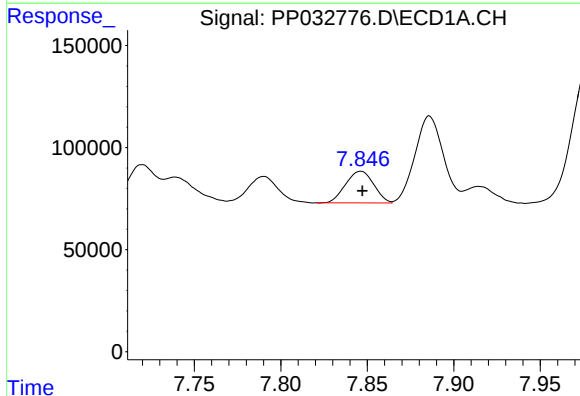


#29 AR-1254-4

R.T.: 7.846 min
Delta R.T.: 0.000 min
Response: 175649
Conc: 89.17 ng/ml

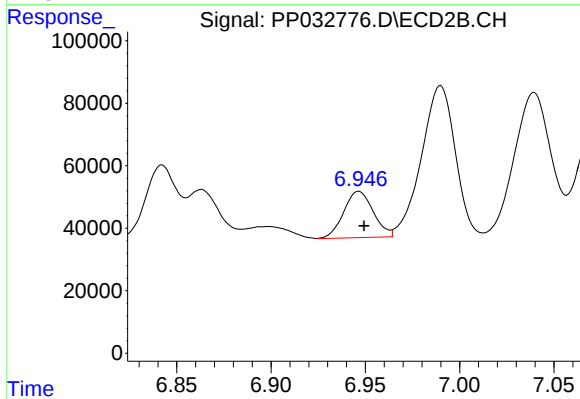

#29 AR-1254-4

R.T.: 6.947 min
Delta R.T.: -0.003 min
Response: 161904
Conc: 97.77 ng/ml

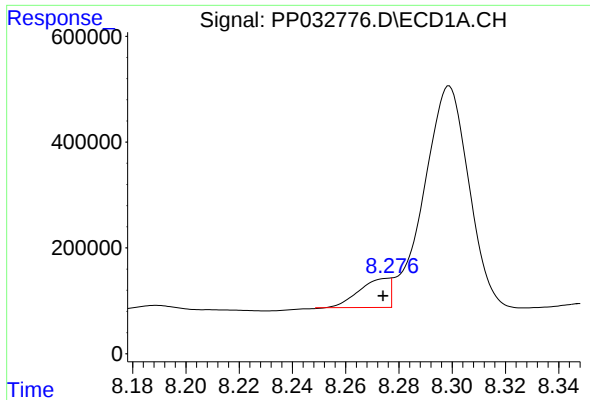


#30 AR-1254-5

R.T.: 8.276 min
Delta R.T.: 0.002 min
Response: 420702
Conc: 201.73 ng/ml m

Instrument :
ECD_P
ClientSampleId :
263K-35A

Manual Integrations
APPROVED

Ankita
1/15/2021 1:49:00 PM

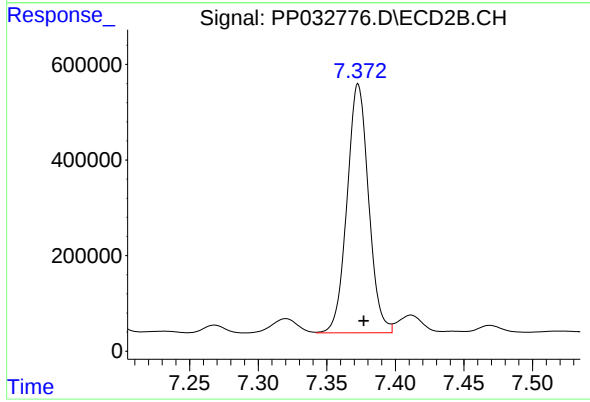

#30 AR-1254-5

R.T.: 7.373 min
Delta R.T.: -0.004 min
Response: 5694800
Conc: 2354.32 ng/ml