

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011621\
 Data File : PP032778.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2021 9:14
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 15 11:55:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 14 08:12:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
24)	L5	AR-1248-4	6.960f	0.000	39402	0	24.293	N.D.	#
26)	L6	AR-1254-1	6.960	0.000	39402	0	23.724	N.D.	#
28)	L6	AR-1254-3	7.564	0.000	33487	0	12.429	N.D.	#
34)	L7	AR-1260-4	8.553f	0.000	13120	0	6.368	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011621\
Data File : PP032778.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2021 9:14
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 15 11:55:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 14 08:12:55 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

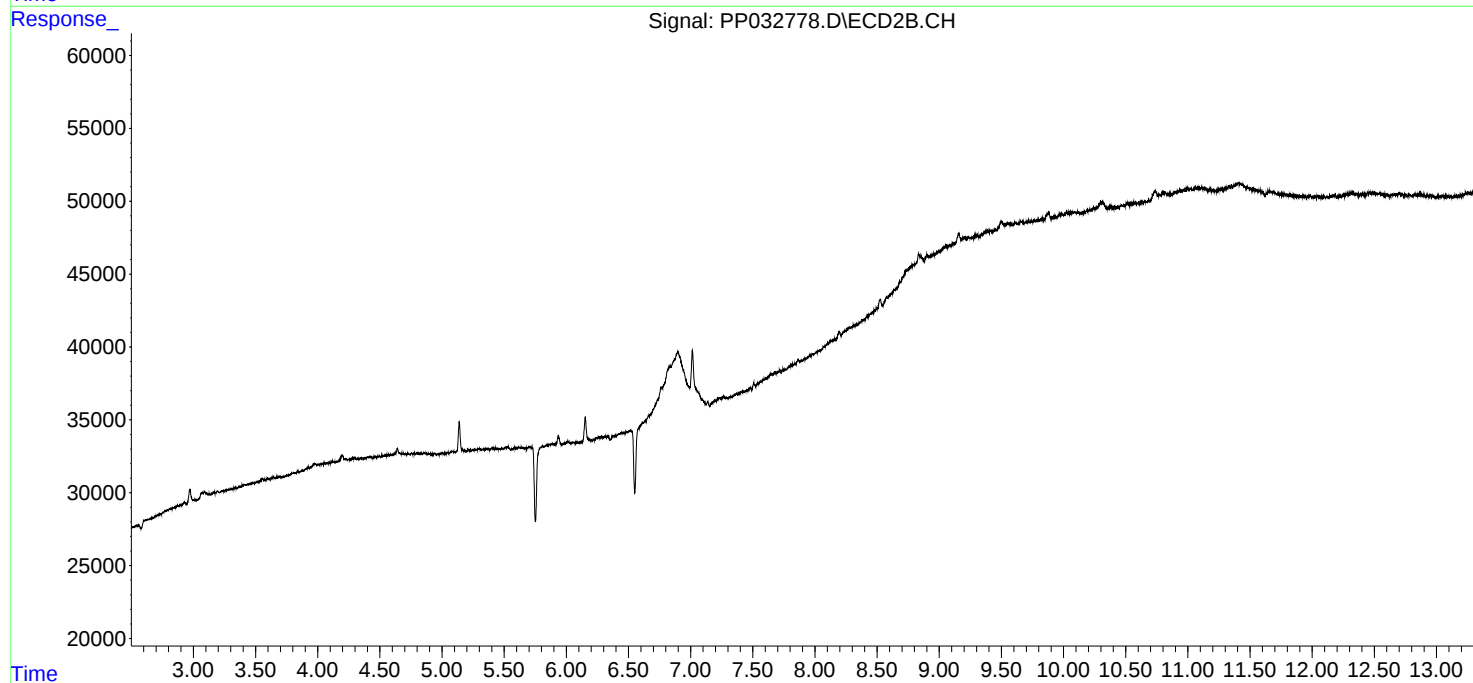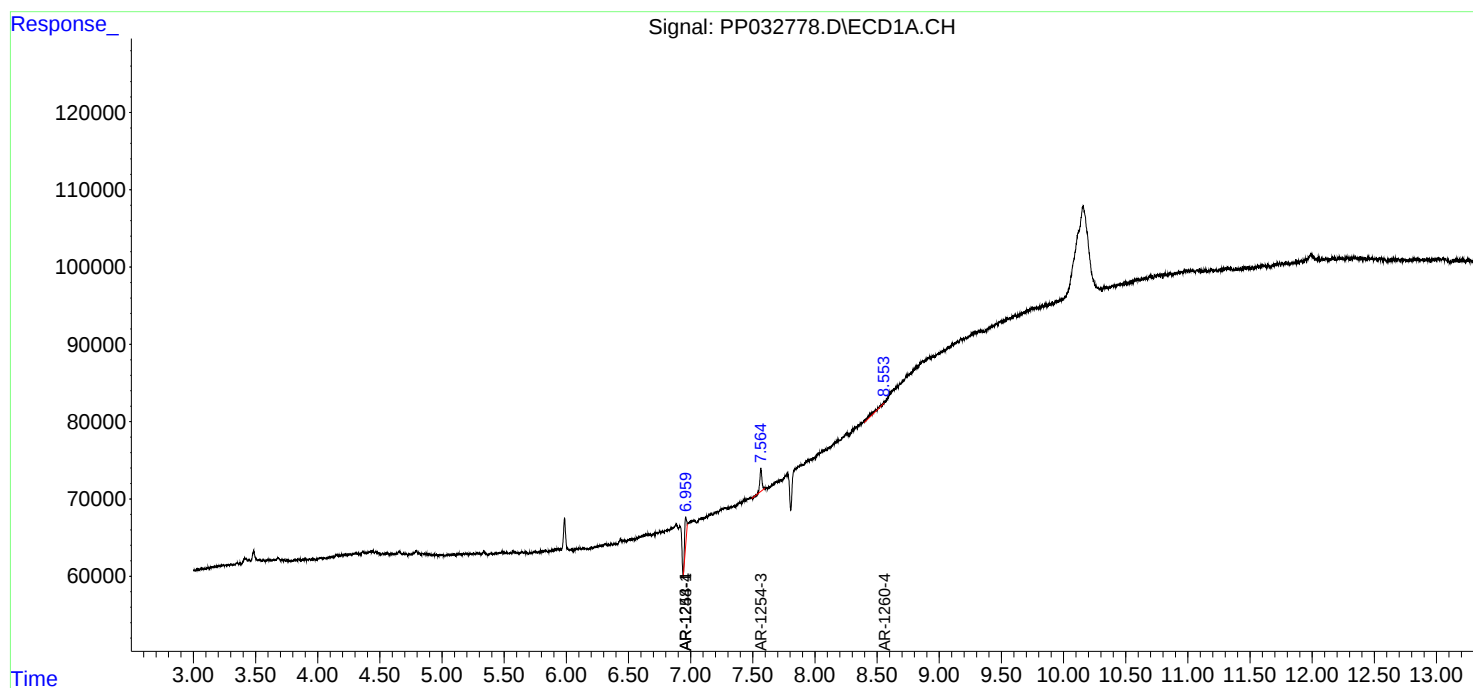


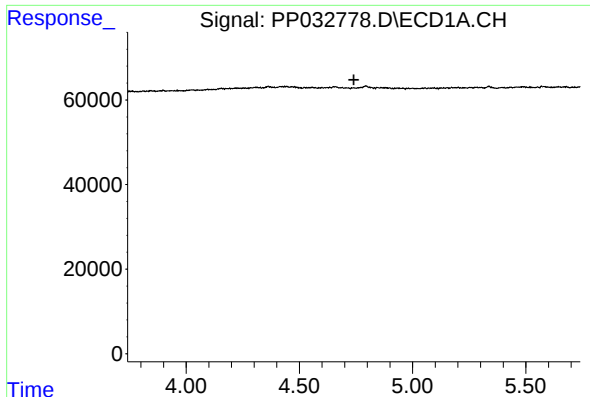

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.741 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
HEXANE

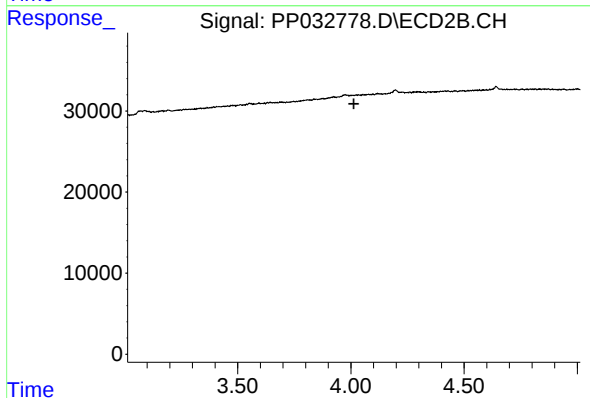


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.013 min
Response: 0
Conc: N.D.

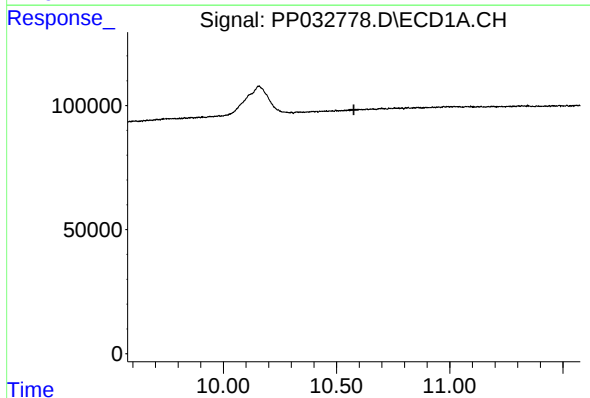


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.577 min
Response: 0
Conc: N.D.

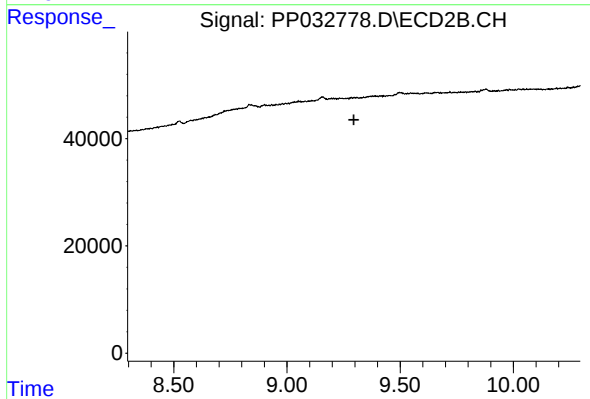

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.296 min
Response: 0
Conc: N.D.

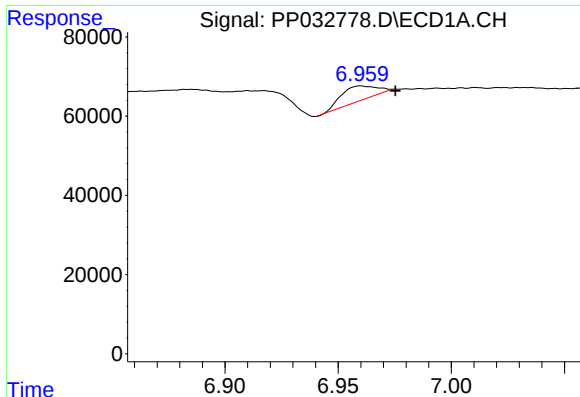

#24 AR-1248-4


R.T.: 6.960 min
Delta R.T.: -0.015 min
Response: 39402
Conc: 24.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

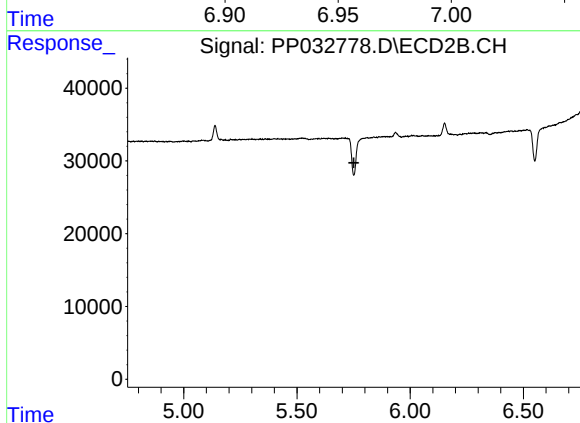


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.752 min
Response: 0
Conc: N.D.

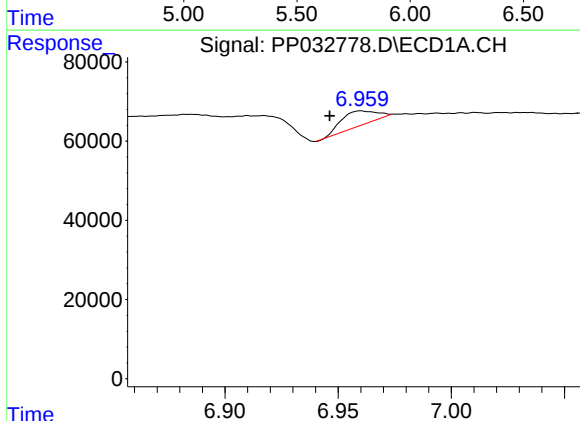


#26 AR-1254-1

R.T.: 6.960 min
Delta R.T.: 0.014 min
Response: 39402
Conc: 23.72 ng/ml

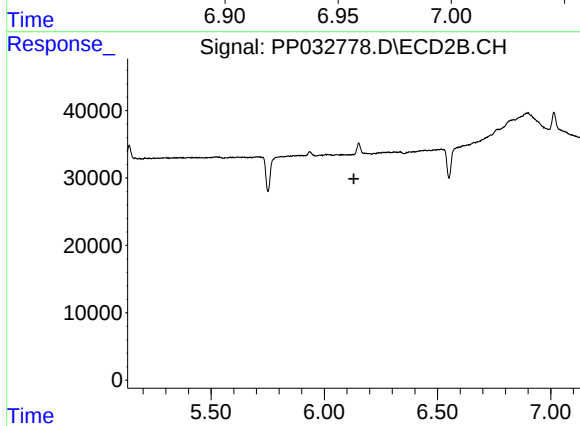

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.131 min
Response: 0
Conc: N.D.

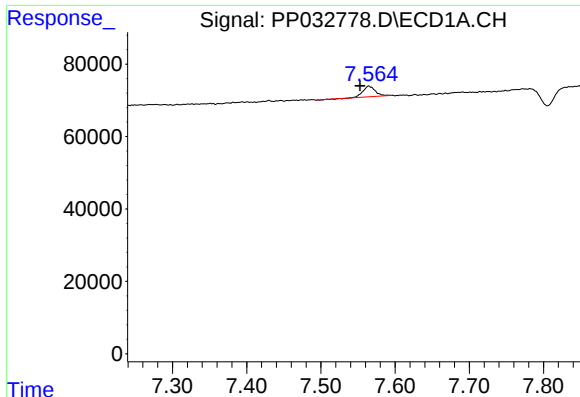

#28 AR-1254-3


R.T.: 7.564 min
Delta R.T.: 0.012 min
Response: 33487
Conc: 12.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
HEXANE

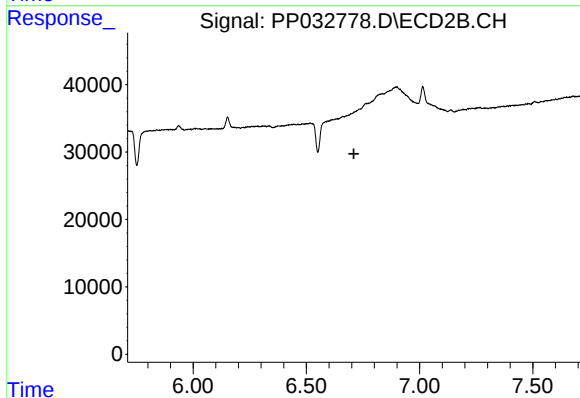


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.710 min
Response: 0
Conc: N.D.

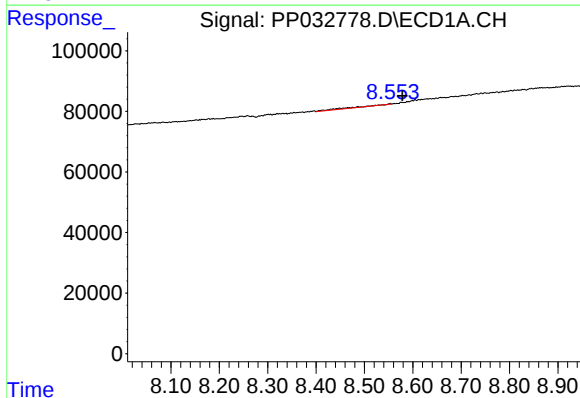

#34 AR-1260-4

R.T.: 8.553 min
Delta R.T.: -0.025 min
Response: 13120
Conc: 6.37 ng/ml

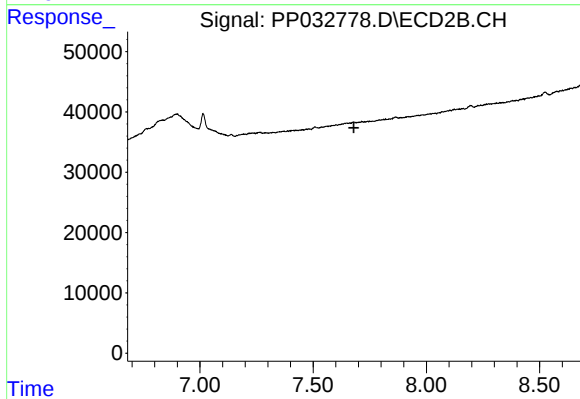

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.680 min
Response: 0
Conc: N.D.