

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011624\
 Data File : PP062943.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2024 20:58
 Operator : YP\AJ
 Sample : P1146-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 4TH-FLOOR-SAMPLE-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 00:51:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 02:58:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.680	65271212	88228401	25.169	25.286
2) SA Decachlor...	10.158	8.784	44394810	64663758	28.073	27.712

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011624\
Data File : PP062943.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2024 20:58
Operator : YP\AJ
Sample : P1146-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
4TH-FLOOR-SAMPLE-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 00:51:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 02:58:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

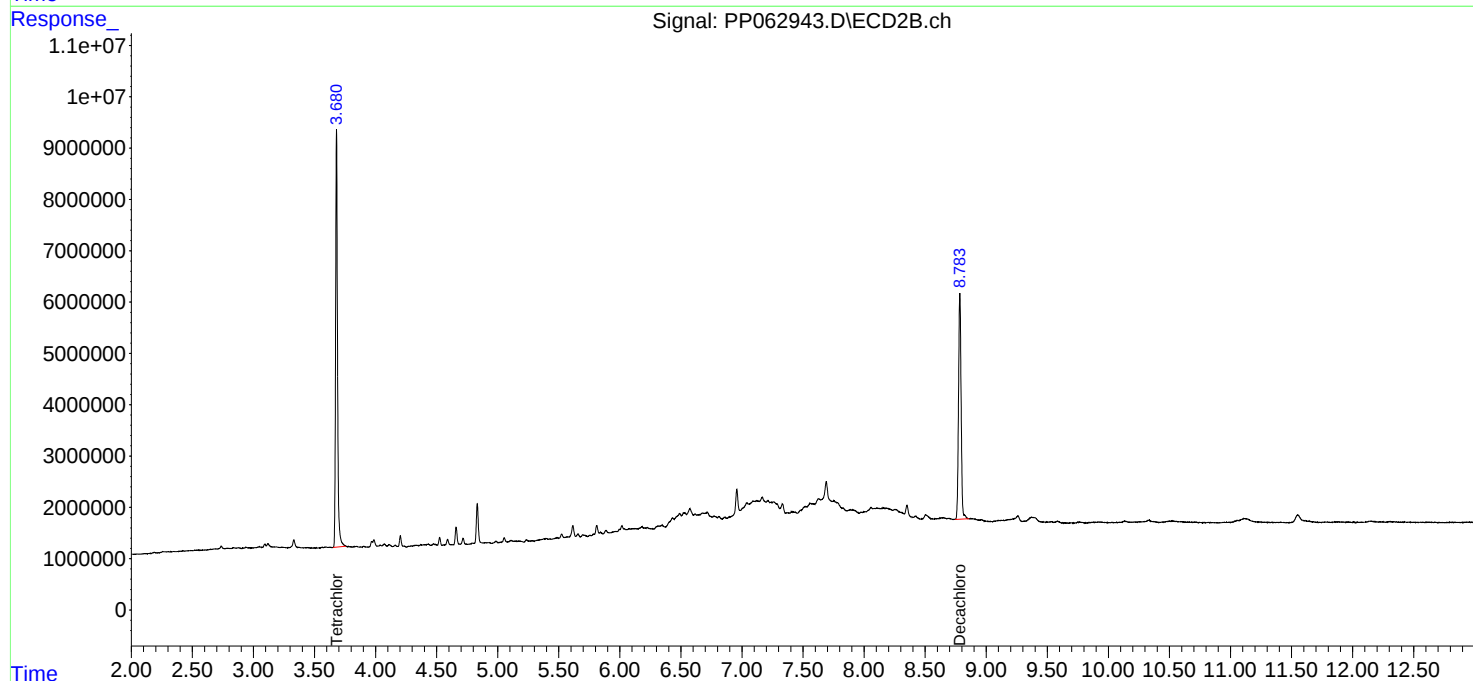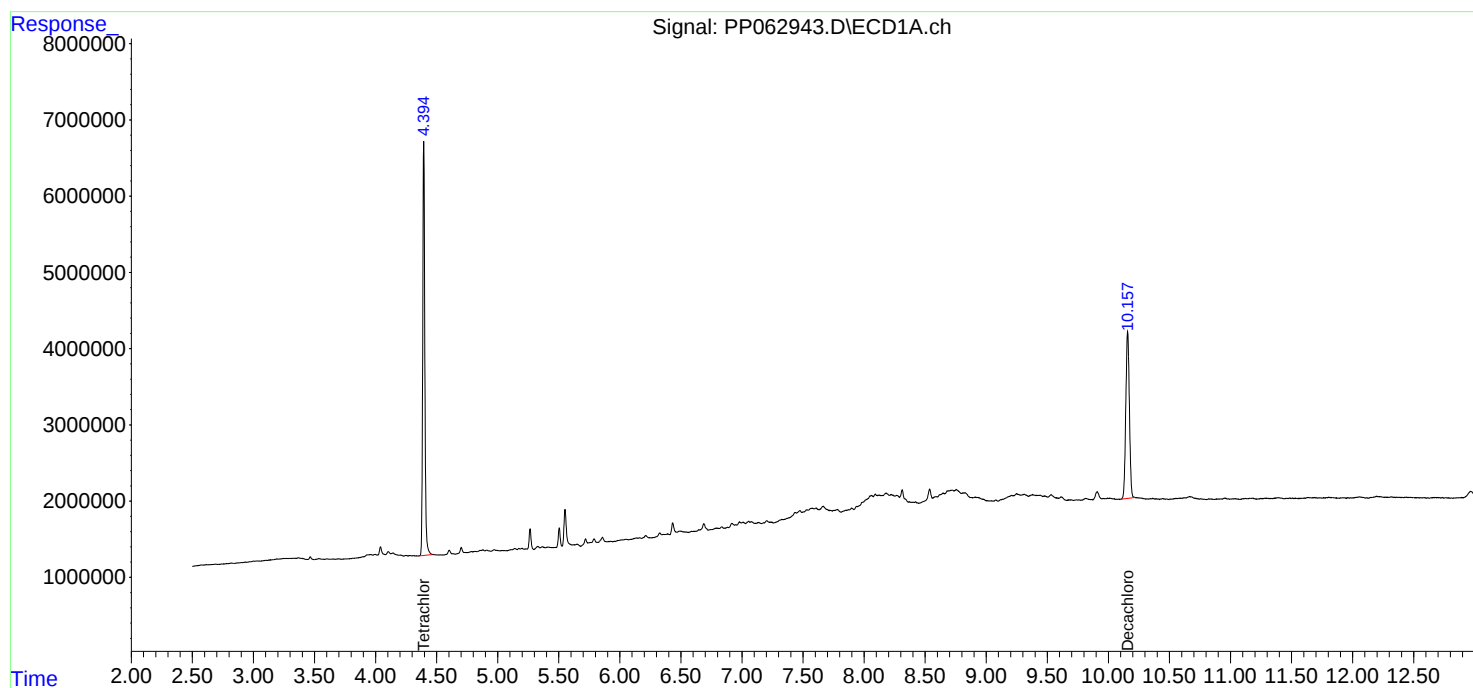


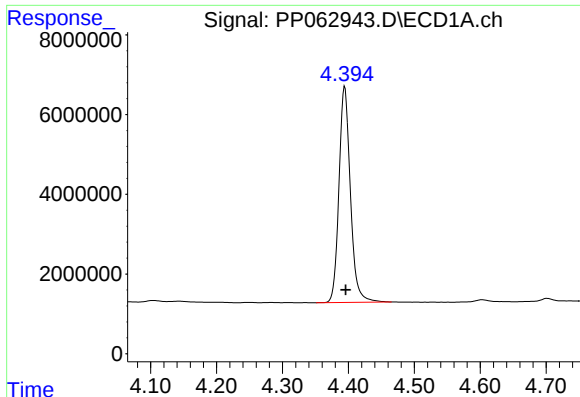

#1 Tetrachloro-m-xylene


R.T.: 4.394 min
Delta R.T.: -0.002 min
Response: 65271212
Conc: 25.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
4TH-FLOOR-SAMPLE-02

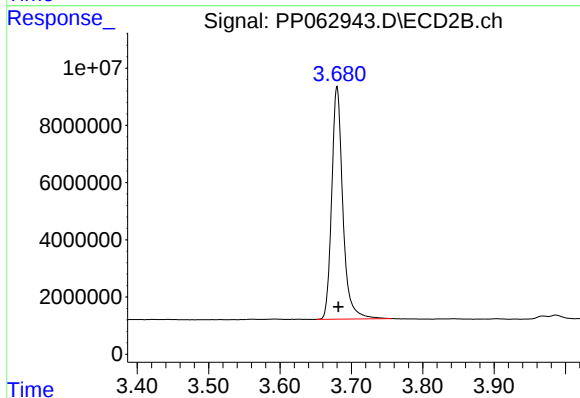


#1 Tetrachloro-m-xylene

R.T.: 3.680 min
Delta R.T.: -0.002 min
Response: 88228401
Conc: 25.29 ng/ml

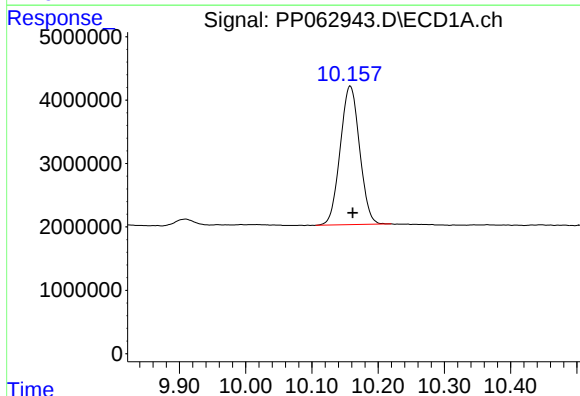

#2 Decachlorobiphenyl

R.T.: 10.158 min
Delta R.T.: -0.004 min
Response: 44394810
Conc: 28.07 ng/ml

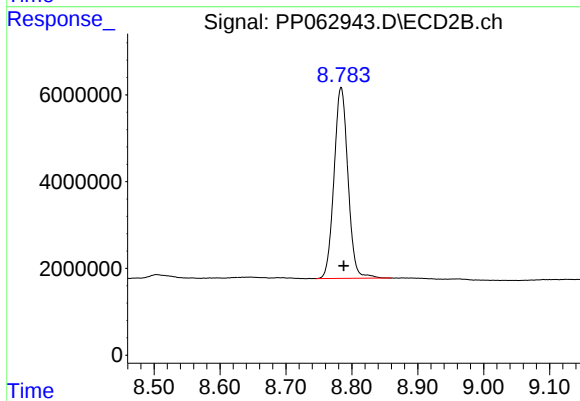

#2 Decachlorobiphenyl

R.T.: 8.784 min
Delta R.T.: -0.004 min
Response: 64663758
Conc: 27.71 ng/ml