

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011625\
 Data File : PP069161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2025 22:28
 Operator : YP\AJ
 Sample : Q1094-03 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 3181

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/17/2025
 Supervised By :Ankita Jodhani 01/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 05:34:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.658	3.974	620327	223407	0.446m	0.229 #
2) SA Decachlor...	10.513	9.104	158357	250416	0.142m	0.208 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011625\
Data File : PP069161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 22:28
Operator : YP\AJ
Sample : Q1094-03 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
3181


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2025
Supervised By :Ankita Jodhani 01/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 05:34:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

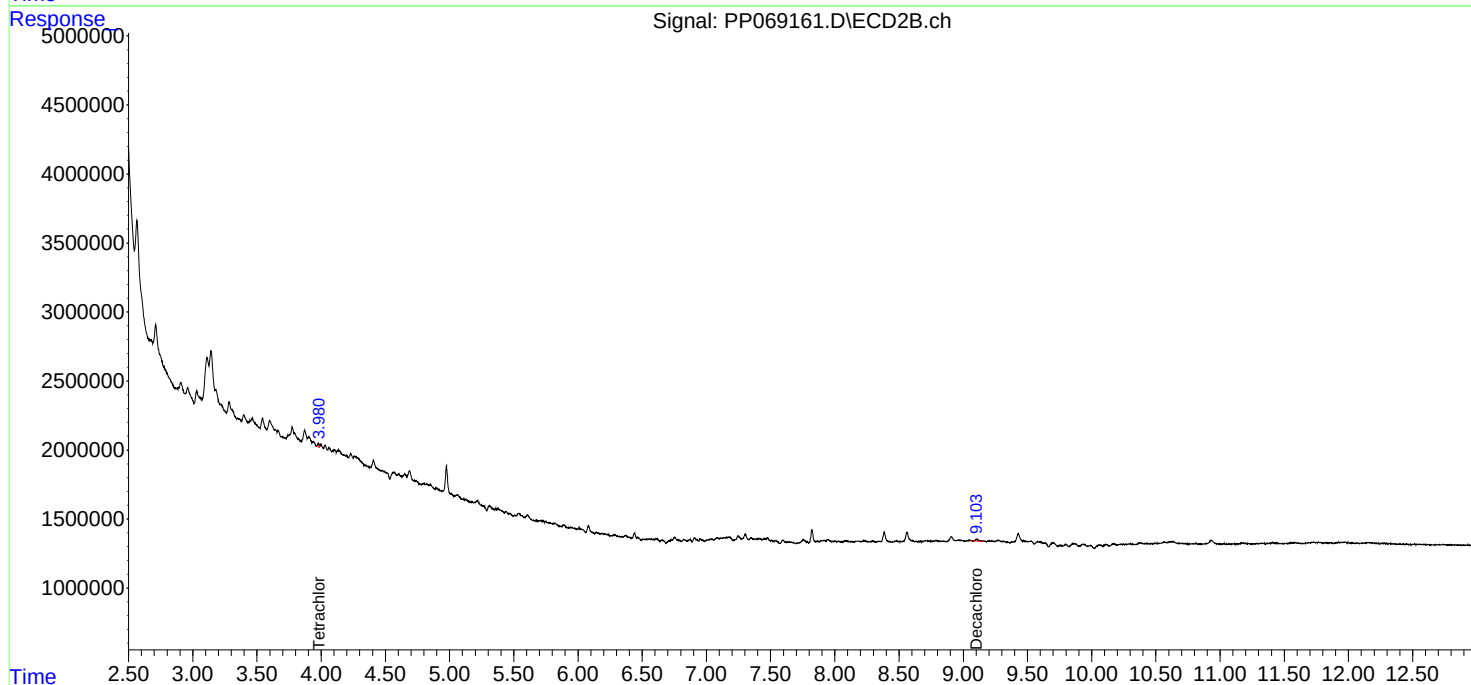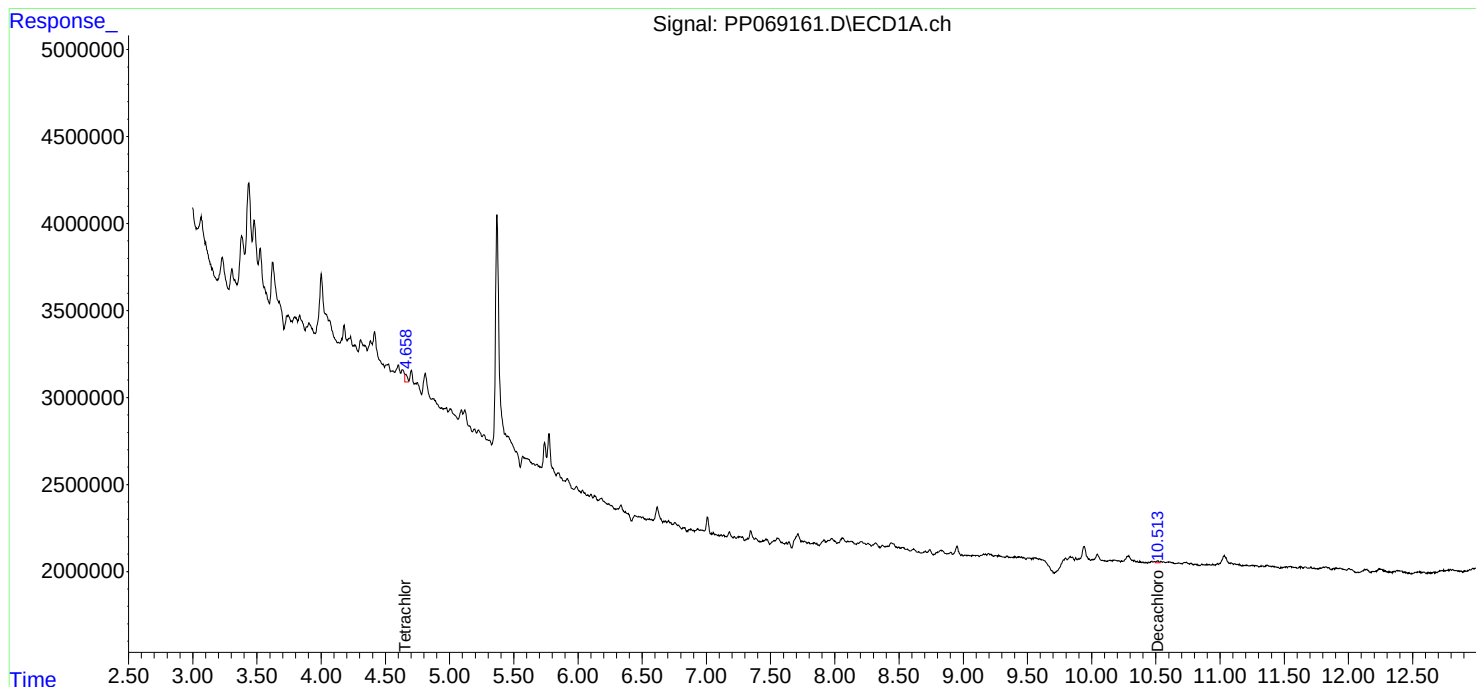

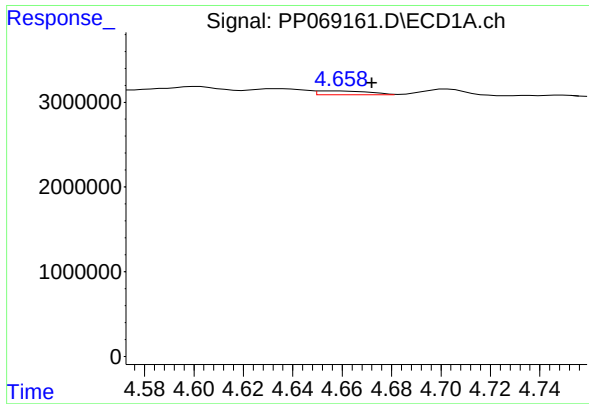


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: -0.014 min
Response: 620327
Conc: 0.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
3181


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2025
Supervised By :Ankita Jodhani 01/17/2025

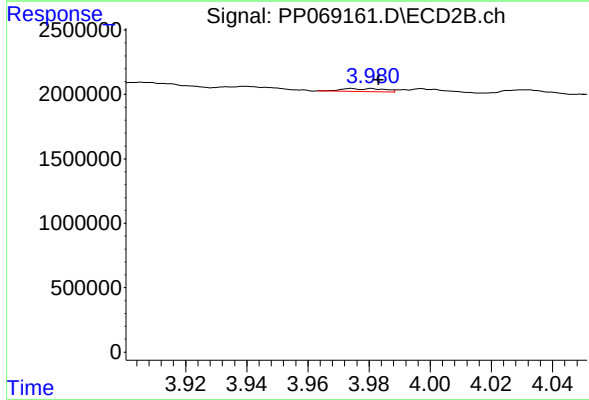


#1 Tetrachloro-m-xylene

R.T.: 3.974 min
Delta R.T.: -0.009 min
Response: 223407
Conc: 0.23 ng/ml

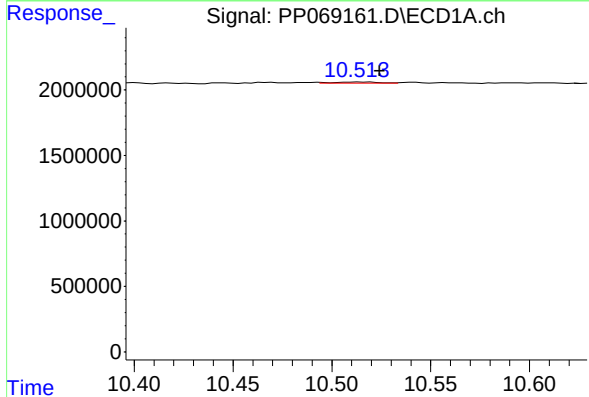

#2 Decachlorobiphenyl

R.T.: 10.513 min
Delta R.T.: -0.012 min
Response: 158357
Conc: 0.14 ng/ml m

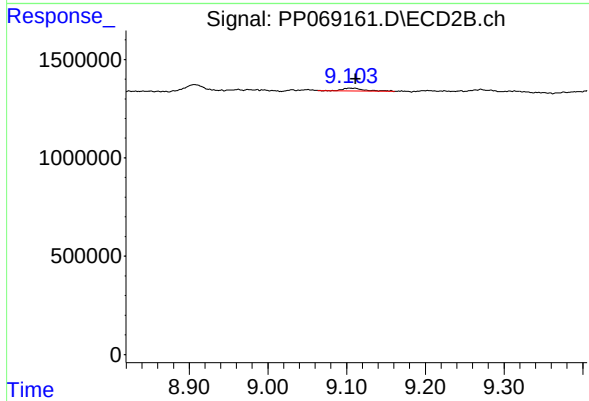

#2 Decachlorobiphenyl

R.T.: 9.104 min
Delta R.T.: -0.008 min
Response: 250416
Conc: 0.21 ng/ml