

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011625\
 Data File : PP069163.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jan 2025 23:01
 Operator : YP\AJ
 Sample : Q1096-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 D3746

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/17/2025
 Supervised By :Ankita Jodhani 01/17/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 05:34:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 07 11:05:55 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.671	3.979	15134710	10441171	10.878	10.696m
2) SA Decachlor...	10.518	9.103	5692195	6099504	5.098	5.077

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011625\
Data File : PP069163.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jan 2025 23:01
Operator : YP\AJ
Sample : Q1096-01
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
D3746


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2025
Supervised By :Ankita Jodhani 01/17/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 05:34:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP010625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 07 11:05:55 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

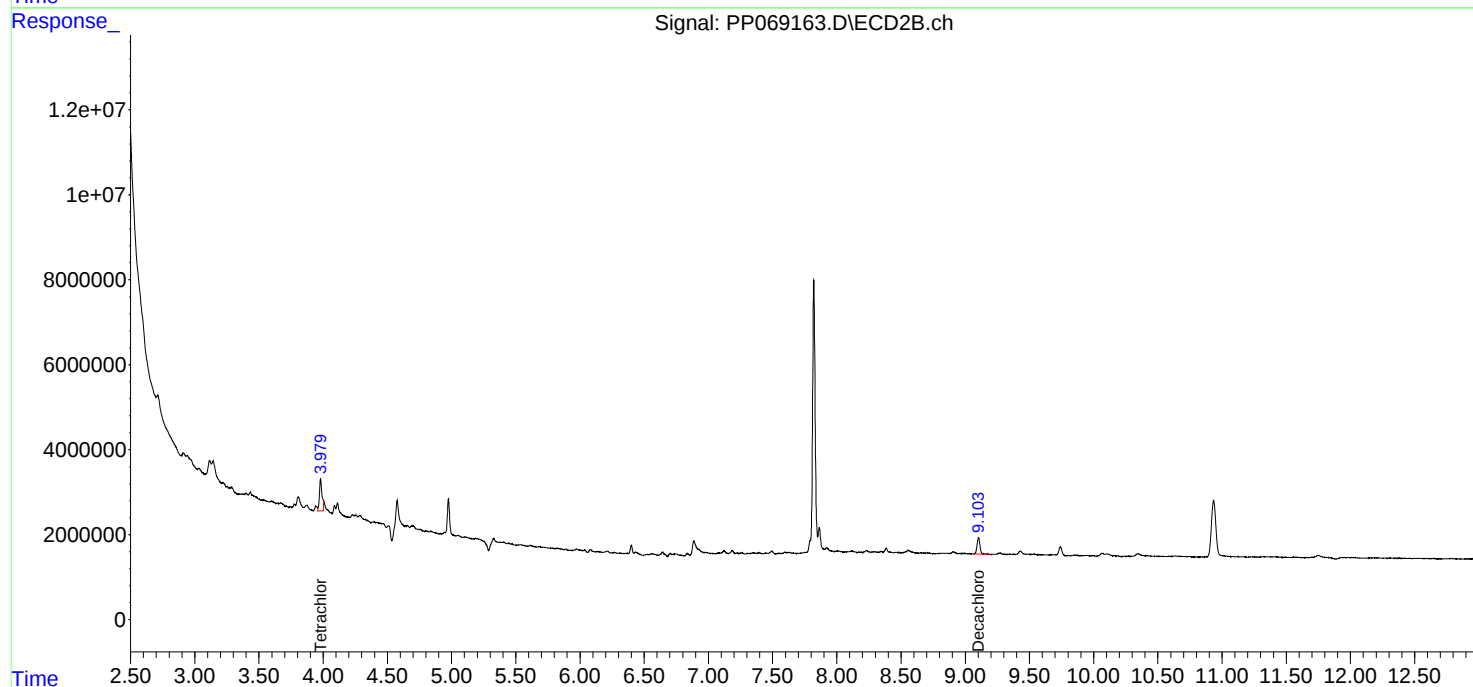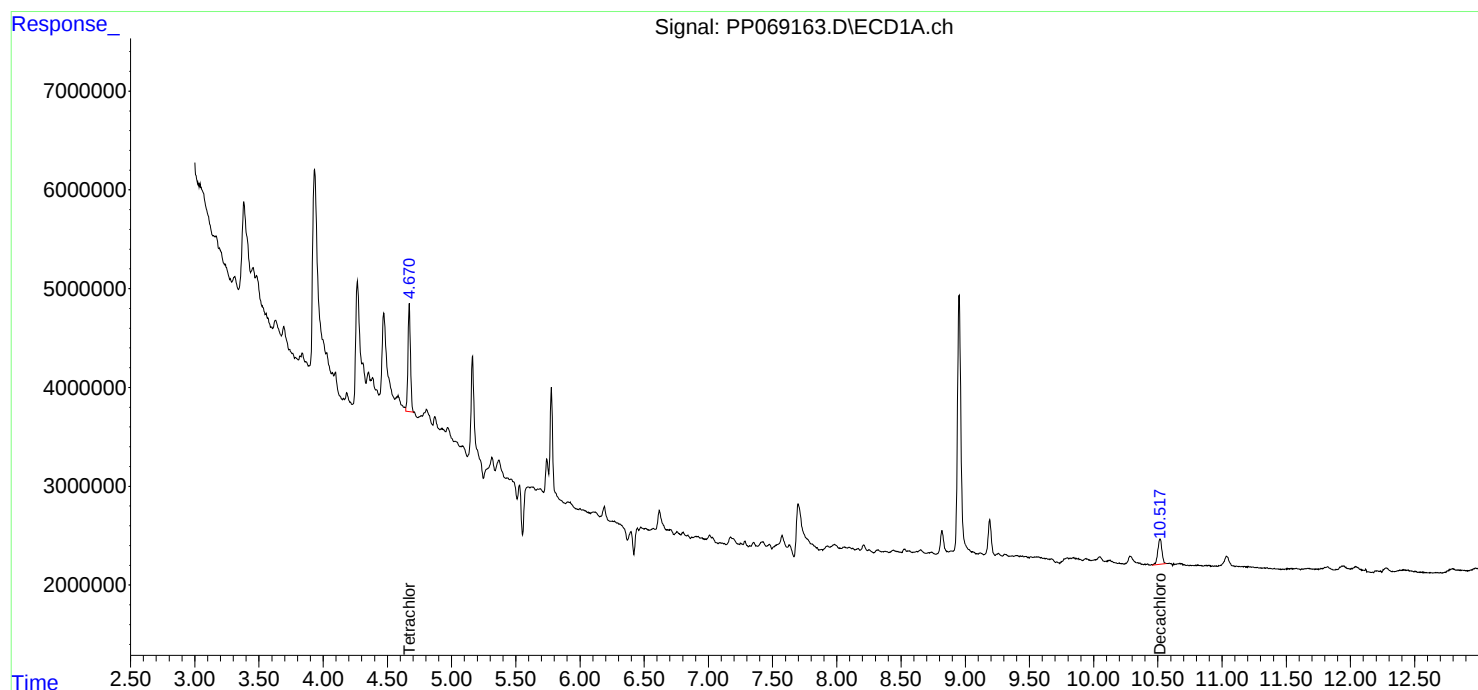

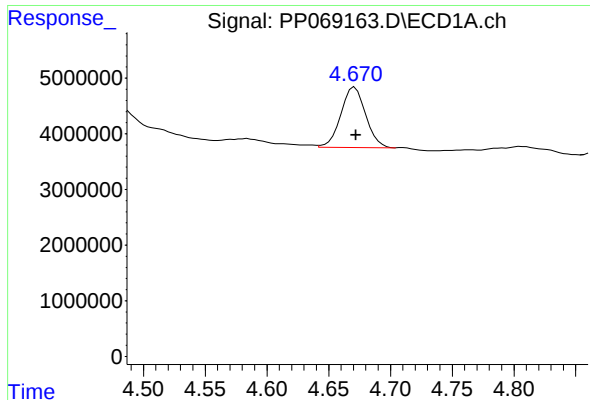


#1 Tetrachloro-m-xylene

R.T.: 4.671 min
Delta R.T.: 0.000 min
Response: 15134710
Conc: 10.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
D3746


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/17/2025
Supervised By :Ankita Jodhani 01/17/2025

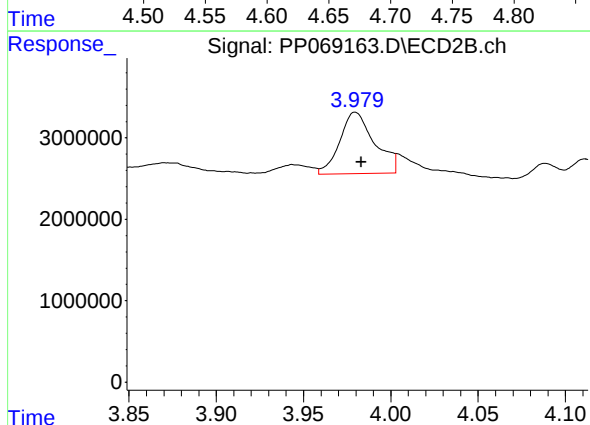


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.004 min
Response: 10441171
Conc: 10.70 ng/ml

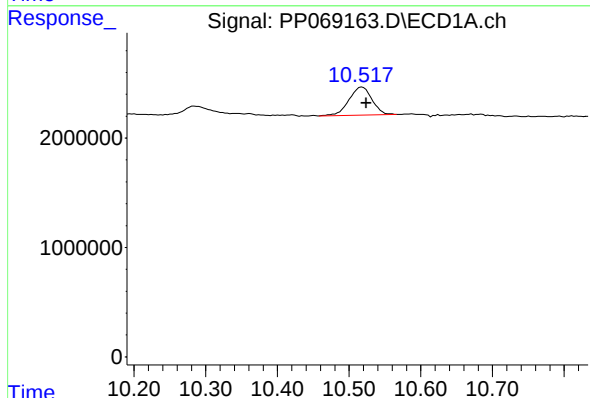

#2 Decachlorobiphenyl

R.T.: 10.518 min
Delta R.T.: -0.006 min
Response: 5692195
Conc: 5.10 ng/ml

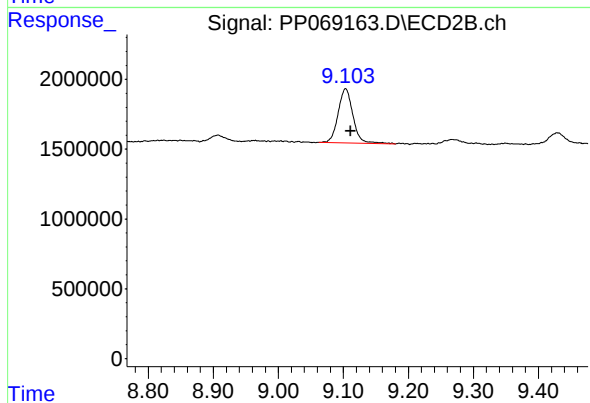

#2 Decachlorobiphenyl

R.T.: 9.103 min
Delta R.T.: -0.008 min
Response: 6099504
Conc: 5.08 ng/ml