

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011719\
 Data File : PP028899.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2019 18:39
 Operator : EI\MA
 Sample : K1147-03MSD
 Misc : hexane
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-1MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:17:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011719.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 17 12:26:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.158	12.269	95845215	147.0E6	371.267	322.213
Target Compounds							
1) T	Dalapon	3.371	3.040	368.3E6	431.6E6	573.300	698.974
2) T	3,5-DICHL...	10.568	10.357	232.2E6	248.1E6	433.166	434.618
5) T	DICAMBA	12.481	12.580	712.1E6	797.6E6	460.485	470.693
6) T	MCP	12.825	12.769	18947624	70593432	39.242	76.529 #
7) T	MCPA	13.064	13.158	132.0E6	141.6E6	171.285	90.262 #
8) T	DICHLORPROP	13.678	13.694	210.6E6	273.4E6	595.745	611.710
9) T	2,4-D	14.031	14.181	307.7E6	373.3E6	865.049	686.006
10) T	Pentachlo...	14.452	14.798	3237.3E6	2798.7E6	419.300	425.735
11) T	2,4,5-TP ...	15.311	15.361	1780.5E6	2727.0E6	637.682	1073.600 #
12) T	2,4,5-T	15.701	16.010	1635.2E6	864.7E6	646.262	403.468 #
13) T	2,4-DB	16.465	16.607	184.5E6	193.6E6	831.085	664.837
14) T	DINOSEB	17.958	17.002	720.3E6	611.0E6	301.748	327.630
15) T	Picloram	17.723	18.386	1907.5E6	1665.6E6	446.994	456.922
16) T	DCPA	18.322	18.264	1457.9E6	1238.1E6	346.447	381.821



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011719\
Data File : PP028899.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2019 18:39
Operator : EI\MA
Sample : K1147-03MSD
Misc : hexane
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:17:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011719.M
Quant Title : 8080.M
QLast Update : Thu Jan 17 12:26:40 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

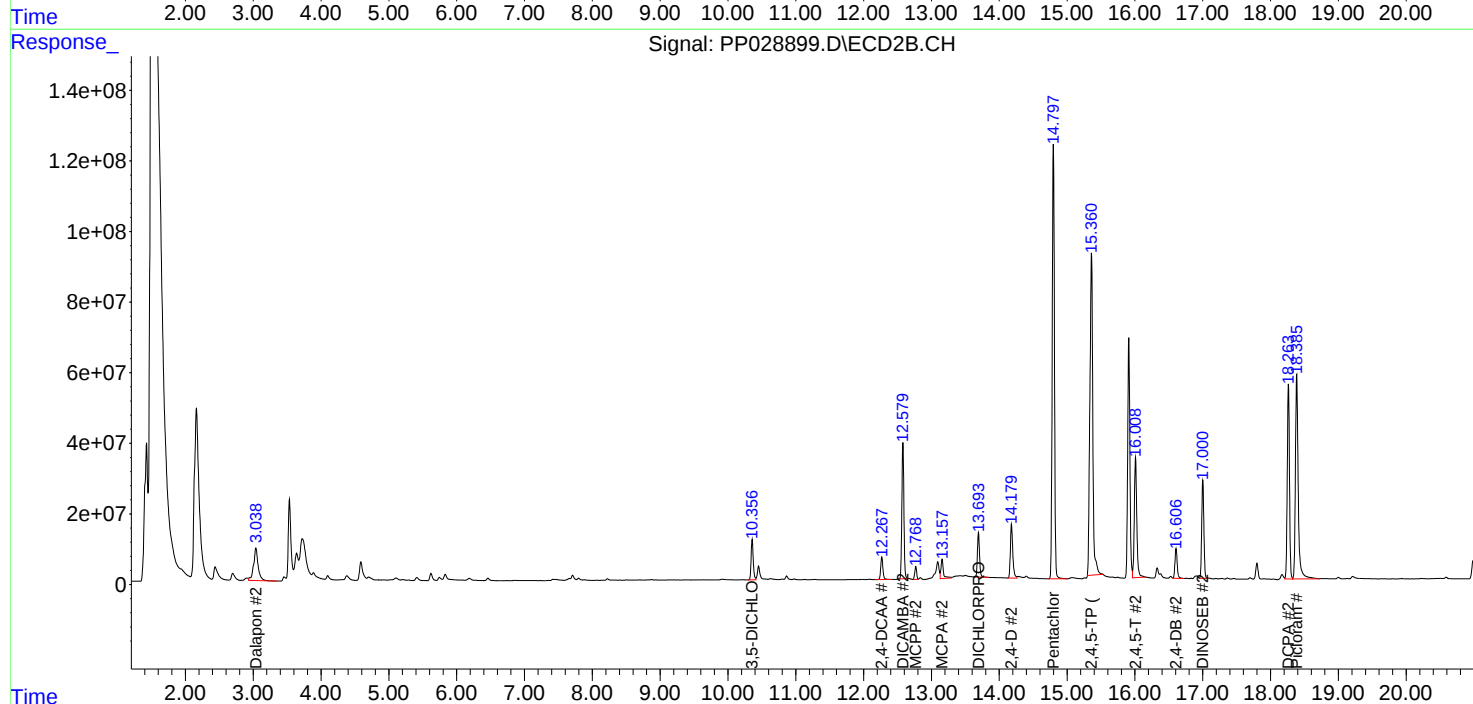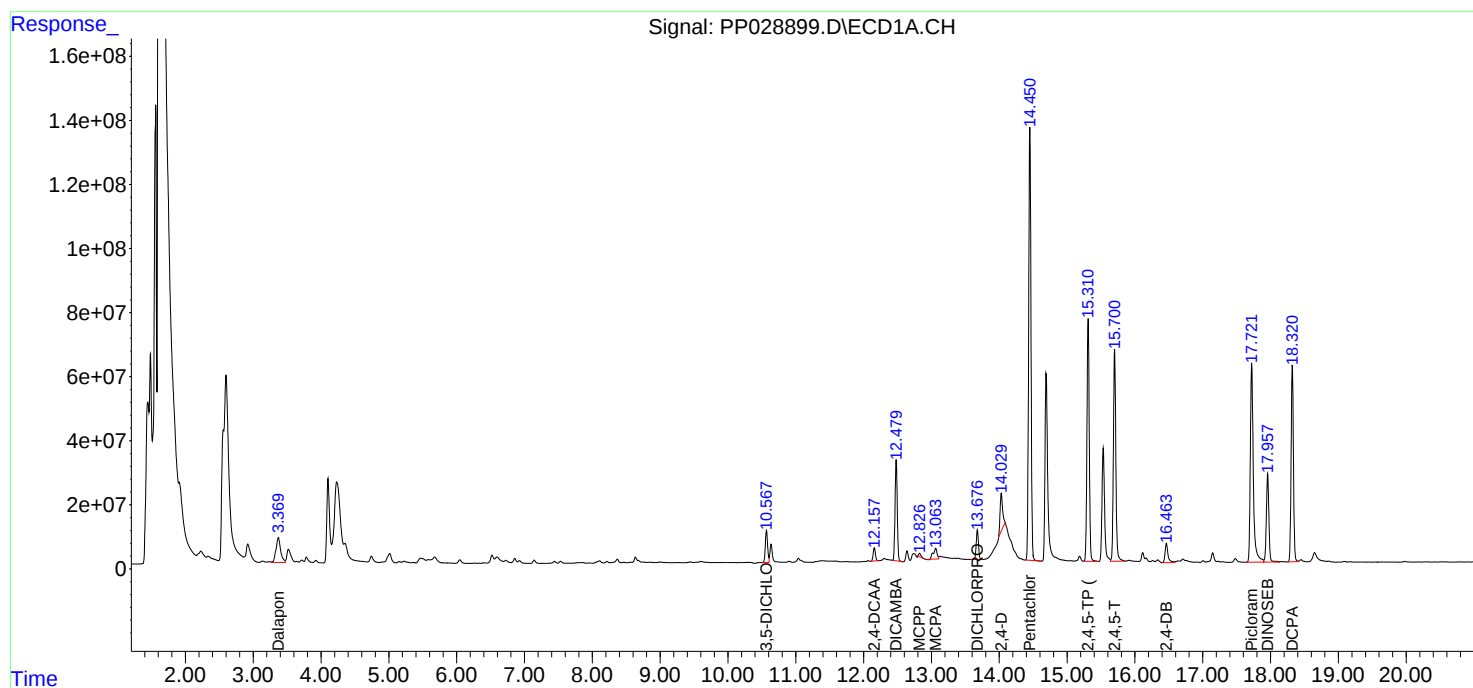


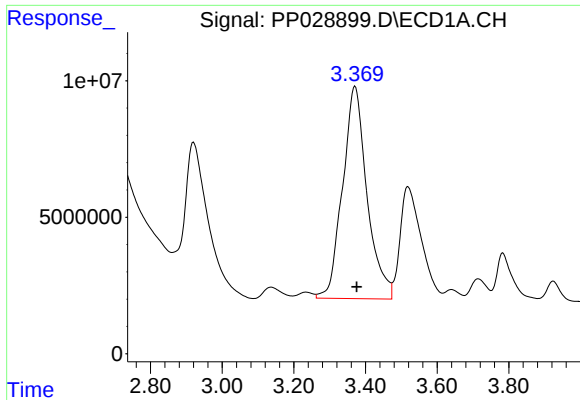

#1 Dalapon


R.T.: 3.371 min
Delta R.T.: -0.004 min
Response: 368268901
Conc: 573.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

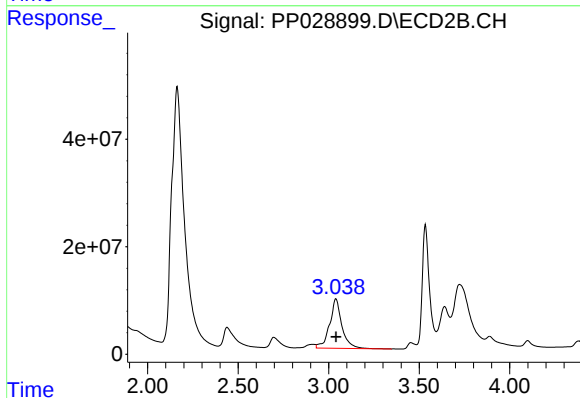


#1 Dalapon

R.T.: 3.040 min
Delta R.T.: -0.002 min
Response: 431642358
Conc: 698.97 ng/ml

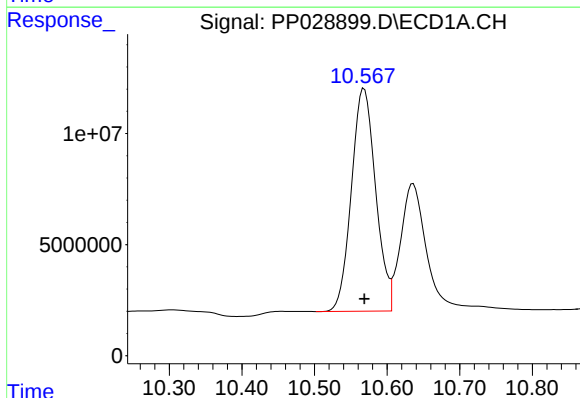


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.568 min
Delta R.T.: 0.000 min
Response: 232236436
Conc: 433.17 ng/ml

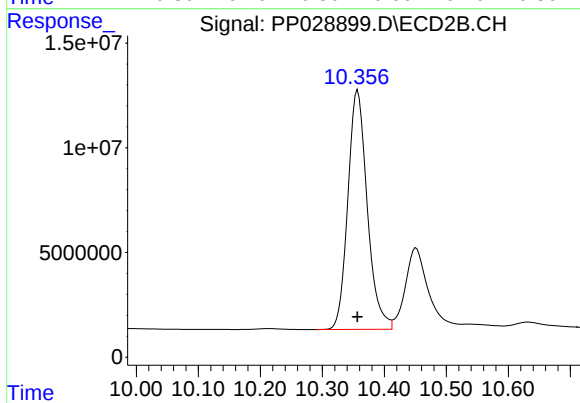

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 10.357 min
Delta R.T.: 0.000 min
Response: 248077715
Conc: 434.62 ng/ml

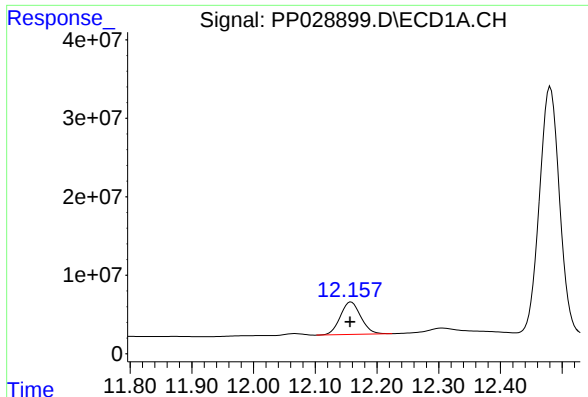

#4 2,4-DCAA


R.T.: 12.158 min
Delta R.T.: 0.001 min
Response: 95845215
Conc: 371.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

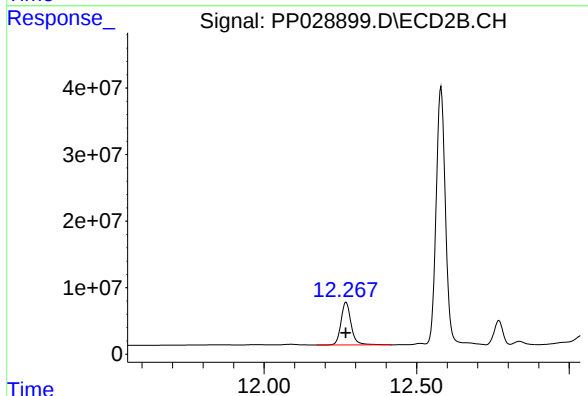


#4 2,4-DCAA

R.T.: 12.269 min
Delta R.T.: 0.000 min
Response: 146973380
Conc: 322.21 ng/ml

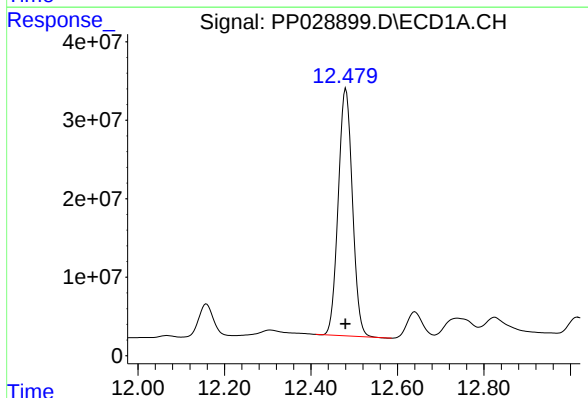


#5 DICAMBA

R.T.: 12.481 min
Delta R.T.: 0.000 min
Response: 712080090
Conc: 460.49 ng/ml

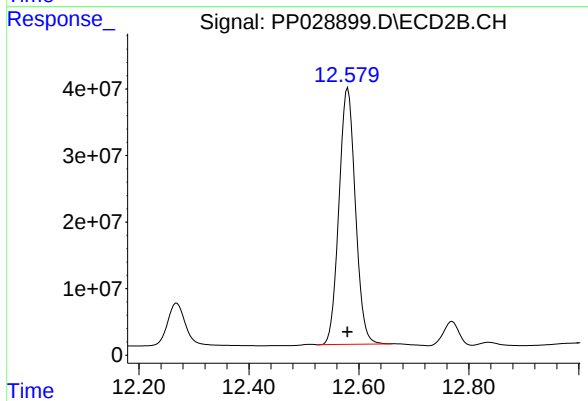

#5 DICAMBA


R.T.: 12.580 min
Delta R.T.: 0.001 min
Response: 797631469
Conc: 470.69 ng/ml

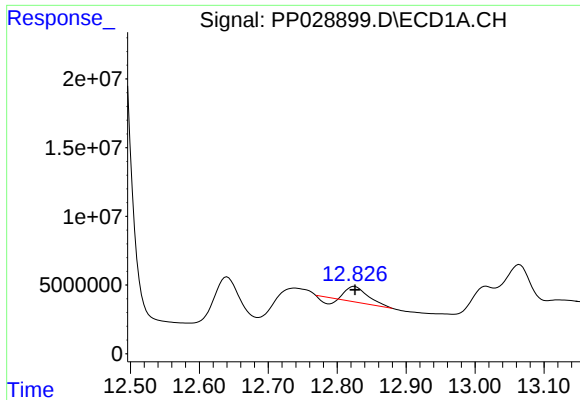

#6 MCP


R.T.: 12.825 min
Delta R.T.: -0.001 min
Response: 18947624
Conc: 39.24 ug/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

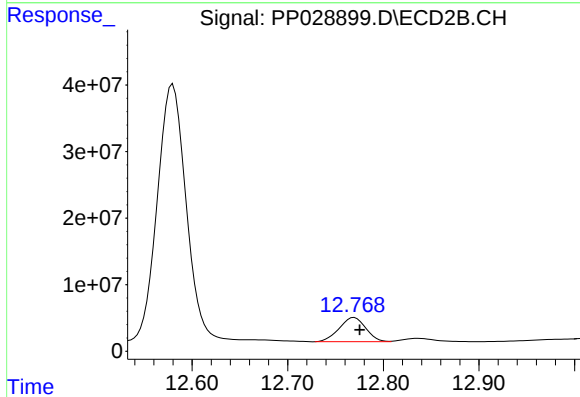


#6 MCP

R.T.: 12.769 min
Delta R.T.: -0.006 min
Response: 70593432
Conc: 76.53 ug/ml

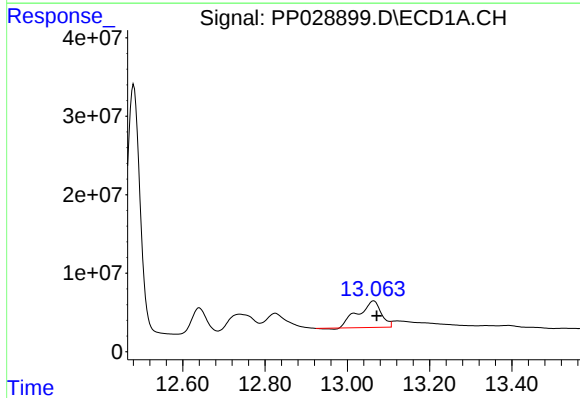


#7 MCPA

R.T.: 13.064 min
Delta R.T.: -0.008 min
Response: 132000604
Conc: 171.28 ug/ml

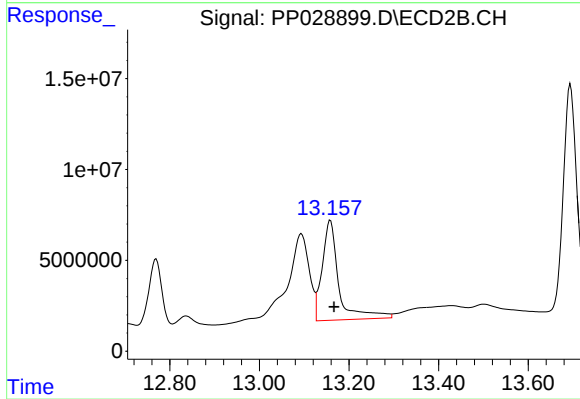

#7 MCPA


R.T.: 13.158 min
Delta R.T.: -0.008 min
Response: 141563565
Conc: 90.26 ug/ml

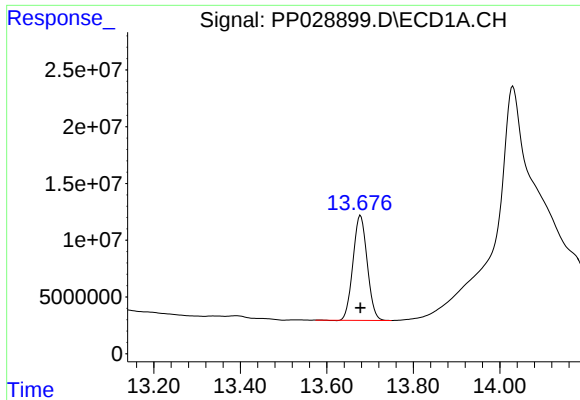

#8 DICHLORPROP


R.T.: 13.678 min
Delta R.T.: 0.000 min
Response: 210576680
Conc: 595.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

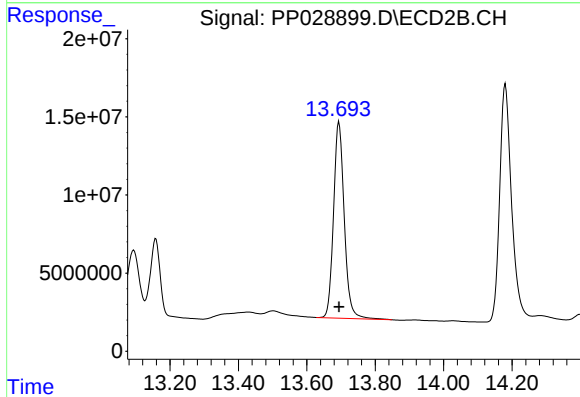


#8 DICHLORPROP

R.T.: 13.694 min
Delta R.T.: 0.000 min
Response: 273375830
Conc: 611.71 ng/ml

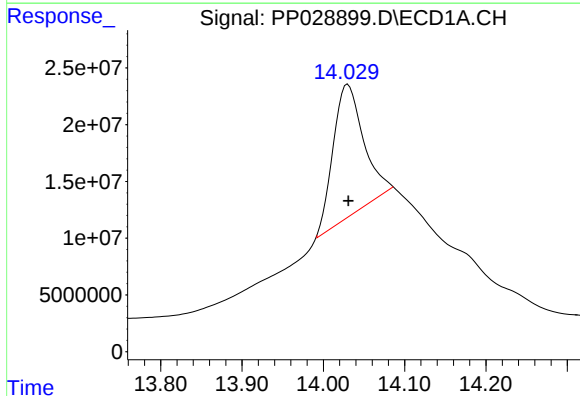


#9 2,4-D

R.T.: 14.031 min
Delta R.T.: 0.000 min
Response: 307699048
Conc: 865.05 ng/ml

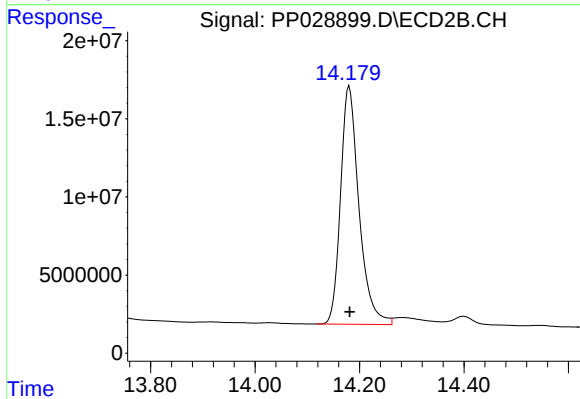

#9 2,4-D


R.T.: 14.181 min
Delta R.T.: 0.000 min
Response: 373318179
Conc: 686.01 ng/ml

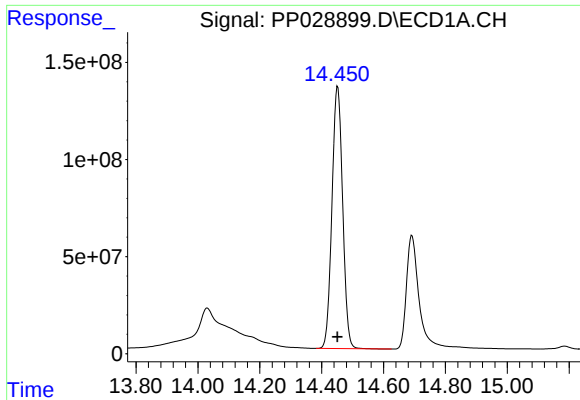

#10 Pentachlorophenol


R.T.: 14.452 min
Delta R.T.: 0.000 min
Response: 3237316798
Conc: 419.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

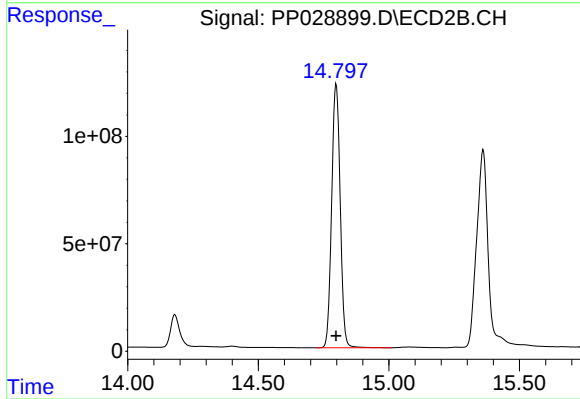


#10 Pentachlorophenol

R.T.: 14.798 min
Delta R.T.: 0.000 min
Response: 2798693113
Conc: 425.73 ng/ml

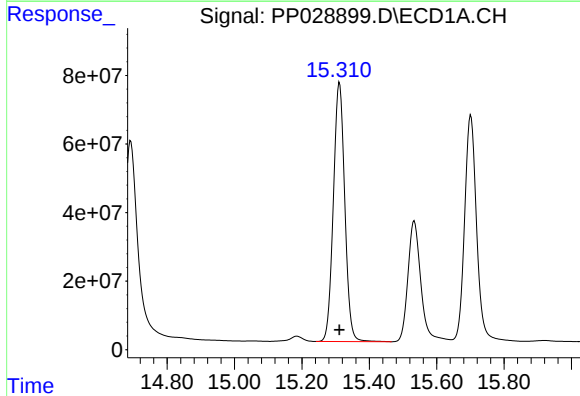


#11 2,4,5-TP (SILVEX)

R.T.: 15.311 min
Delta R.T.: 0.000 min
Response: 1780451442
Conc: 637.68 ng/ml

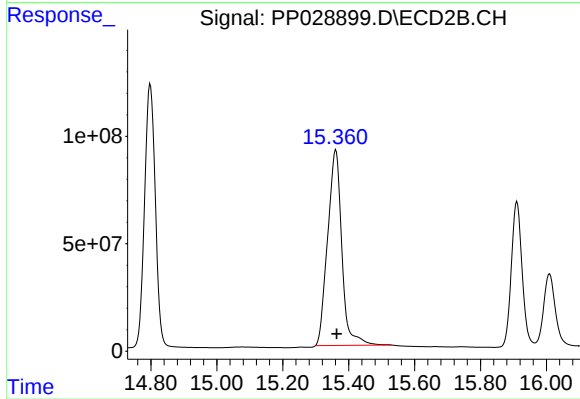

#11 2,4,5-TP (SILVEX)


R.T.: 15.361 min
Delta R.T.: -0.003 min
Response: 2727037237
Conc: 1073.60 ng/ml

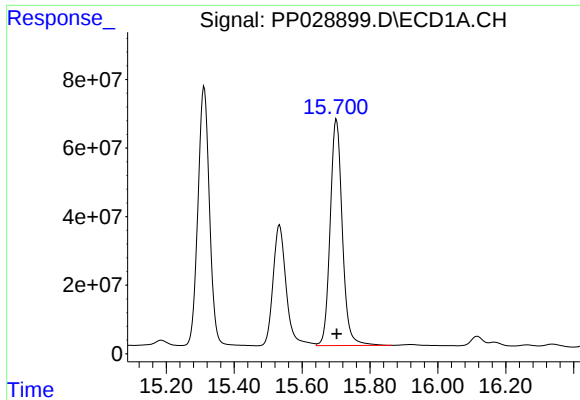

#12 2,4,5-T


R.T.: 15.701 min
Delta R.T.: 0.000 min
Response: 1635212403
Conc: 646.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

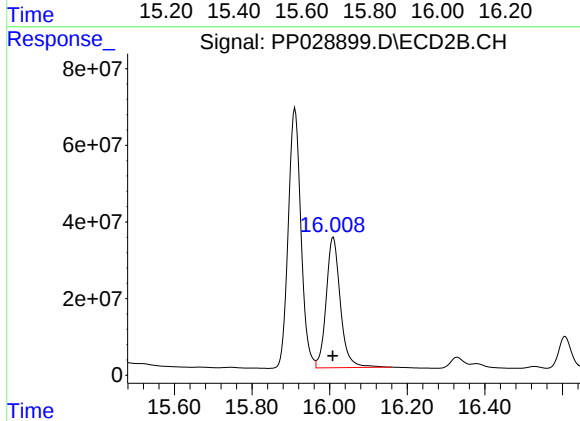


#12 2,4,5-T

R.T.: 16.010 min
Delta R.T.: 0.001 min
Response: 864722855
Conc: 403.47 ng/ml

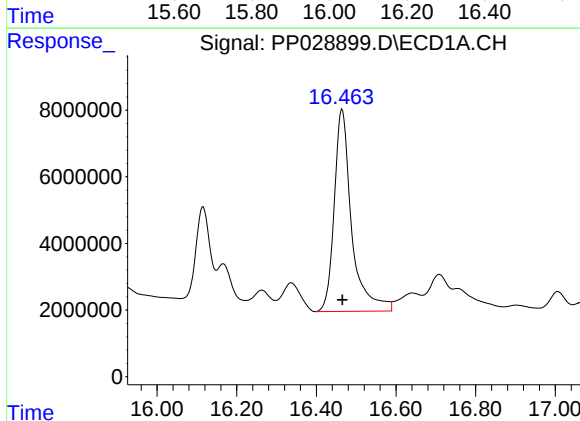


#13 2,4-DB

R.T.: 16.465 min
Delta R.T.: 0.000 min
Response: 184462889
Conc: 831.08 ng/ml

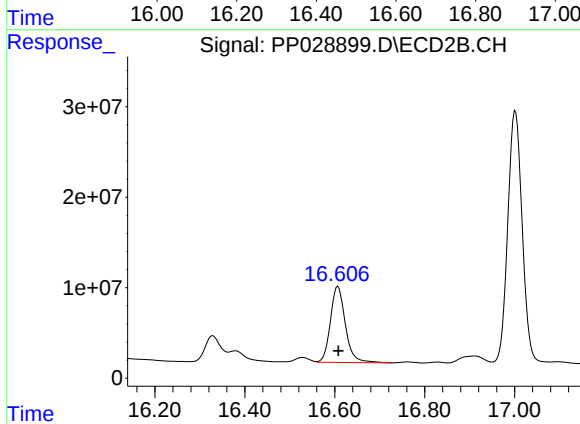

#13 2,4-DB


R.T.: 16.607 min
Delta R.T.: 0.000 min
Response: 193643146
Conc: 664.84 ng/ml

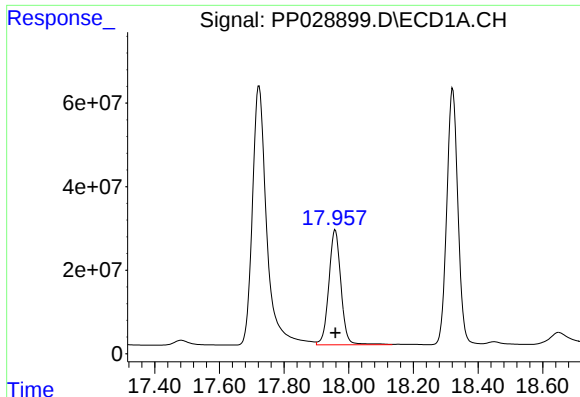

#14 DINOSEB


R.T.: 17.958 min
Delta R.T.: 0.000 min
Response: 720273360
Conc: 301.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

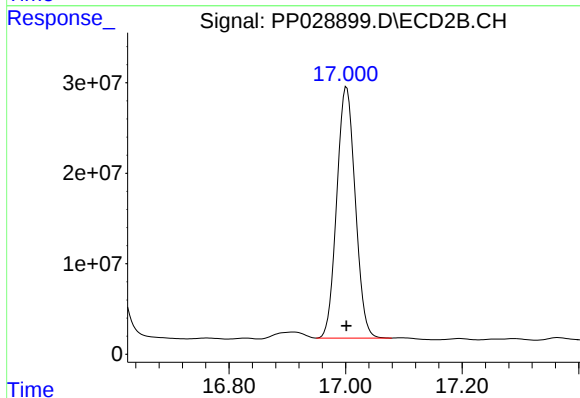


#14 DINOSEB

R.T.: 17.002 min
Delta R.T.: 0.000 min
Response: 611045839
Conc: 327.63 ng/ml

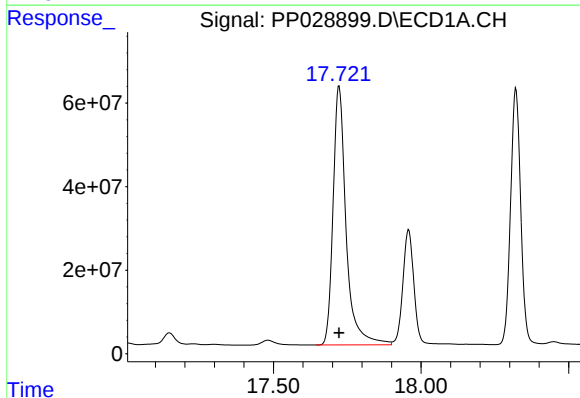


#15 Picloram

R.T.: 17.723 min
Delta R.T.: 0.000 min
Response: 1907456160
Conc: 446.99 ng/ml

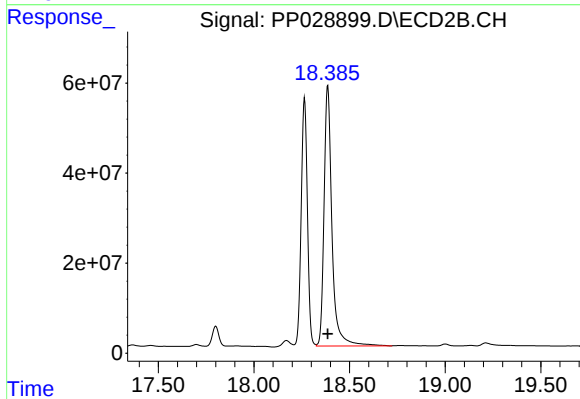

#15 Picloram


R.T.: 18.386 min
Delta R.T.: 0.000 min
Response: 1665600022
Conc: 456.92 ng/ml

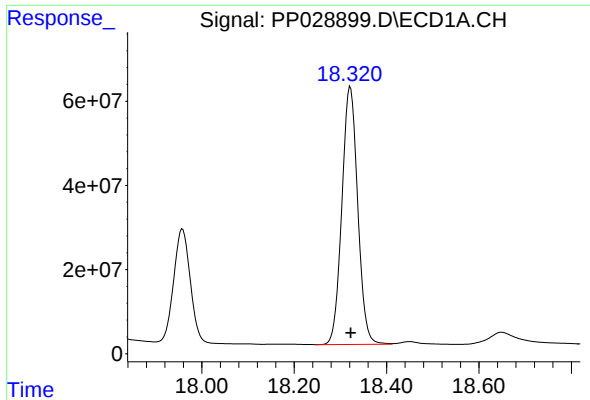

#16 DCPA

R.T.: 18.322 min
Delta R.T.: 0.000 min
Response: 1457853099
Conc: 346.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-1MSD

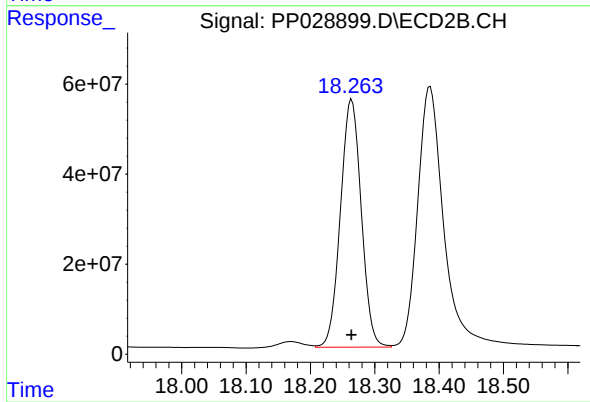

#16 DCPA

R.T.: 18.264 min
Delta R.T.: 0.000 min
Response: 1238063992
Conc: 381.82 ng/ml