

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011719\
 Data File : PP028911.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2019 22:53
 Operator : EI\MA
 Sample : K1139-18RE
 Misc : hexane
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 K1016-06MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 00:22:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011719.M
 Quant Title : 8080.M
 QLast Update : Thu Jan 17 12:26:40 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	12.166	12.270	213.7E6	257.8E6	827.799	565.255 #
Target Compounds							
1) T	Dalapon	3.335	3.004	180.5E6	557.4E6	280.932	902.607 #
2) T	3,5-DICHL...	10.552	0.000	16823702	0	31.379	N.D. #
6) T	MCP	12.856	0.000	9130420	0	18.910	N.D. #
7) T	MCPA	13.107	0.000	139.5E6	0	181.027	N.D. #
8) T	DICHLORPROP	0.000	13.716	0	25554431	N.D.	57.181 #
9) T	2,4-D	14.069	0.000	99742000	0	280.409	N.D. #
10) T	Pentachlo...	14.443	0.000	7396939	0	0.958	N.D. #
15) T	Picloram	17.740	18.399	3990875	7548303	0.935	2.071 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011719\
Data File : PP028911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2019 22:53
Operator : EI\MA
Sample : K1139-18RE
Misc : hexane
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
K1016-06MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 00:22:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011719.M
Quant Title : 8080.M
QLast Update : Thu Jan 17 12:26:40 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

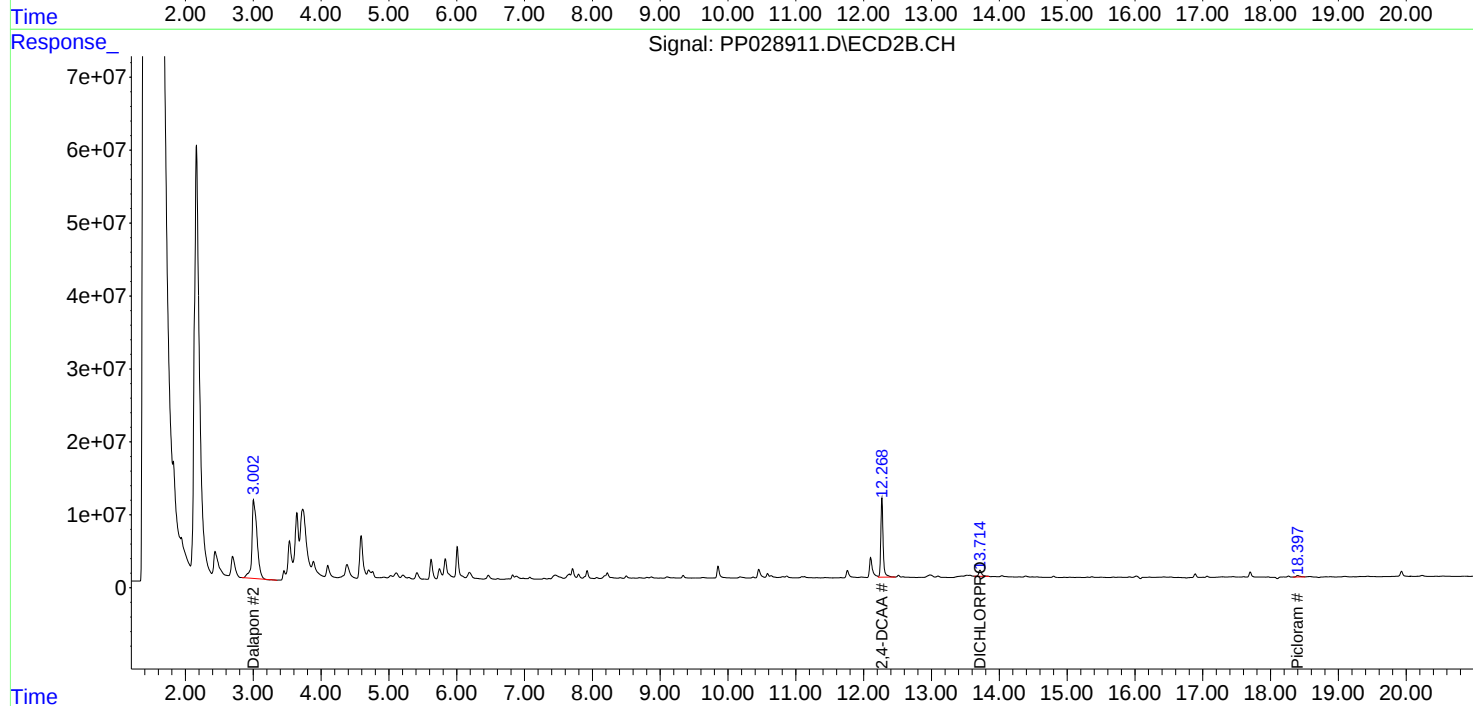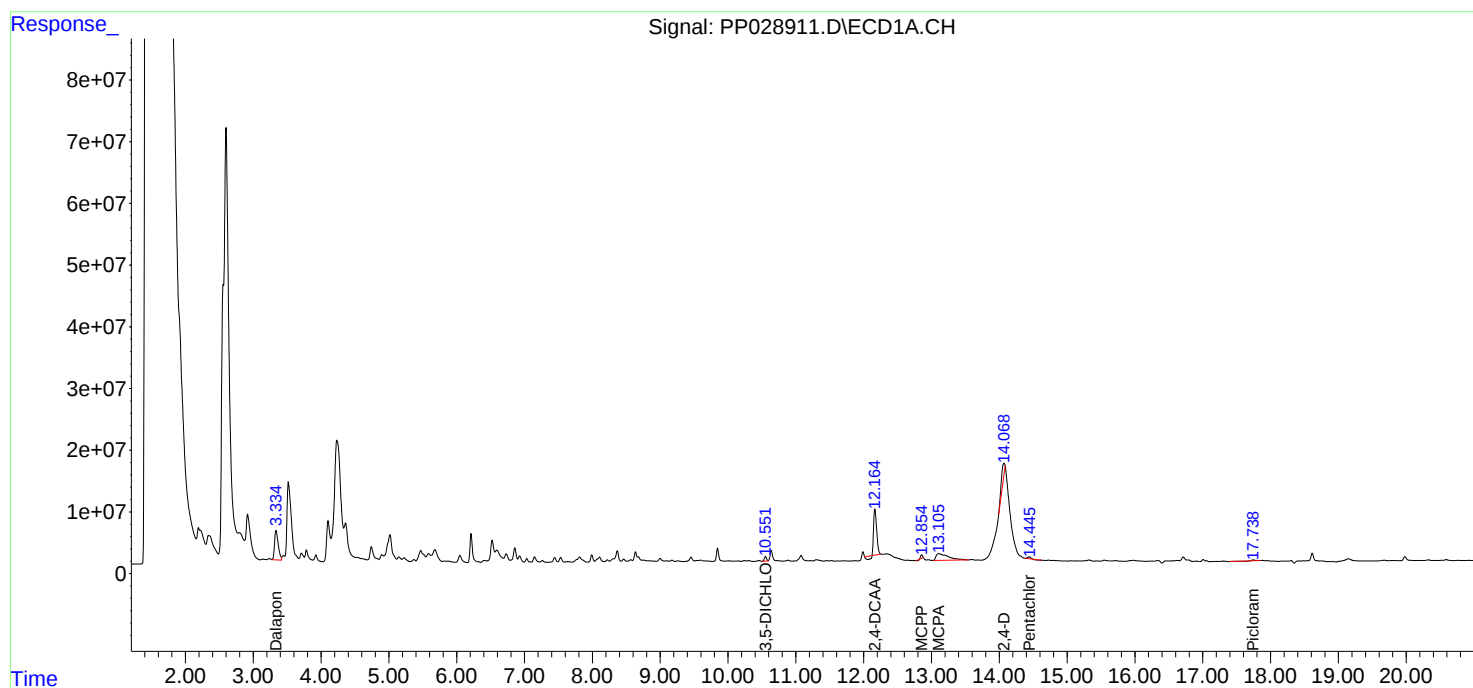


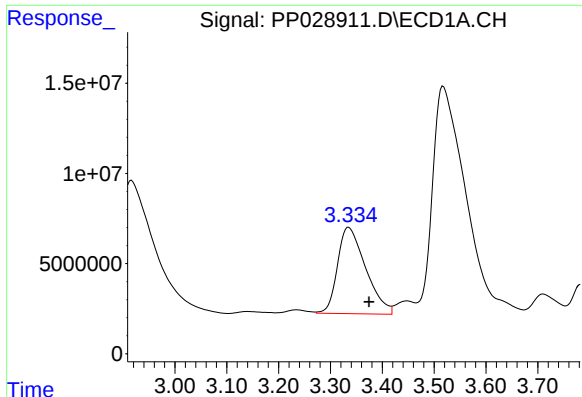

#1 Dalapon


R.T.: 3.335 min
Delta R.T.: -0.040 min
Response: 180461584
Conc: 280.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
K1016-06MSD

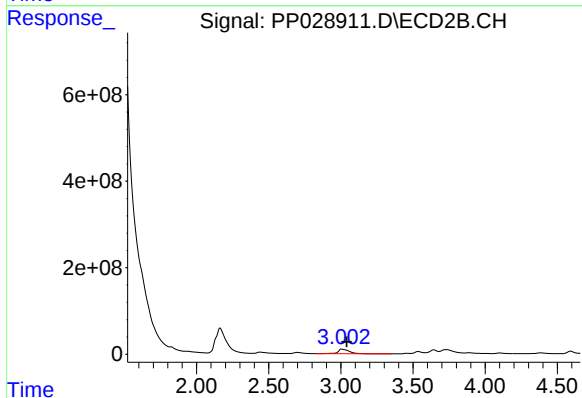


#1 Dalapon

R.T.: 3.004 min
Delta R.T.: -0.038 min
Response: 557393536
Conc: 902.61 ng/ml

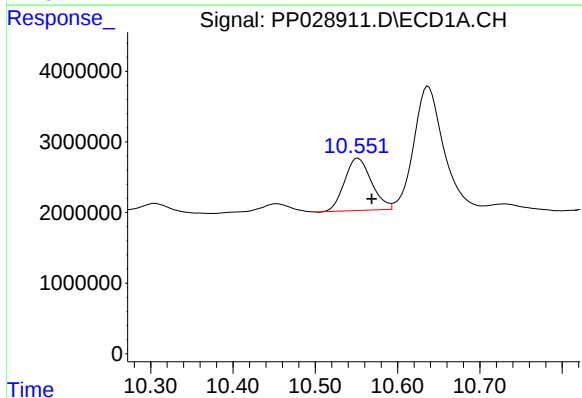


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.552 min
Delta R.T.: -0.016 min
Response: 16823702
Conc: 31.38 ng/ml

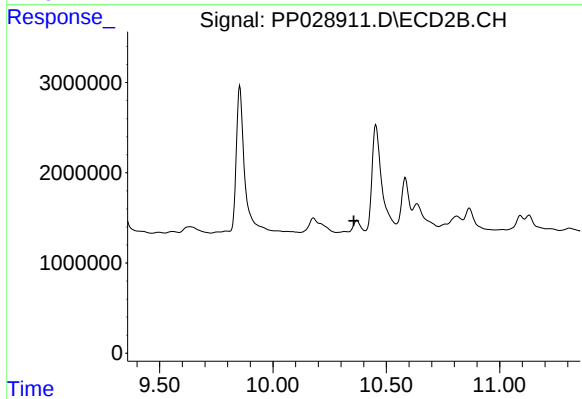

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 10.357 min
Response: 0
Conc: N.D.

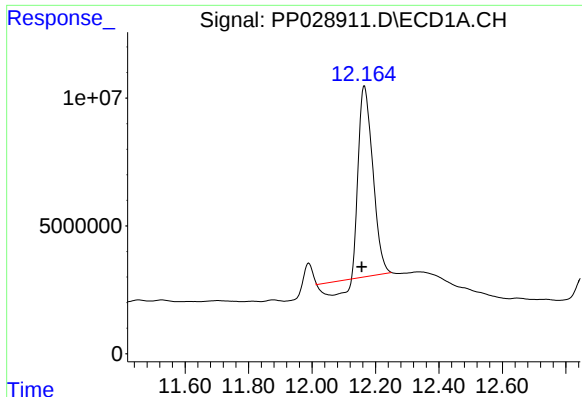

#4 2,4-DCAA


R.T.: 12.166 min
Delta R.T.: 0.009 min
Response: 213702322
Conc: 827.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
K1016-06MSD

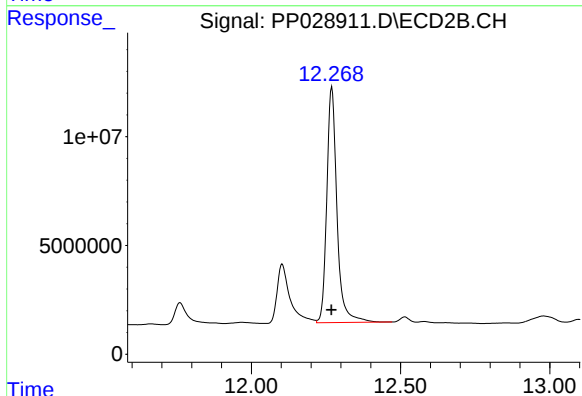


#4 2,4-DCAA

R.T.: 12.270 min
Delta R.T.: 0.002 min
Response: 257833851
Conc: 565.26 ng/ml

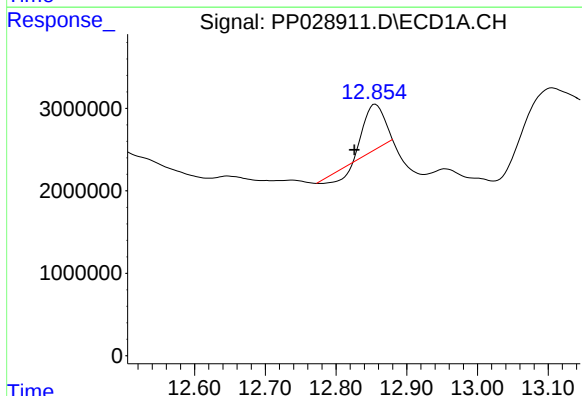


#6 MCP

R.T.: 12.856 min
Delta R.T.: 0.030 min
Response: 9130420
Conc: 18.91 ug/ml

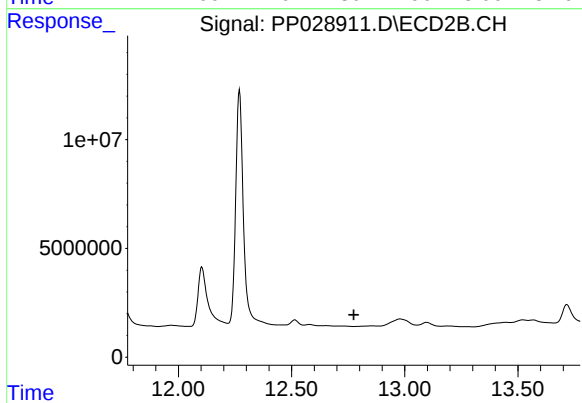

#6 MCP


R.T.: 0.000 min
Exp R.T.: 12.775 min
Response: 0
Conc: N.D.

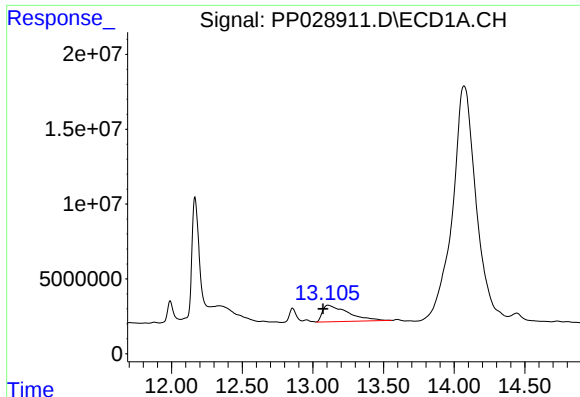

#7 MCPA


R.T.: 13.107 min
Delta R.T.: 0.035 min
Response: 139508728
Conc: 181.03 ug/ml

Instrument :
ECD_P
ClientSampleId :
K1016-06MSD

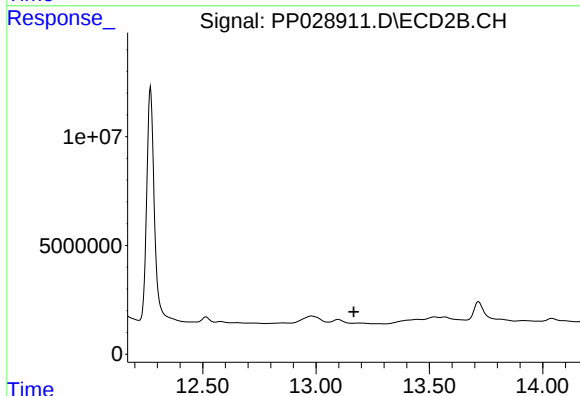


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 13.167 min
Response: 0
Conc: N.D.

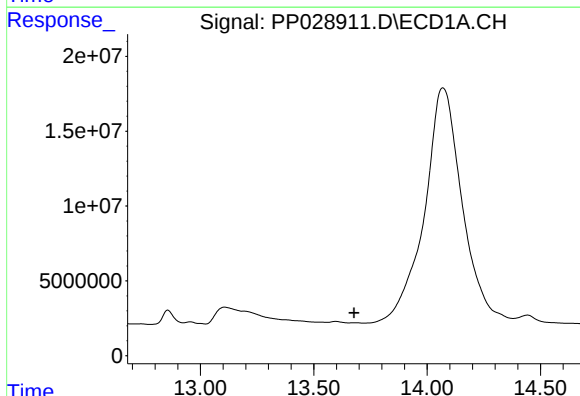


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.678 min
Response: 0
Conc: N.D.

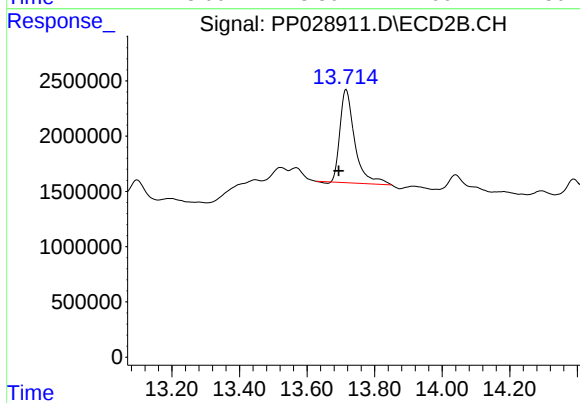

#8 DICHLORPROP


R.T.: 13.716 min
Delta R.T.: 0.022 min
Response: 25554431
Conc: 57.18 ng/ml

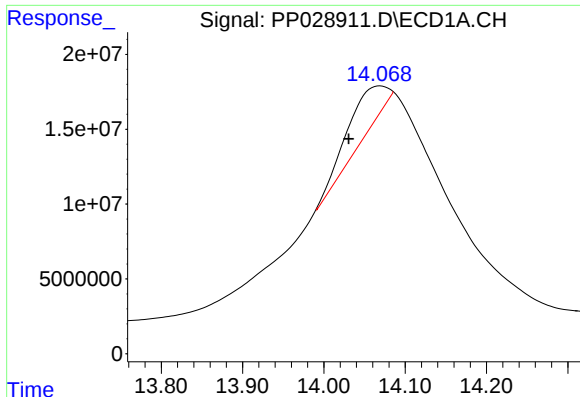

#9 2,4-D


R.T.: 14.069 min
Delta R.T.: 0.039 min
Response: 99742000
Conc: 280.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
K1016-06MSD

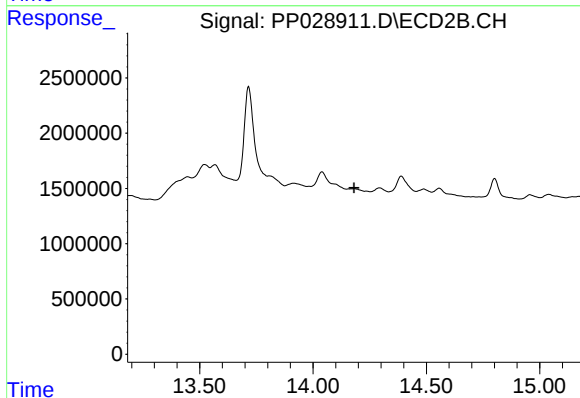


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 14.181 min
Response: 0
Conc: N.D.

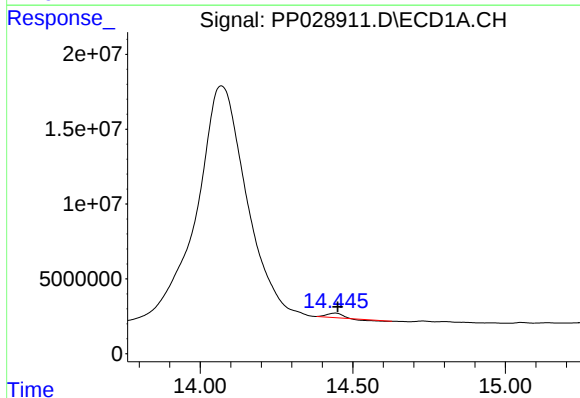


#10 Pentachlorophenol

R.T.: 14.443 min
Delta R.T.: -0.009 min
Response: 7396939
Conc: 0.96 ng/ml

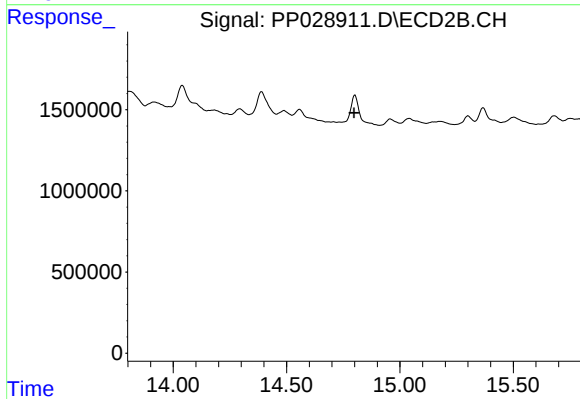

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 14.798 min
Response: 0
Conc: N.D.

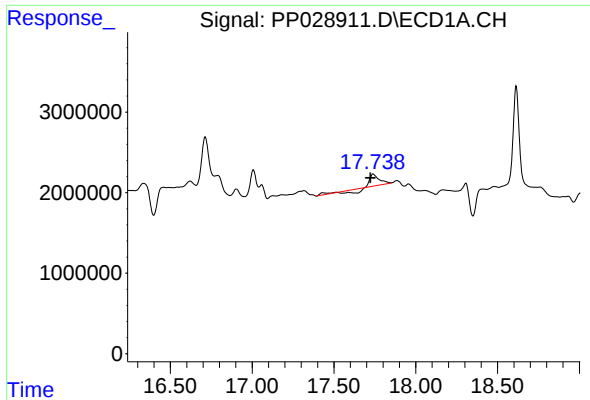

#15 Picloram

R.T.: 17.740 min
Delta R.T.: 0.017 min
Response: 3990875
Conc: 0.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
K1016-06MSD

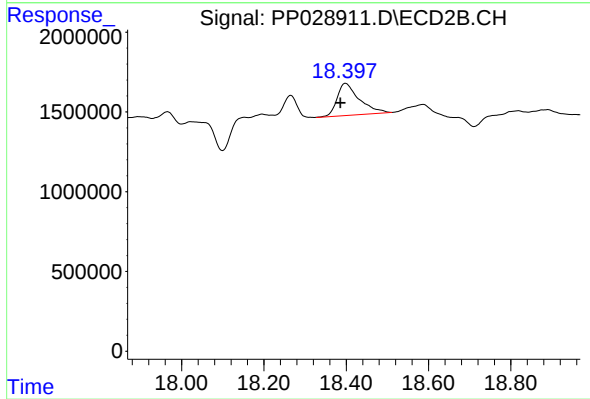

#15 Picloram

R.T.: 18.399 min
Delta R.T.: 0.013 min
Response: 7548303
Conc: 2.07 ng/ml