

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP042990.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2022 17:07
 Operator : AJ\MA
 Sample : N1126-04 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 02:55:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.876	4.042	43674	46014	1.846	1.842
2)	SA Decachlor...	10.813	9.382	31255	32381	2.138	1.660
Target Compounds							
6)	L1 AR-1016-4	0.000	5.573	0	9269	N.D.	14.915 #
20)	L4 AR-1242-5	0.000	6.185	0	17060	N.D.	23.708 #
22)	L5 AR-1248-2	0.000	5.573	0	9269	N.D.	11.421 #
26)	L6 AR-1254-1	0.000	6.185	0	17060	N.D.	11.001 #
27)	L6 AR-1254-2	7.314	6.344	19350	17260	15.374	12.714
28)	L6 AR-1254-3	7.693	6.768	13639	25250	10.513	11.805
29)	L6 AR-1254-4	0.000	7.008	0	11674	N.D.	9.357 #
30)	L6 AR-1254-5	8.417	7.439	29715	8192	31.716	4.804 #
33)	L7 AR-1260-3	0.000	7.254	0	13468	N.D.	9.319 #
35)	L7 AR-1260-5	9.035	0.000	1068	0	0.649	N.D. #
36)	L8 AR-1262-1	0.000	7.439	0	8192	N.D.	9.049 #
37)	L8 AR-1262-2	9.035	0.000	1068	0	0.617	N.D. #
39)	L8 AR-1262-4	9.422	0.000	33362	0	61.847	N.D. #
42)	L9 AR-1268-2	9.422	0.000	33362	0	17.467	N.D. #
43)	L9 AR-1268-3	9.640f	0.000	12996	0	7.714	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP042990.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2022 17:07
Operator : AJ\MA
Sample : N1126-04 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 02:55:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

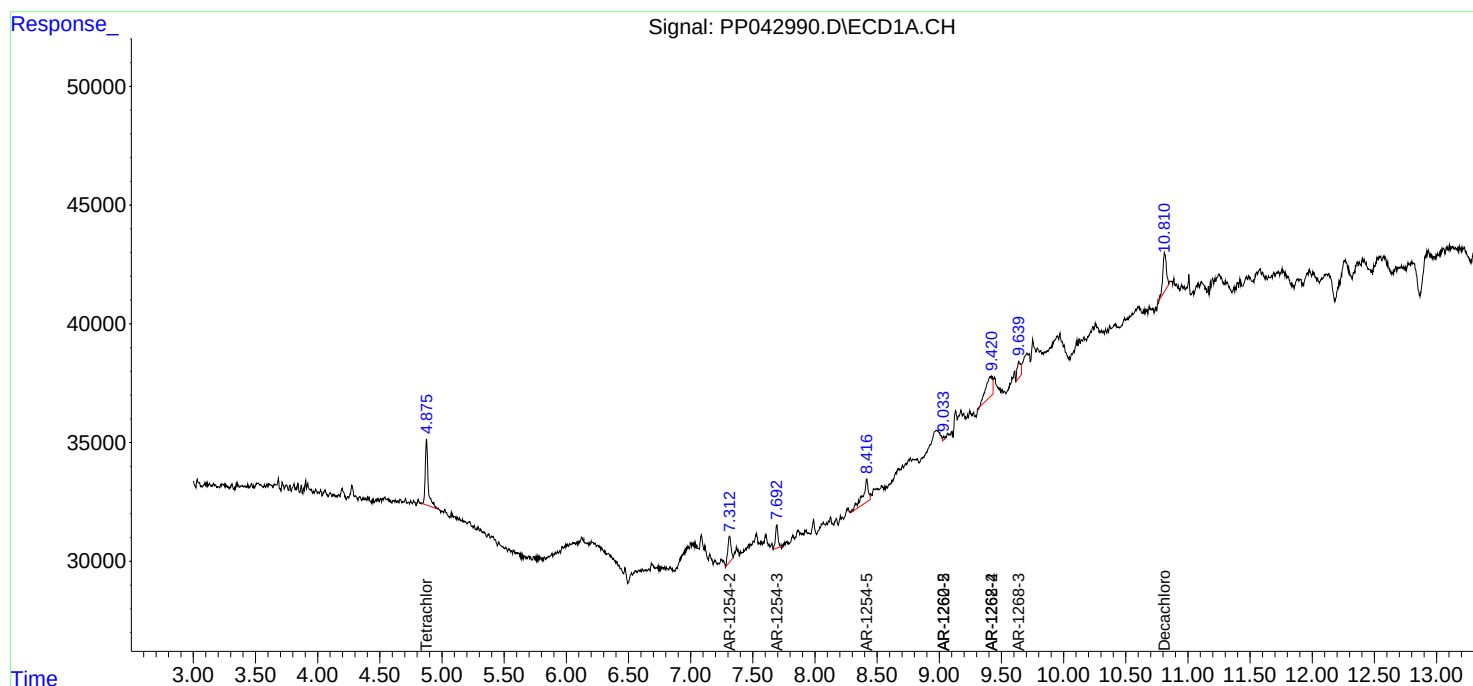


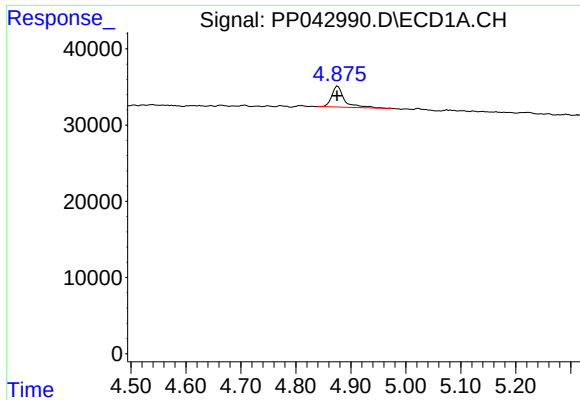

#1 Tetrachloro-m-xylene


R.T.: 4.876 min
Delta R.T.: 0.001 min
Response: 43674
Conc: 1.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

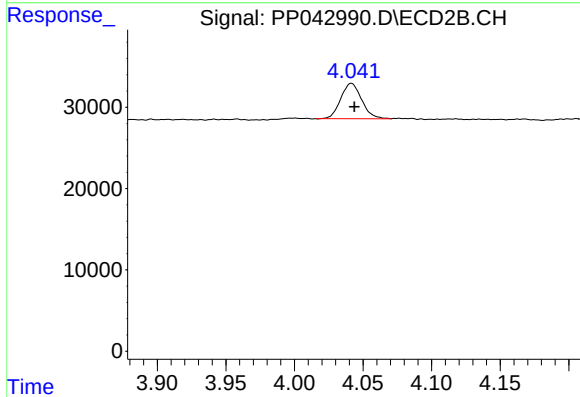


#1 Tetrachloro-m-xylene

R.T.: 4.042 min
Delta R.T.: -0.002 min
Response: 46014
Conc: 1.84 ng/ml

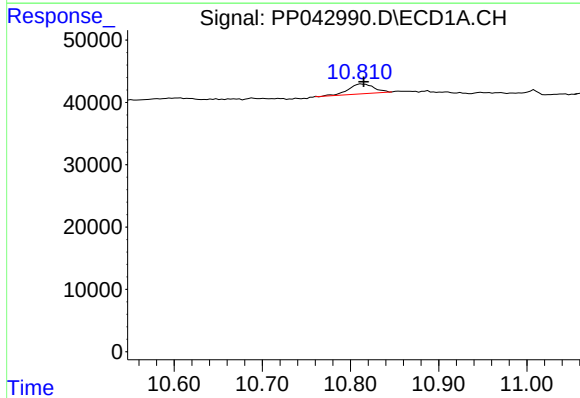


#2 Decachlorobiphenyl

R.T.: 10.813 min
Delta R.T.: -0.002 min
Response: 31255
Conc: 2.14 ng/ml

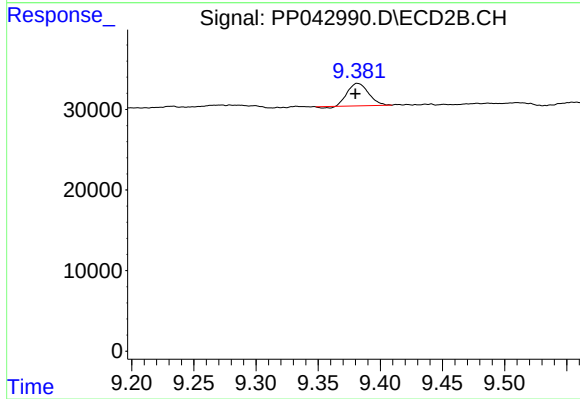

#2 Decachlorobiphenyl


R.T.: 9.382 min
Delta R.T.: 0.002 min
Response: 32381
Conc: 1.66 ng/ml

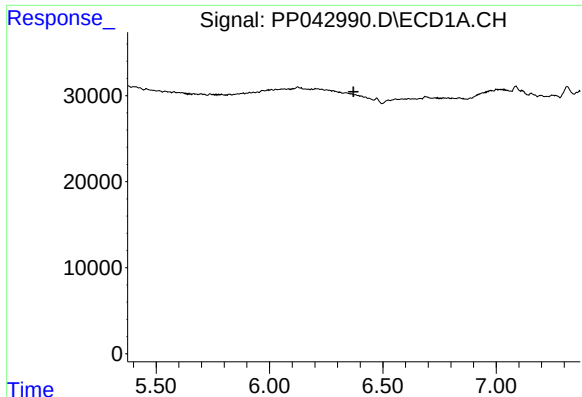

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T.: 6.371 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

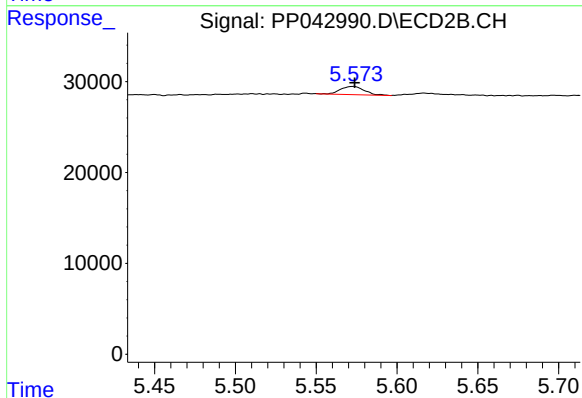


#6 AR-1016-4

R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 9269
Conc: 14.91 ng/ml

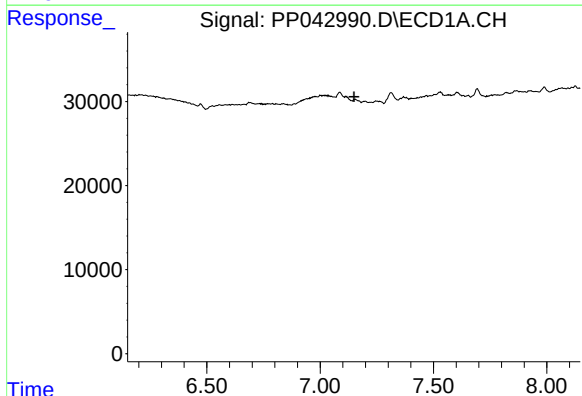


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.149 min
Response: 0
Conc: N.D.

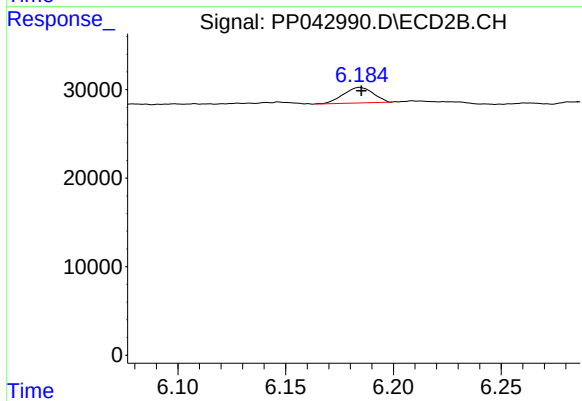

#20 AR-1242-5

R.T.: 6.185 min
Delta R.T.: 0.000 min
Response: 17060
Conc: 23.71 ng/ml

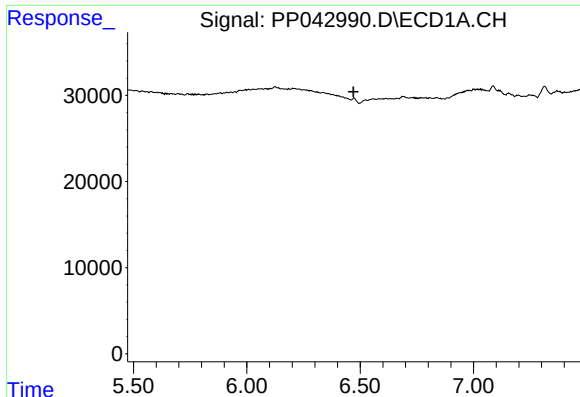

#22 AR-1248-2

R.T.: 0.000 min
Exp R.T.: 6.471 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

#22 AR-1248-2


R.T.: 5.573 min
Delta R.T.: 0.000 min
Response: 9269
Conc: 11.42 ng/ml

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.082 min
Response: 0
Conc: N.D.

#26 AR-1254-1


R.T.: 6.185 min
Delta R.T.: -0.001 min
Response: 17060
Conc: 11.00 ng/ml

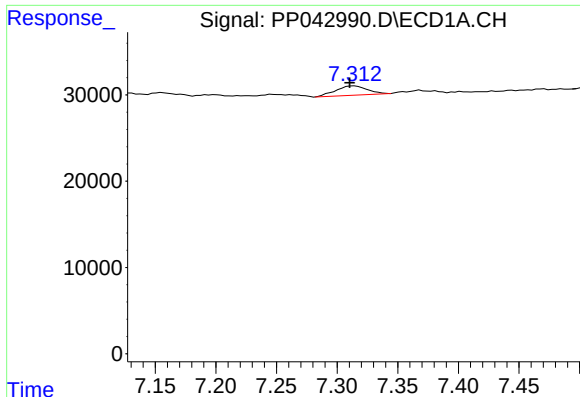

#27 AR-1254-2


R.T.: 7.314 min
Delta R.T.: 0.003 min
Response: 19350
Conc: 15.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

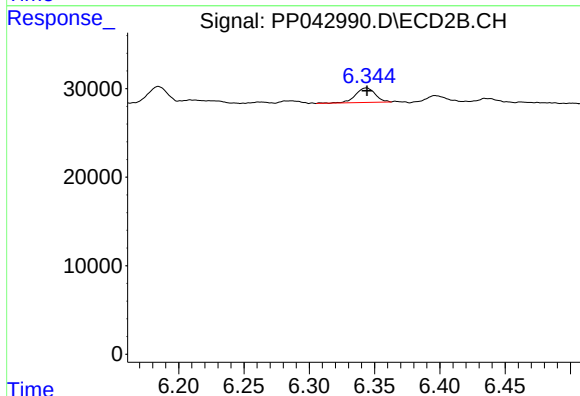


#27 AR-1254-2

R.T.: 6.344 min
Delta R.T.: 0.000 min
Response: 17260
Conc: 12.71 ng/ml

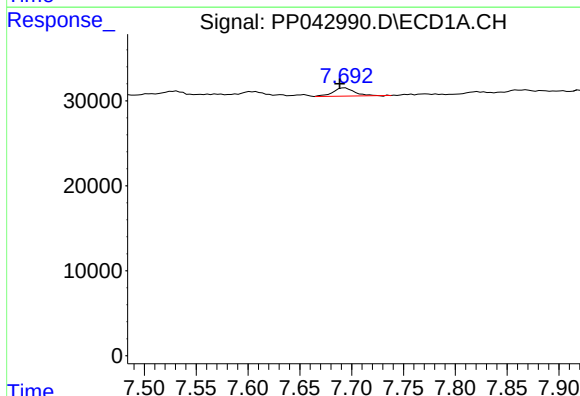


#28 AR-1254-3

R.T.: 7.693 min
Delta R.T.: 0.005 min
Response: 13639
Conc: 10.51 ng/ml

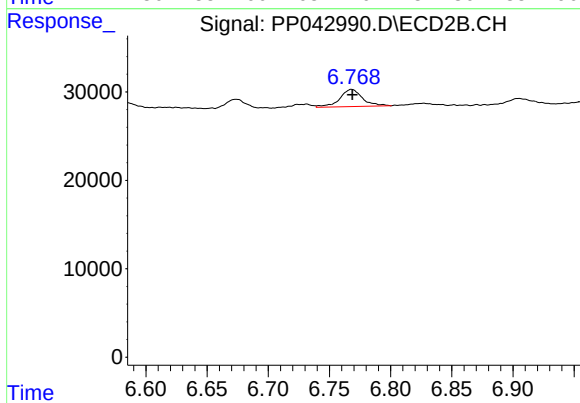

#28 AR-1254-3


R.T.: 6.768 min
Delta R.T.: 0.000 min
Response: 25250
Conc: 11.80 ng/ml

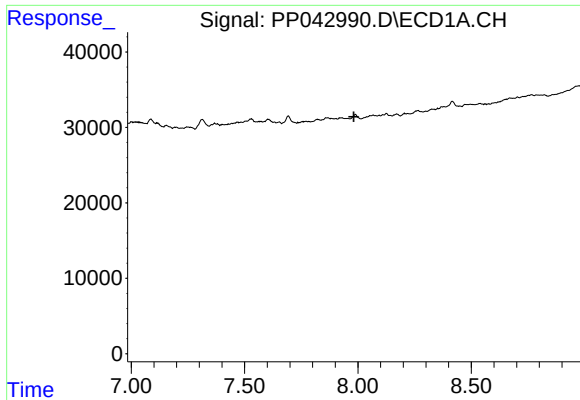

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

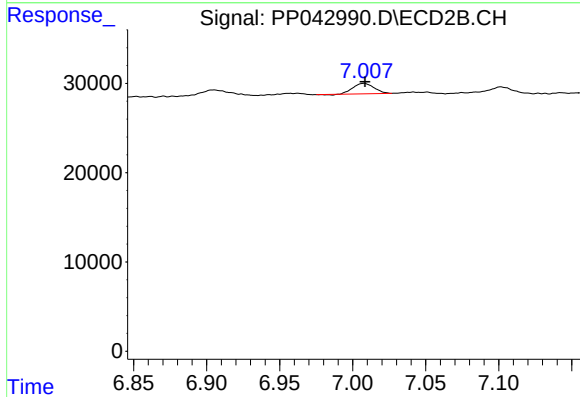


#29 AR-1254-4

R.T.: 7.008 min
Delta R.T.: 0.000 min
Response: 11674
Conc: 9.36 ng/ml

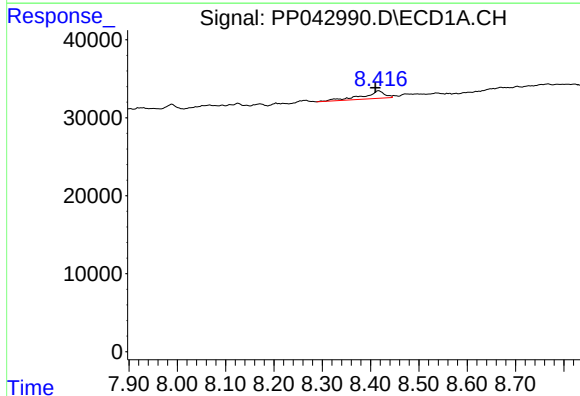


#30 AR-1254-5

R.T.: 8.417 min
Delta R.T.: 0.007 min
Response: 29715
Conc: 31.72 ng/ml

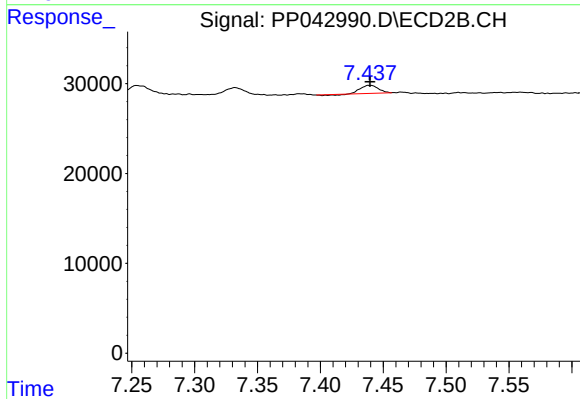

#30 AR-1254-5


R.T.: 7.439 min
Delta R.T.: -0.001 min
Response: 8192
Conc: 4.80 ng/ml

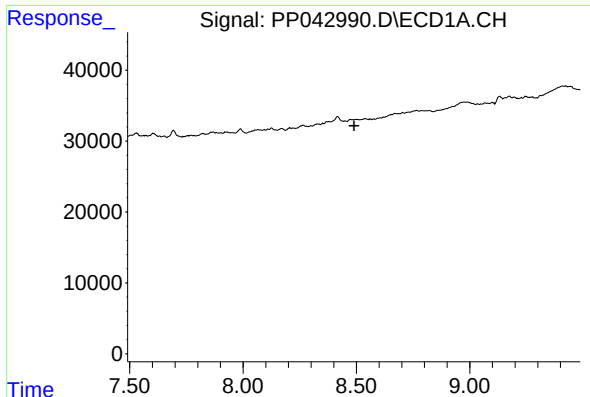

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

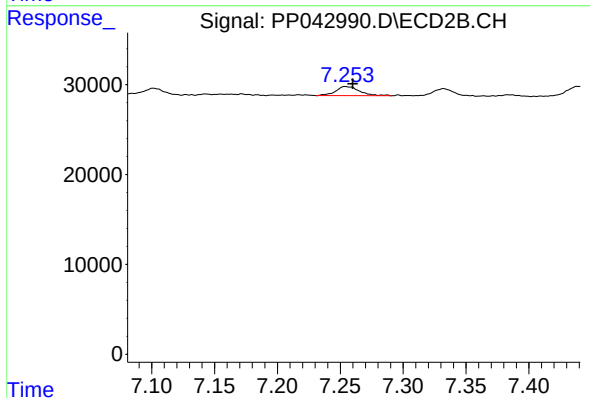


#33 AR-1260-3

R.T.: 7.254 min
Delta R.T.: -0.006 min
Response: 13468
Conc: 9.32 ng/ml

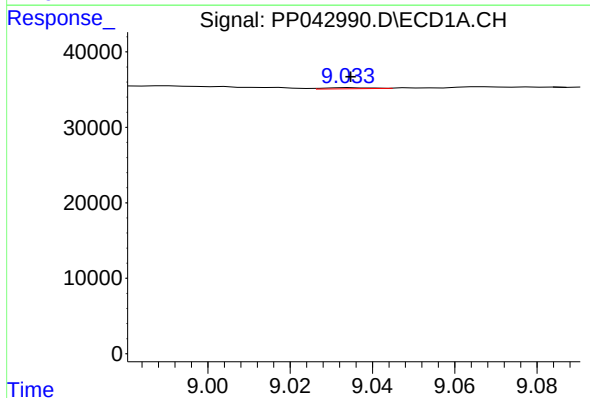


#35 AR-1260-5

R.T.: 9.035 min
Delta R.T.: 0.000 min
Response: 1068
Conc: 0.65 ng/ml

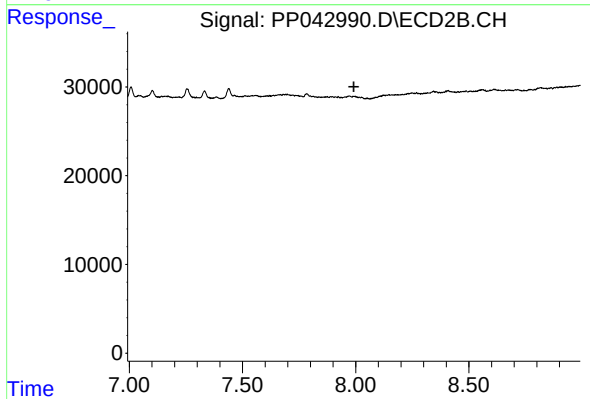

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 7.992 min
Response: 0
Conc: N.D.

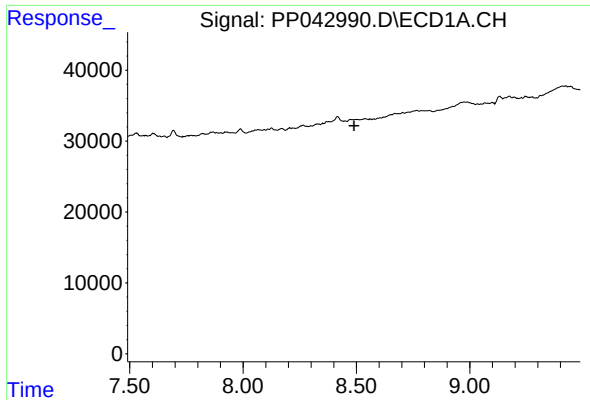

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

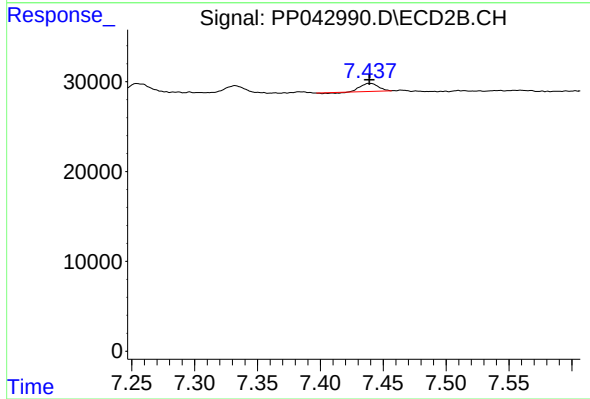


#36 AR-1262-1

R.T.: 7.439 min
Delta R.T.: 0.000 min
Response: 8192
Conc: 9.05 ng/ml

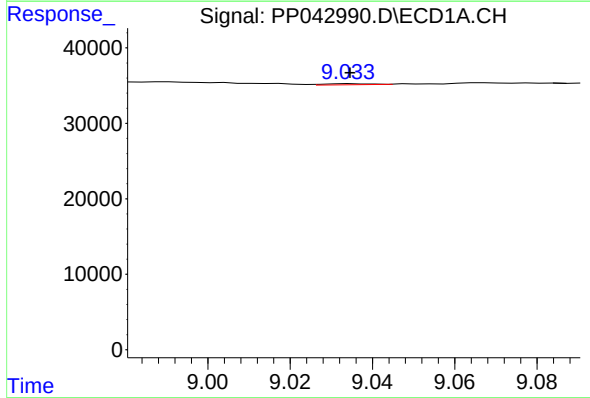


#37 AR-1262-2

R.T.: 9.035 min
Delta R.T.: 0.000 min
Response: 1068
Conc: 0.62 ng/ml

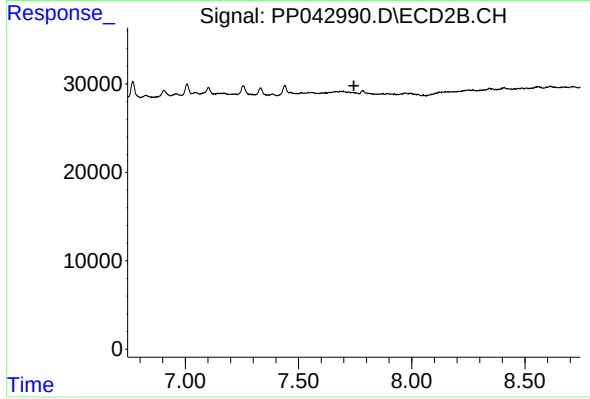

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 7.744 min
Response: 0
Conc: N.D.

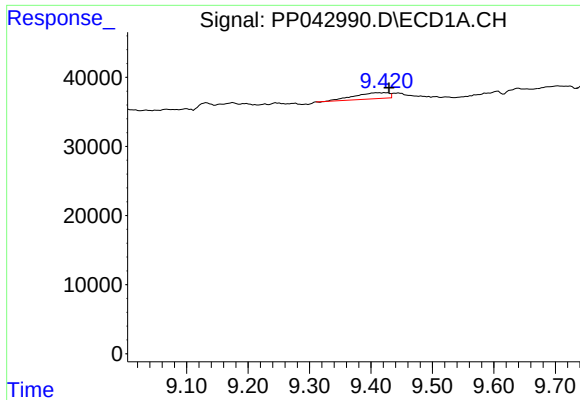

#39 AR-1262-4


R.T.: 9.422 min
Delta R.T.: -0.007 min
Response: 33362
Conc: 61.85 ng/ml

Instrument :
ECD_P
ClientSampleId :

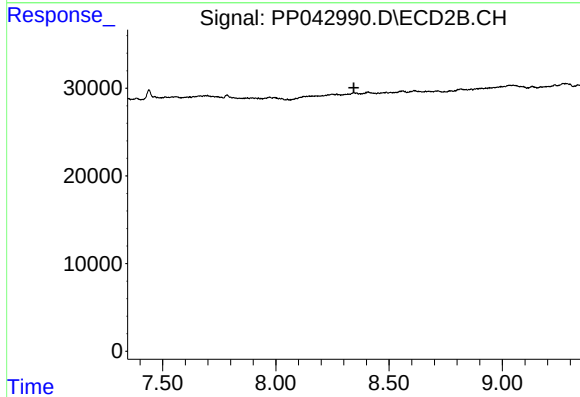


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

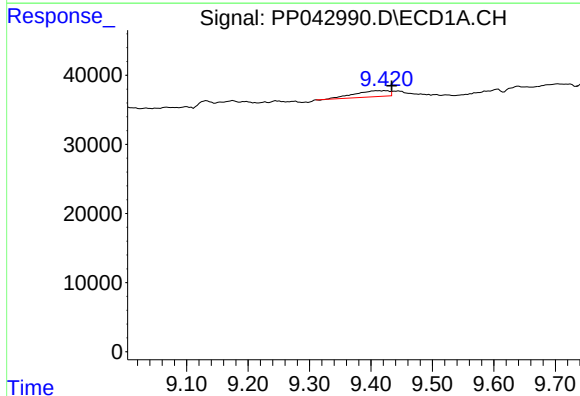


#42 AR-1268-2

R.T.: 9.422 min
Delta R.T.: -0.011 min
Response: 33362
Conc: 17.47 ng/ml

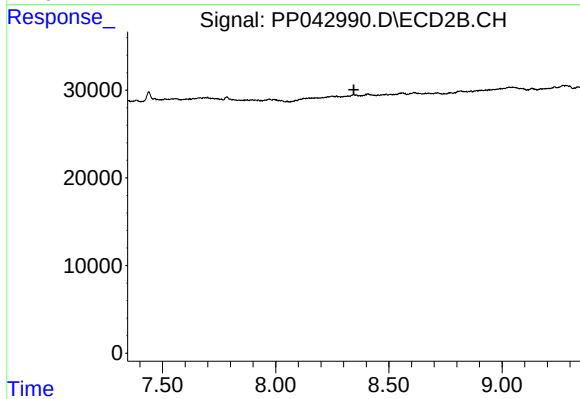

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

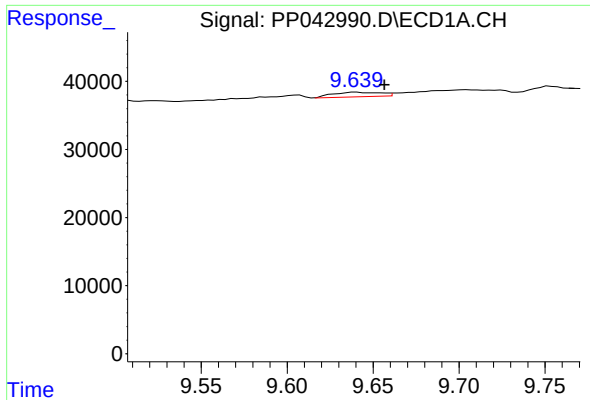

#43 AR-1268-3

R.T.: 9.640 min
Delta R.T.: -0.016 min
Response: 12996
Conc: 7.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

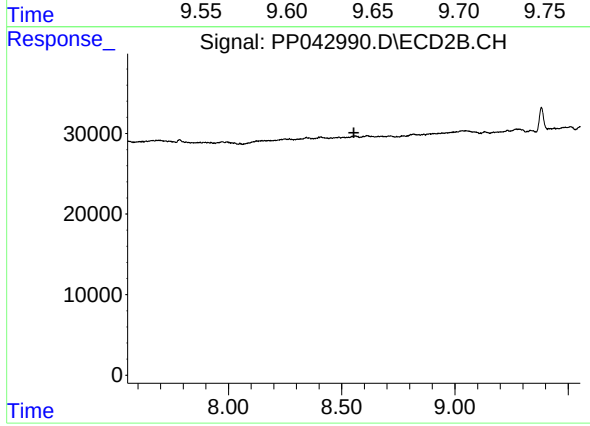

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.554 min
Response: 0
Conc: N.D.