

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP043006.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2022 22:00
 Operator : AJ\MA
 Sample : N1163-02 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 03:00:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.880	4.045	29083	39453	1.229	1.580 #
2)	SA Decachlor...	10.816	9.383	38274	40067	2.618	2.054
Target Compounds							
31)	L7 AR-1260-1	0.000	6.908	0	3958	N.D.	3.062 #
32)	L7 AR-1260-2	8.112	0.000	917	0	0.888	N.D. #
33)	L7 AR-1260-3	8.518f	7.275f	3453	9710	4.577	6.719 #
35)	L7 AR-1260-5	9.046	7.977f	10614	13161	6.451	5.247
36)	L8 AR-1262-1	8.518f	0.000	3453	0	3.270	N.D. #
37)	L8 AR-1262-2	9.046	0.000	10614	0	6.132	N.D. #
38)	L8 AR-1262-3	0.000	8.306f	0	17146	N.D.	15.368 #
41)	L9 AR-1268-1	0.000	8.306f	0	17146	N.D.	5.563 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP043006.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2022 22:00
Operator : AJ\MA
Sample : N1163-02 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 03:00:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

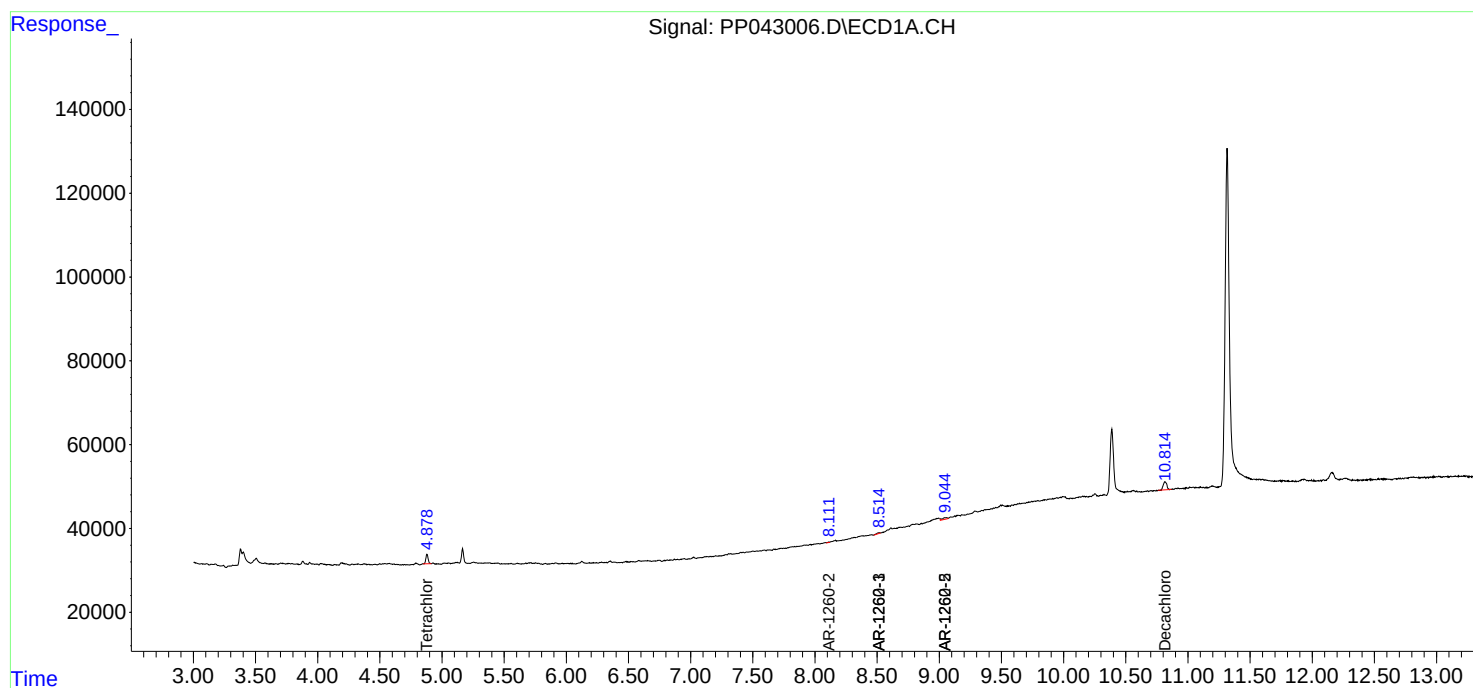


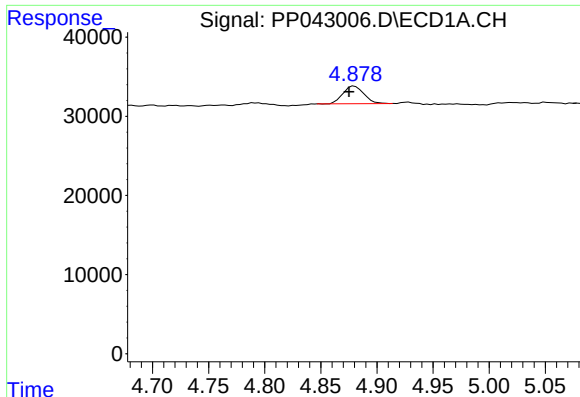

#1 Tetrachloro-m-xylene


R.T.: 4.880 min
Delta R.T.: 0.005 min
Response: 29083
Conc: 1.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

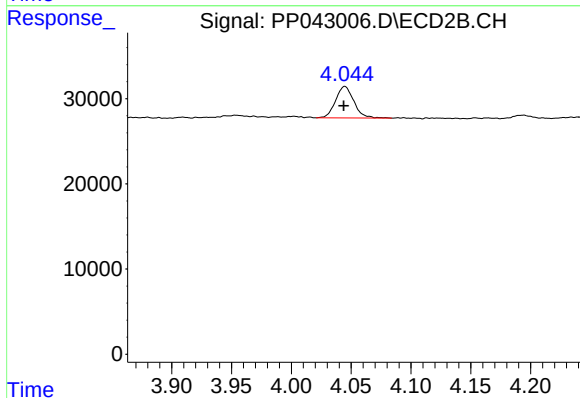


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.001 min
Response: 39453
Conc: 1.58 ng/ml

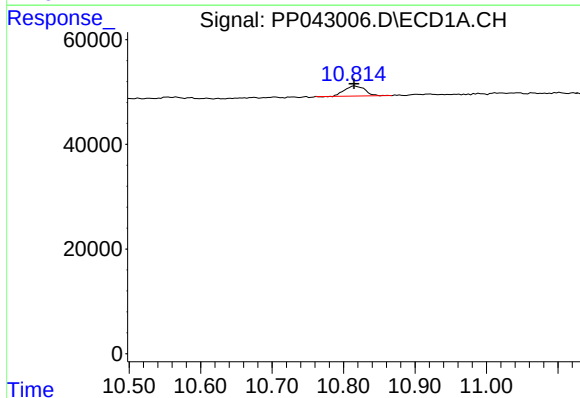


#2 Decachlorobiphenyl

R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 38274
Conc: 2.62 ng/ml

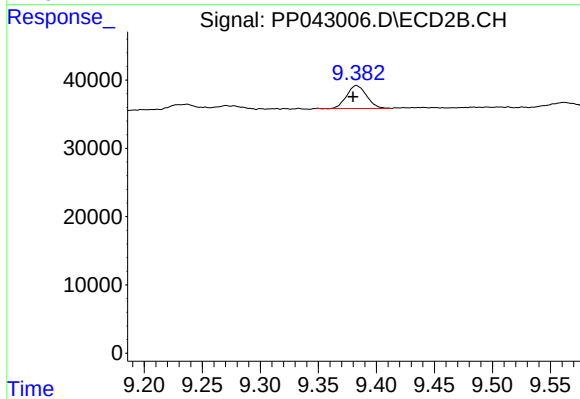

#2 Decachlorobiphenyl


R.T.: 9.383 min
Delta R.T.: 0.003 min
Response: 40067
Conc: 2.05 ng/ml

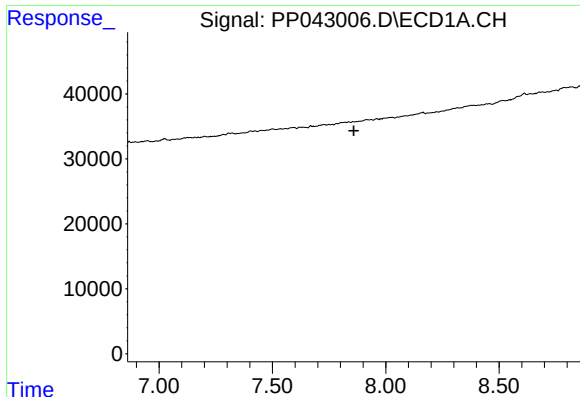

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.859 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

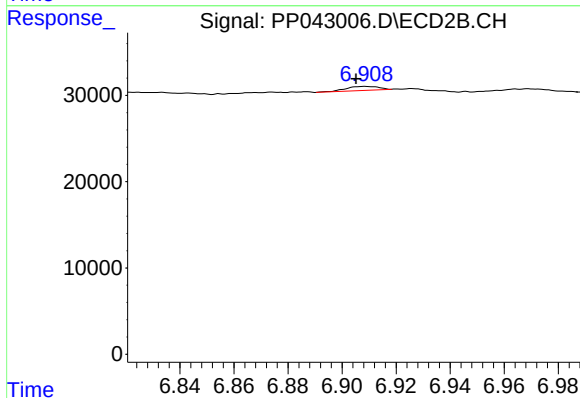


#31 AR-1260-1

R.T.: 6.908 min
Delta R.T.: 0.003 min
Response: 3958
Conc: 3.06 ng/ml

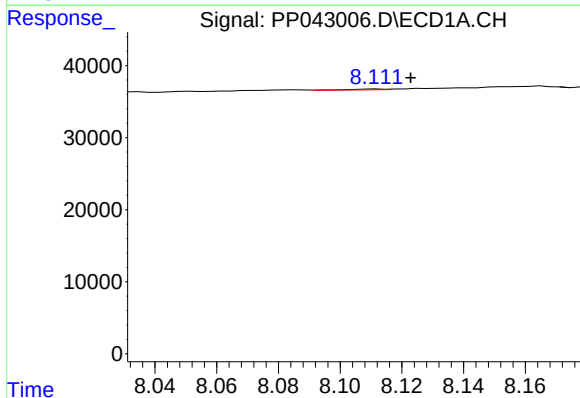


#32 AR-1260-2

R.T.: 8.112 min
Delta R.T.: -0.011 min
Response: 917
Conc: 0.89 ng/ml

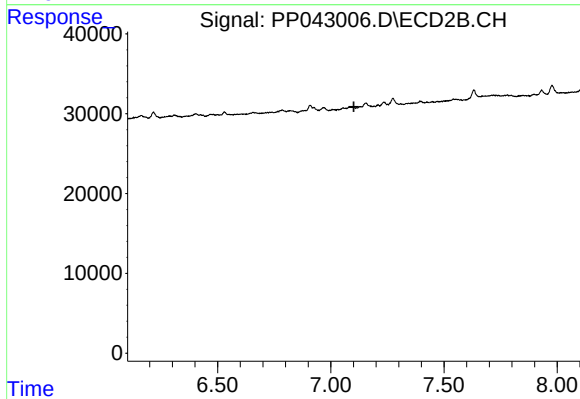

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.102 min
Response: 0
Conc: N.D.

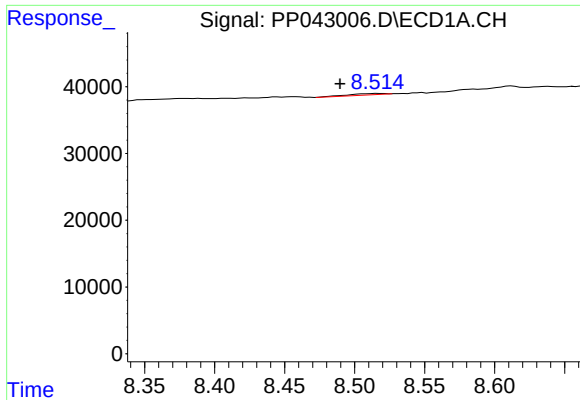

#33 AR-1260-3


R.T.: 8.518 min
Delta R.T.: 0.028 min
Response: 3453
Conc: 4.58 ng/ml

Instrument :
ECD_P
ClientSampleId :

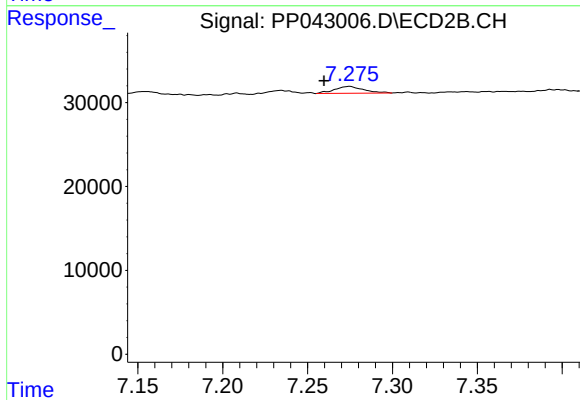


#33 AR-1260-3

R.T.: 7.275 min
Delta R.T.: 0.015 min
Response: 9710
Conc: 6.72 ng/ml

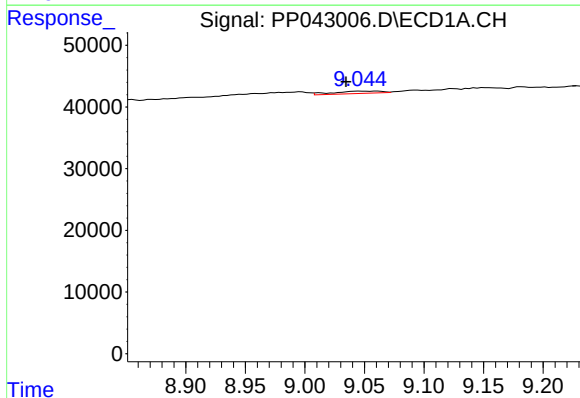


#35 AR-1260-5

R.T.: 9.046 min
Delta R.T.: 0.011 min
Response: 10614
Conc: 6.45 ng/ml

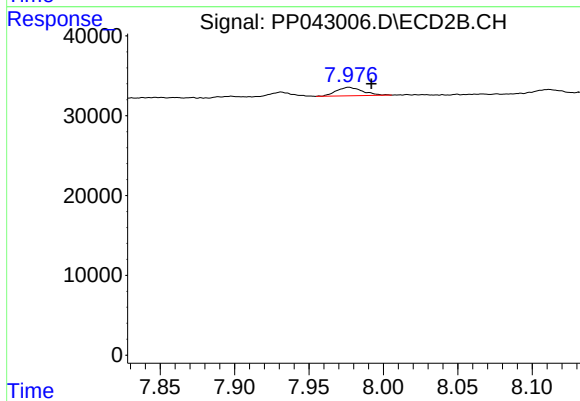

#35 AR-1260-5


R.T.: 7.977 min
Delta R.T.: -0.015 min
Response: 13161
Conc: 5.25 ng/ml

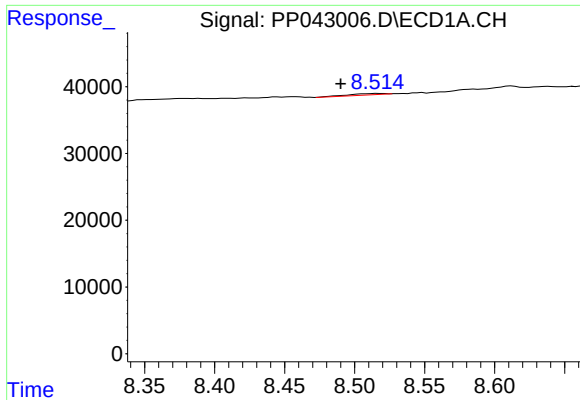

#36 AR-1262-1


R.T.: 8.518 min
Delta R.T.: 0.028 min
Response: 3453
Conc: 3.27 ng/ml

Instrument :
ECD_P
ClientSampleId :

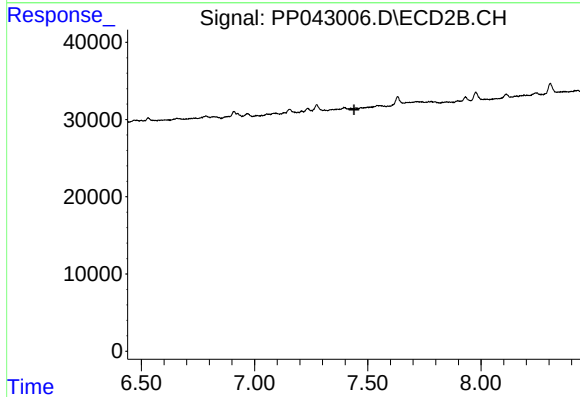


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.439 min
Response: 0
Conc: N.D.

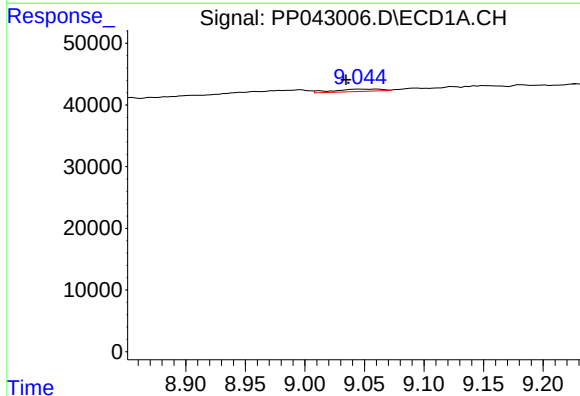


#37 AR-1262-2

R.T.: 9.046 min
Delta R.T.: 0.011 min
Response: 10614
Conc: 6.13 ng/ml

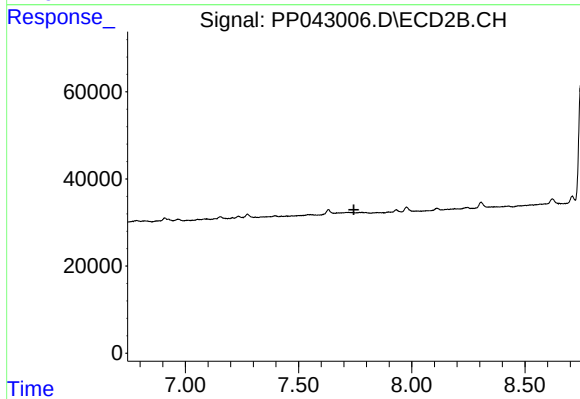

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

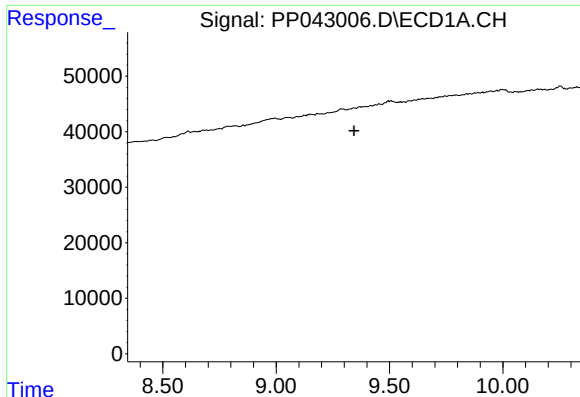

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 9.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

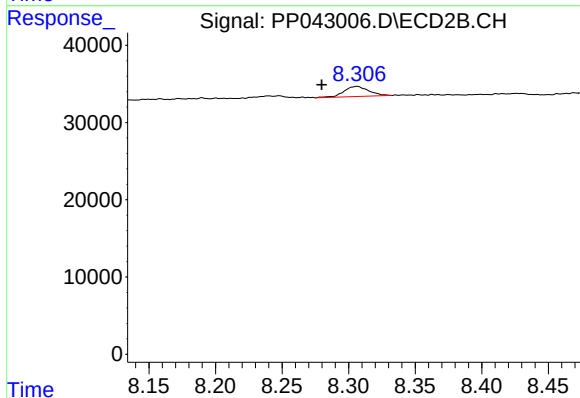


#38 AR-1262-3

R.T.: 8.306 min
Delta R.T.: 0.027 min
Response: 17146
Conc: 15.37 ng/ml

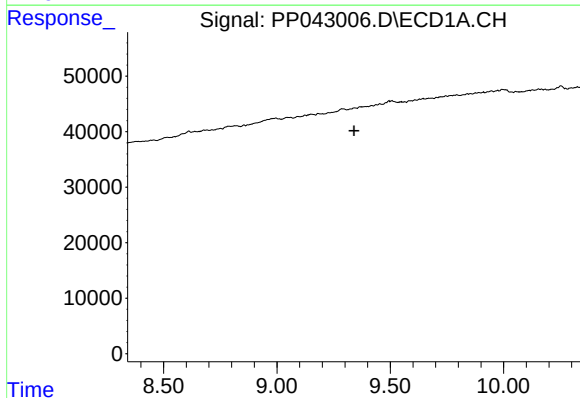

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.341 min
Response: 0
Conc: N.D.

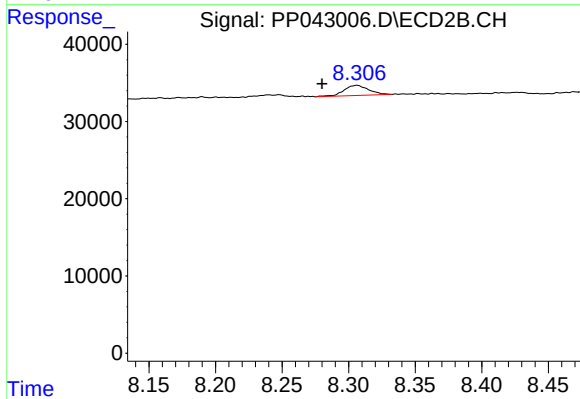

#41 AR-1268-1

R.T.: 8.306 min
Delta R.T.: 0.026 min
Response: 17146
Conc: 5.56 ng/ml