

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP043017.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 1:30
 Operator : AJ\MA
 Sample : N1163-08 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 03:03:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.877	4.043	24711	37534	1.044	1.503 #
2)	SA Decachlor...	10.813	9.379	36029	38464	2.465	1.972
Target Compounds							
29)	L6 AR-1254-4	8.009f	0.000	7550	0	8.638	N.D. #
30)	L6 AR-1254-5	8.411	0.000	10038	0	10.713	N.D. #
32)	L7 AR-1260-2	8.118	0.000	8903	0	8.620	N.D. #
33)	L7 AR-1260-3	8.511f	0.000	6662	0	8.830	N.D. #
35)	L7 AR-1260-5	0.000	7.973f	0	11679	N.D.	4.657 #
36)	L8 AR-1262-1	8.511f	0.000	6662	0	6.309	N.D. #
38)	L8 AR-1262-3	0.000	8.303f	0	11794	N.D.	10.571 #
41)	L9 AR-1268-1	0.000	8.303f	0	11794	N.D.	3.827 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP043017.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 1:30
Operator : AJ\MA
Sample : N1163-08 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 03:03:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

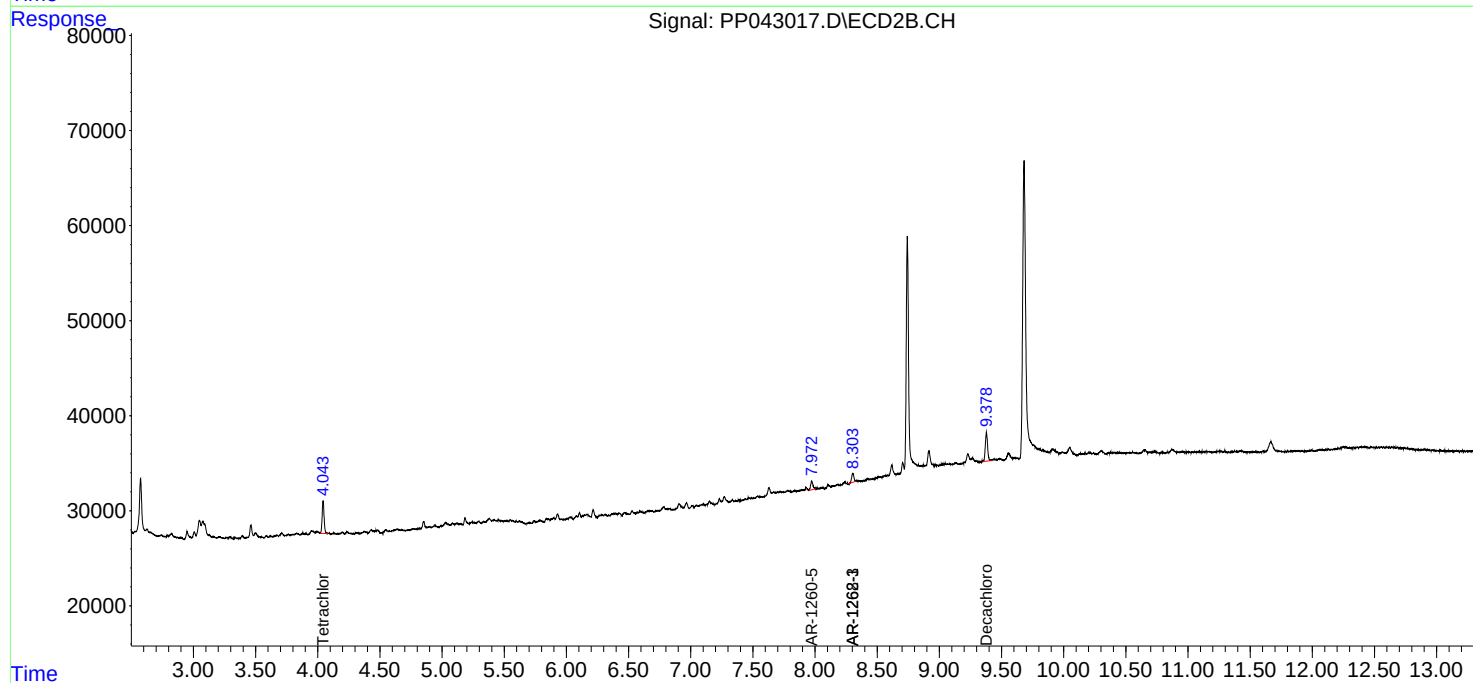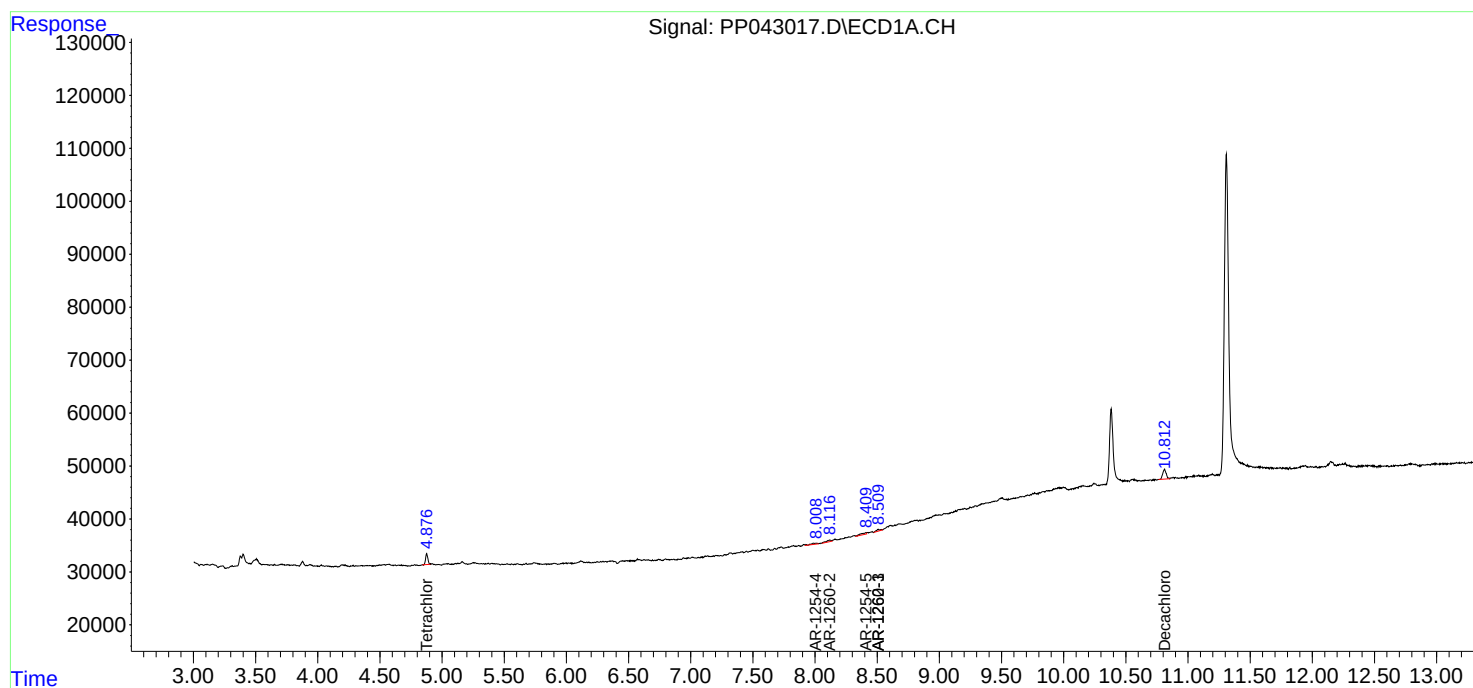


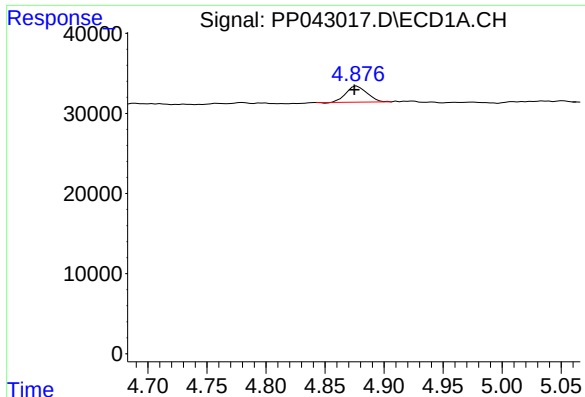

#1 Tetrachloro-m-xylene


R.T.: 4.877 min
Delta R.T.: 0.002 min
Response: 24711
Conc: 1.04 ng/ml

Instrument :
ECD_P
ClientSampleId :

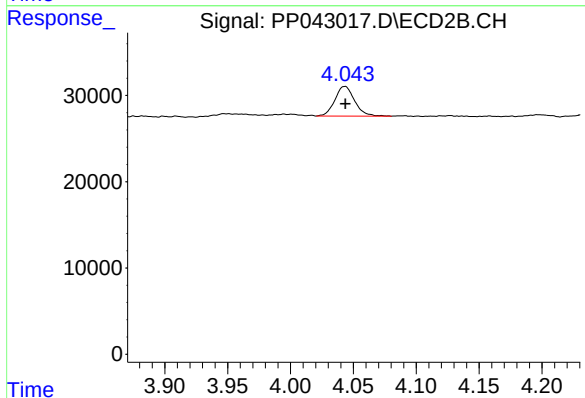


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 37534
Conc: 1.50 ng/ml

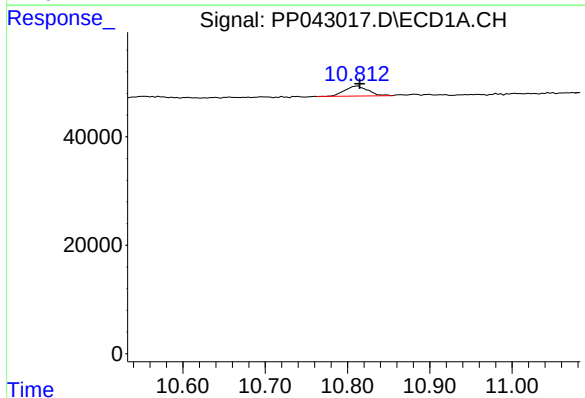


#2 Decachlorobiphenyl

R.T.: 10.813 min
Delta R.T.: -0.002 min
Response: 36029
Conc: 2.46 ng/ml

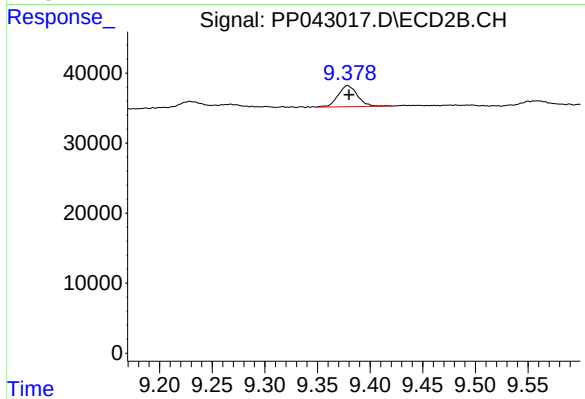

#2 Decachlorobiphenyl


R.T.: 9.379 min
Delta R.T.: -0.001 min
Response: 38464
Conc: 1.97 ng/ml

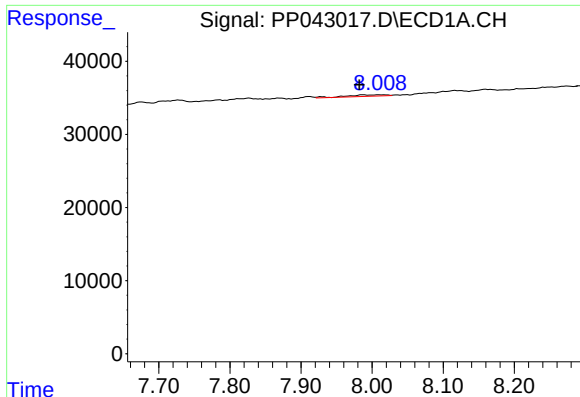

#29 AR-1254-4


R.T.: 8.009 min
Delta R.T.: 0.027 min
Response: 7550
Conc: 8.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

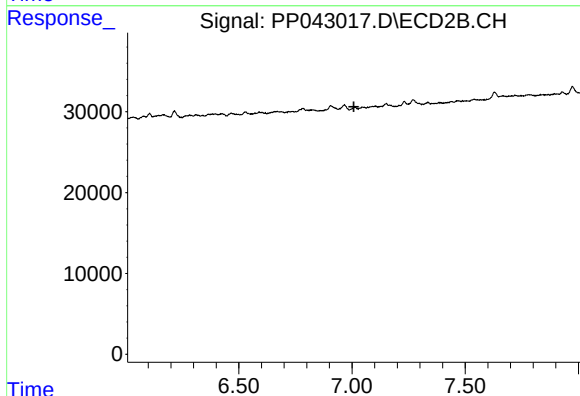


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

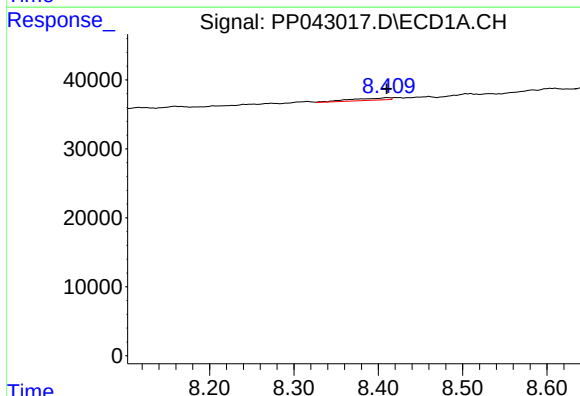


#30 AR-1254-5

R.T.: 8.411 min
Delta R.T.: 0.001 min
Response: 10038
Conc: 10.71 ng/ml

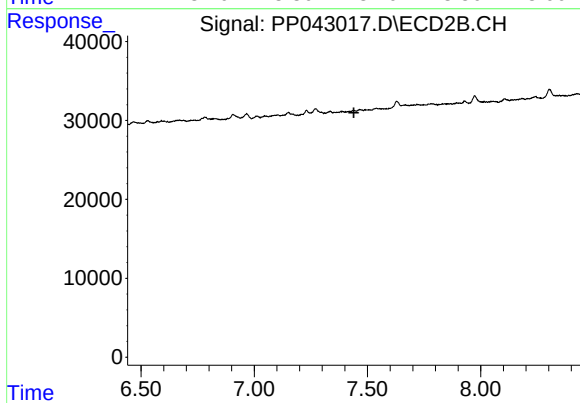

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

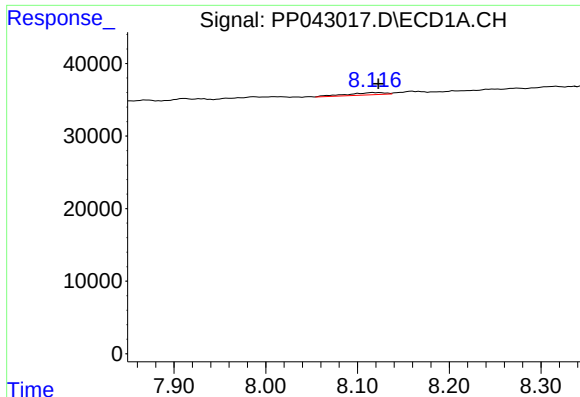

#32 AR-1260-2


R.T.: 8.118 min
Delta R.T.: -0.005 min
Response: 8903
Conc: 8.62 ng/ml

Instrument :
ECD_P
ClientSampleId :

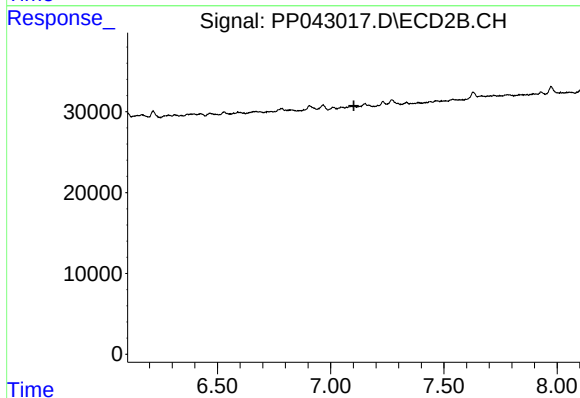


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.102 min
Response: 0
Conc: N.D.

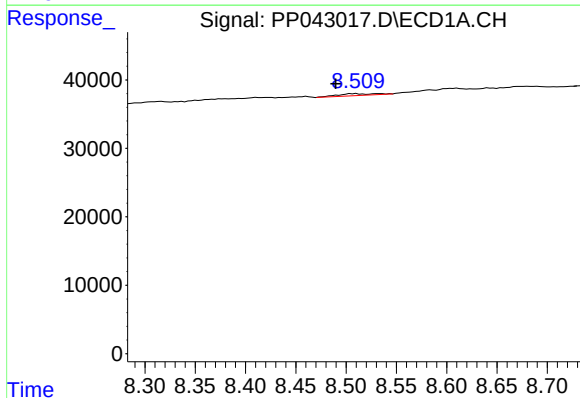


#33 AR-1260-3

R.T.: 8.511 min
Delta R.T.: 0.021 min
Response: 6662
Conc: 8.83 ng/ml

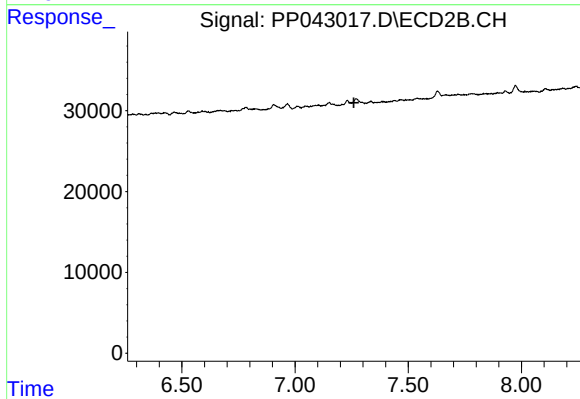

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 7.260 min
Response: 0
Conc: N.D.

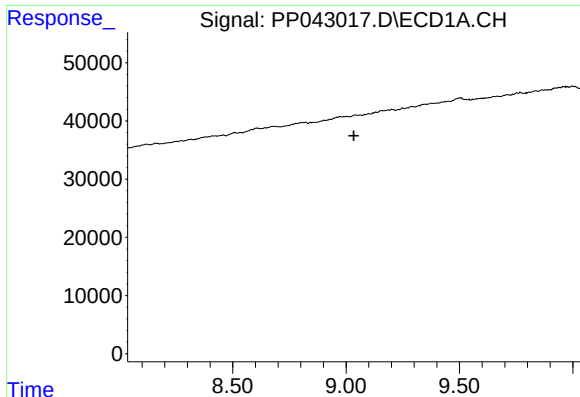

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 9.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

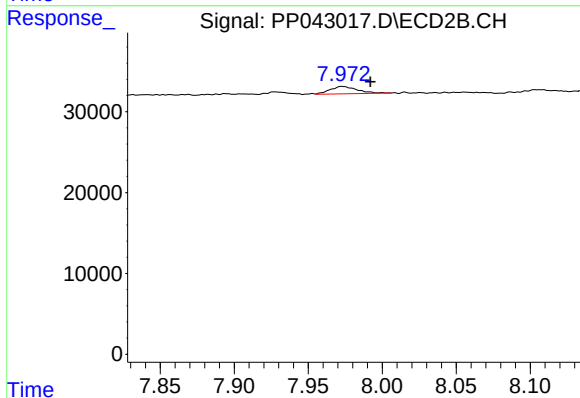


#35 AR-1260-5

R.T.: 7.973 min
Delta R.T.: -0.019 min
Response: 11679
Conc: 4.66 ng/ml

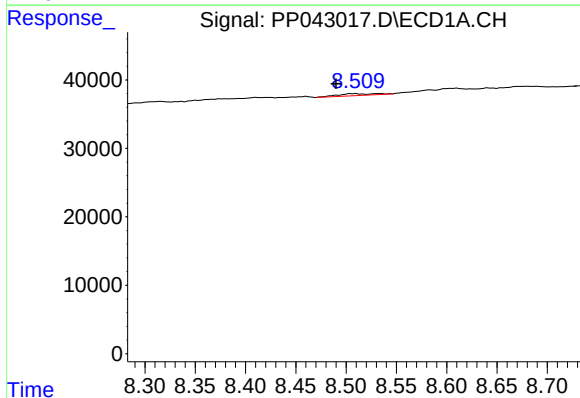


#36 AR-1262-1

R.T.: 8.511 min
Delta R.T.: 0.021 min
Response: 6662
Conc: 6.31 ng/ml

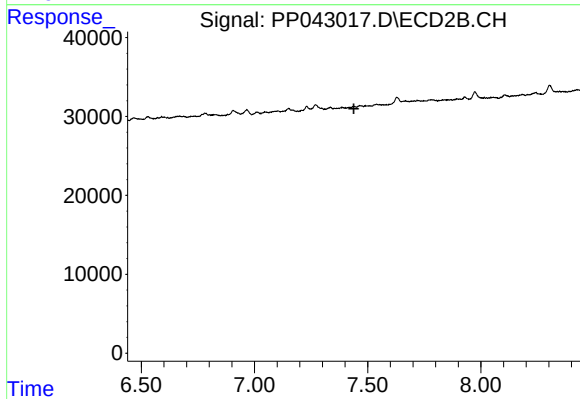

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.439 min
Response: 0
Conc: N.D.

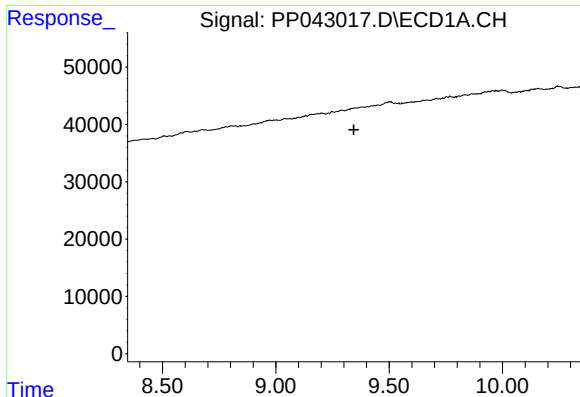

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

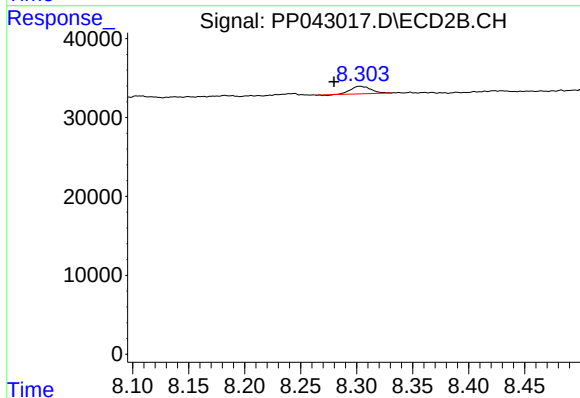


#38 AR-1262-3

R.T.: 8.303 min
Delta R.T.: 0.023 min
Response: 11794
Conc: 10.57 ng/ml

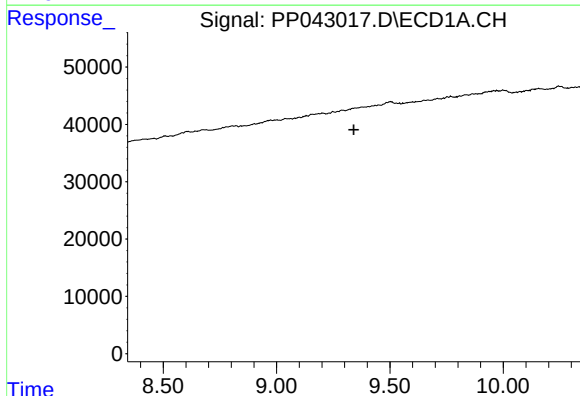

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.341 min
Response: 0
Conc: N.D.

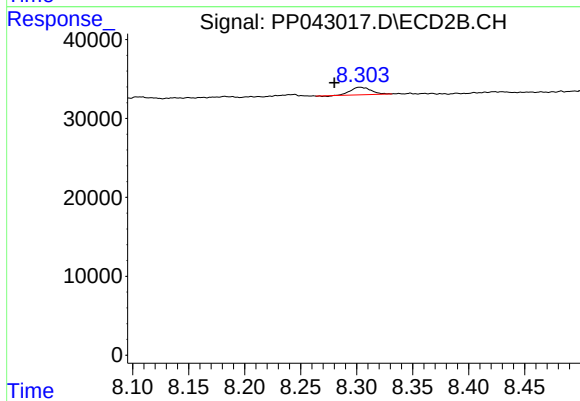

#41 AR-1268-1

R.T.: 8.303 min
Delta R.T.: 0.023 min
Response: 11794
Conc: 3.83 ng/ml