

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP043019.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2022 2:04
 Operator : AJ\MA
 Sample : N1163-10 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 18 03:04:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.878	4.044	32306	42636	1.365	1.707 #
2)	SA Decachlor...	10.813	9.381	48225	39978	3.299	2.049 #
Target Compounds							
30)	L6 AR-1254-5	8.423	0.000	3410	0	3.640	N.D. #
31)	L7 AR-1260-1	7.830f	6.908	8965	10536	9.401	8.151
33)	L7 AR-1260-3	0.000	7.271	0	14380	N.D.	9.949 #
35)	L7 AR-1260-5	9.042	7.976f	8432	16834	5.125	6.712 #
37)	L8 AR-1262-2	9.042	0.000	8432	0	4.871	N.D. #
38)	L8 AR-1262-3	0.000	8.304f	0	17282	N.D.	15.490 #
41)	L9 AR-1268-1	0.000	8.304f	0	17282	N.D.	5.607 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP043019.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2022 2:04
Operator : AJ\MA
Sample : N1163-10 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 18 03:04:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

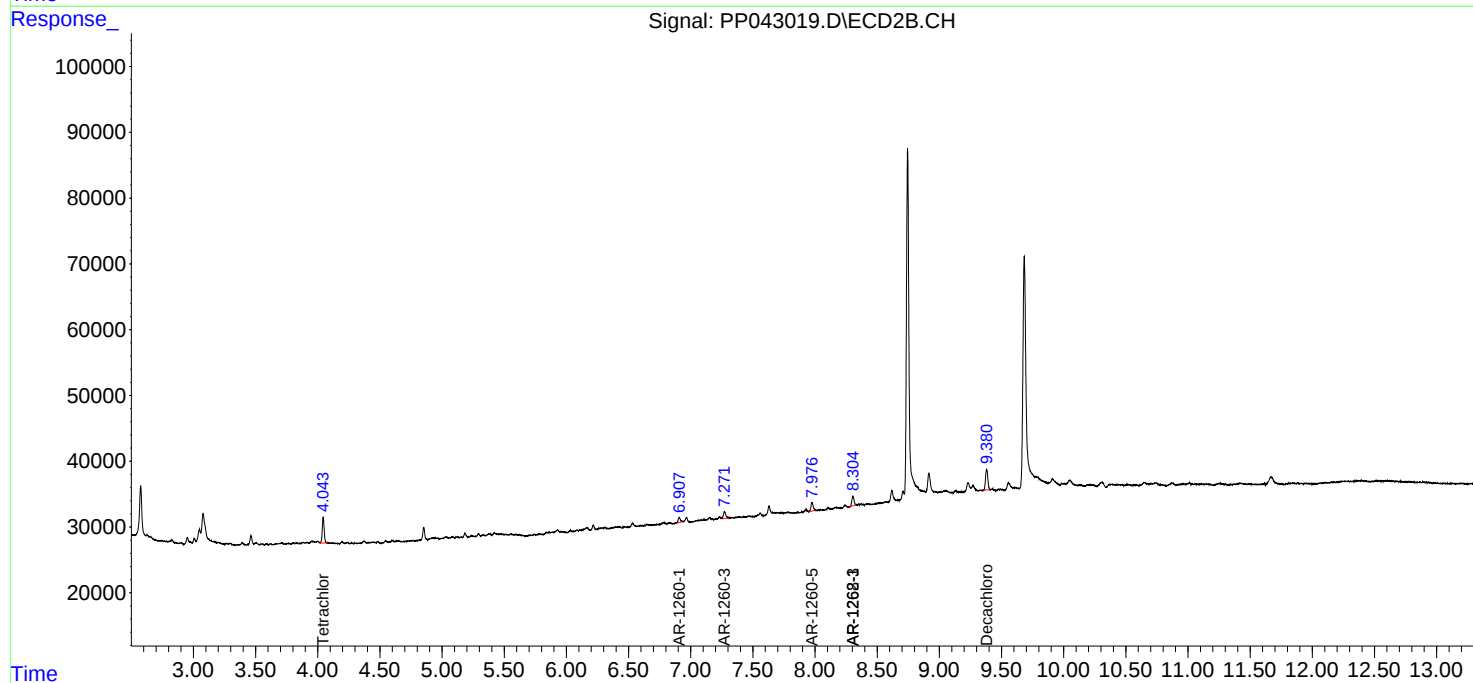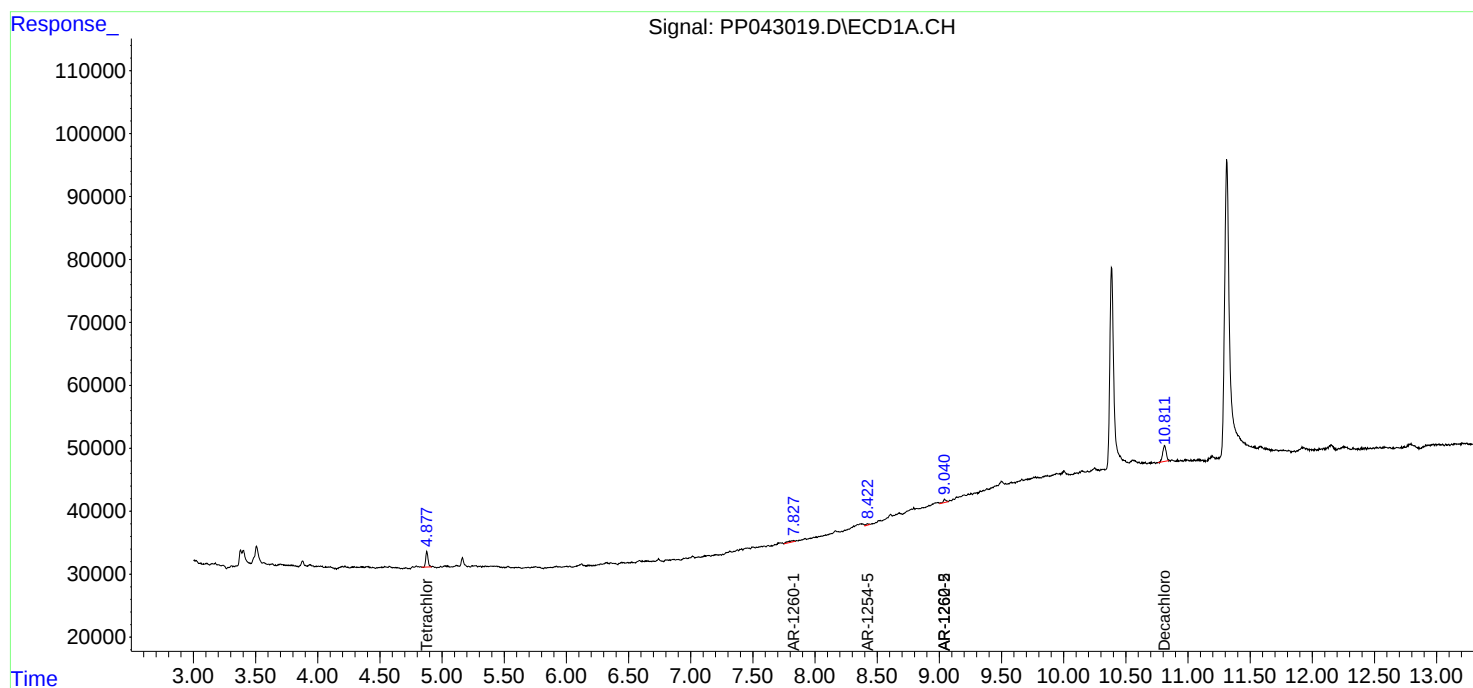


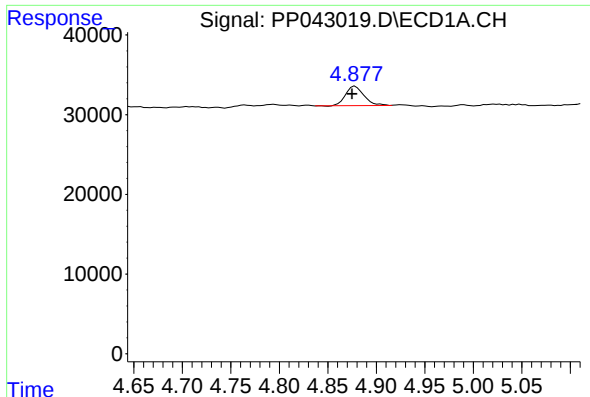

#1 Tetrachloro-m-xylene


R.T.: 4.878 min
Delta R.T.: 0.003 min
Response: 32306
Conc: 1.37 ng/ml

Instrument :
ECD_P
ClientSampleId :

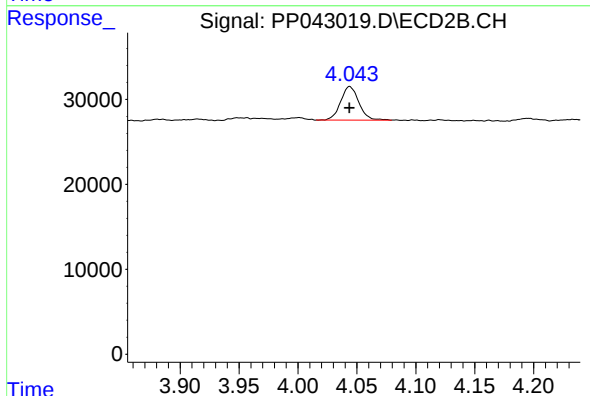


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 42636
Conc: 1.71 ng/ml

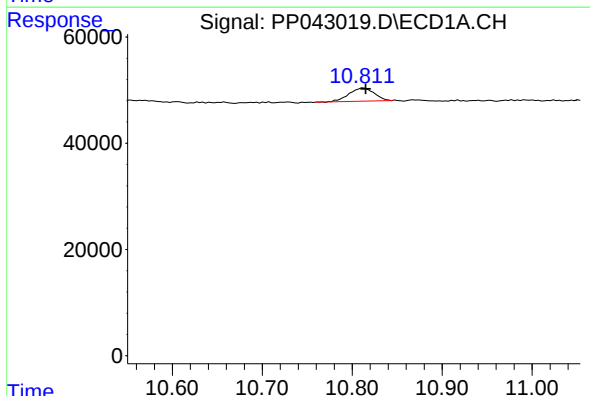


#2 Decachlorobiphenyl

R.T.: 10.813 min
Delta R.T.: -0.002 min
Response: 48225
Conc: 3.30 ng/ml

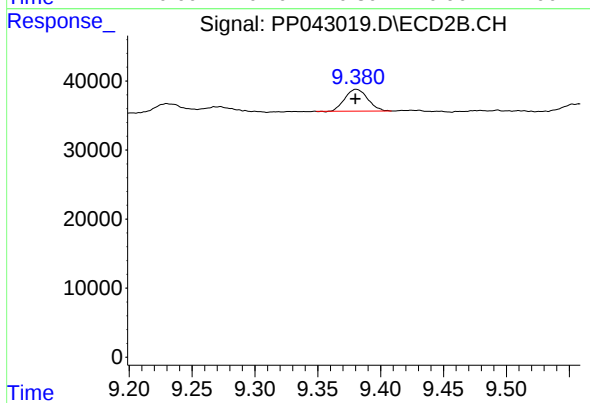

#2 Decachlorobiphenyl


R.T.: 9.381 min
Delta R.T.: 0.000 min
Response: 39978
Conc: 2.05 ng/ml

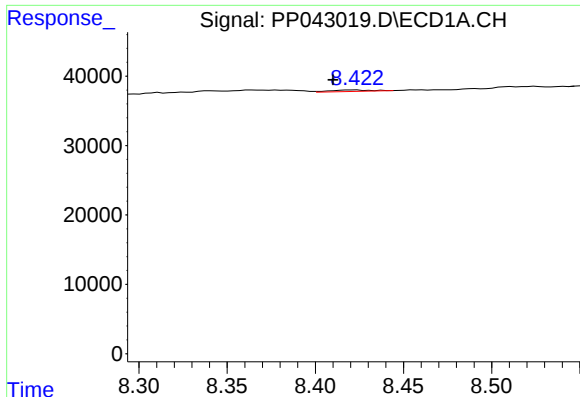

#30 AR-1254-5


R.T.: 8.423 min
Delta R.T.: 0.013 min
Response: 3410
Conc: 3.64 ng/ml

Instrument :
ECD_P
ClientSampleId :

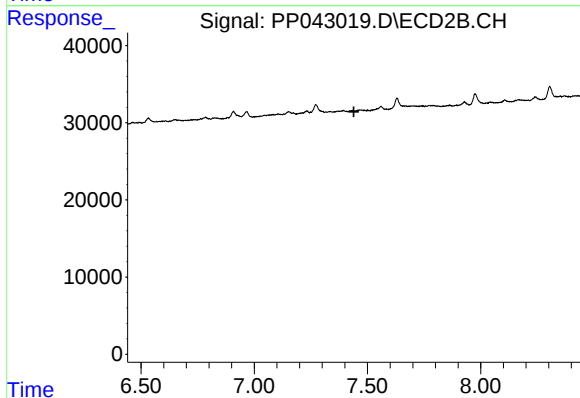


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

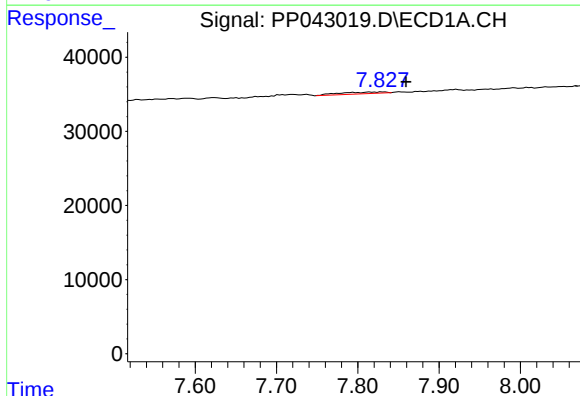


#31 AR-1260-1

R.T.: 7.830 min
Delta R.T.: -0.030 min
Response: 8965
Conc: 9.40 ng/ml

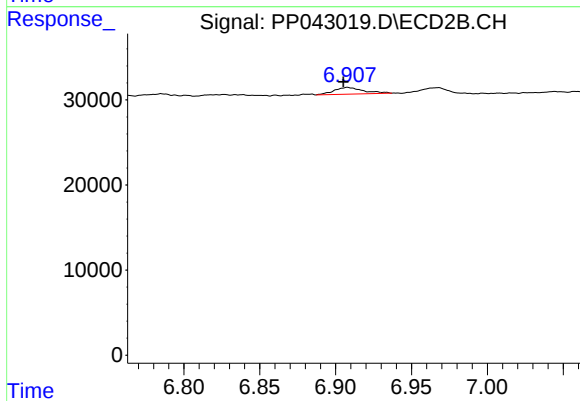

#31 AR-1260-1


R.T.: 6.908 min
Delta R.T.: 0.003 min
Response: 10536
Conc: 8.15 ng/ml

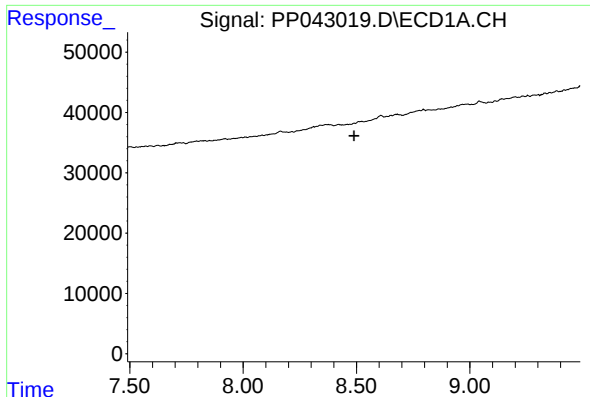

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.490 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

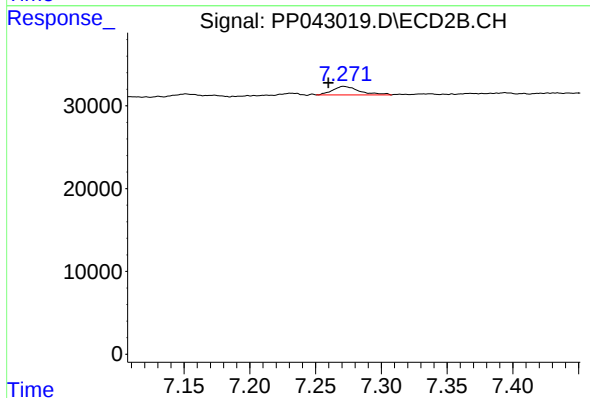


#33 AR-1260-3

R.T.: 7.271 min
Delta R.T.: 0.011 min
Response: 14380
Conc: 9.95 ng/ml

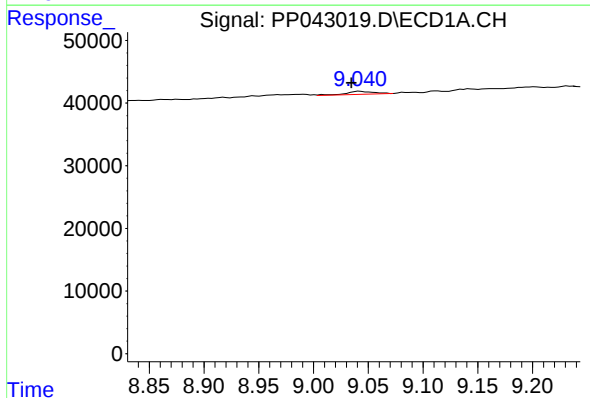


#35 AR-1260-5

R.T.: 9.042 min
Delta R.T.: 0.008 min
Response: 8432
Conc: 5.12 ng/ml

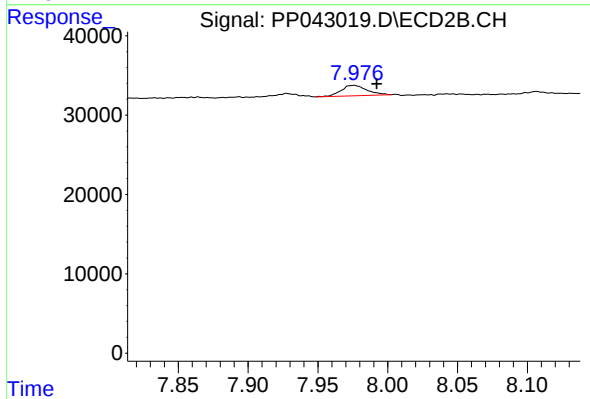

#35 AR-1260-5


R.T.: 7.976 min
Delta R.T.: -0.016 min
Response: 16834
Conc: 6.71 ng/ml

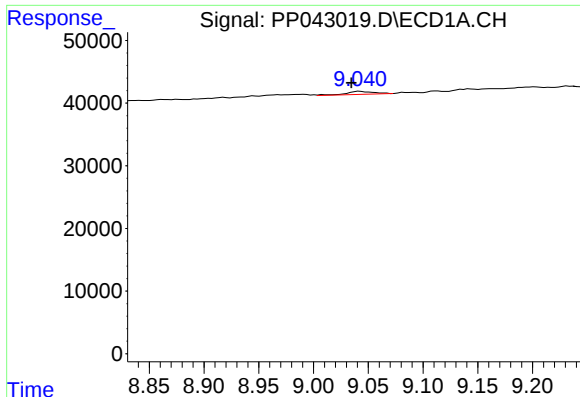

#37 AR-1262-2


R.T.: 9.042 min
Delta R.T.: 0.008 min
Response: 8432
Conc: 4.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

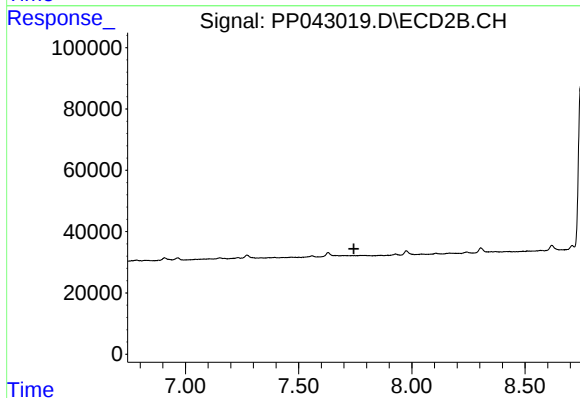


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

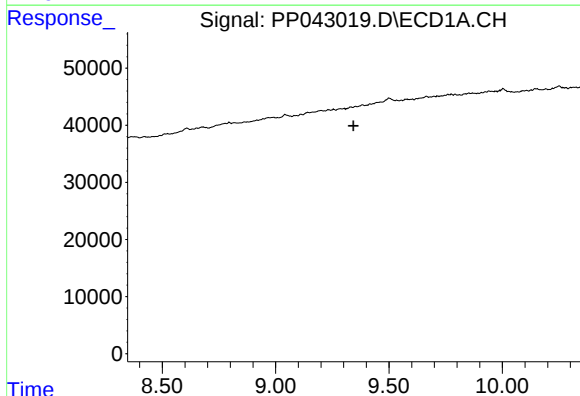


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.344 min
Response: 0
Conc: N.D.

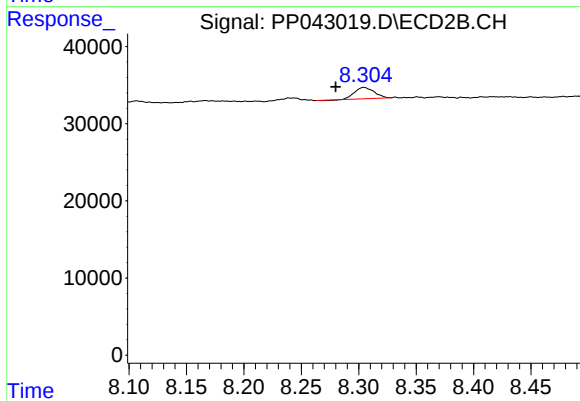

#38 AR-1262-3


R.T.: 8.304 min
Delta R.T.: 0.025 min
Response: 17282
Conc: 15.49 ng/ml

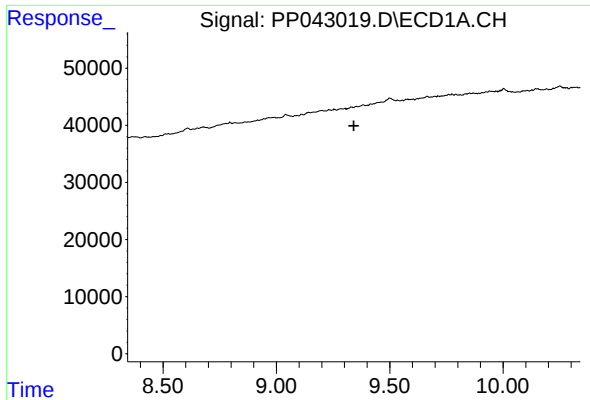

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

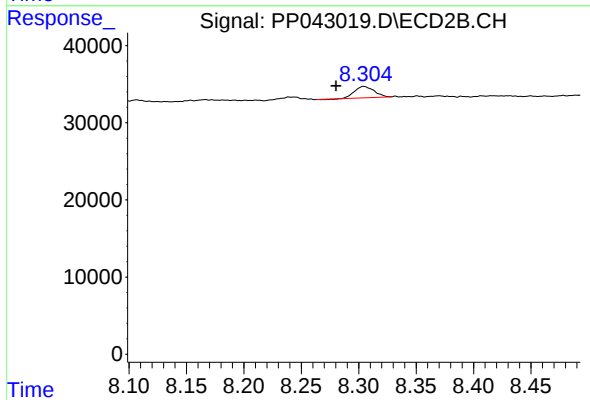

#41 AR-1268-1

R.T.: 8.304 min
Delta R.T.: 0.024 min
Response: 17282
Conc: 5.61 ng/ml