

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP042974.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2022 12:15
 Operator : AJ\MA
 Sample : N1143-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WEST-BOILER-ROOM-NORTH-SIDEWALL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 16:36:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.879	4.044	473268	534223	20.002	21.389
2)	SA Decachlor...	10.821	9.386	320156	432089	21.901	22.151

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP042974.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2022 12:15
Operator : AJ\MA
Sample : N1143-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
WEST-BOILER-ROOM-NORTH-SIDEWALL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 16:36:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

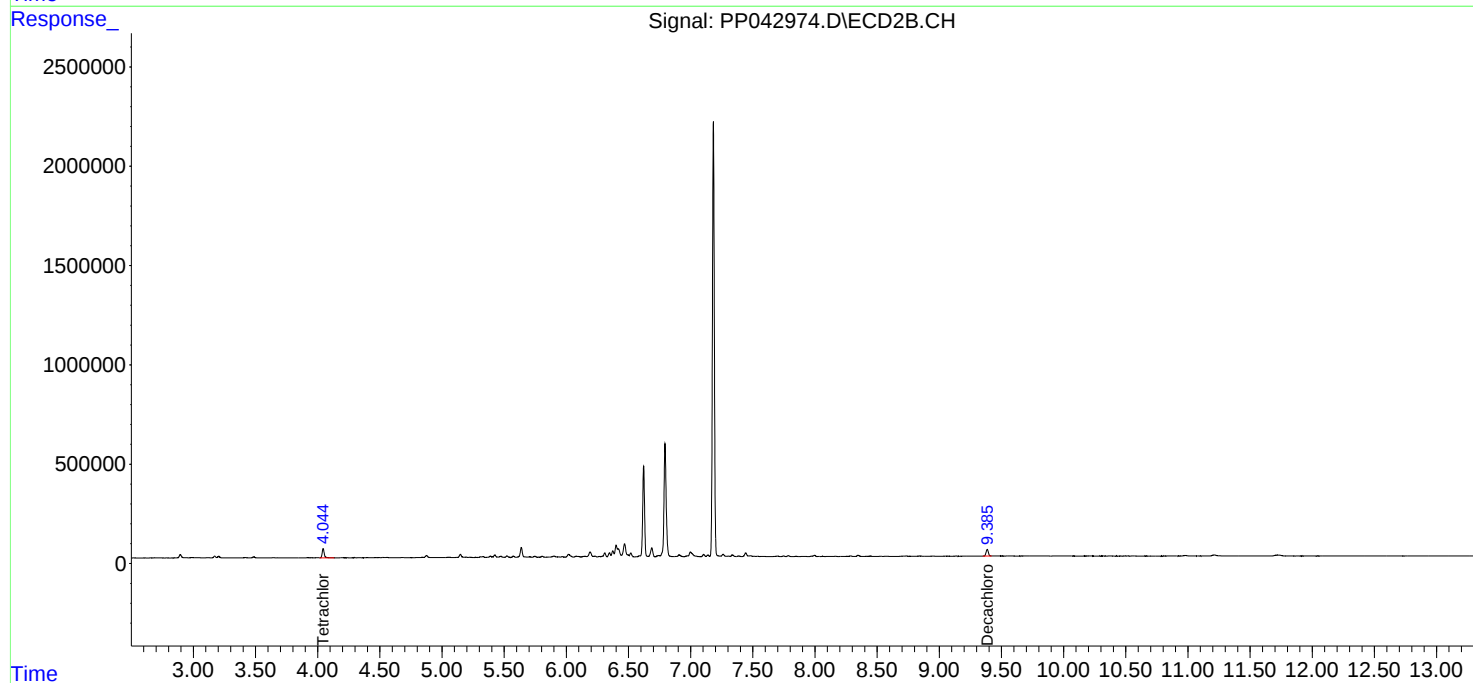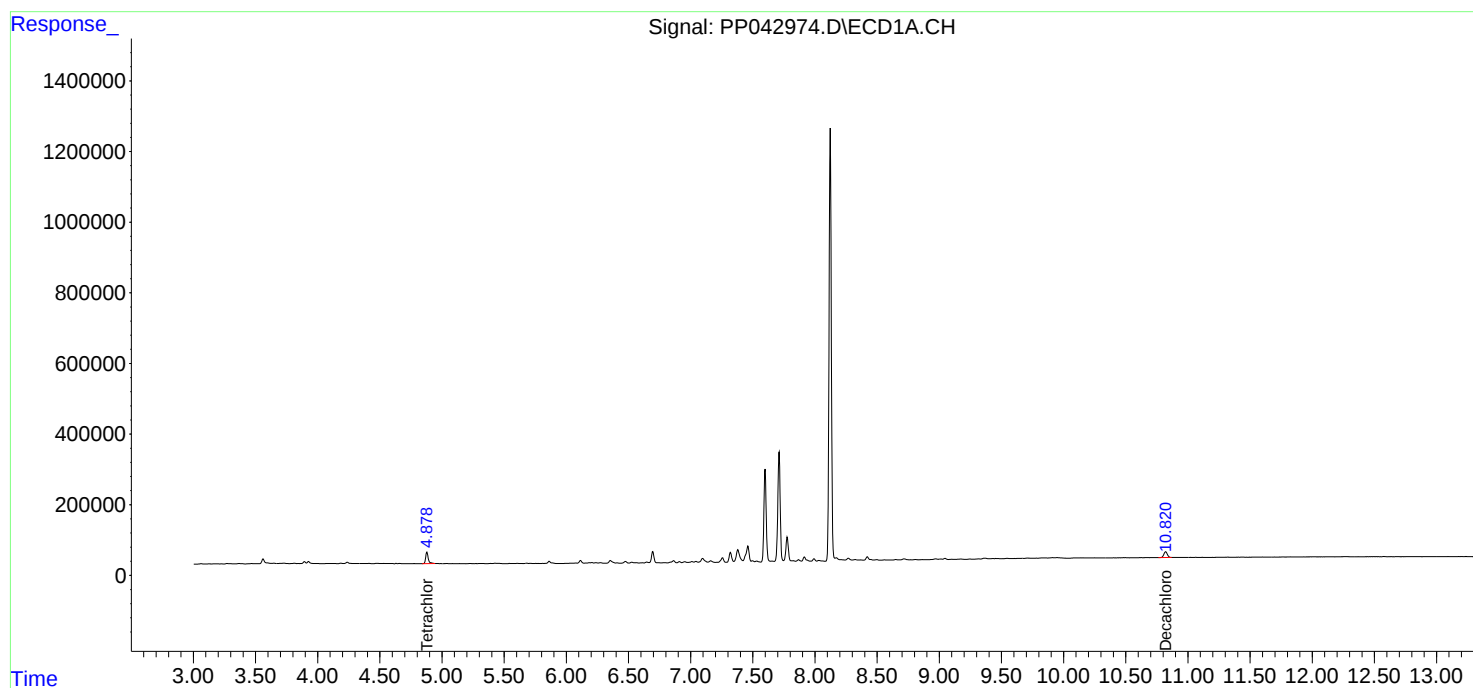


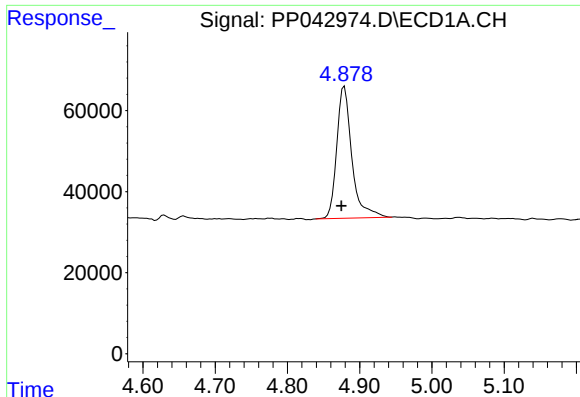

#1 Tetrachloro-m-xylene


R.T.: 4.879 min
Delta R.T.: 0.004 min
Response: 473268
Conc: 20.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
WEST-BOILER-ROOM-NORTH-SIDEWALL

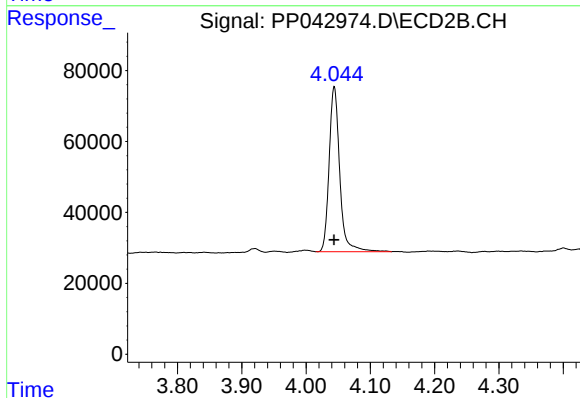


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 534223
Conc: 21.39 ng/ml

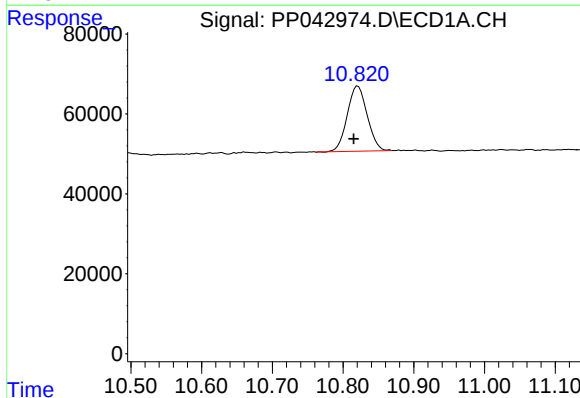

#2 Decachlorobiphenyl

R.T.: 10.821 min
Delta R.T.: 0.006 min
Response: 320156
Conc: 21.90 ng/ml

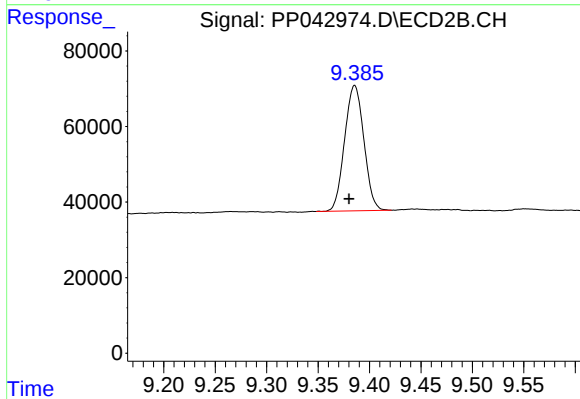

#2 Decachlorobiphenyl

R.T.: 9.386 min
Delta R.T.: 0.006 min
Response: 432089
Conc: 22.15 ng/ml