

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
 Data File : PP042976.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jan 2022 12:48
 Operator : AJ\MA
 Sample : N1167-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MR-PIPE-B

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
 Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 17 16:37:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.877	4.043	583857	641259	24.676	25.675
2) SA Decachlor...	10.819	9.383	391563	548247	26.785	28.106
Target Compounds						
16) L4 AR-1242-1	6.181	5.308	19191	24148	32.391	30.133
17) L4 AR-1242-2	6.205	5.329	41057	42351	46.019	37.403
18) L4 AR-1242-3	6.271	5.524	18757	26976	33.806m	42.308 #
19) L4 AR-1242-4	6.374	5.618	13668	48842	30.040m	79.514 #
20) L4 AR-1242-5	7.156	6.186	56742	70107	126.498	97.430

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP011722\
Data File : PP042976.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jan 2022 12:48
Operator : AJ\MA
Sample : N1167-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MR-PIPE-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 17 16:37:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

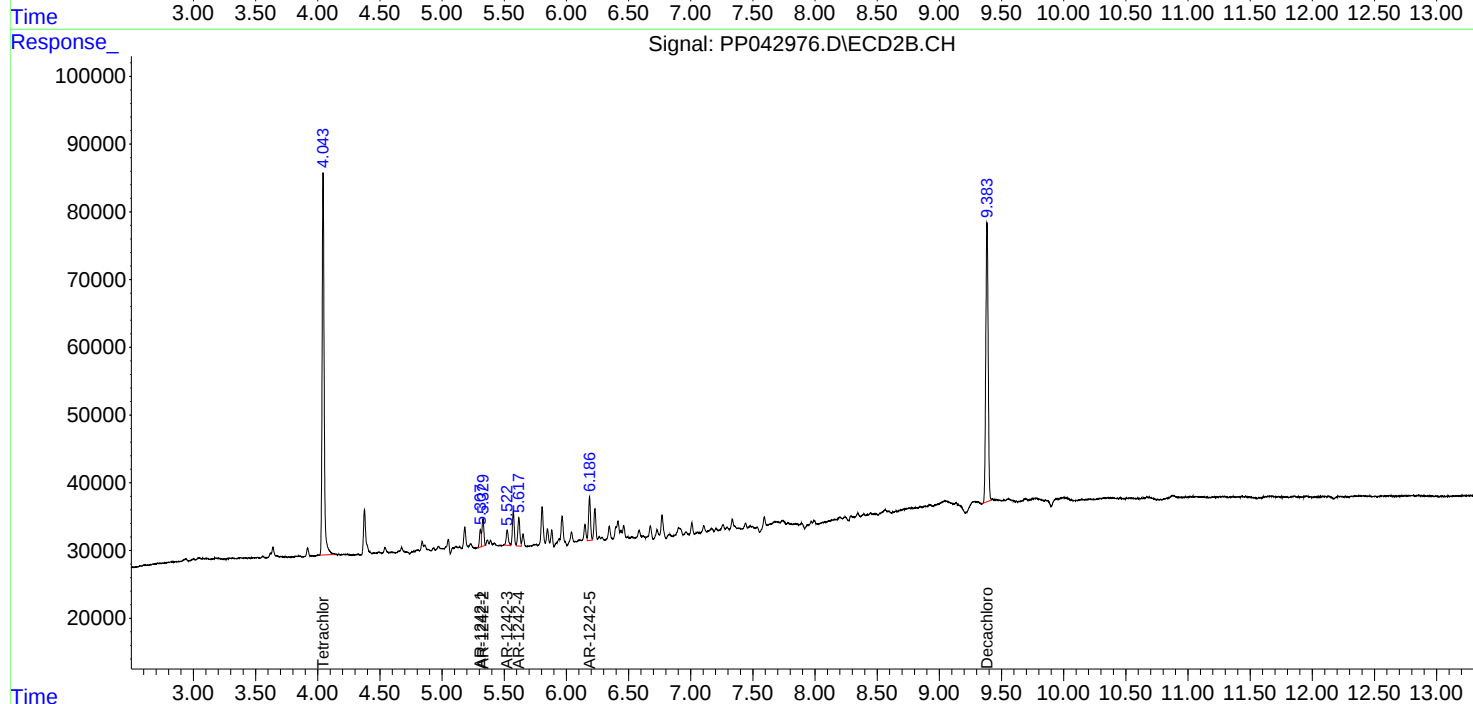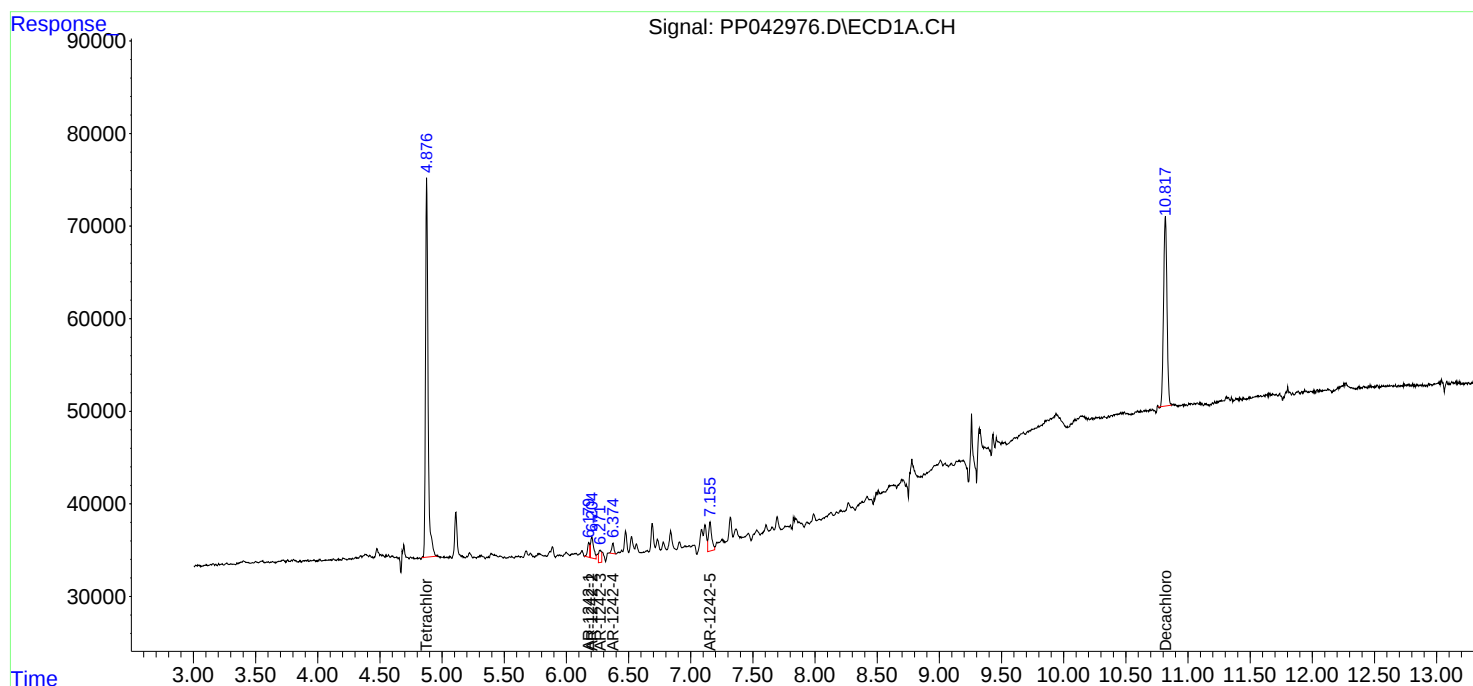

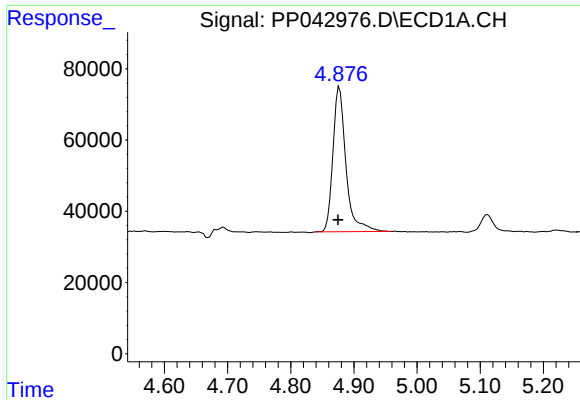


#1 Tetrachloro-m-xylene

R.T.: 4.877 min
Delta R.T.: 0.002 min
Response: 583857
Conc: 24.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

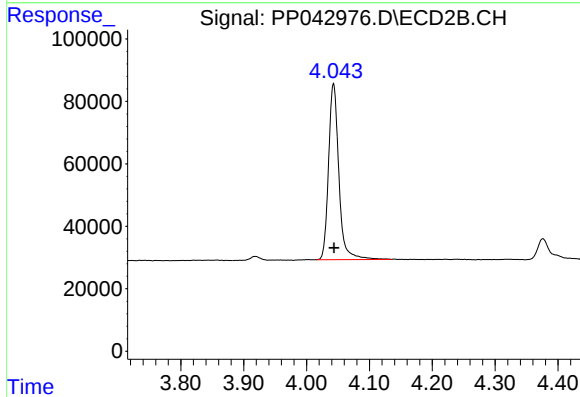


#1 Tetrachloro-m-xylene

R.T.: 4.043 min
Delta R.T.: 0.000 min
Response: 641259
Conc: 25.67 ng/ml

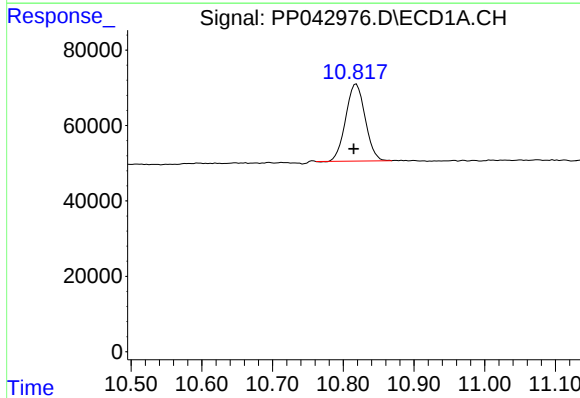


#2 Decachlorobiphenyl

R.T.: 10.819 min
Delta R.T.: 0.004 min
Response: 391563
Conc: 26.79 ng/ml

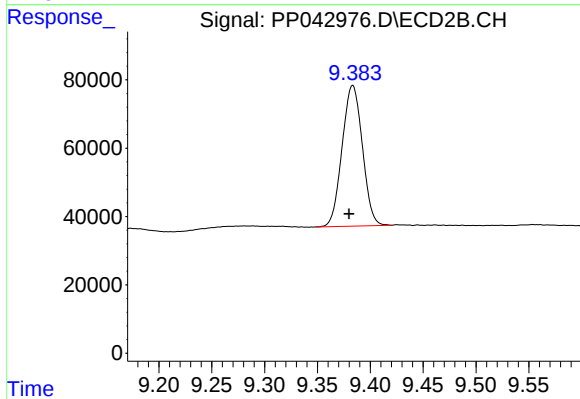

#2 Decachlorobiphenyl

R.T.: 9.383 min
Delta R.T.: 0.003 min
Response: 548247
Conc: 28.11 ng/ml

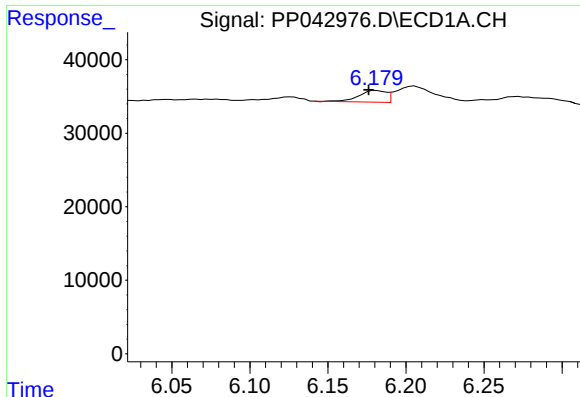


#16 AR-1242-1

R.T.: 6.181 min
Delta R.T.: 0.005 min
Response: 19191
Conc: 32.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

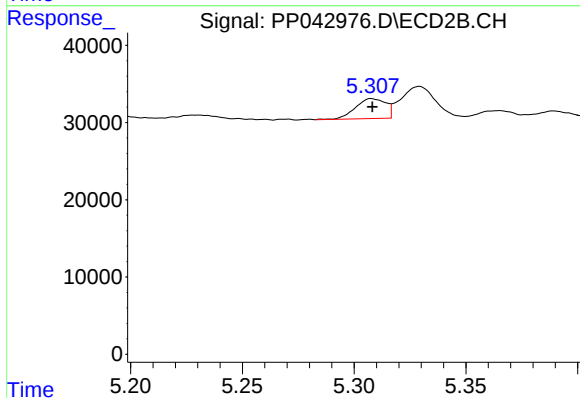


#16 AR-1242-1

R.T.: 5.308 min
Delta R.T.: 0.000 min
Response: 24148
Conc: 30.13 ng/ml

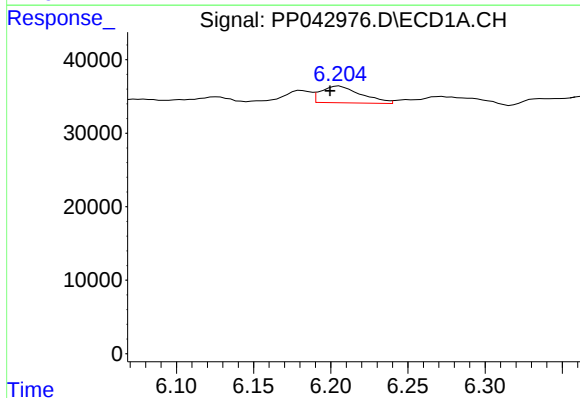


#17 AR-1242-2

R.T.: 6.205 min
Delta R.T.: 0.006 min
Response: 41057
Conc: 46.02 ng/ml

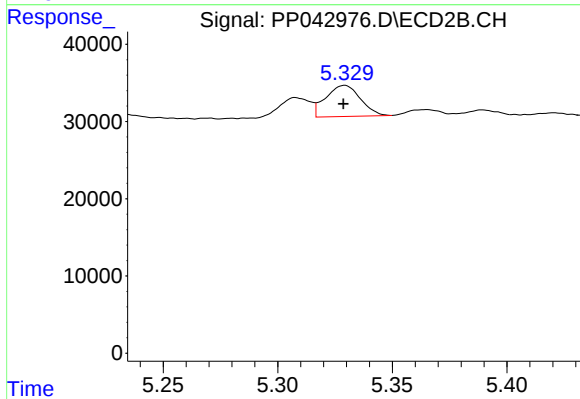

#17 AR-1242-2

R.T.: 5.329 min
Delta R.T.: 0.000 min
Response: 42351
Conc: 37.40 ng/ml

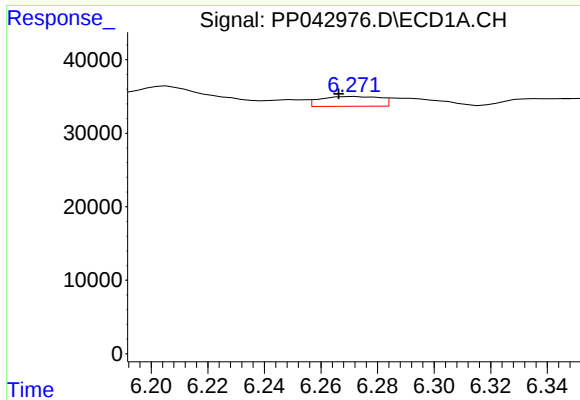


#18 AR-1242-3

R.T.: 6.271 min
Delta R.T.: 0.005 min
Response: 18757
Conc: 33.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-B


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

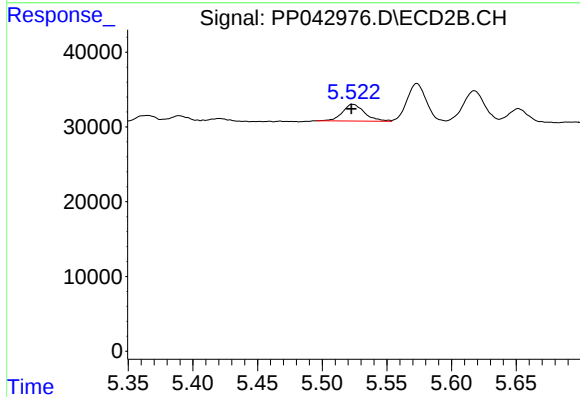


#18 AR-1242-3

R.T.: 5.524 min
Delta R.T.: 0.001 min
Response: 26976
Conc: 42.31 ng/ml

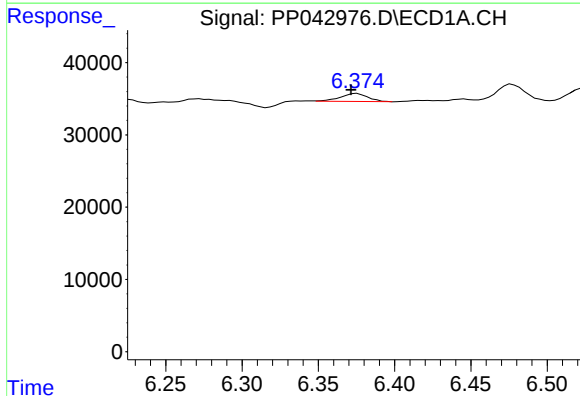


#19 AR-1242-4

R.T.: 6.374 min
Delta R.T.: 0.003 min
Response: 13668
Conc: 30.04 ng/ml m

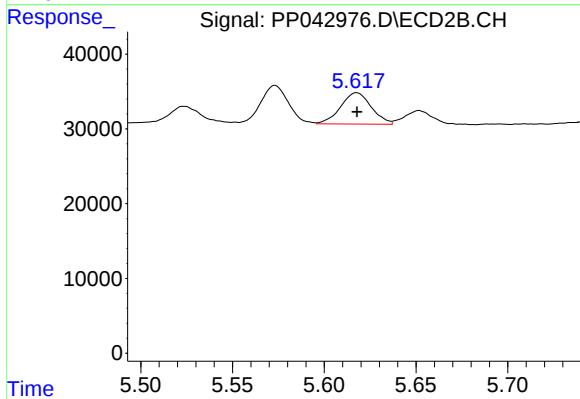

#19 AR-1242-4

R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 48842
Conc: 79.51 ng/ml

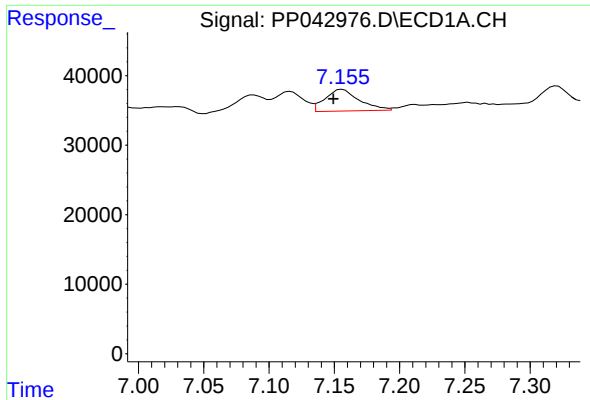


#20 AR-1242-5

R.T.: 7.156 min
Delta R.T.: 0.007 min
Response: 56742
Conc: 126.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
MR-PIPE-B

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/18/2022
Supervised By :Yogesh Patel 01/18/2022

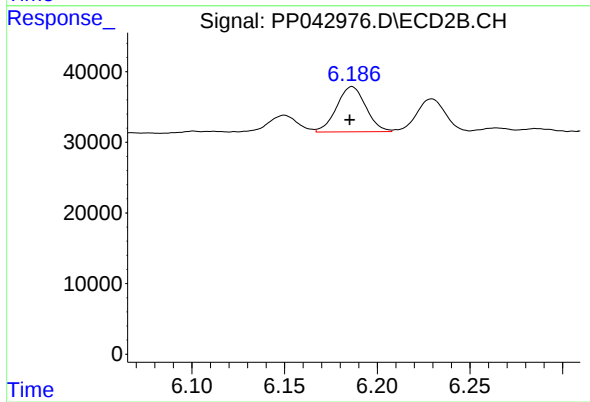

#20 AR-1242-5

R.T.: 6.186 min
Delta R.T.: 0.001 min
Response: 70107
Conc: 97.43 ng/ml